

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX041518\
 Data File : VX000892.D
 Acq On : 15 Apr 2018 13:13
 Operator : JC/MD
 Sample : PB108205ZHE#02 5X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB108205ZHE#02 5X

Quant Time: Apr 16 08:15:48 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 10 15:49:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	276914	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	370959	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	341389	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	225309	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	162988	46.68	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.36%	
35) Dibromofluoromethane	5.51	113	132014	46.19	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.38%	
50) Toluene-d8	8.72	98	510626	47.98	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.96%	
62) 4-Bromofluorobenzene	11.15	95	199164	45.24	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.48%	


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX041518\
Data File : VX000892.D
Acq On : 15 Apr 2018 13:13
Operator : JC/MD
Sample : PB108205ZHE#02 5X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB108205ZHE#02 5X

Quant Time: Apr 16 08:15:48 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 10 15:49:28 2018
Response via : Initial Calibration

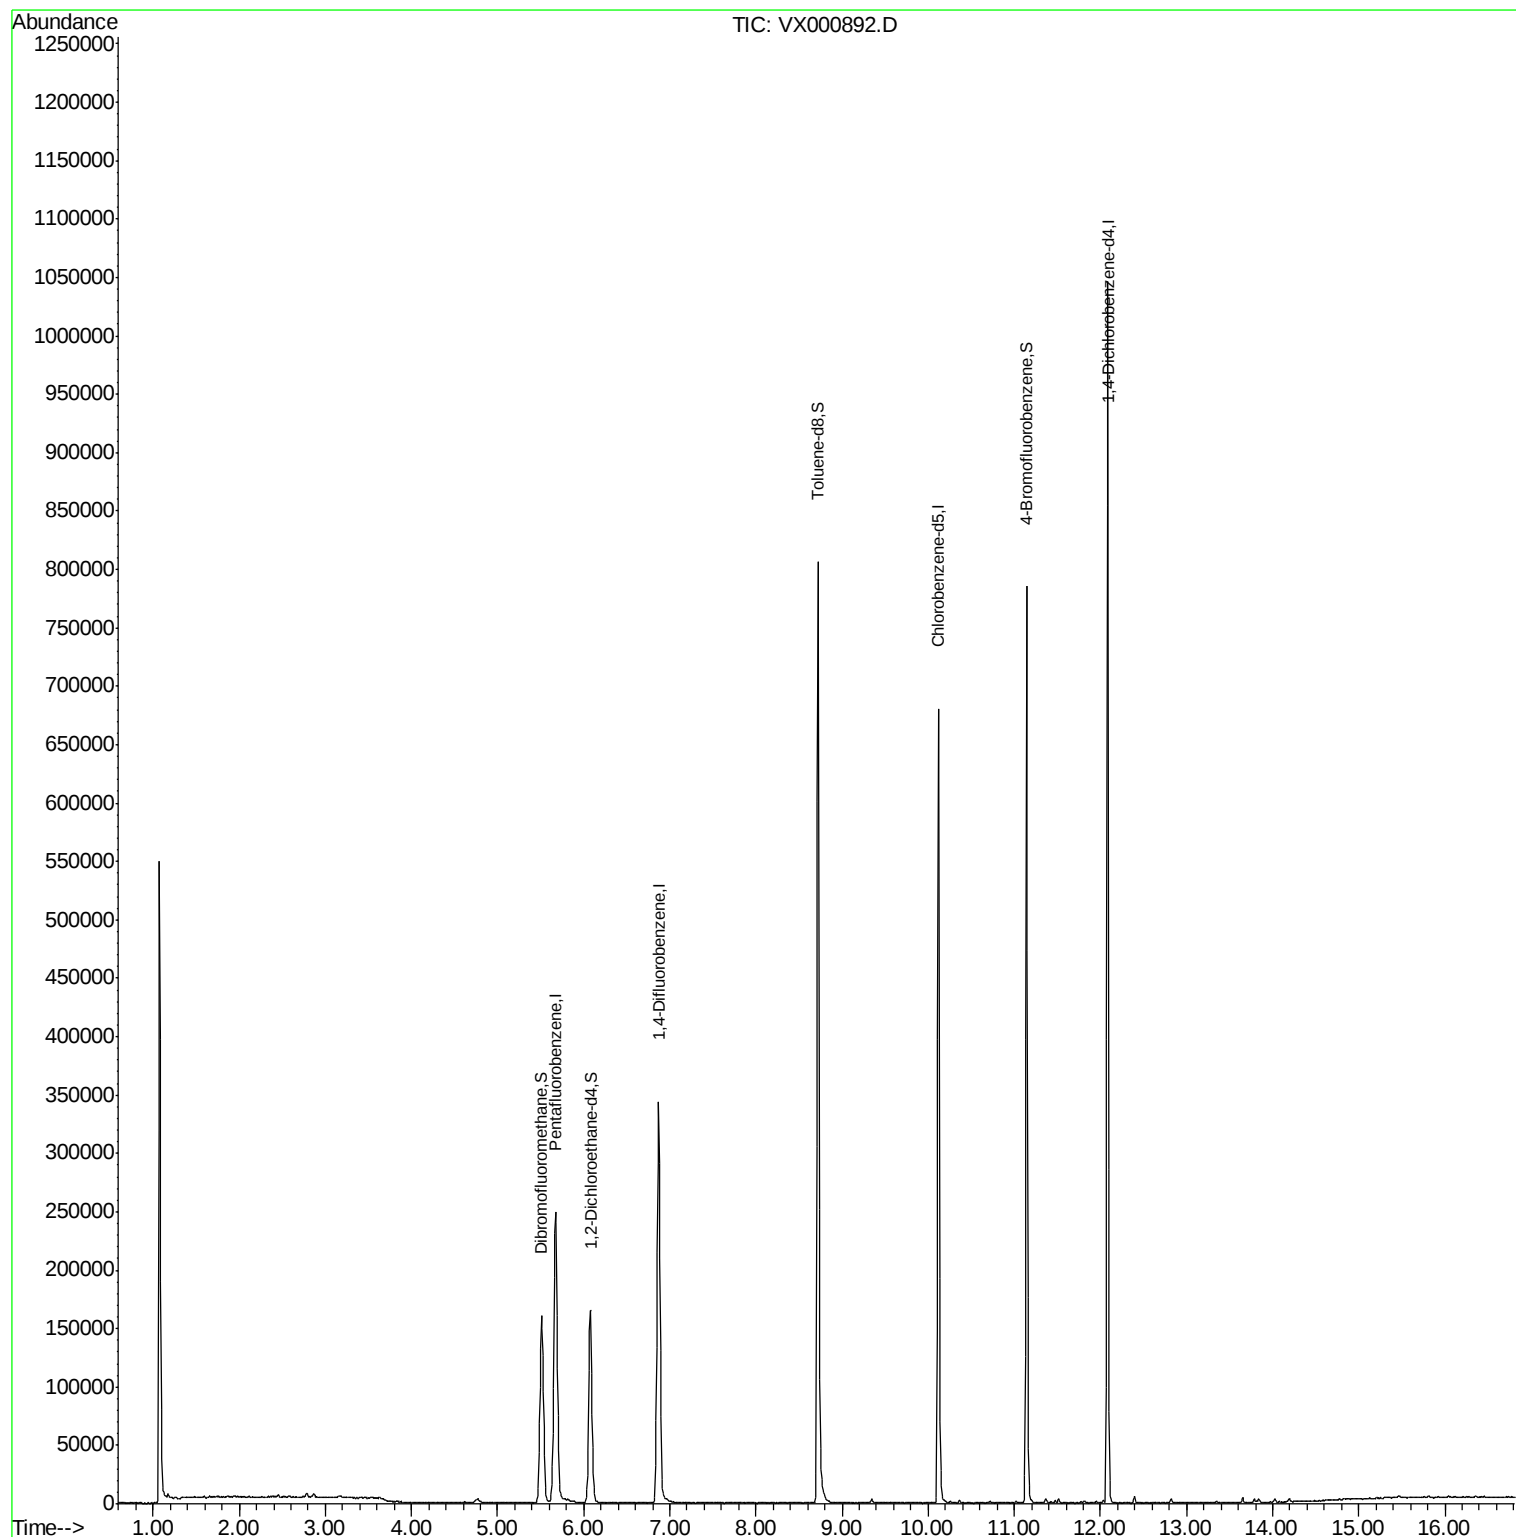



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.00 min

Lab File: VX000892.D

Acq: 15 Apr 2018 13:13

Instrument :

MSVOA_X

ClientSampleId :


PB108205ZHE#02 5X

Tot Ion:168 Resp: 276914

Ion Ratio Lower Upper




168 100

99 47.1 38.3 57.5

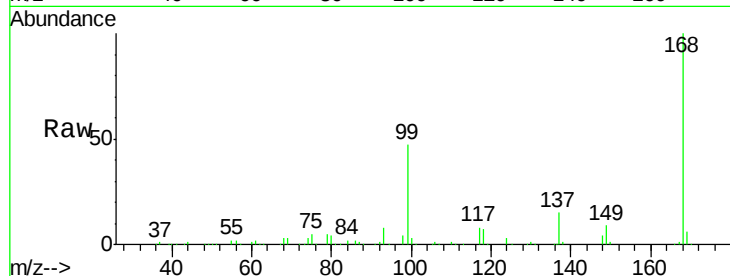

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

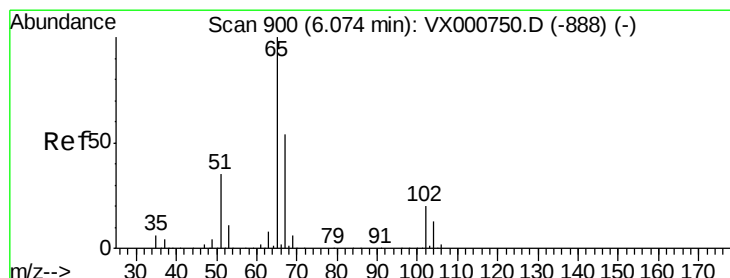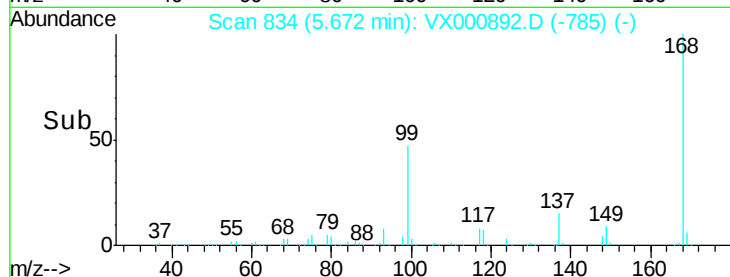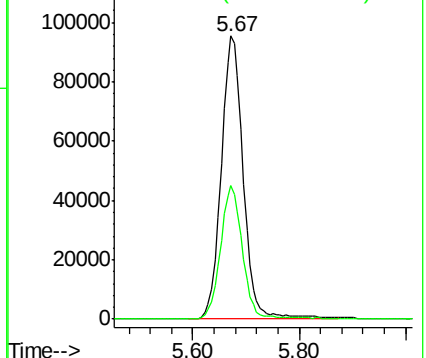

#33

1,2-Dichloroethane-d4

Concen: 46.68 ug/l

RT: 6.07 min Scan# 900

Delta R.T. -0.00 min

Lab File: VX000892.D


Acq: 15 Apr 2018 13:13

Tgt Ion: 65 Resp: 162988

Ion Ratio Lower Upper



65 100


67 51.5 0.0 103.8

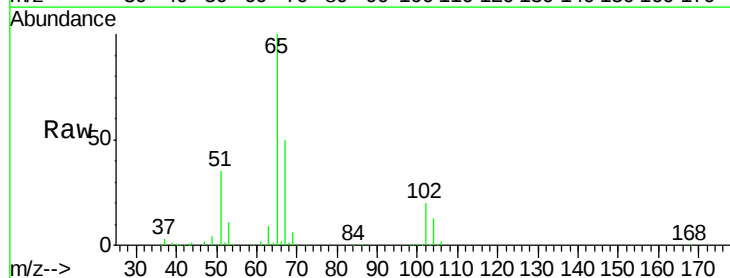

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

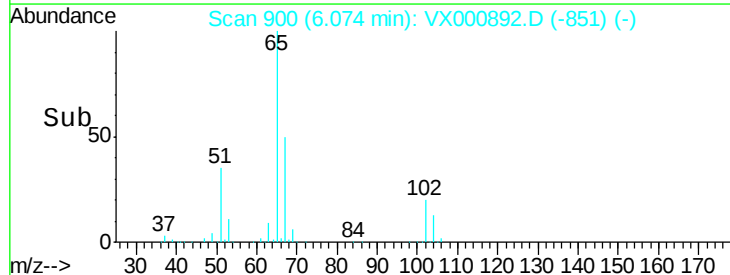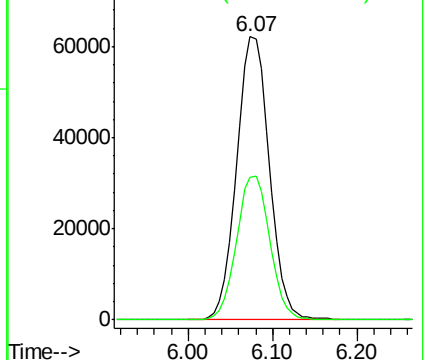

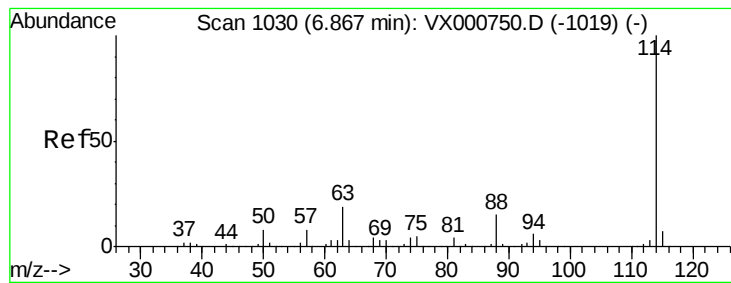

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1031

Delta R.T. 0.01 min

Lab File: VX000892.D

Acq: 15 Apr 2018 13:13

Instrument :

MSVOA_X

ClientSampleId :

PB108205ZHE#02 5X


Tot Ion:114 Resp: 370959

Ion Ratio Lower Upper

114 100

63 19.2 0.0 38.4




88 15.7 0.0 31.0

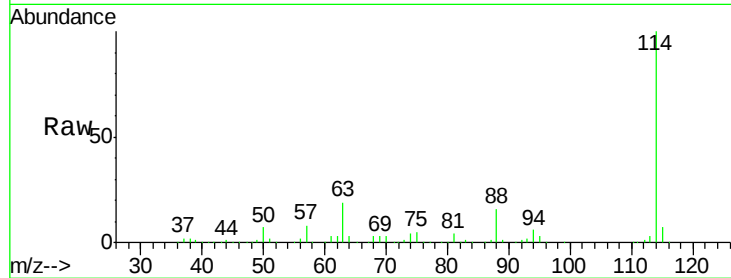

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

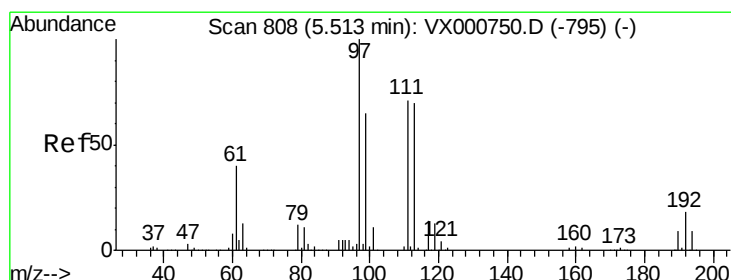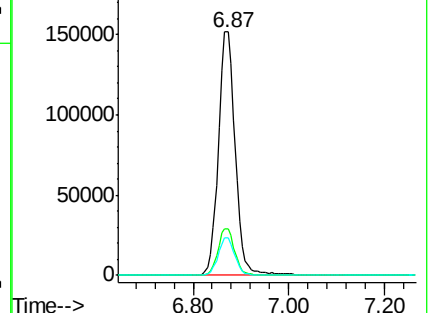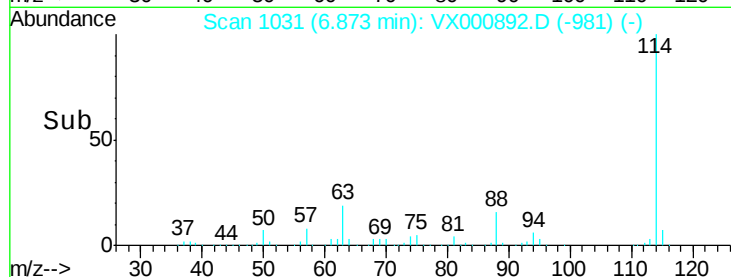

#35

Dibromofluoromethane

Concen: 46.19 ug/l

RT: 5.51 min Scan# 808

Delta R.T. -0.00 min

Lab File: VX000892.D

Acq: 15 Apr 2018 13:13


Tgt Ion:113 Resp: 132014

Ion Ratio Lower Upper

113 100

111 102.6 81.5 122.3



192 25.9 20.4 30.6

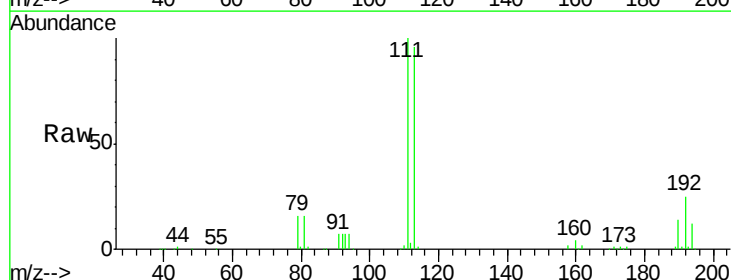


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



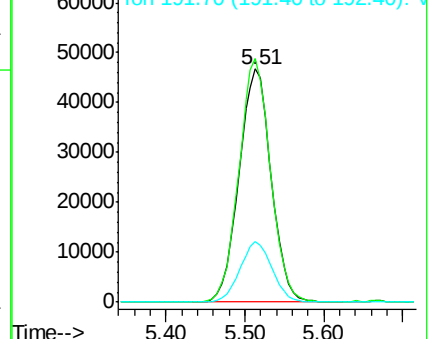
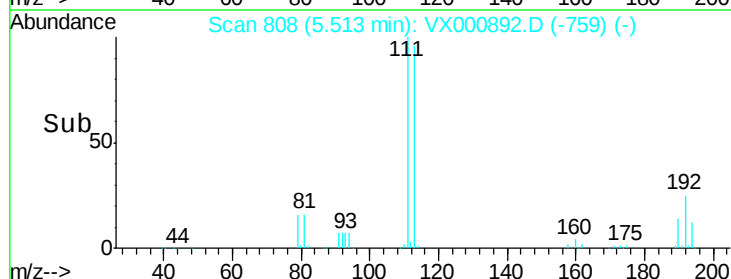


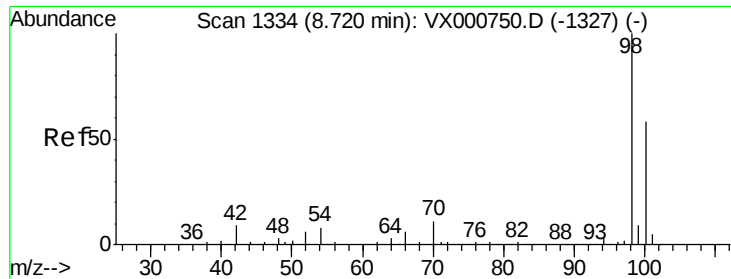

#50
Toluene-d8
Concen: 47.98 ug/l
RT: 8.72 min Scan# 1334
Delta R.T. -0.00 min
Lab File: VX000892.D
Acq: 15 Apr 2018 13:13




Instrument :
MSVOA_X
ClientSampleId :
PB108205ZHE#02 5X

Tot Ion: 98 Resp: 510626
Ion Ratio Lower Upper
98 100
100 64.8 52.6 79.0

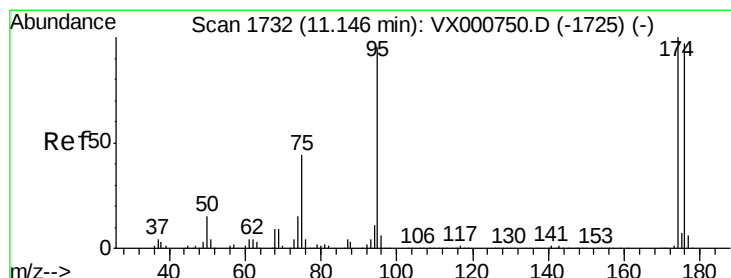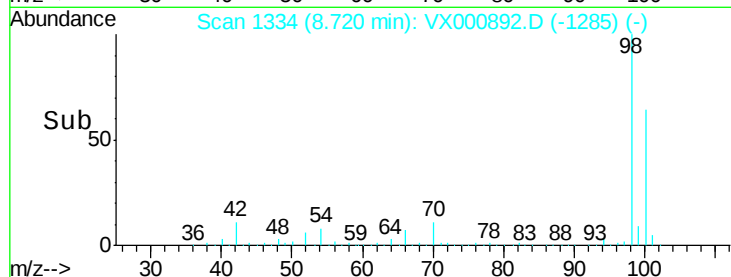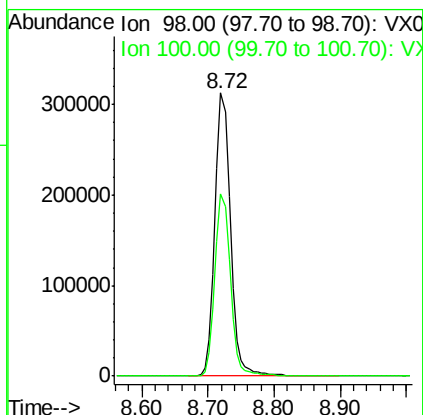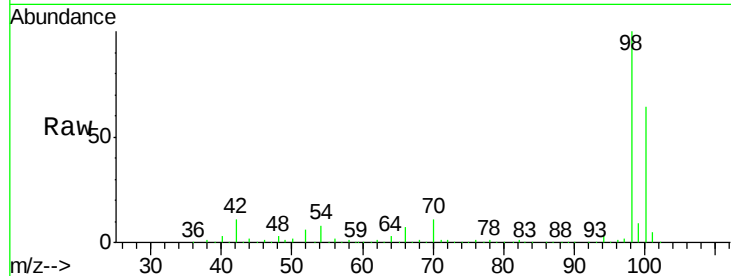

#62
4-Bromofluorobenzene
Concen: 45.24 ug/l
RT: 11.15 min Scan# 1732
Delta R.T. -0.00 min
Lab File: VX000892.D
Acq: 15 Apr 2018 13:13

Tgt Ion: 95 Resp: 199164
Ion Ratio Lower Upper
95 100
174 99.0 0.0 198.4
176 95.6 0.0 194.4

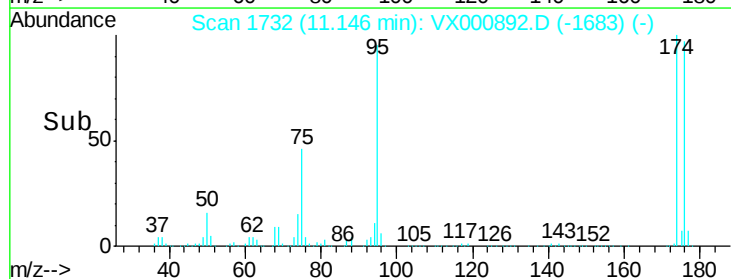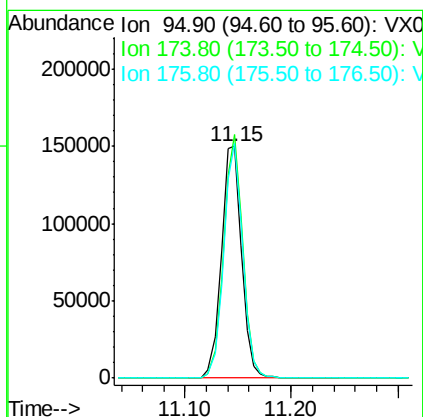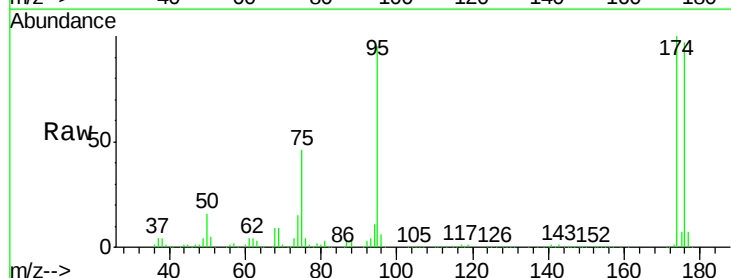







#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1564
Delta R.T. -0.00 min
Lab File: VX000892.D
Acq: 15 Apr 2018 13:13

Instrument :
MSVOA_X
ClientSampleId :
PB108205ZHE#02 5X

Tot Ion:117 Resp: 341389
Ion Ratio Lower Upper
117 100
82 51.9 41.9 62.9
119 32.2 26.0 39.0

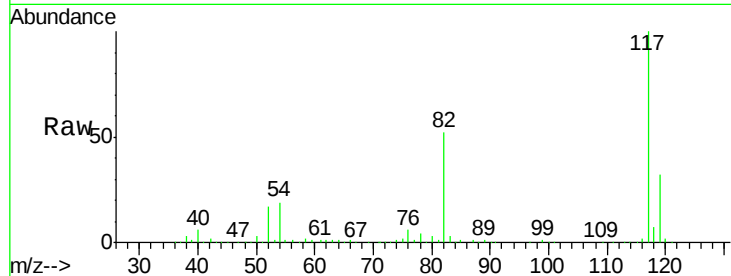


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

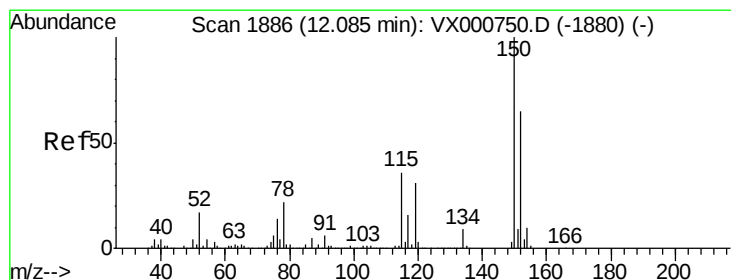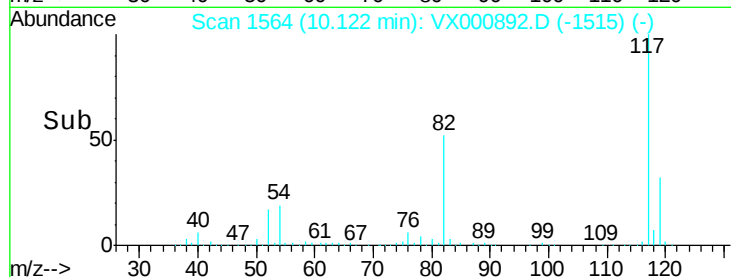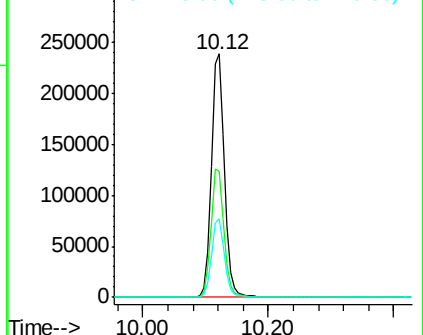

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.09 min Scan# 1886
Delta R.T. -0.00 min
Lab File: VX000892.D
Acq: 15 Apr 2018 13:13

Tgt Ion:152 Resp: 225309
Ion Ratio Lower Upper
152 100
115 53.9 37.9 113.7
150 157.3 0.0 348.0

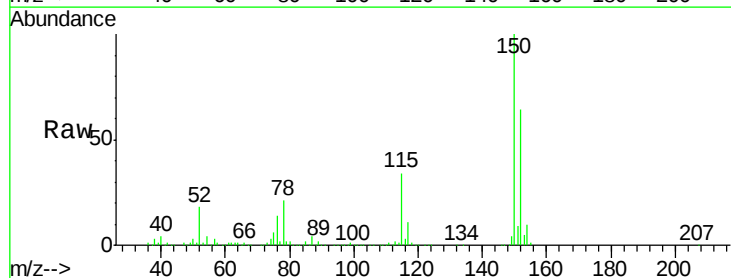

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

