

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX041618\
 Data File : VX000918.D
 Acq On : 16 Apr 2018 14:59
 Operator : JC/MD
 Sample : J2348-05
 Misc : 4.58g/5.0mL/100uL/5mL/MSVOA_X/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 155

Quant Time: Apr 16 17:30:44 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 10 15:49:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	249589	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	342585	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	322839	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	215670	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	148042	47.04	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.08%	
35) Dibromofluoromethane	5.51	113	115532	43.77	ug/l	0.00
Spiked Amount 50.000			Recovery	=	87.54%	
50) Toluene-d8	8.72	98	474904	48.32	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.64%	
62) 4-Bromofluorobenzene	11.15	95	191534	47.11	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.22%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX041618\
Data File : VX000918.D
Acq On : 16 Apr 2018 14:59
Operator : JC/MD
Sample : J2348-05
Misc : 4.58g/5.0mL/100uL/5mL/MSVOA_X/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
155

Quant Time: Apr 16 17:30:44 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 10 15:49:28 2018
Response via : Initial Calibration

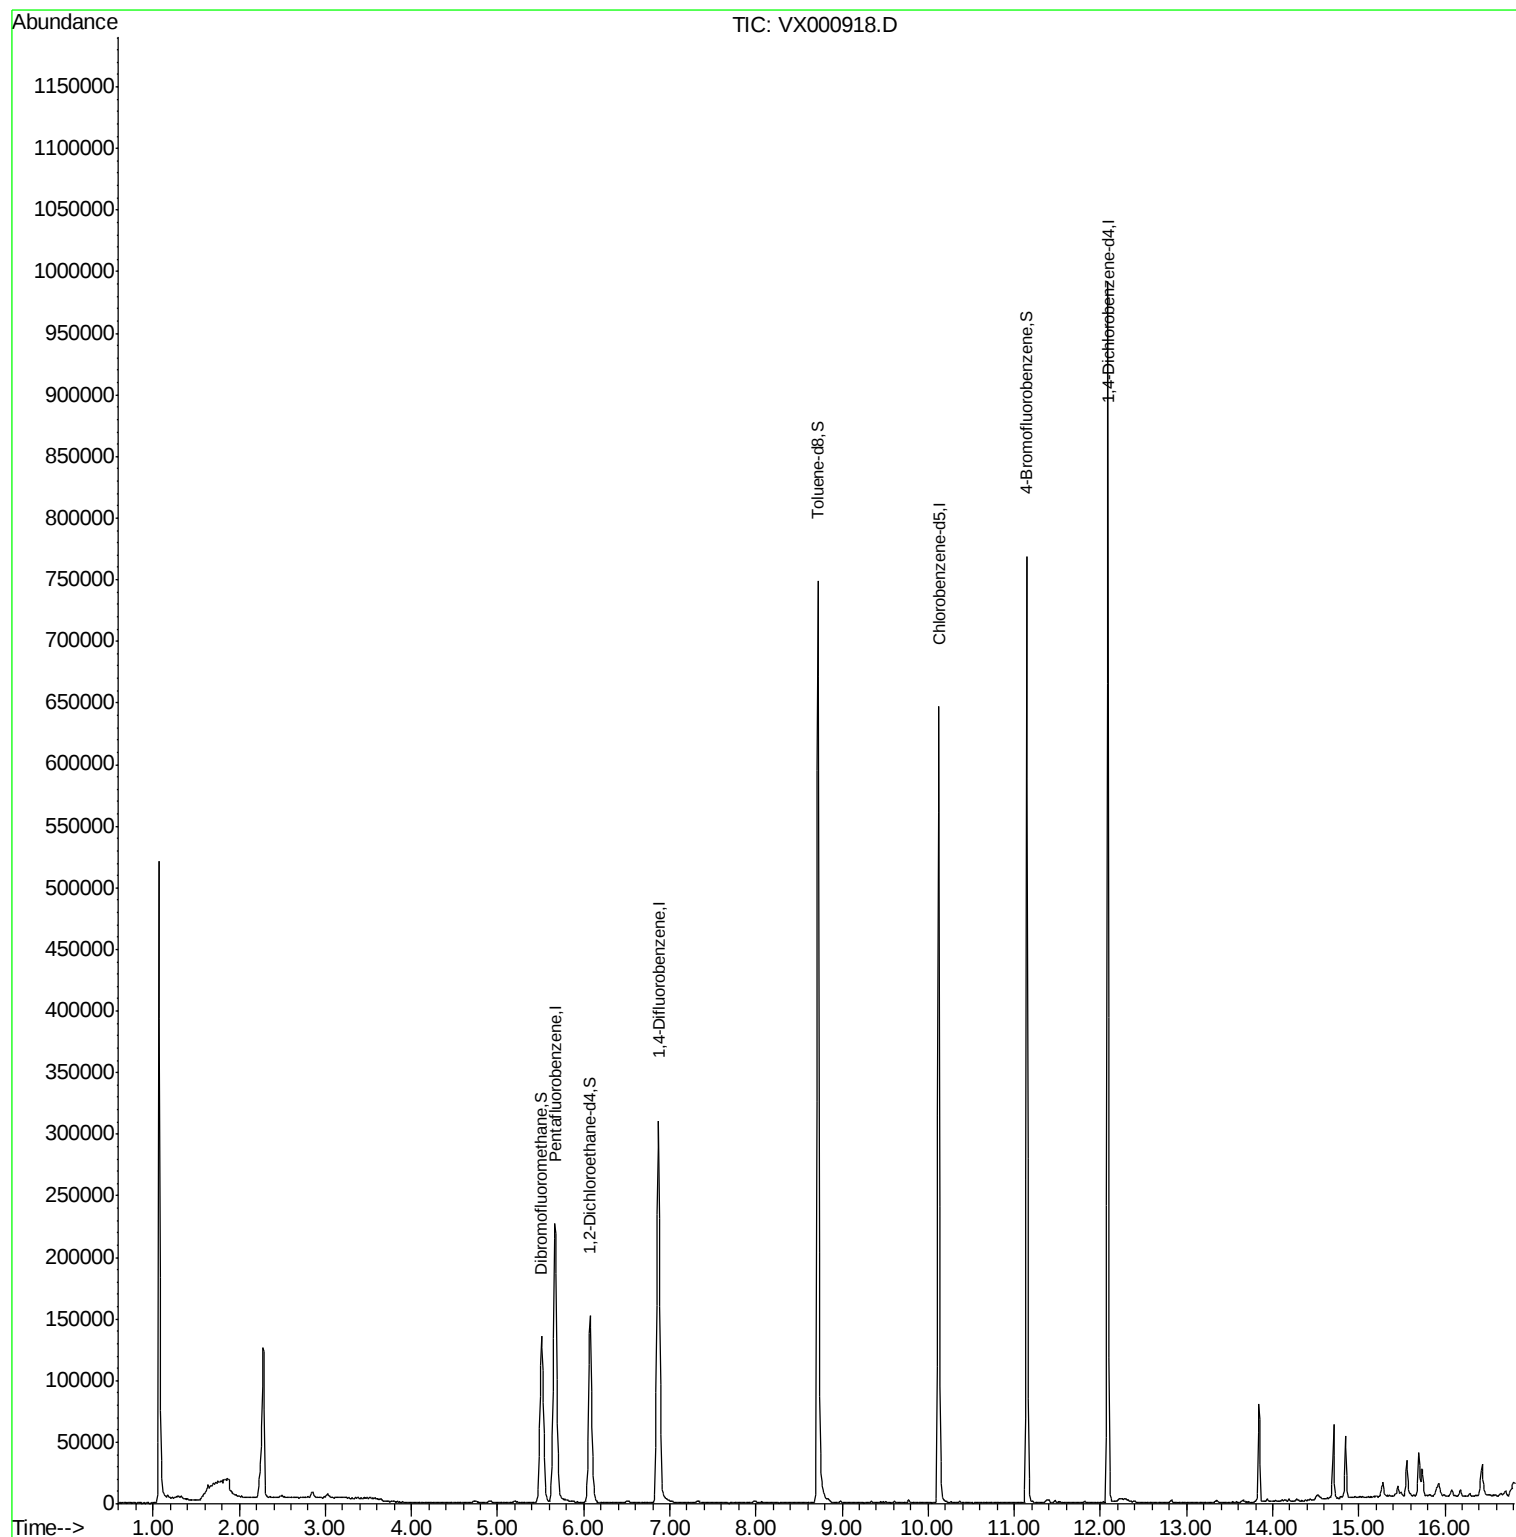

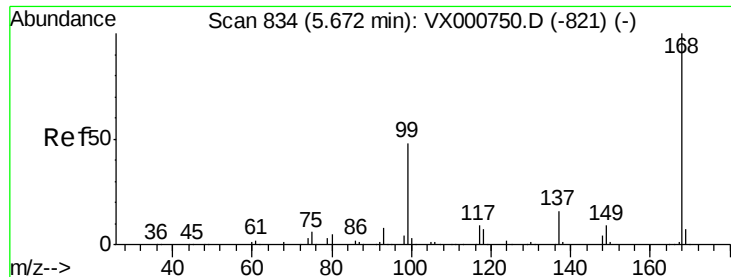

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.01 min

Lab File: VX000918.D

Acq: 16 Apr 2018 14:59


Instrument :
MSVOA_X
ClientSampleId :
155

Tot Ion:168 Resp: 249589

Ion Ratio Lower Upper

168 100

99 48.1 38.3 57.5

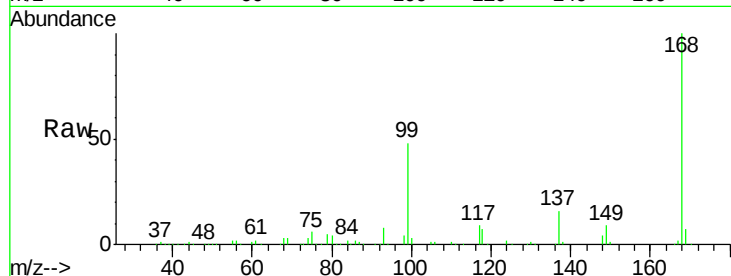

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

80000

60000



40000

20000

0

Time-->

5.50 5.60 5.70 5.80 5.90

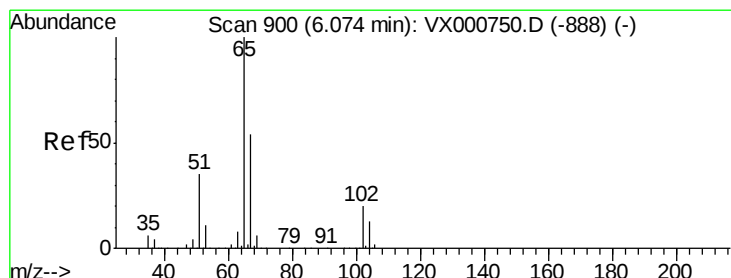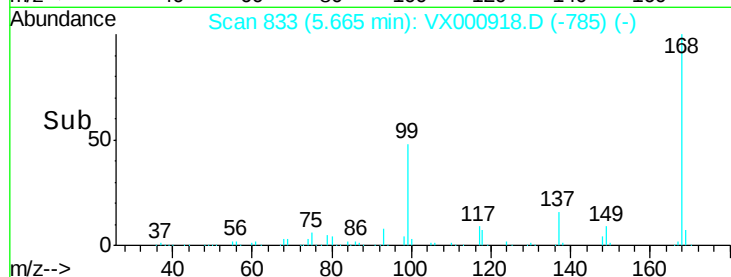

#33

1,2-Dichloroethane-d4

Concen: 47.04 ug/l

RT: 6.07 min Scan# 900

Delta R.T. -0.00 min

Lab File: VX000918.D


Acq: 16 Apr 2018 14:59

Tgt Ion: 65 Resp: 148042

Ion Ratio Lower Upper

65 100

67 51.5 0.0 103.8

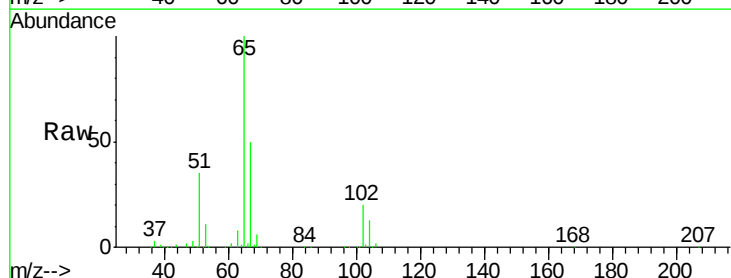

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

60000


40000


20000

0

Time-->

6.00 6.10 6.20

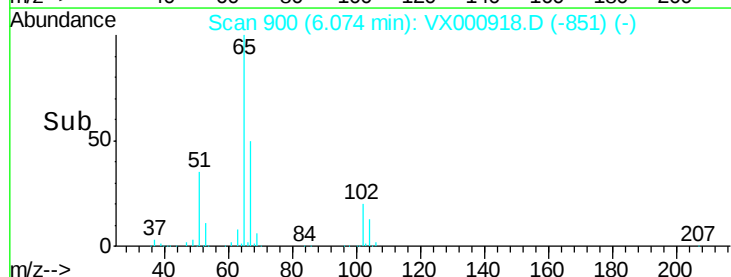

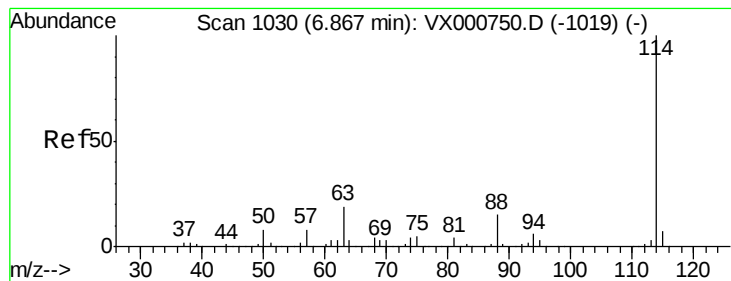

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. -0.00 min

Lab File: VX000918.D

Acq: 16 Apr 2018 14:59

Instrument :

MSVOA_X

ClientSampleId :

155


Tot Ion:114 Resp: 342585

Ion Ratio Lower Upper

114 100

63 18.9 0.0 38.4




88 15.1 0.0 31.0

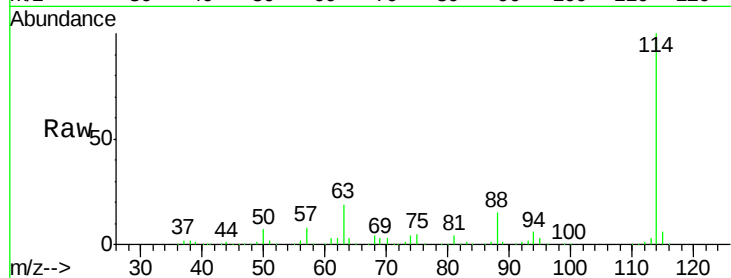

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

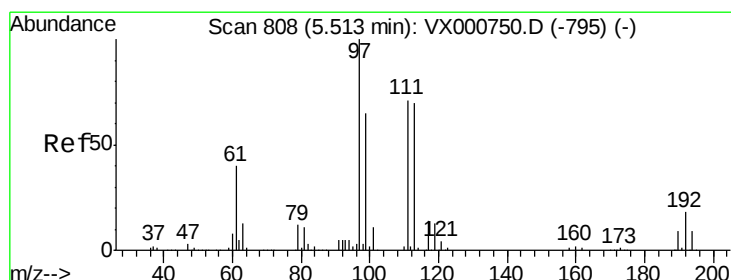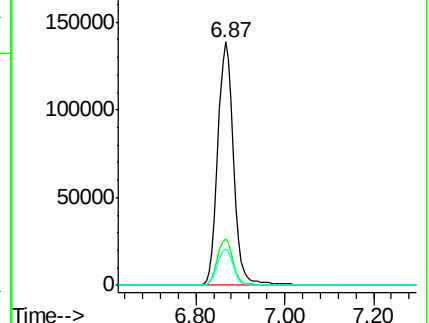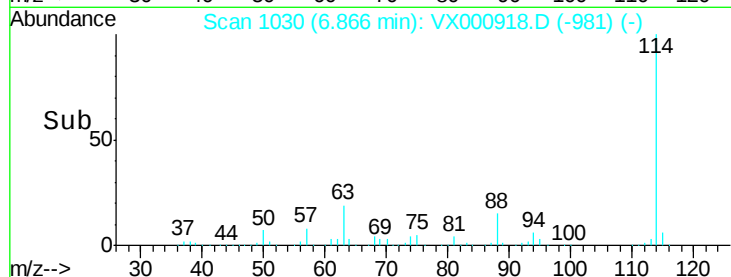

#35

Dibromofluoromethane

Concen: 43.77 ug/l

RT: 5.51 min Scan# 808

Delta R.T. -0.00 min

Lab File: VX000918.D

Acq: 16 Apr 2018 14:59


Tgt Ion:113 Resp: 115532

Ion Ratio Lower Upper

113 100

111 100.4 81.5 122.3



192 25.8 20.4 30.6

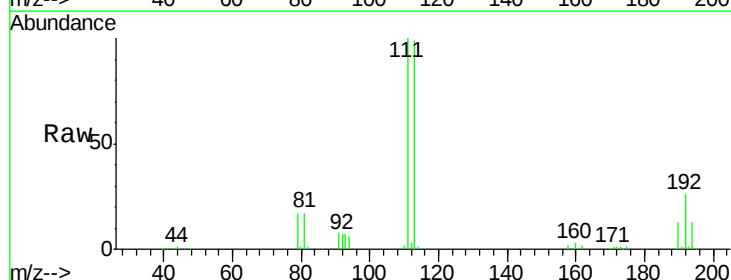


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

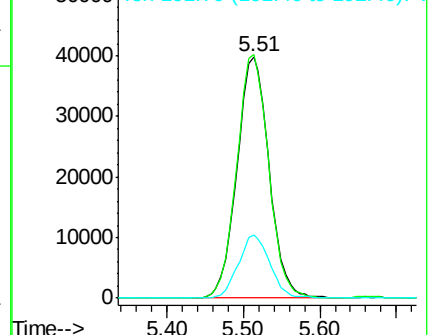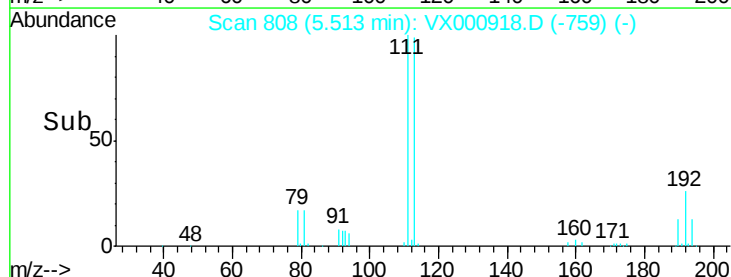

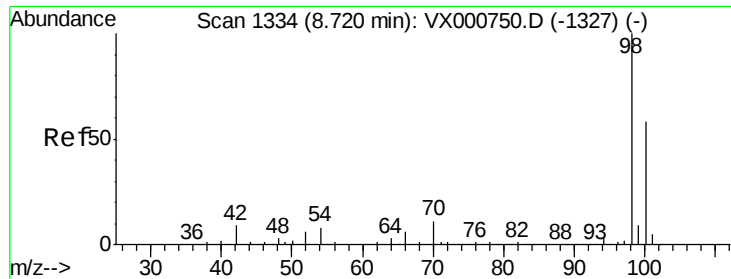

#50

Toluene-d8

Concen: 48.32 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. -0.00 min

Lab File: VX000918.D

Acq: 16 Apr 2018 14:59

Instrument :

MSVOA_X

ClientSampleId :


155

Tot Ion: 98 Resp: 474904

Ion Ratio Lower Upper

98 100

100 64.5 52.6 79.0

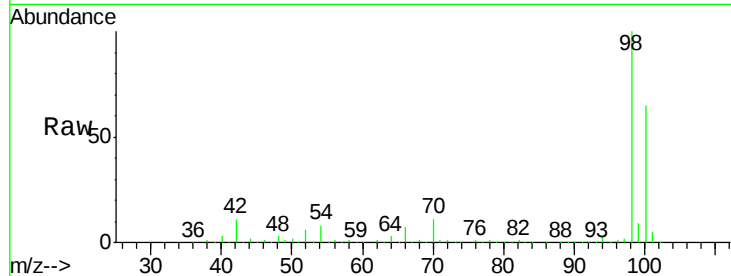

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

8.72

300000



200000

100000

0

Time-->

8.60 8.80 9.00

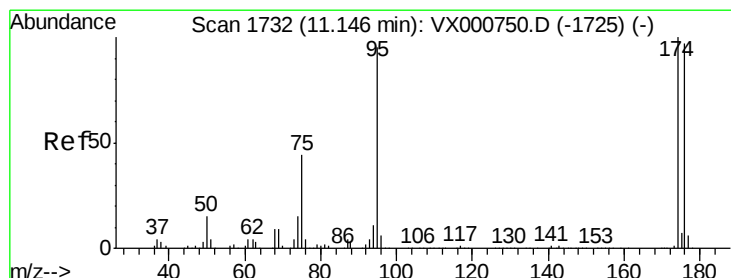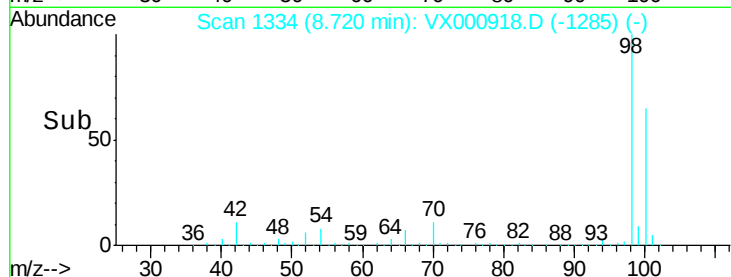

#62

4-Bromofluorobenzene

Concen: 47.11 ug/l

RT: 11.15 min Scan# 1732

Delta R.T. -0.00 min

Lab File: VX000918.D

Acq: 16 Apr 2018 14:59


Tgt Ion: 95 Resp: 191534

Ion Ratio Lower Upper

95 100

174 97.9 0.0 198.4

176 95.3 0.0 194.4

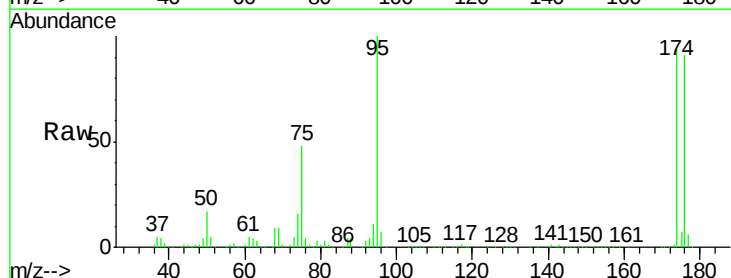

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

11.15

200000

150000


100000

50000

0

Time-->

11.10 11.20

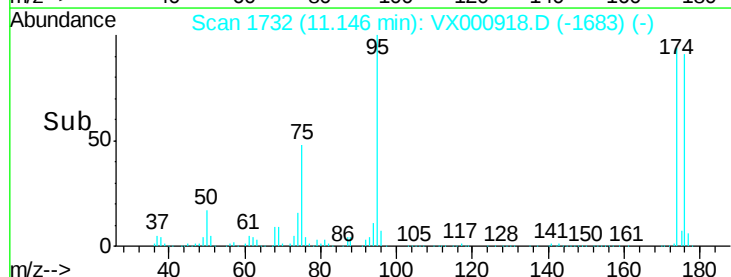







#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1564
Delta R.T. -0.00 min
Lab File: VX000918.D
Acq: 16 Apr 2018 14:59

Instrument :
MSVOA_X
ClientSampleId :
155

Tot Ion:117 Resp: 322839
Ion Ratio Lower Upper
117 100
82 51.5 41.9 62.9
119 32.4 26.0 39.0

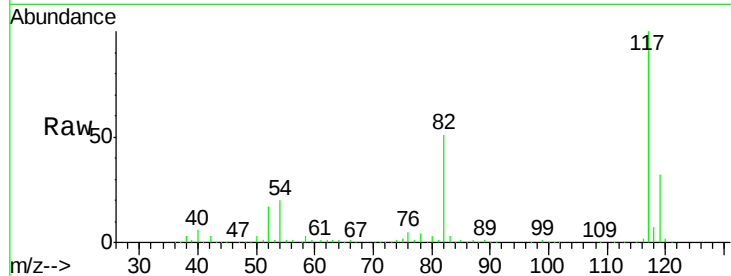


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX
Ion 118.90 (118.60 to 119.60): V

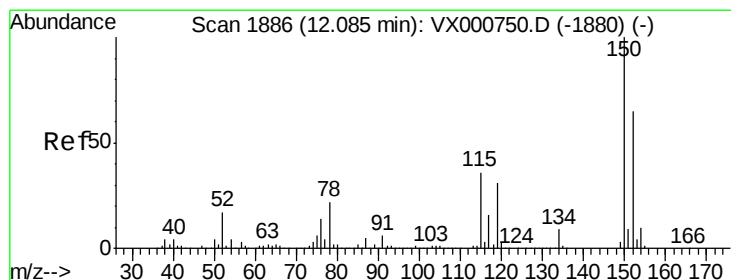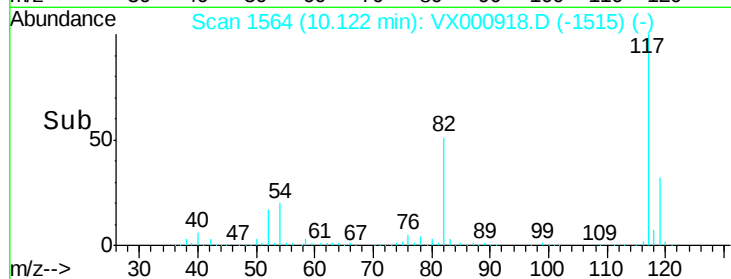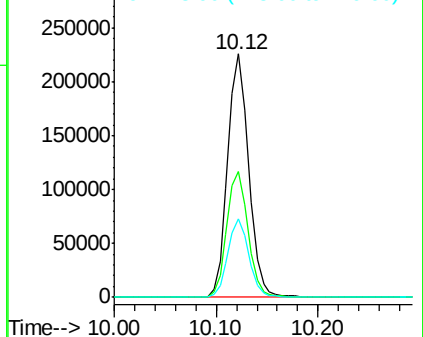

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.08 min Scan# 1886
Delta R.T. -0.00 min
Lab File: VX000918.D
Acq: 16 Apr 2018 14:59

Tgt Ion:152 Resp: 215670
Ion Ratio Lower Upper
152 100
115 53.7 37.9 113.7
150 154.4 0.0 348.0

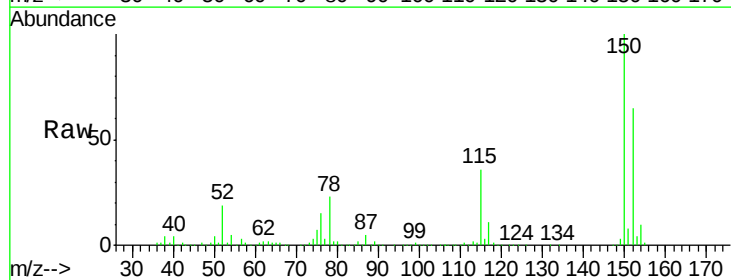

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

