

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX041618\
 Data File : VX000941.D
 Acq On : 17 Apr 2018 01:36
 Operator : JC/MD
 Sample : VX0416WBL02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0416WBL02

Quant Time: Apr 17 07:20:12 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 10 15:49:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	260640	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	362039	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	332682	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	216860	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.08	65	159908	48.66	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.32%	
35) Dibromofluoromethane	5.51	113	125947	45.15	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.30%	
50) Toluene-d8	8.72	98	498793	48.03	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.06%	
62) 4-Bromofluorobenzene	11.14	95	191934	44.67	ug/l	0.00
Spiked Amount	50.000		Recovery	=	89.34%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX041618\
Data File : VX000941.D
Acq On : 17 Apr 2018 01:36
Operator : JC/MD
Sample : VX0416WBL02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0416WBL02

Quant Time: Apr 17 07:20:12 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 10 15:49:28 2018
Response via : Initial Calibration

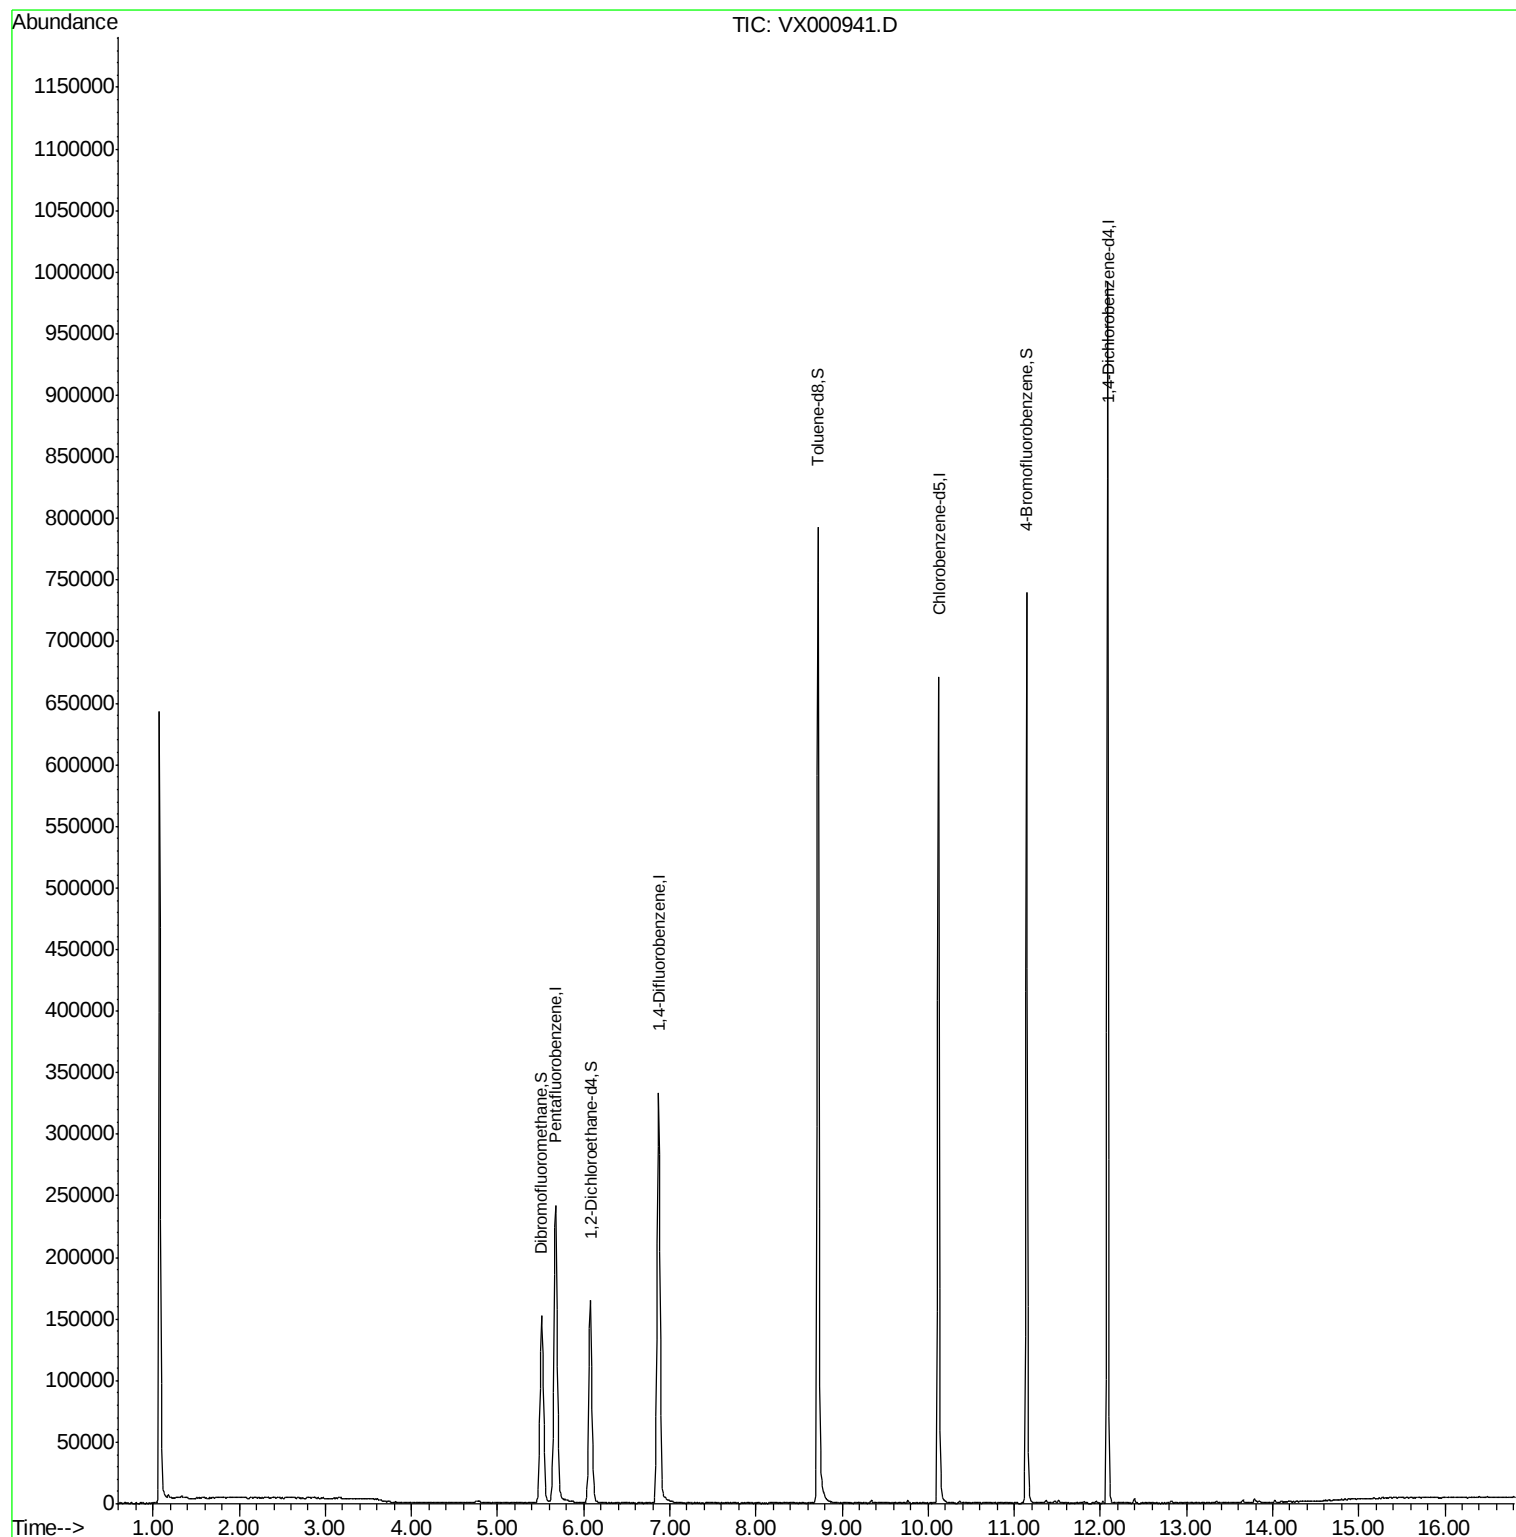



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.00 min

Lab File: VX000941.D

Acq: 17 Apr 2018 01:36

Instrument :

MSVOA_X

ClientSampleId :


VX0416WBL02

Tot Ion:168 Resp: 260640

Ion Ratio Lower Upper

168 100

99 47.0 38.3 57.5

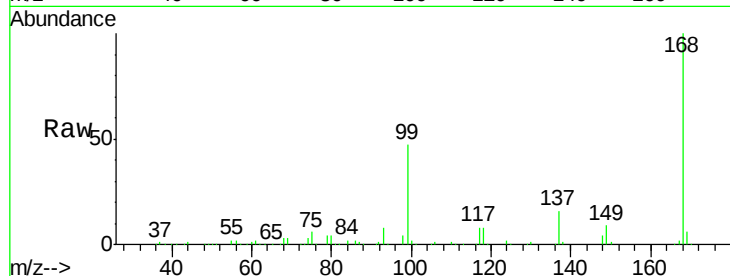

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

100000

80000

60000

40000

20000

0



Time-->

5.50

5.60

5.70

5.80

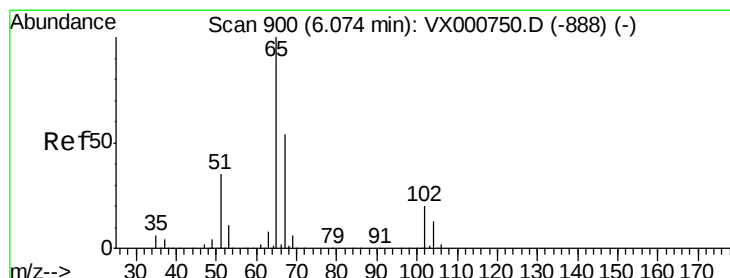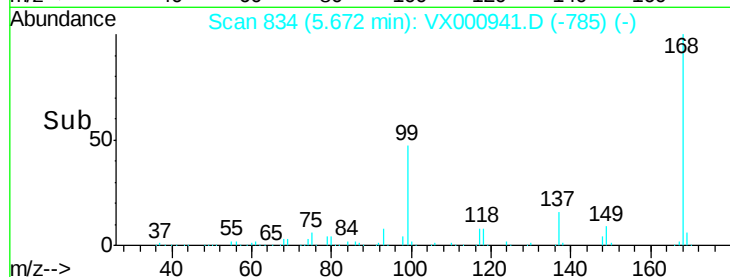

#33

1,2-Dichloroethane-d4

Concen: 48.66 ug/l

RT: 6.08 min Scan# 901

Delta R.T. 0.01 min

Lab File: VX000941.D


Acq: 17 Apr 2018 01:36

Tgt Ion: 65 Resp: 159908

Ion Ratio Lower Upper

65 100

67 51.5 0.0 103.8

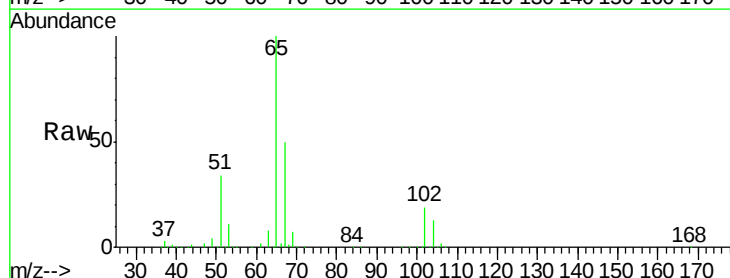

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.08

60000

40000

20000


0


Time-->

6.00

6.10

6.20

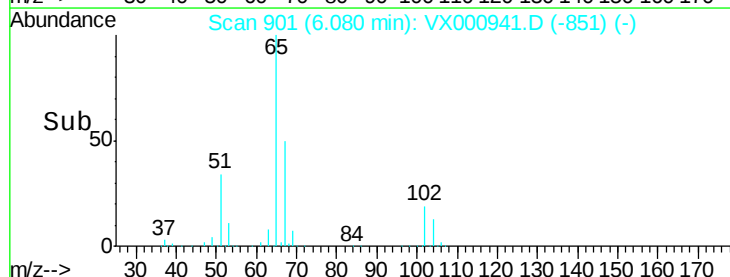

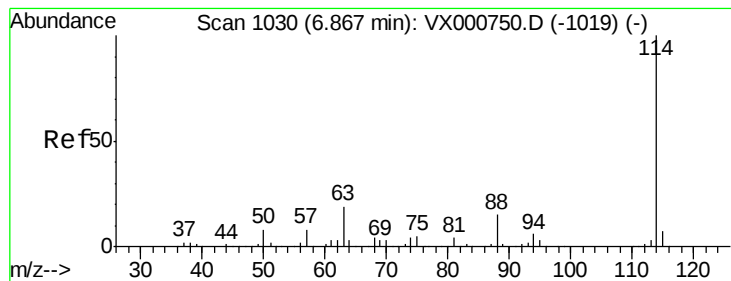

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1031

Delta R.T. 0.01 min

Lab File: VX000941.D

Acq: 17 Apr 2018 01:36

Instrument :

MSVOA_X

ClientSampleId :

VX0416WBL02


Tot Ion:114 Resp: 362039

Ion Ratio Lower Upper

114 100

63 18.2 0.0 38.4




88 15.4 0.0 31.0

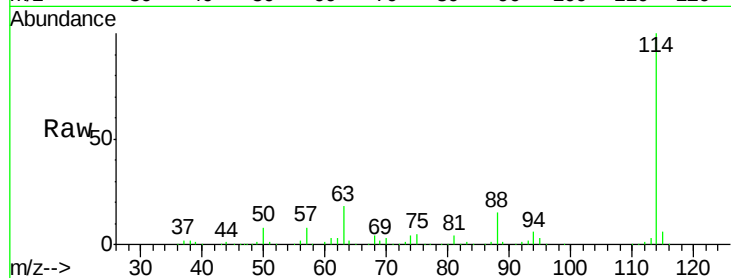

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

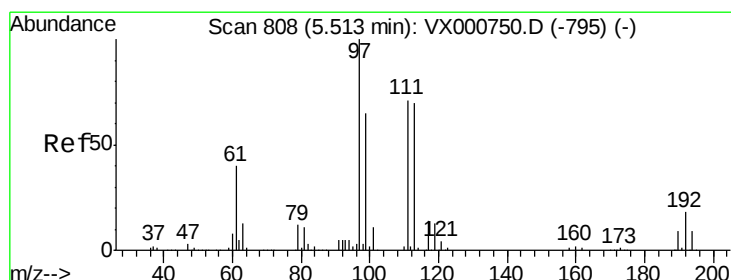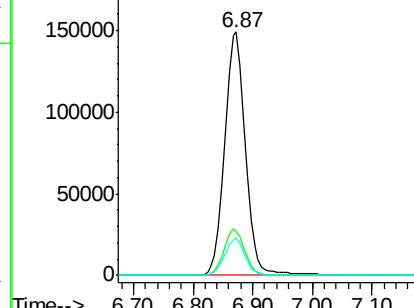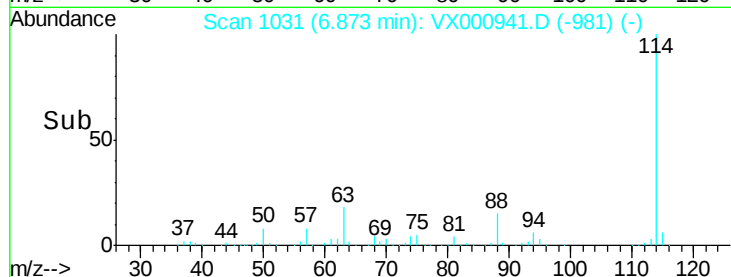

#35

Dibromofluoromethane

Concen: 45.15 ug/l

RT: 5.51 min Scan# 808

Delta R.T. -0.00 min

Lab File: VX000941.D

Acq: 17 Apr 2018 01:36


Tgt Ion:113 Resp: 125947

Ion Ratio Lower Upper

113 100

111 102.0 81.5 122.3



192 25.4 20.4 30.6

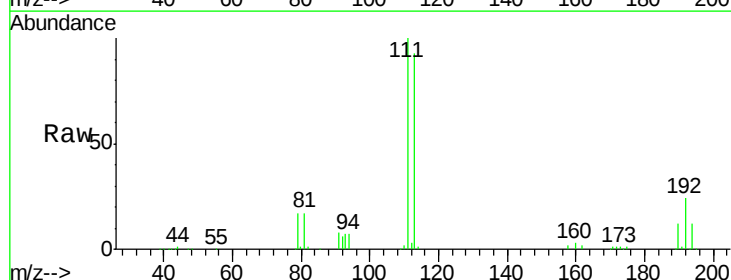


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



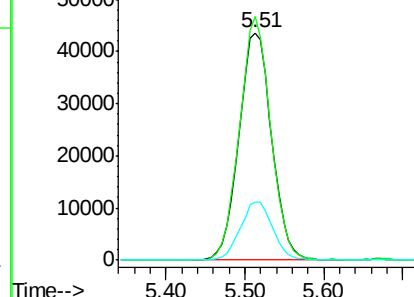
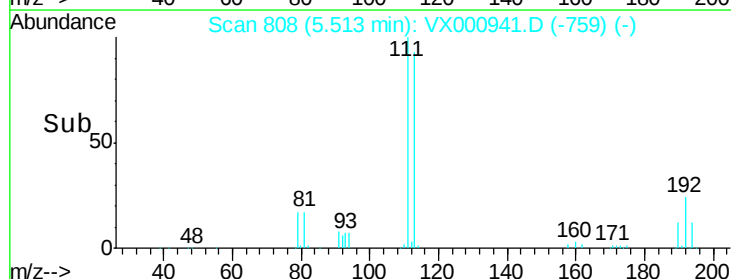


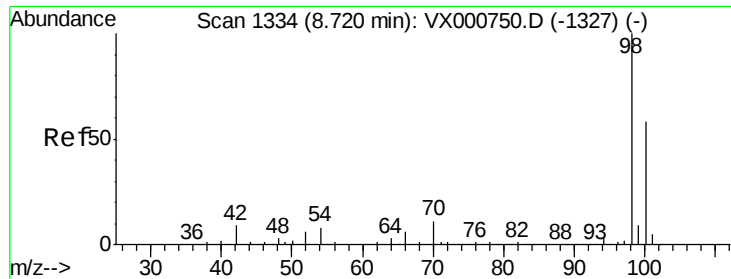

#50
Toluene-d8
Concen: 48.03 ug/l
RT: 8.72 min Scan# 1334
Delta R.T. -0.00 min
Lab File: VX000941.D
Acq: 17 Apr 2018 01:36




Instrument :
MSVOA_X
ClientSampleId :
VX0416WBL02

Tot Ion: 98 Resp: 498793
Ion Ratio Lower Upper
98 100
100 64.9 52.6 79.0

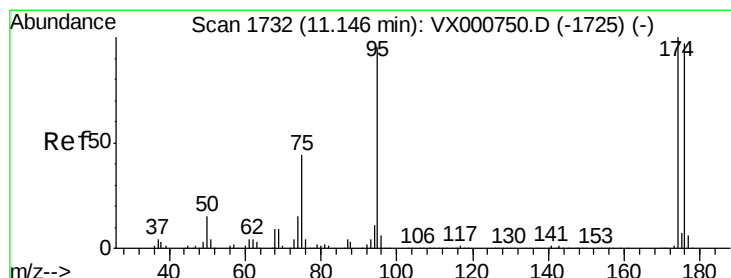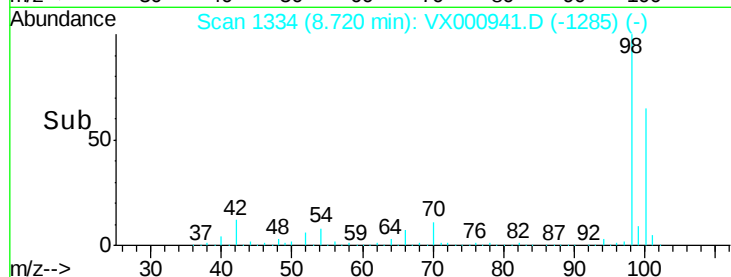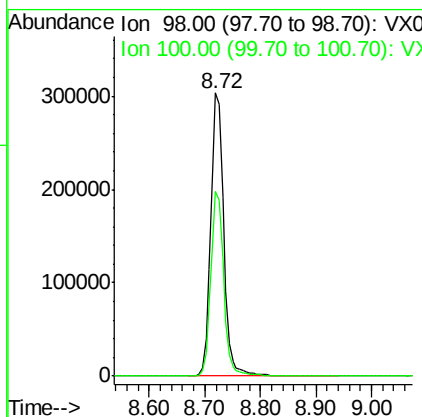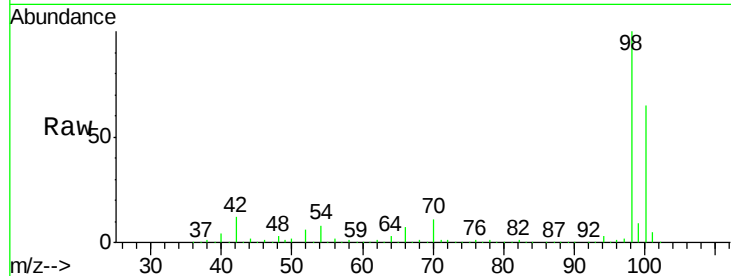

#62
4-Bromofluorobenzene
Concen: 44.67 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. -0.01 min
Lab File: VX000941.D
Acq: 17 Apr 2018 01:36

Tgt Ion: 95 Resp: 191934
Ion Ratio Lower Upper
95 100
174 98.7 0.0 198.4
176 95.6 0.0 194.4

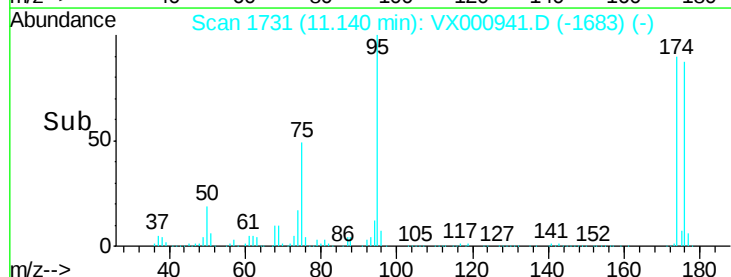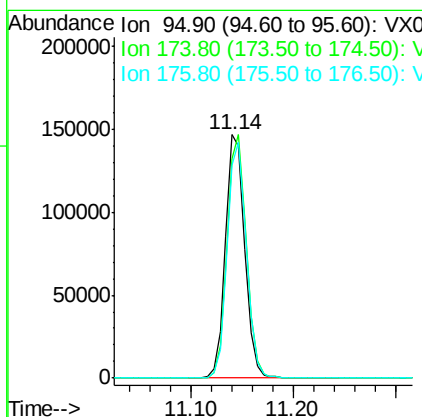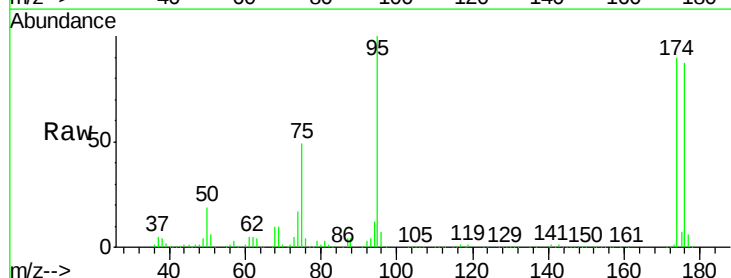







#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1564
Delta R.T. -0.00 min
Lab File: VX000941.D
Acq: 17 Apr 2018 01:36

Instrument :
MSVOA_X
ClientSampleId :
VX0416WBL02

Tot Ion:117 Resp: 332682
Ion Ratio Lower Upper
117 100
82 51.8 41.9 62.9
119 32.2 26.0 39.0

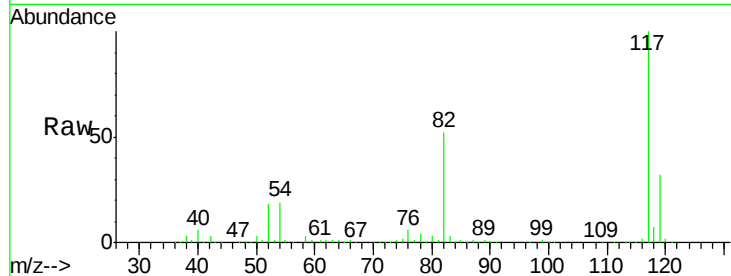


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

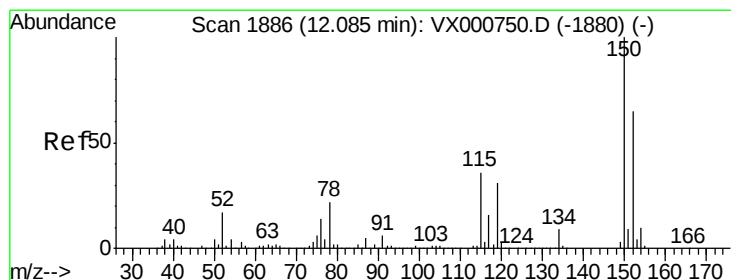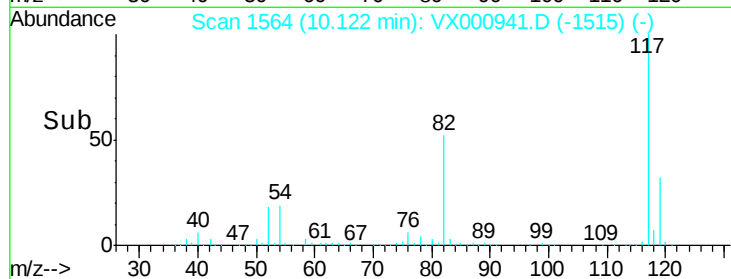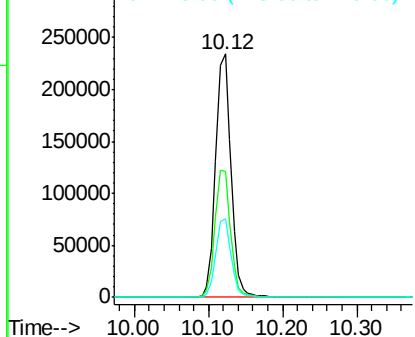

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.09 min Scan# 1886
Delta R.T. -0.00 min
Lab File: VX000941.D
Acq: 17 Apr 2018 01:36

Tgt Ion:152 Resp: 216860
Ion Ratio Lower Upper
152 100
115 53.2 37.9 113.7
150 155.9 0.0 348.0

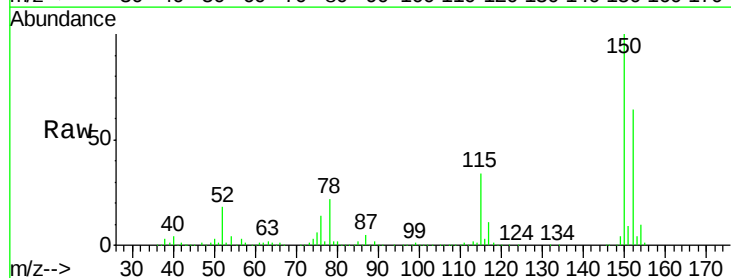

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

