


Data Path : W:\HPCHEM1\MSVOA X\Data\VX041618\  
Data File : VX000912.D  
Acq On : 16 Apr 2018 11:56  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA\_X\METHOD\82X041018W.M  
Title : SW846 8260  
Last Update : Tue Apr 10 15:49:28 2018

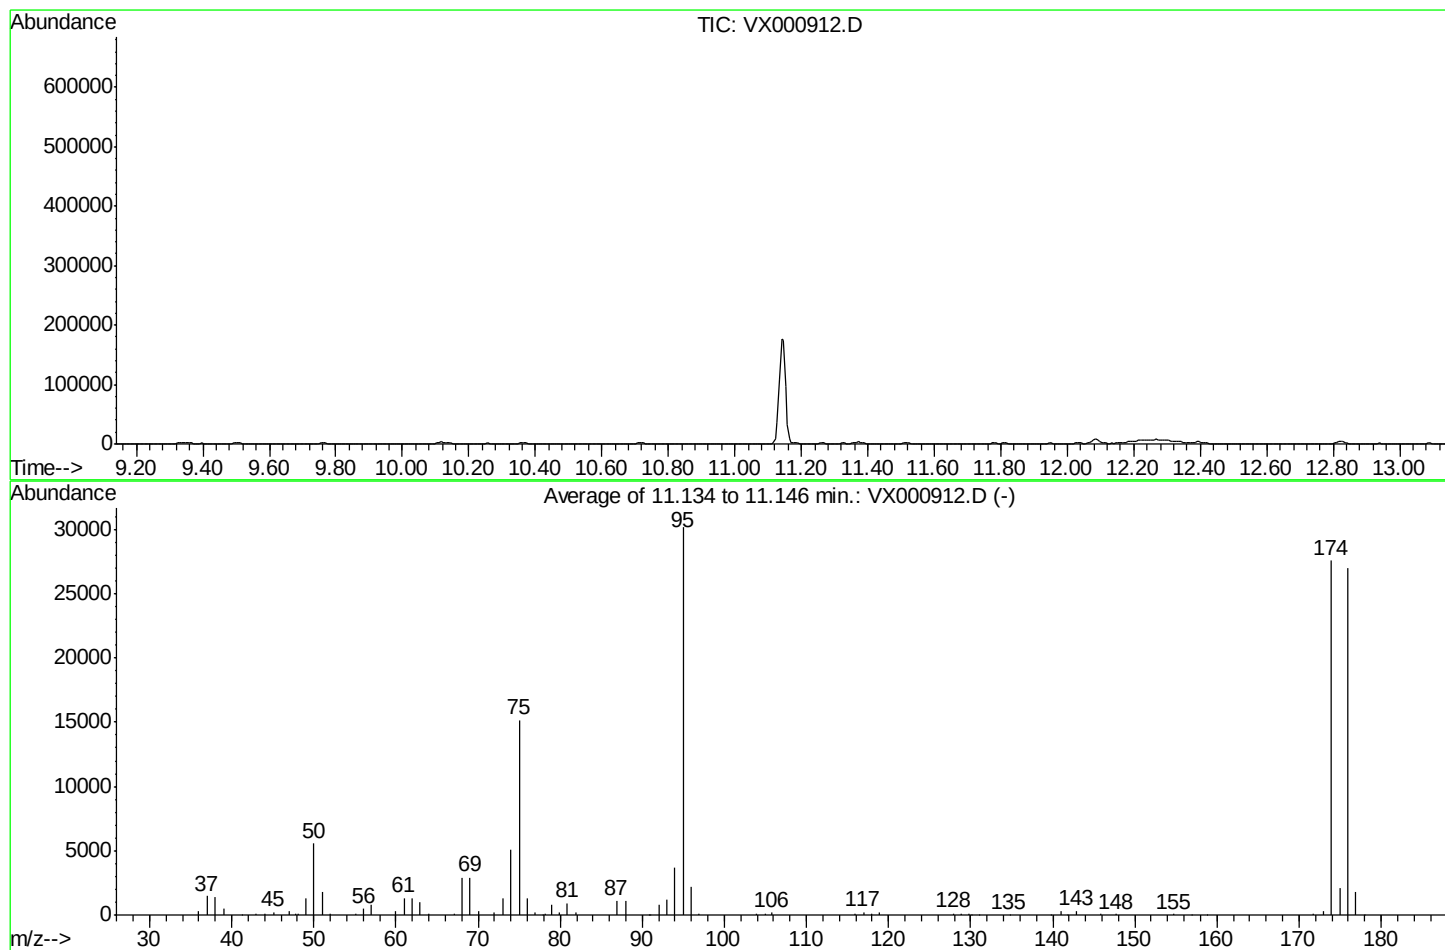

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 18.5      | 5574    | PASS             |
| 75          | 95           | 30           | 60           | 50.2      | 15141   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 30154   | PASS             |
| 96          | 95           | 5            | 9            | 7.3       | 2214    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.2       | 341     | PASS             |
| 174         | 95           | 50           | 100          | 91.4      | 27570   | PASS             |
| 175         | 174          | 5            | 9            | 7.6       | 2106    | PASS             |
| 176         | 174          | 95           | 101          | 97.9      | 26981   | PASS             |
| 177         | 176          | 5            | 9            | 6.6       | 1772    | PASS             |