


Data Path : W:\HPCHEM1\MSVOA X\Data\VX041618\
Data File : VX000939.D
Acq On : 17 Apr 2018 00:20
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
Title : SW846 8260
Last Update : Tue Apr 10 15:49:28 2018

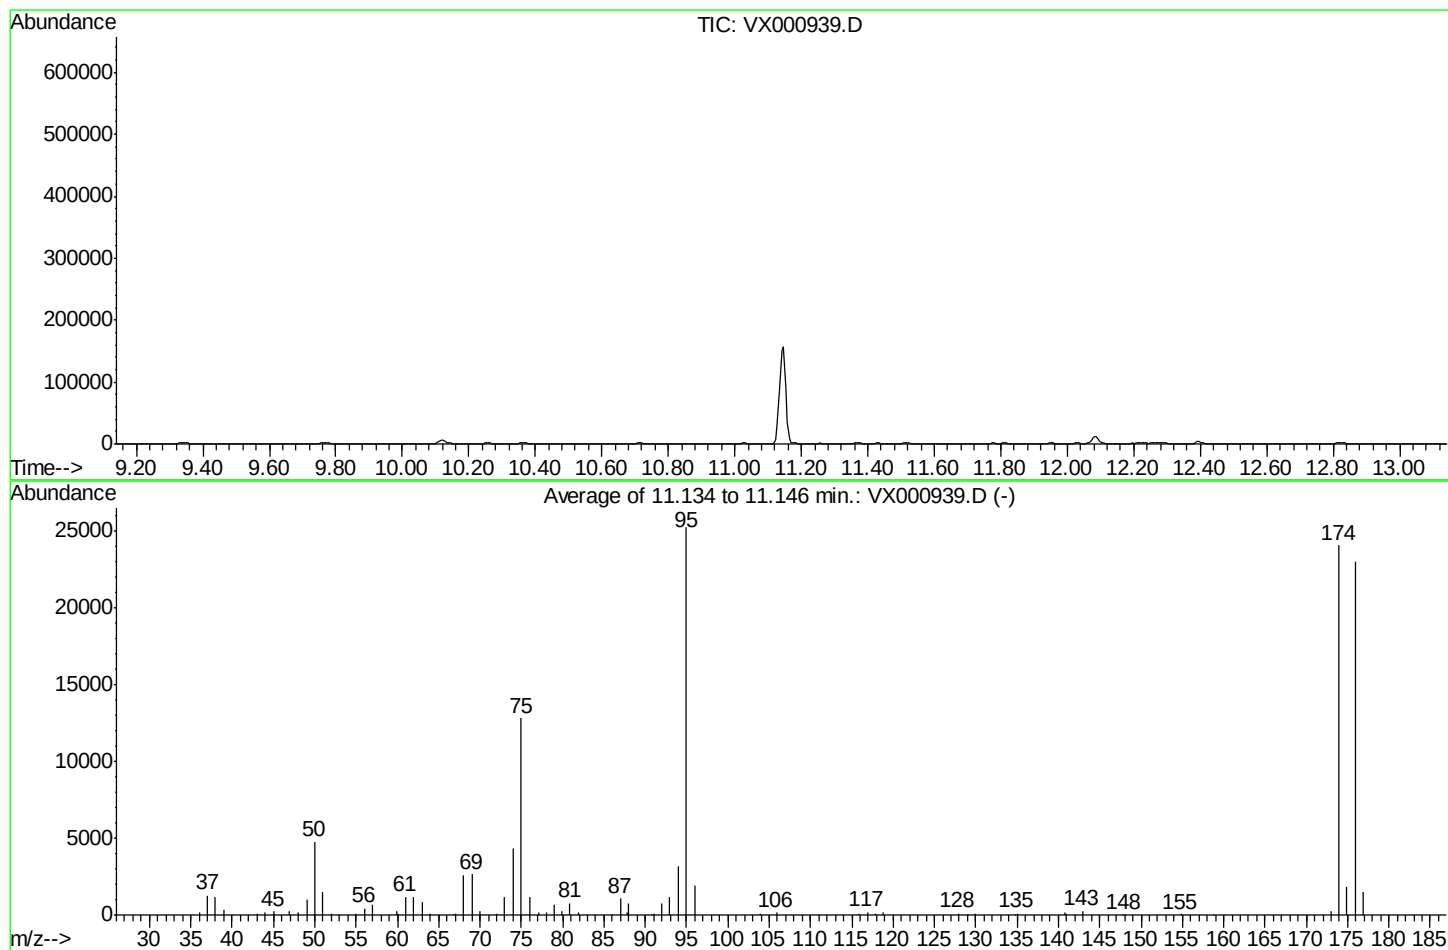

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	4775	PASS
75	95	30	60	50.8	12816	PASS
95	95	100	100	100.0	25229	PASS
96	95	5	9	7.6	1917	PASS
173	174	0.00	2	1.0	238	PASS
174	95	50	100	95.3	24038	PASS
175	174	5	9	7.5	1804	PASS
176	174	95	101	95.6	22987	PASS
177	176	5	9	6.7	1541	PASS