

Data Path : W:\HPCHEM1\MSVOA X\Data\VX041718\
 Data File : VX000979.D
 Acq On : 17 Apr 2018 21:31
 Operator : JC/MD
 Sample : PB108300ZHE#10 5X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
ClientSampled :
 PB108300ZHE#10 5X

Quant Time: Apr 18 05:54:30 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 10 15:49:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	249142	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	345918	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	320178	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	200728	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	156933	49.96	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.92%	
35) Dibromofluoromethane	5.51	113	121747	45.68	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.36%	
50) Toluene-d8	8.72	98	485559	48.93	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.86%	
62) 4-Bromofluorobenzene	11.14	95	183681	44.74	ug/l	0.00
Spiked Amount	50.000		Recovery	=	89.48%	
Target Compounds						
16) Acetone	2.45	43	3649	3.37	ug/l	92
18) Methyl Acetate	2.78	43	4792	1.71	ug/l	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\Data\VX041718\
 Data File : VX000979.D
 Acq On : 17 Apr 2018 21:31
 Operator : JC/MD
 Sample : PB108300ZHE#10 5X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
Client Sampled :
 PB108300ZHE#10 5X

Quant Time: Apr 18 05:54:30 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 10 15:49:28 2018
 Response via : Initial Calibration




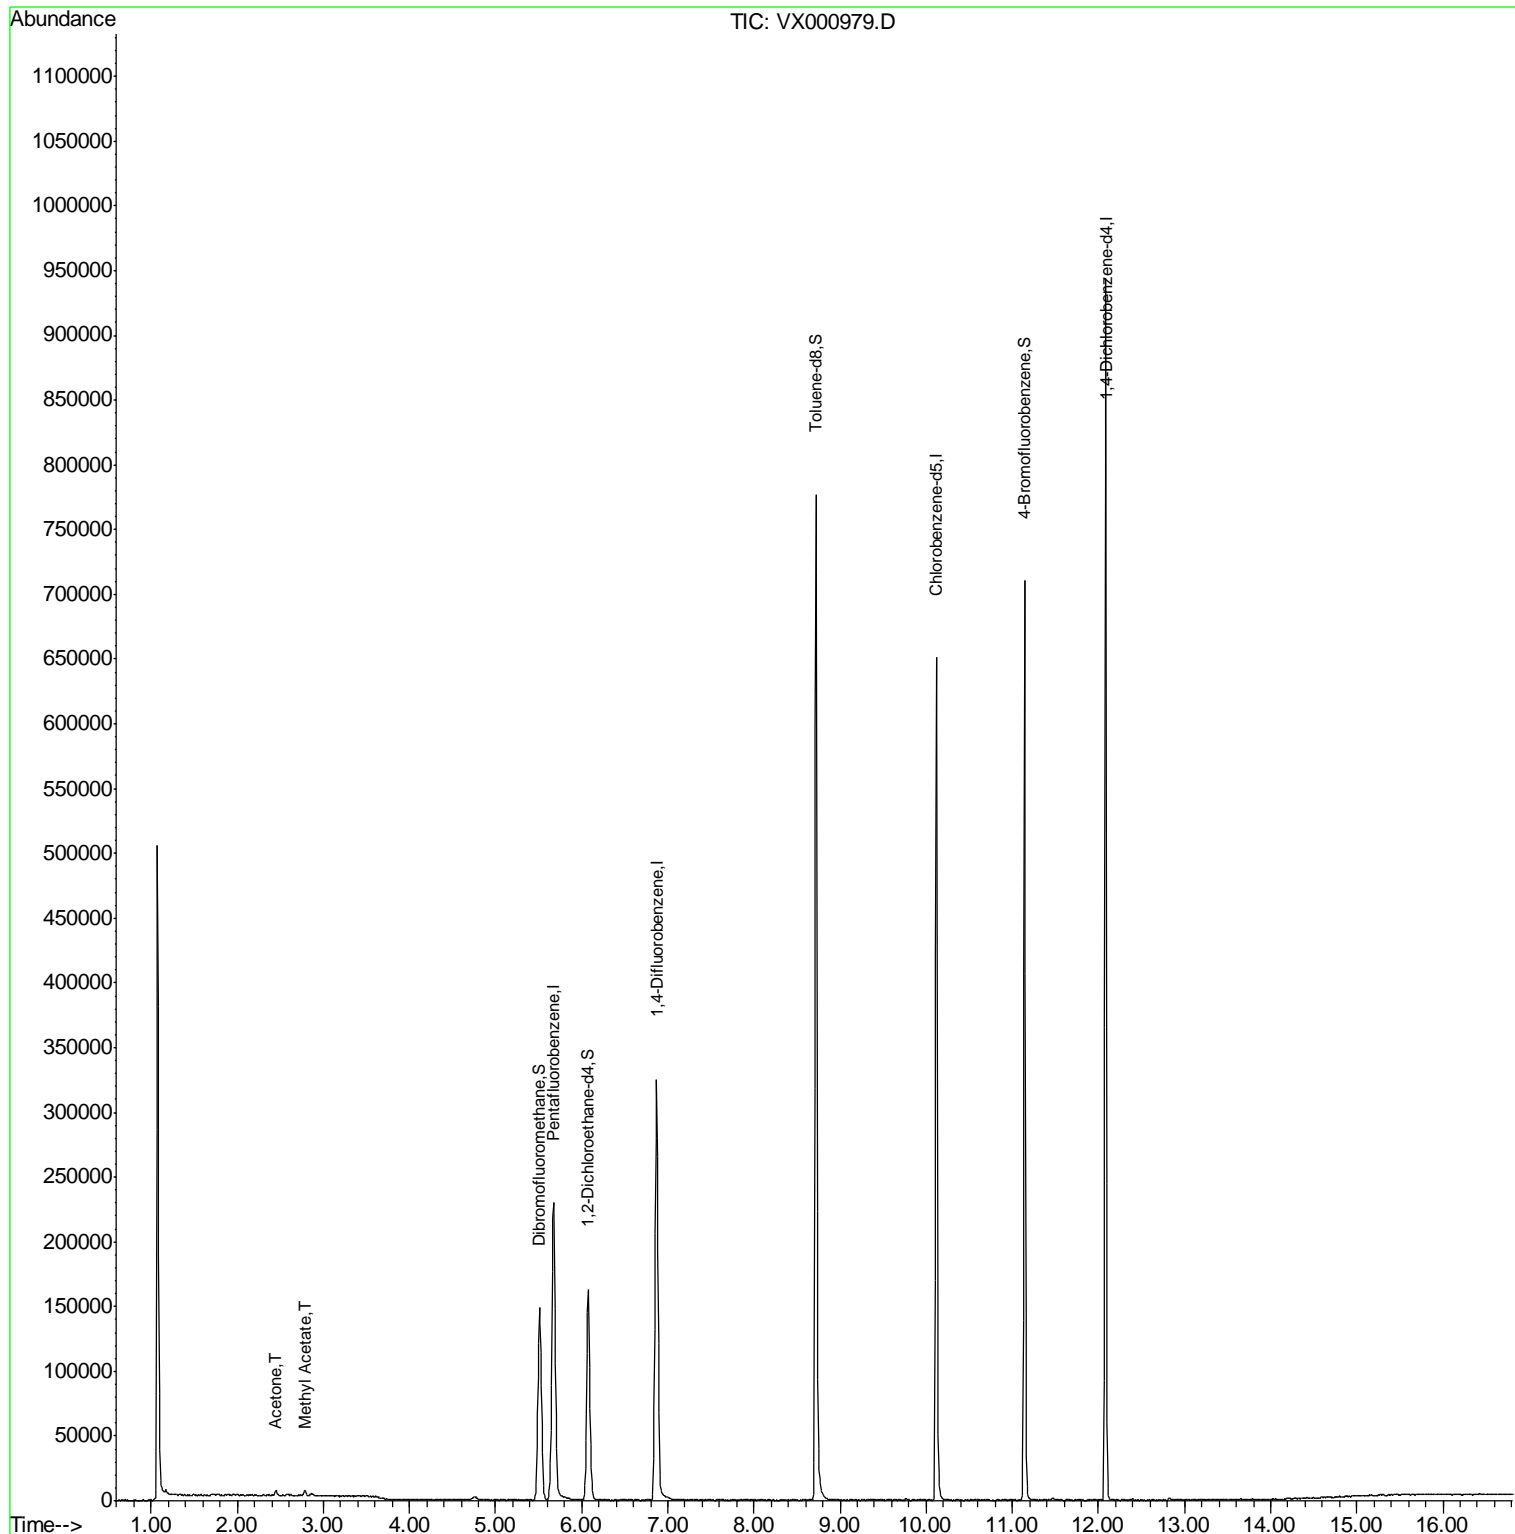


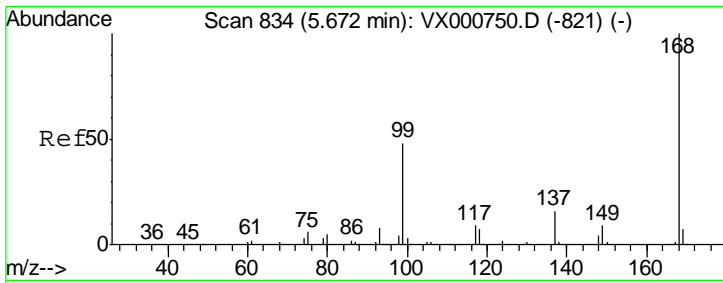

#1
 Pentafluorobenzene
 Concen: 50.00 ug/l
 RT: 5.67 min Scan# 834
 Delta R.T. -0.00 min
 Lab File: VX000979.D
 Acq: 17 Apr 2018 21:31




Instrument : MSVOA_X
 ClientSampleId : PB108300ZHE#10 5X


Tgt Ion	Resp	Lower	Upper
168	100		
99	49.3	38.3	57.5

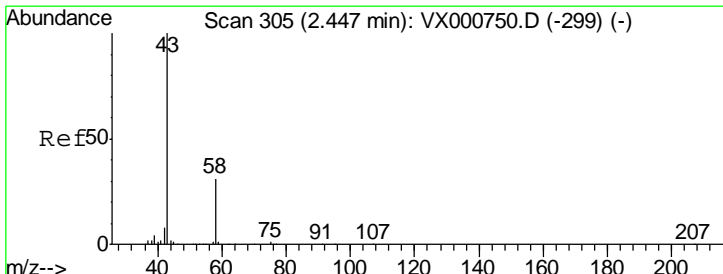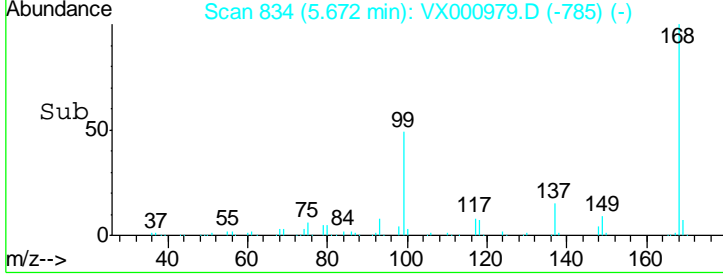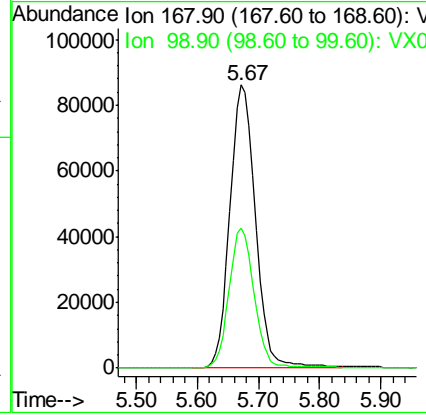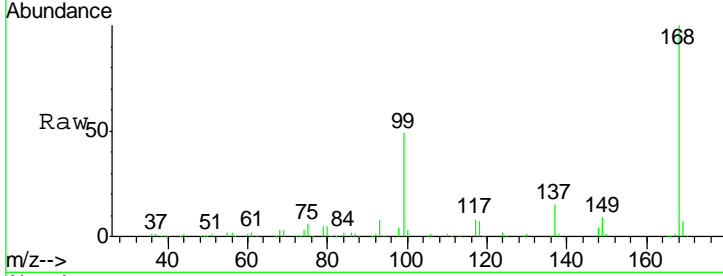

#16
 Acetone
 Concen: 3.37 ug/l
 RT: 2.45 min Scan# 305
 Delta R.T. -0.00 min
 Lab File: VX000979.D
 Acq: 17 Apr 2018 21:31

Tgt Ion	Resp	Lower	Upper
43	100		
58	26.6	24.6	37.0


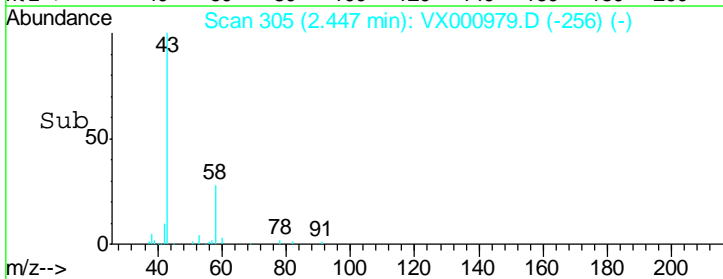
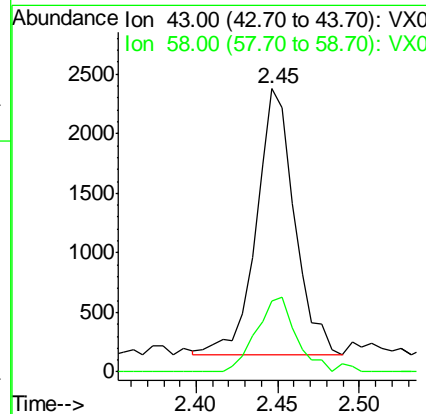
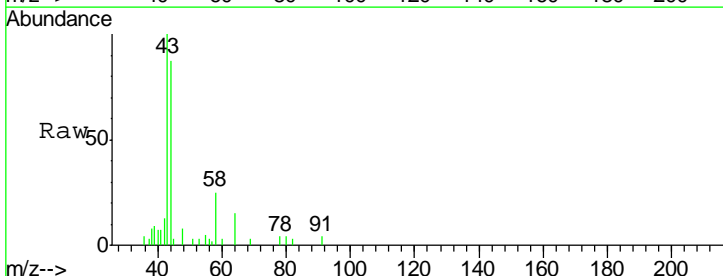


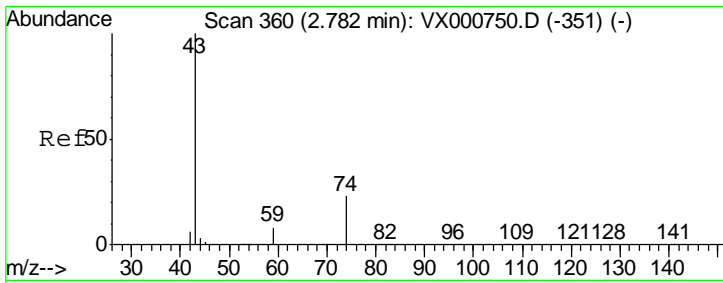

#18
 Methyl Acetate
 Concen: 1.71 ug/l
 RT: 2.78 min Scan# 360
 Delta R.T. -0.00 min
 Lab File: VX000979.D
 Acq: 17 Apr 2018 21:31




Instrument :
 MSVOA_X
ClientSampled :
 PB108300ZHE#10 5X


Tgt Ion	Resp	Lower	Upper
43	100		
74	20.5	19.1	28.7

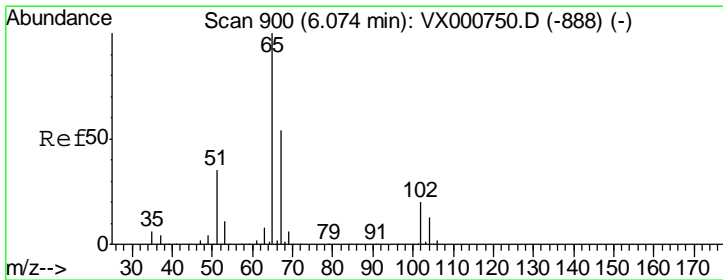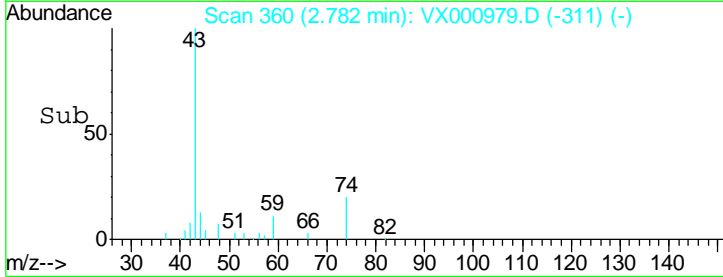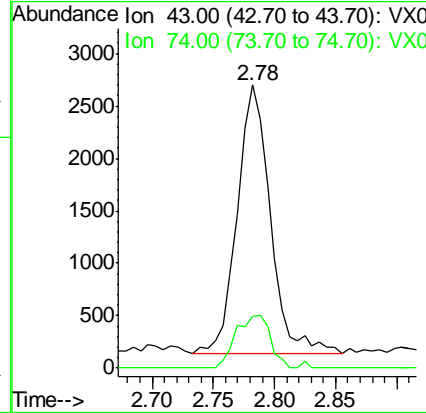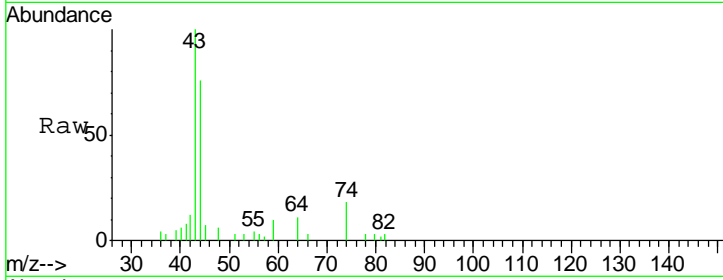

#33
 1,2-Dichloroethane-d4
 Concen: 49.96 ug/l
 RT: 6.07 min Scan# 900
 Delta R.T. -0.00 min
 Lab File: VX000979.D
 Acq: 17 Apr 2018 21:31

Tgt Ion	Resp	Lower	Upper
65	100		
67	51.8	0.0	103.8


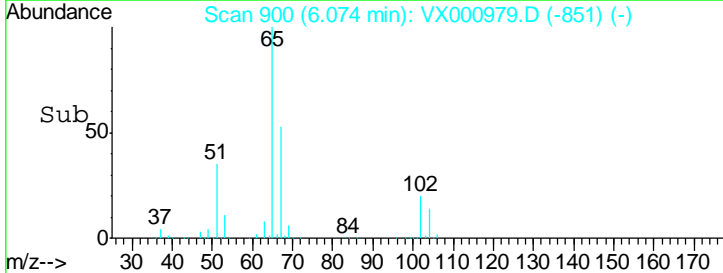
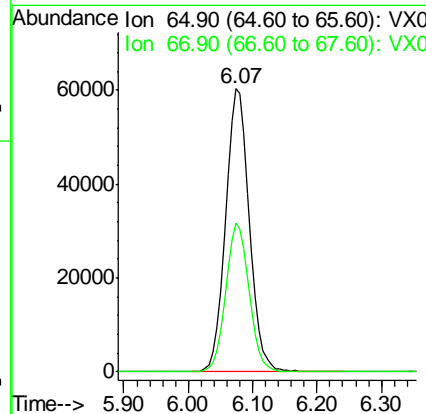
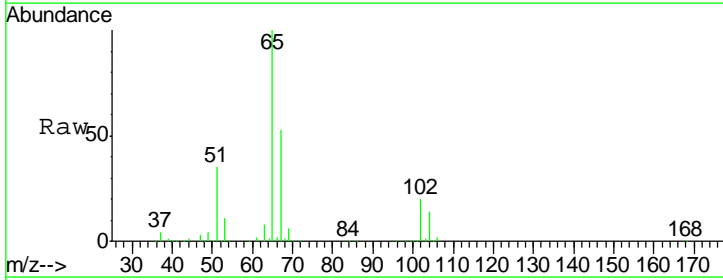


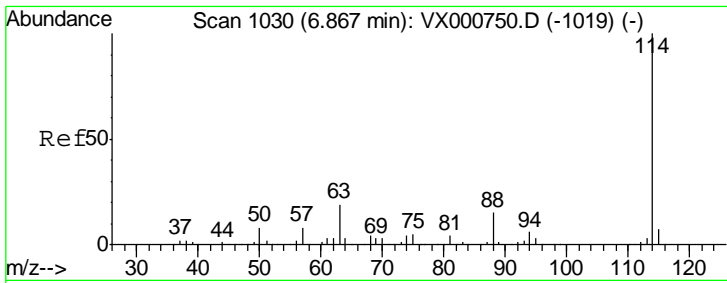

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.87 min Scan# 1030
 Delta R.T. -0.00 min
 Lab File: VX000979.D
 Acq: 17 Apr 2018 21:31




Instrument : MSVOA_X
 ClientSampleId : PB108300ZHE#10 5X


Tgt Ion	Resp	Lower	Upper
114	100		
63	20.1	0.0	38.4
88	15.0	0.0	31.0

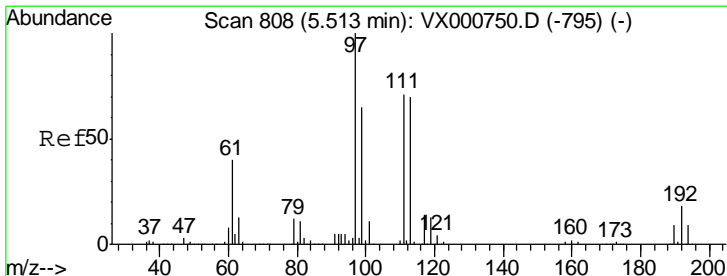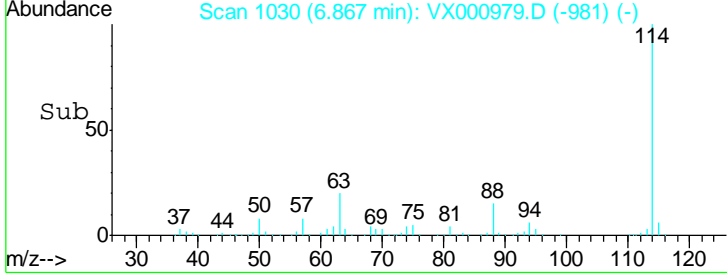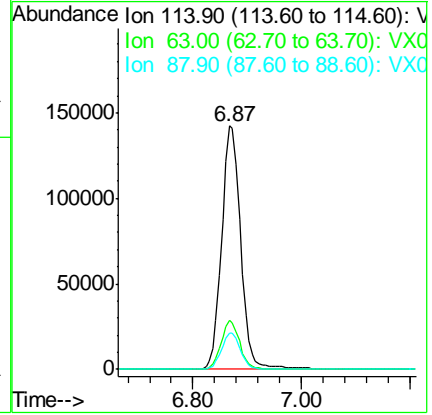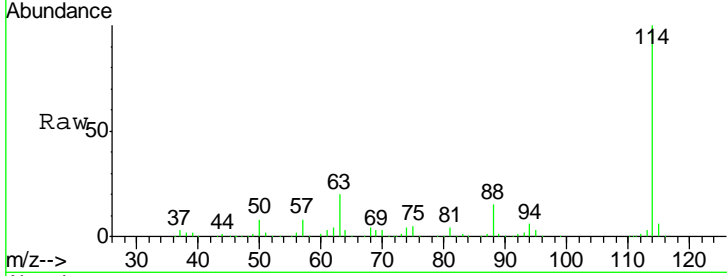

#35
 Dibromofluoromethane
 Concen: 45.68 ug/l
 RT: 5.51 min Scan# 808
 Delta R.T. -0.00 min
 Lab File: VX000979.D
 Acq: 17 Apr 2018 21:31

Tgt Ion	Resp	Lower	Upper
113	100		
111	102.0	81.5	122.3
192	25.7	20.4	30.6


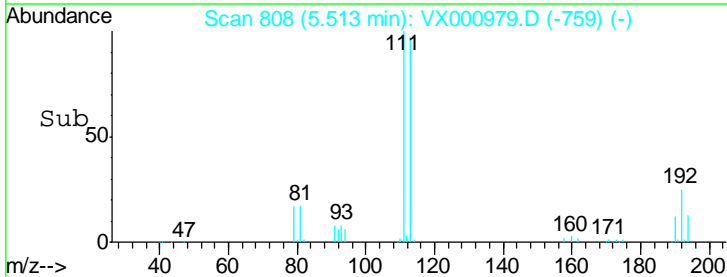
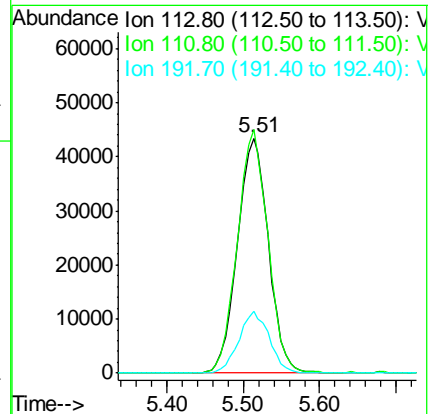
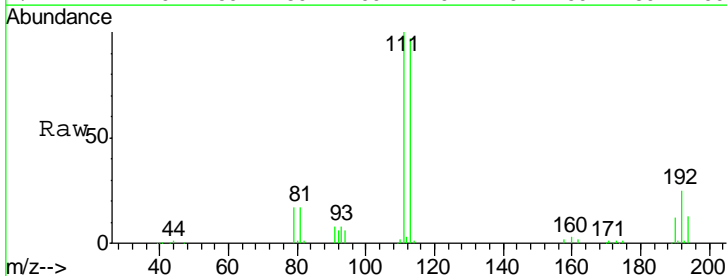


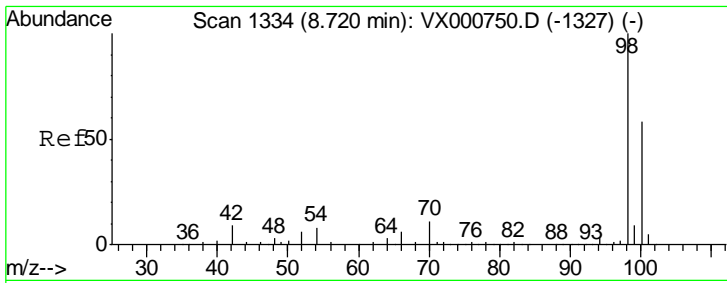

#50
 Toluene-d8
 Concen: 48.93 ug/l
 RT: 8.72 min Scan# 1334
 Delta R.T. -0.00 min
 Lab File: VX000979.D
 Acq: 17 Apr 2018 21:31




Instrument : MSVOA_X
 ClientSampled : PB108300ZHE#10 5X


Tgt Ion: 98 Resp: 485559
 Ion Ratio Lower Upper
 98 100
 100 64.3 52.6 79.0

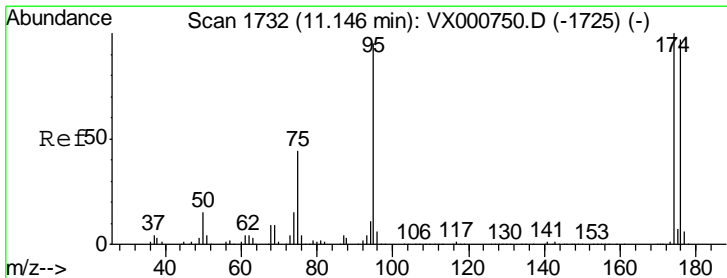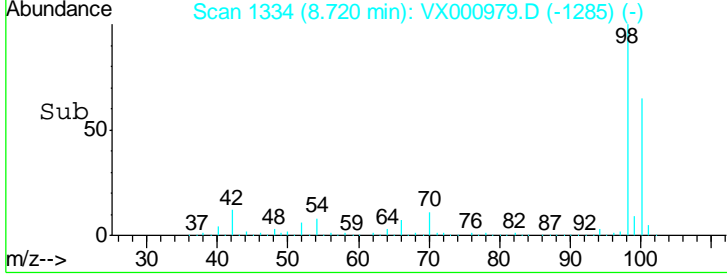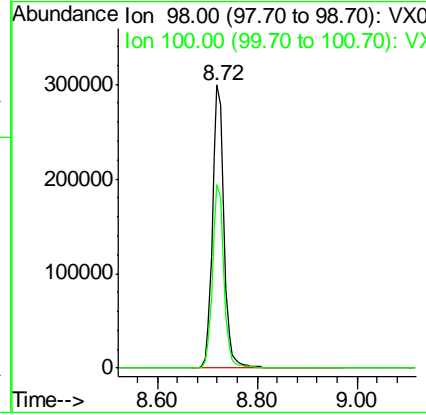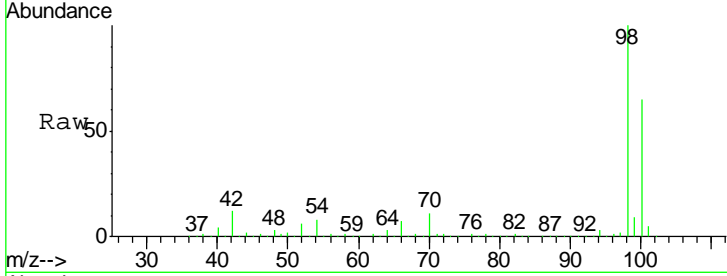

#62
 4-Bromofluorobenzene
 Concen: 44.74 ug/l
 RT: 11.14 min Scan# 1731
 Delta R.T. -0.01 min
 Lab File: VX000979.D
 Acq: 17 Apr 2018 21:31

Tgt Ion: 95 Resp: 183681
 Ion Ratio Lower Upper
 95 100
 174 97.0 0.0 198.4
 176 95.0 0.0 194.4


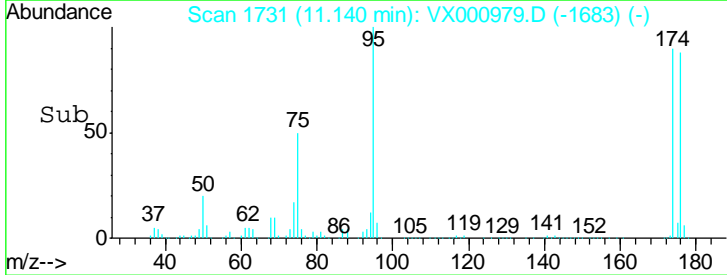
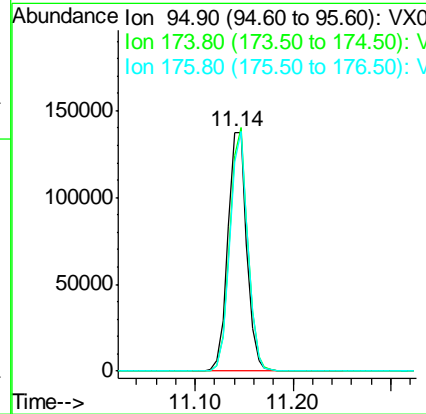
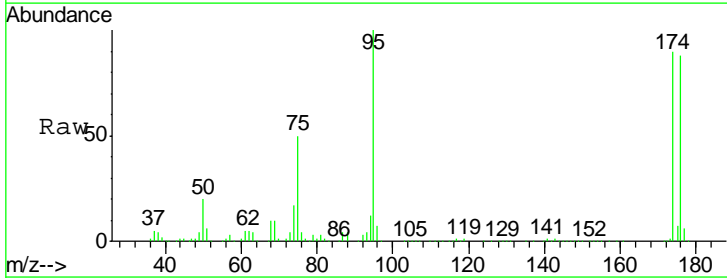


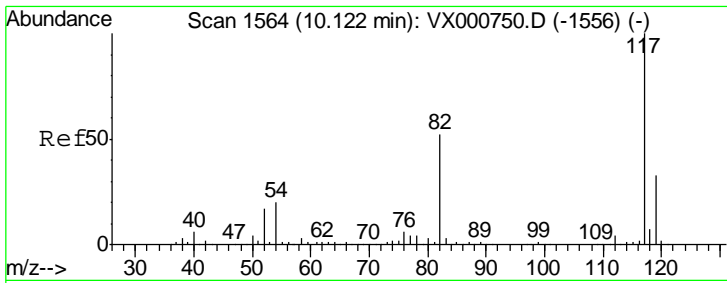

#63
 Chlorobenzene-d5
 Concen: 50.00 ug/l
 RT: 10.12 min Scan# 1563
 Delta R.T. -0.01 min
 Lab File: VX000979.D
 Acq: 17 Apr 2018 21:31

Instrument : MSVOA_X
 ClientSampleId : PB108300ZHE#10 5X

Tgt Ion	Resp	Lower	Upper
117	100		
82	53.1	41.9	62.9
119	32.0	26.0	39.0

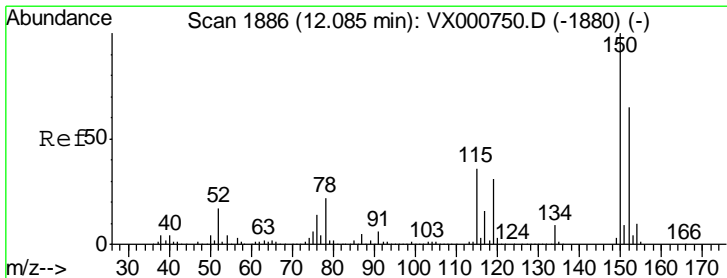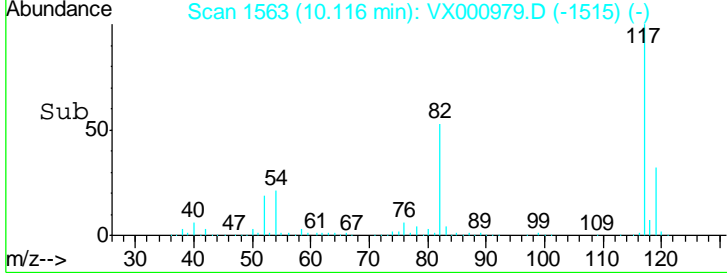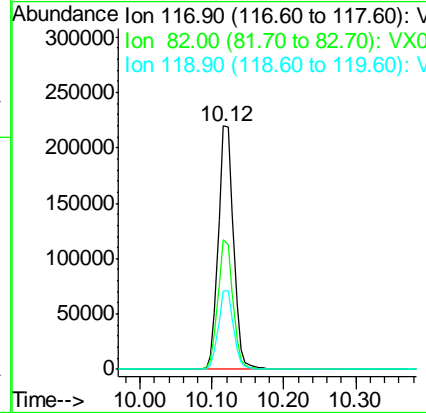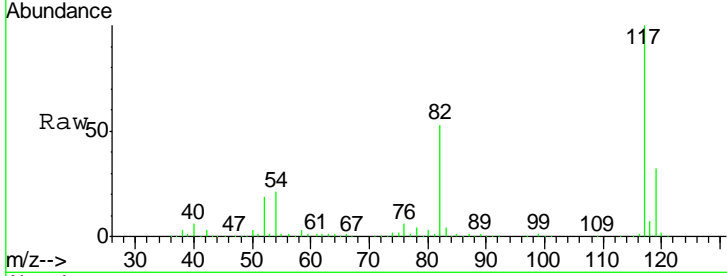

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.00 ug/l
 RT: 12.09 min Scan# 1886
 Delta R.T. -0.00 min
 Lab File: VX000979.D
 Acq: 17 Apr 2018 21:31

Tgt Ion	Resp	Lower	Upper
152	100		
115	54.0	37.9	113.7
150	156.6	0.0	348.0

