


Data Path : W:\HPCHEM1\MSVOA_X\Data\VX041718\
Data File : VX000965.D
Acq On : 17 Apr 2018 12:02
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
Title : SW846 8260
Last Update : Tue Apr 10 15:49:28 2018

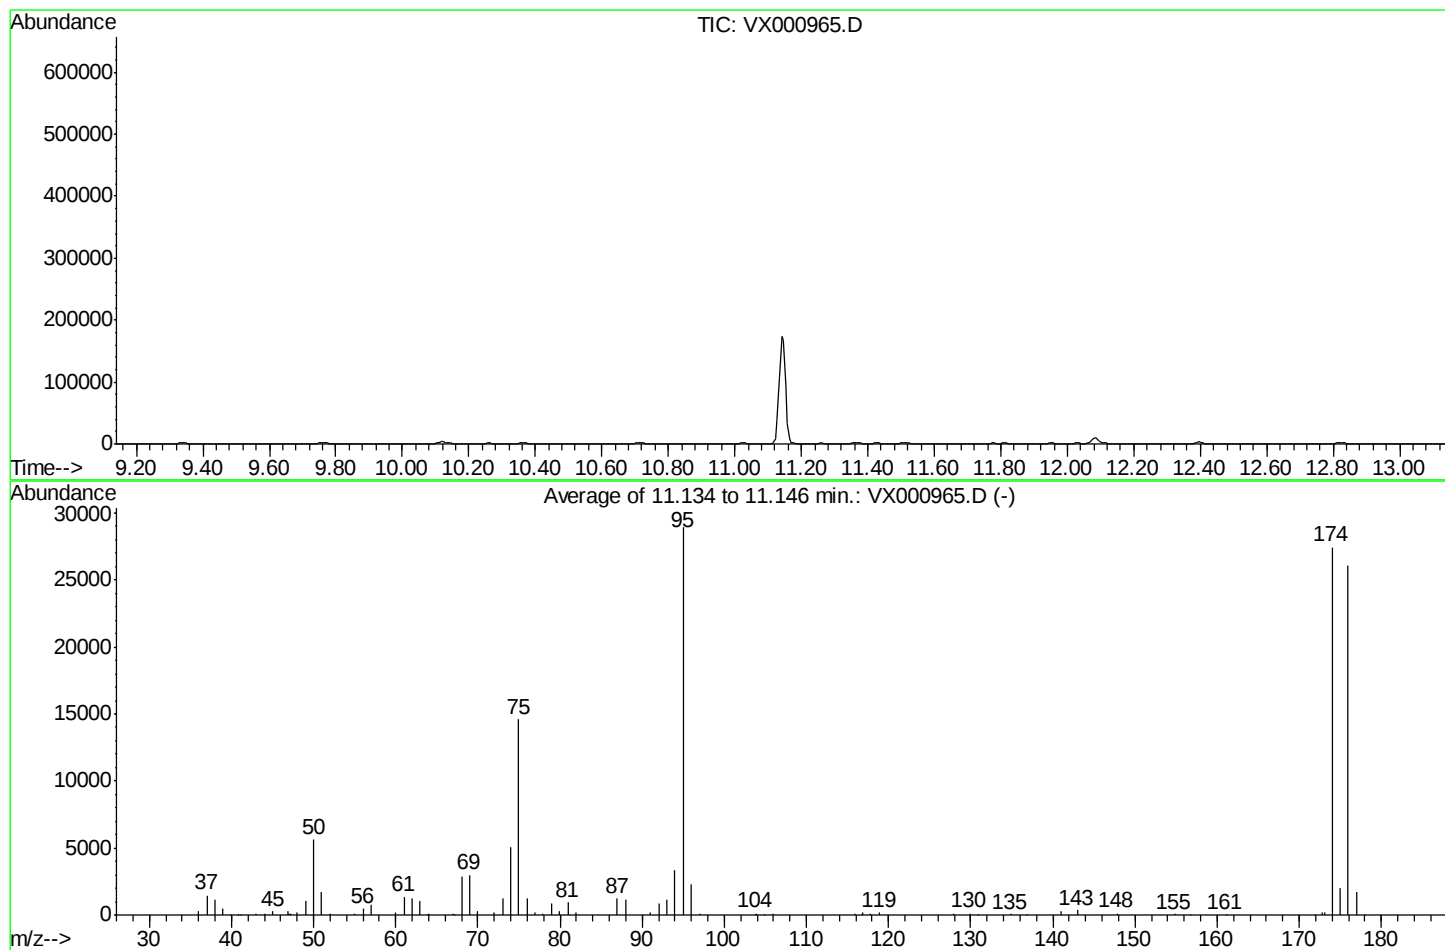

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	5596	PASS
75	95	30	60	50.4	14592	PASS
95	95	100	100	100.0	28930	PASS
96	95	5	9	7.8	2256	PASS
173	174	0.00	2	0.8	218	PASS
174	95	50	100	94.8	27426	PASS
175	174	5	9	7.2	1980	PASS
176	174	95	101	95.2	26117	PASS
177	176	5	9	6.6	1725	PASS