



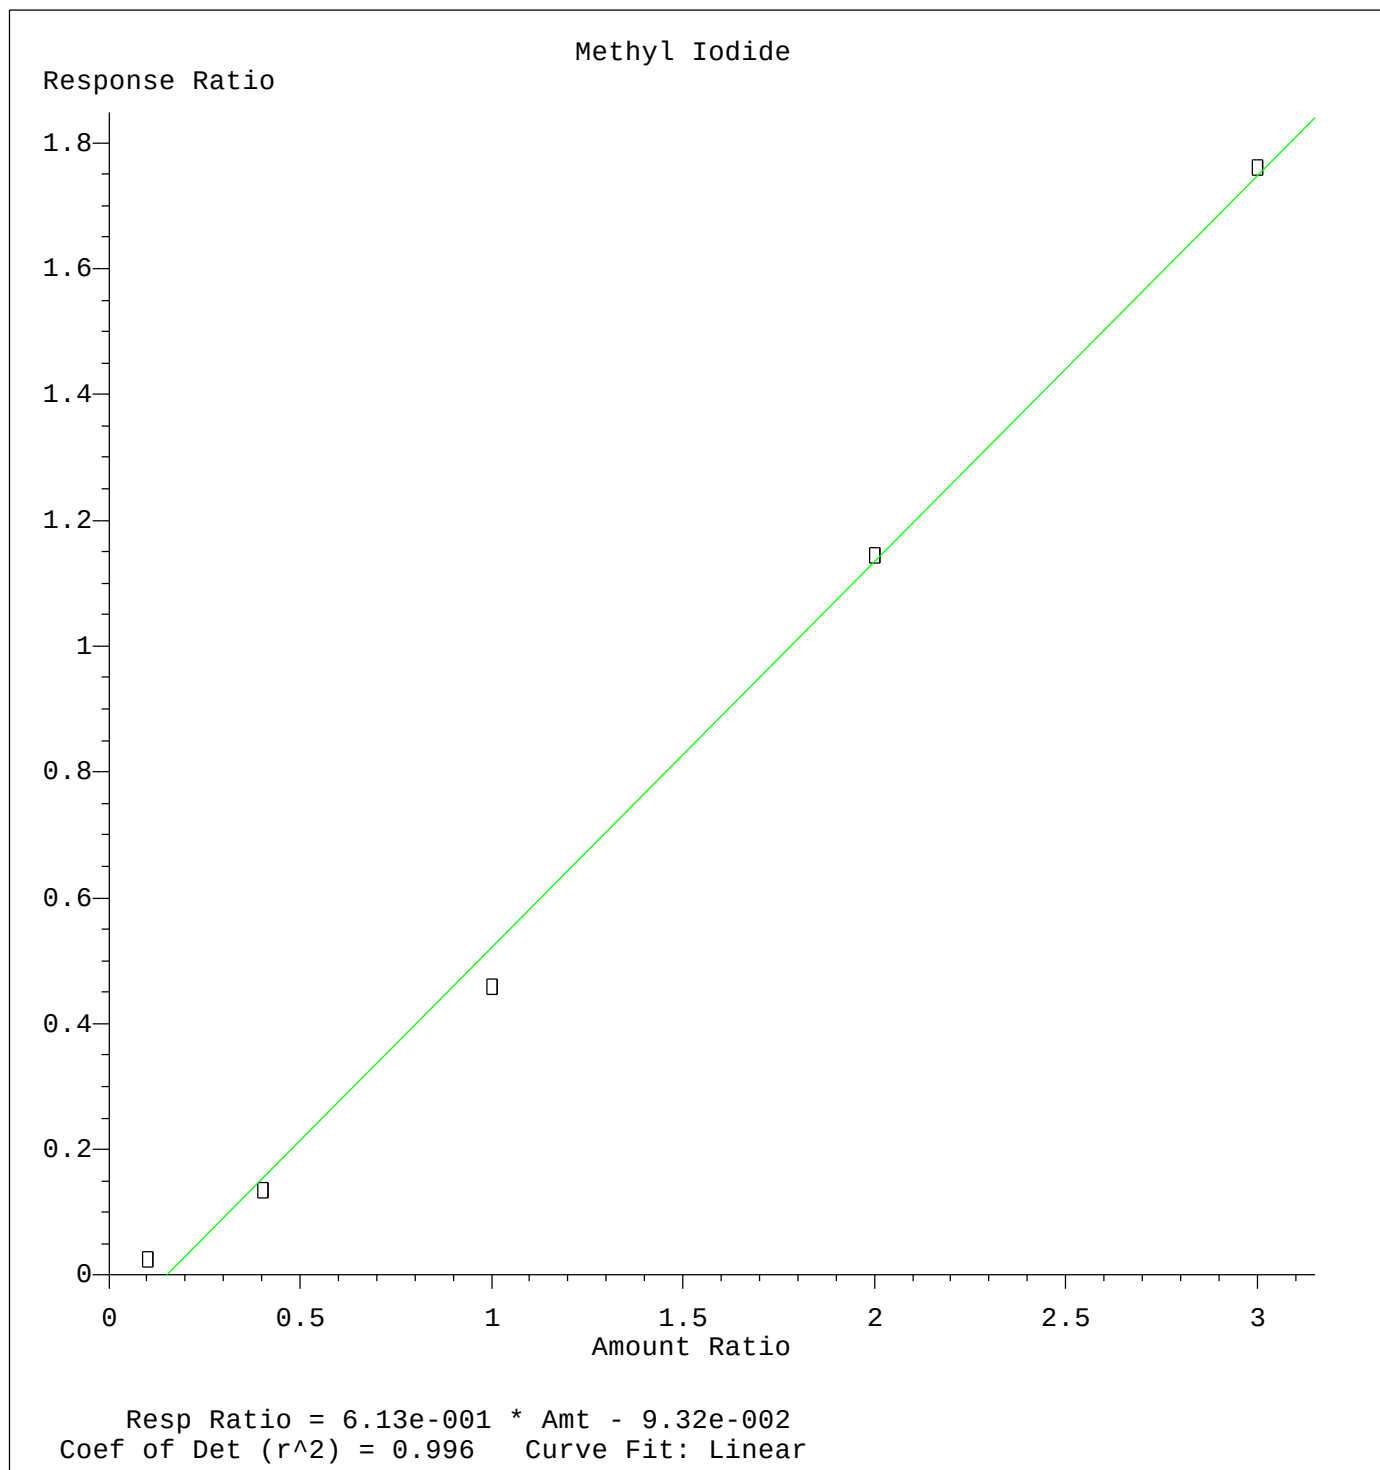


Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X041918W.M
Calibration Table Last Updated: Fri Apr 20 14:48:32 2018

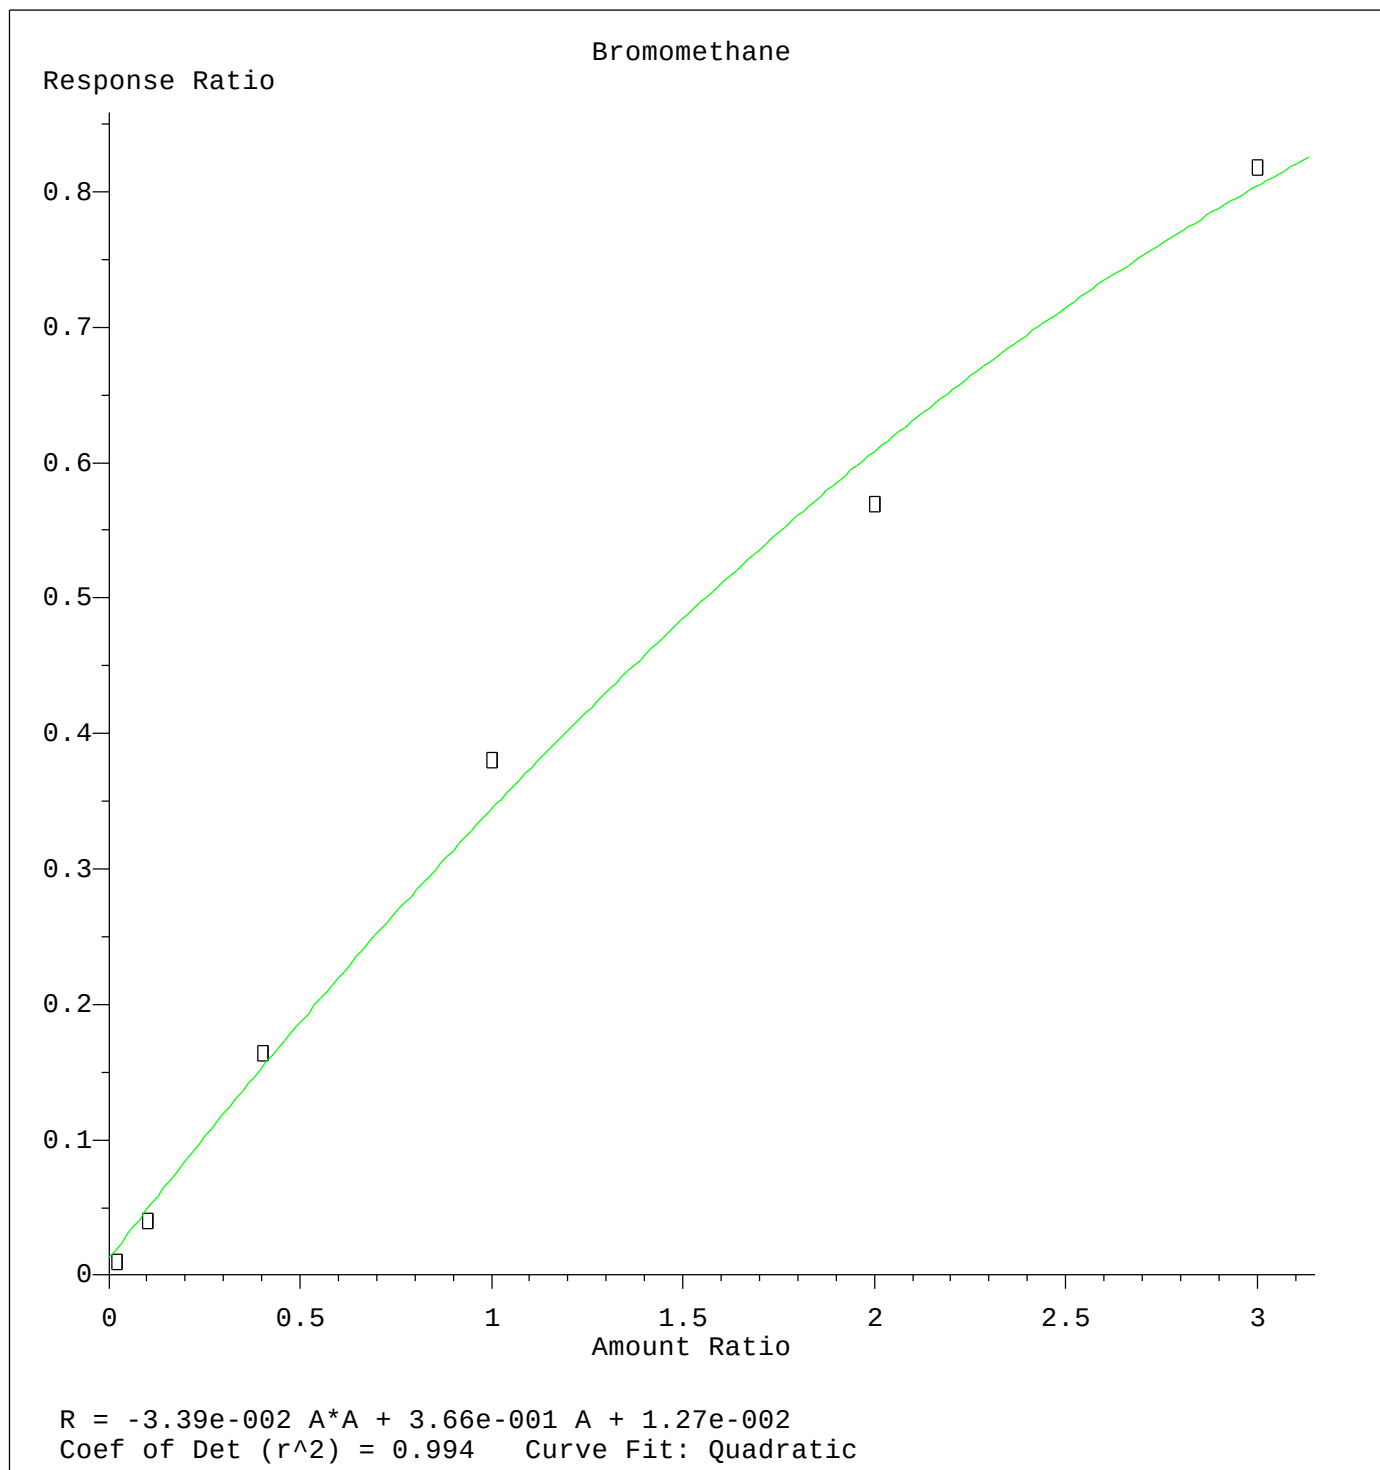

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X041918W.M
Calibration Table Last Updated: Fri Apr 20 14:48:32 2018


trans-1,4-Dichloro-2-butene

Response Ratio

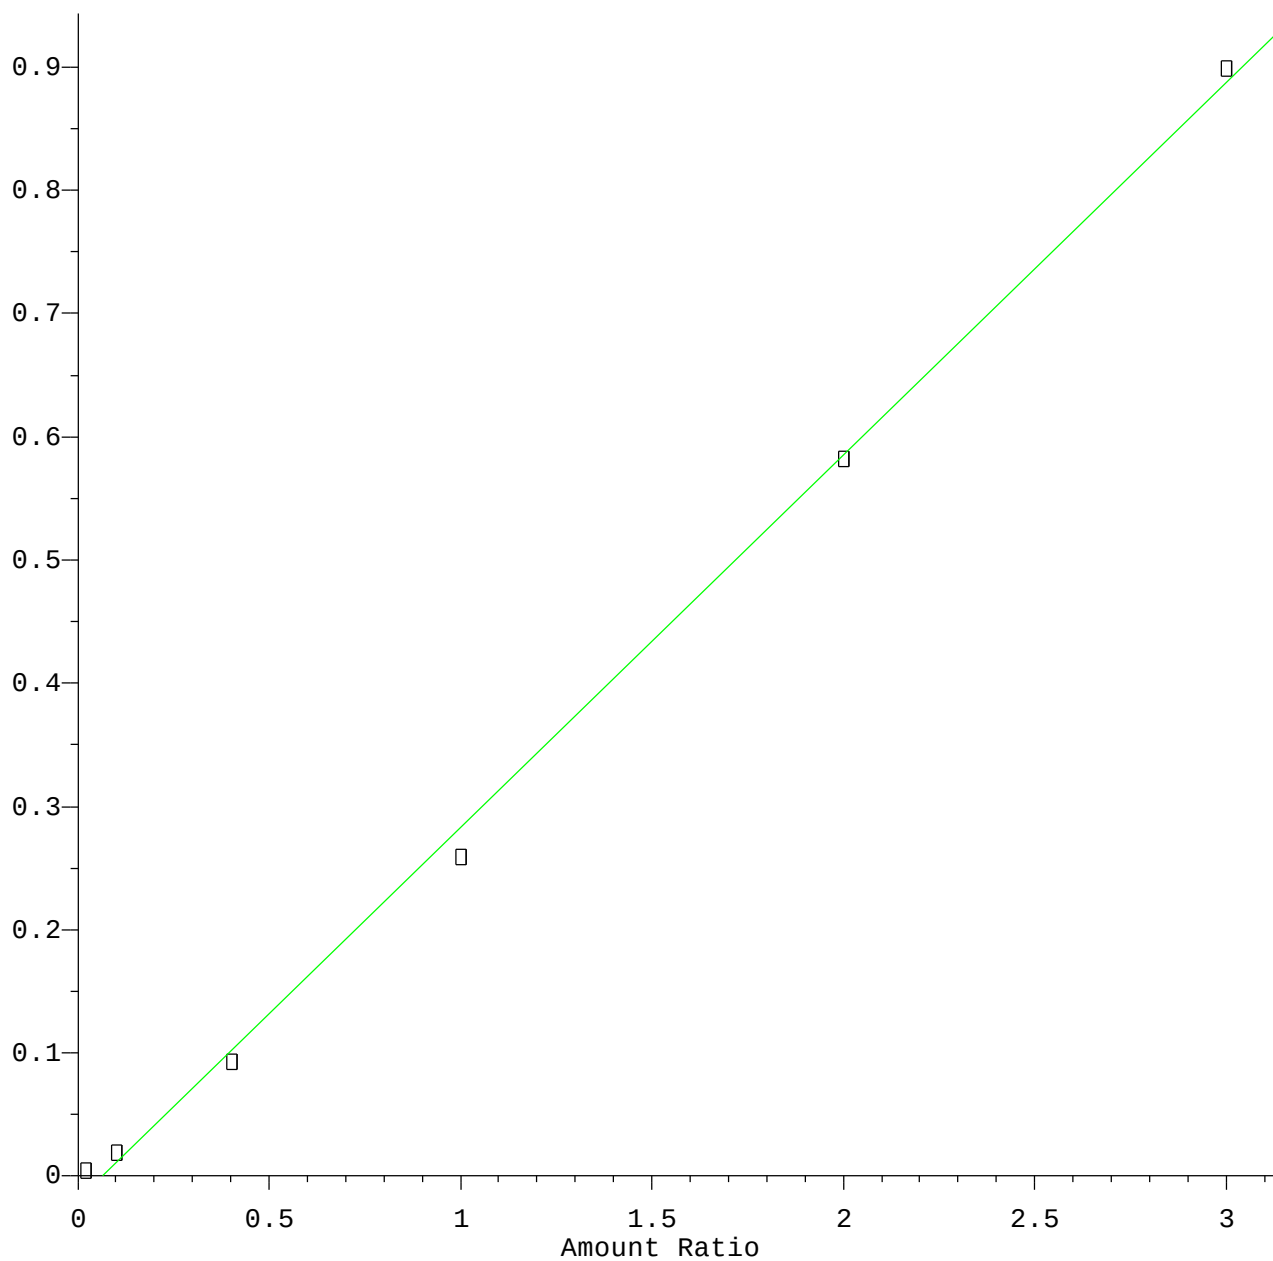


Resp Ratio = $3.02 \times 10^{-1} \times \text{Amt} - 1.96 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X041918W.M
Calibration Table Last Updated: Fri Apr 20 14:48:32 2018

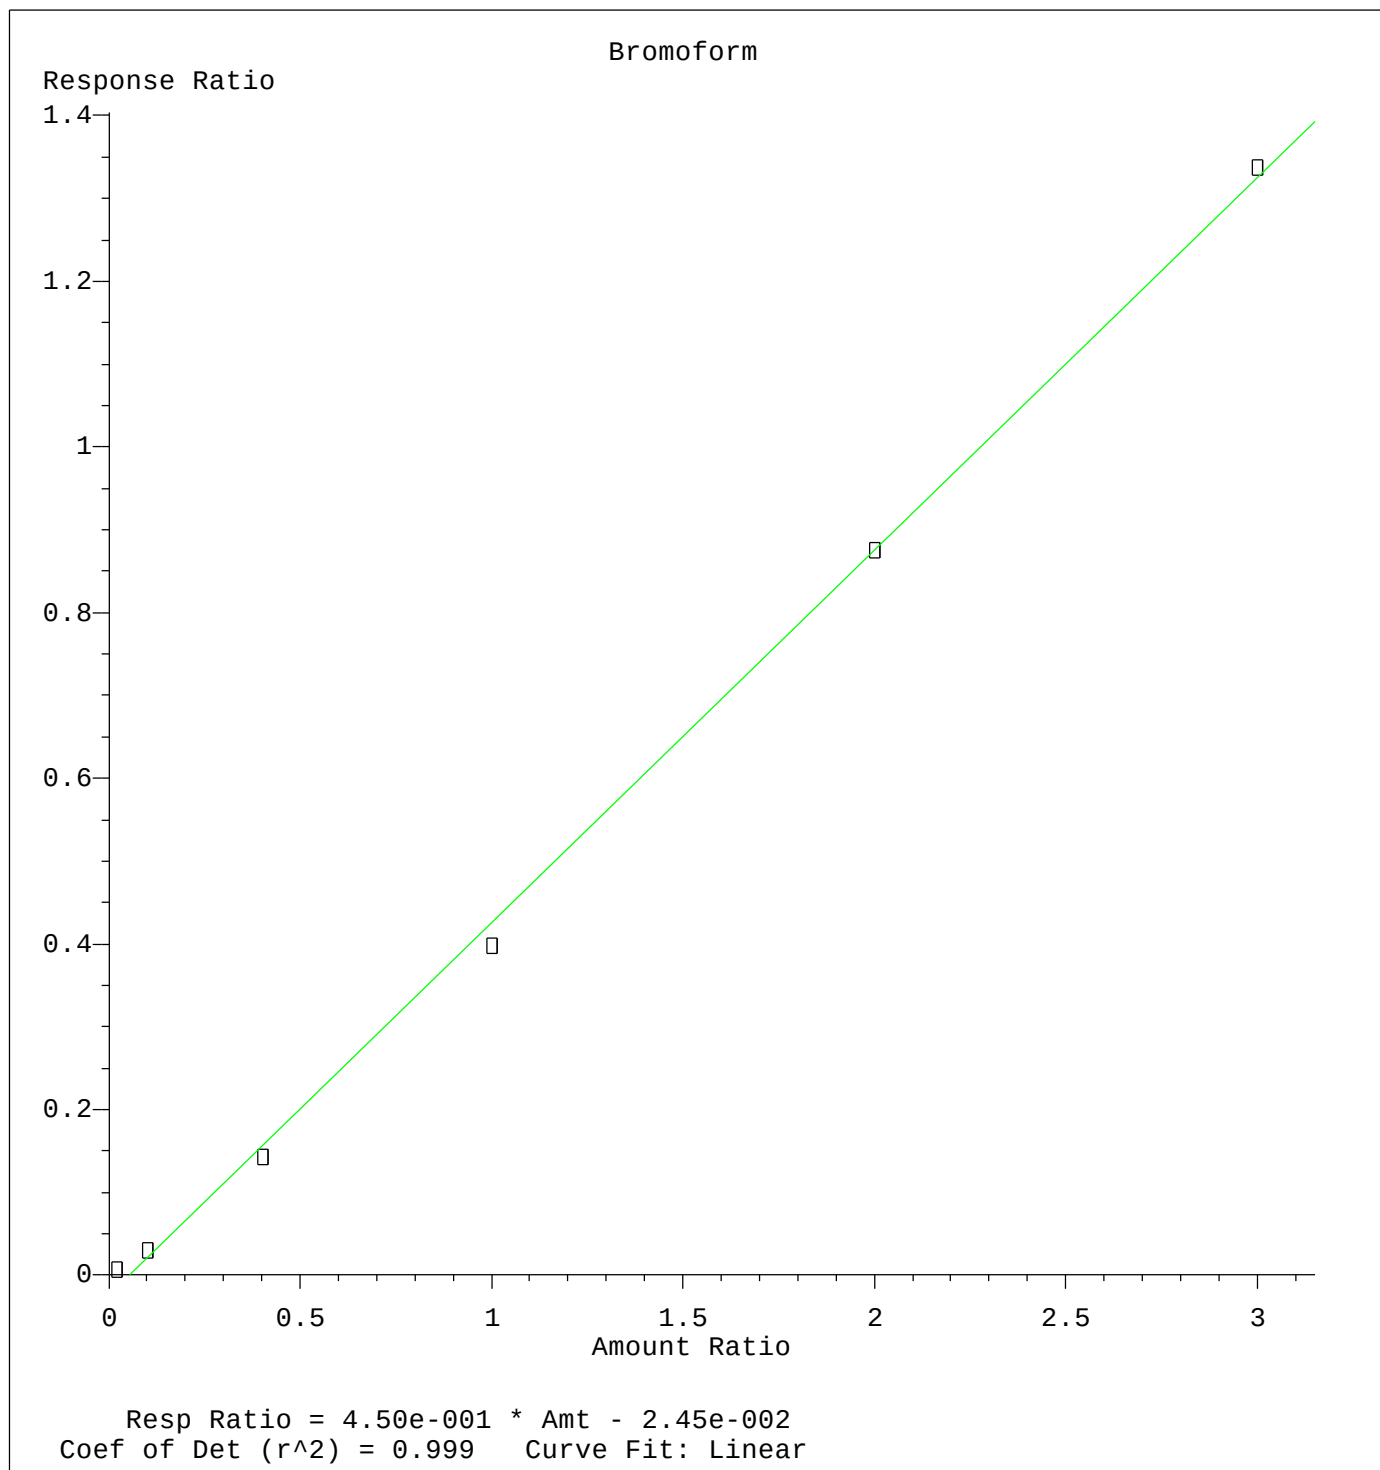

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X041918W.M
Calibration Table Last Updated: Fri Apr 20 14:48:32 2018

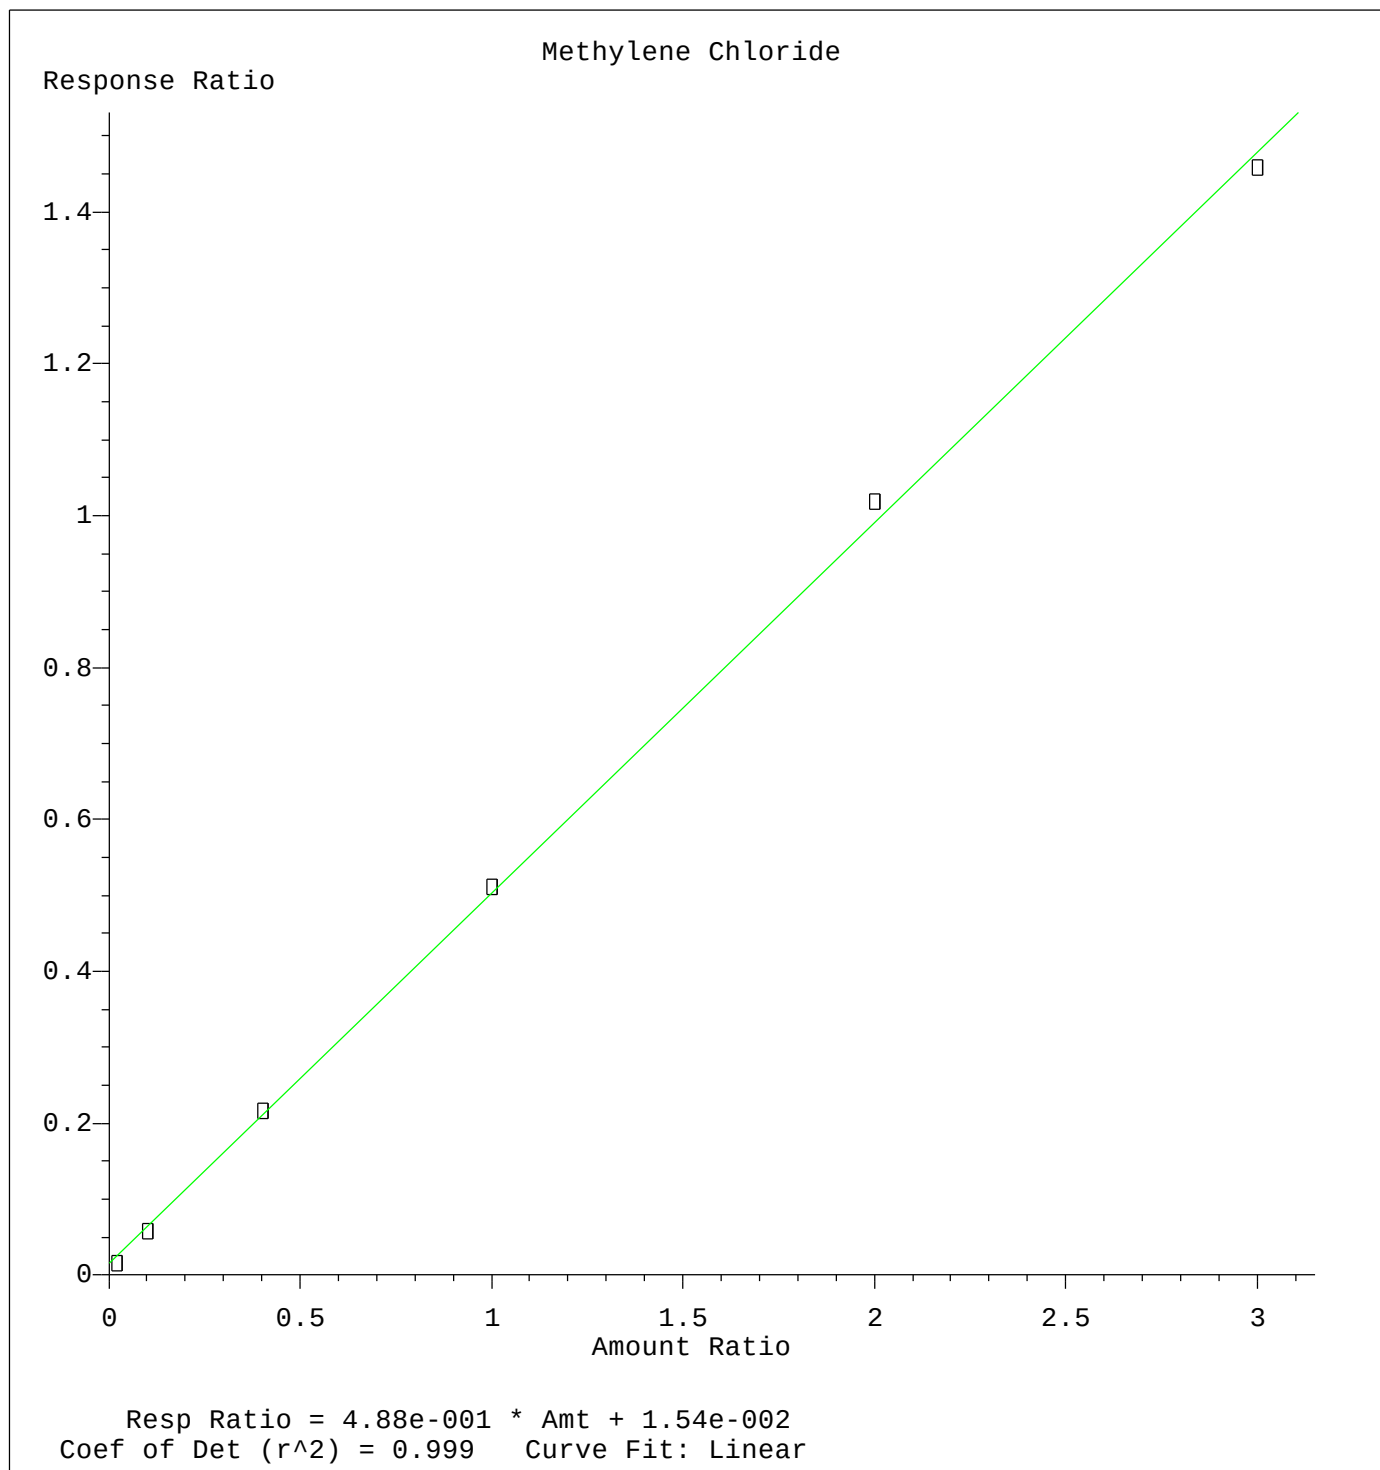

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X041918W.M
Calibration Table Last Updated: Fri Apr 20 14:48:32 2018

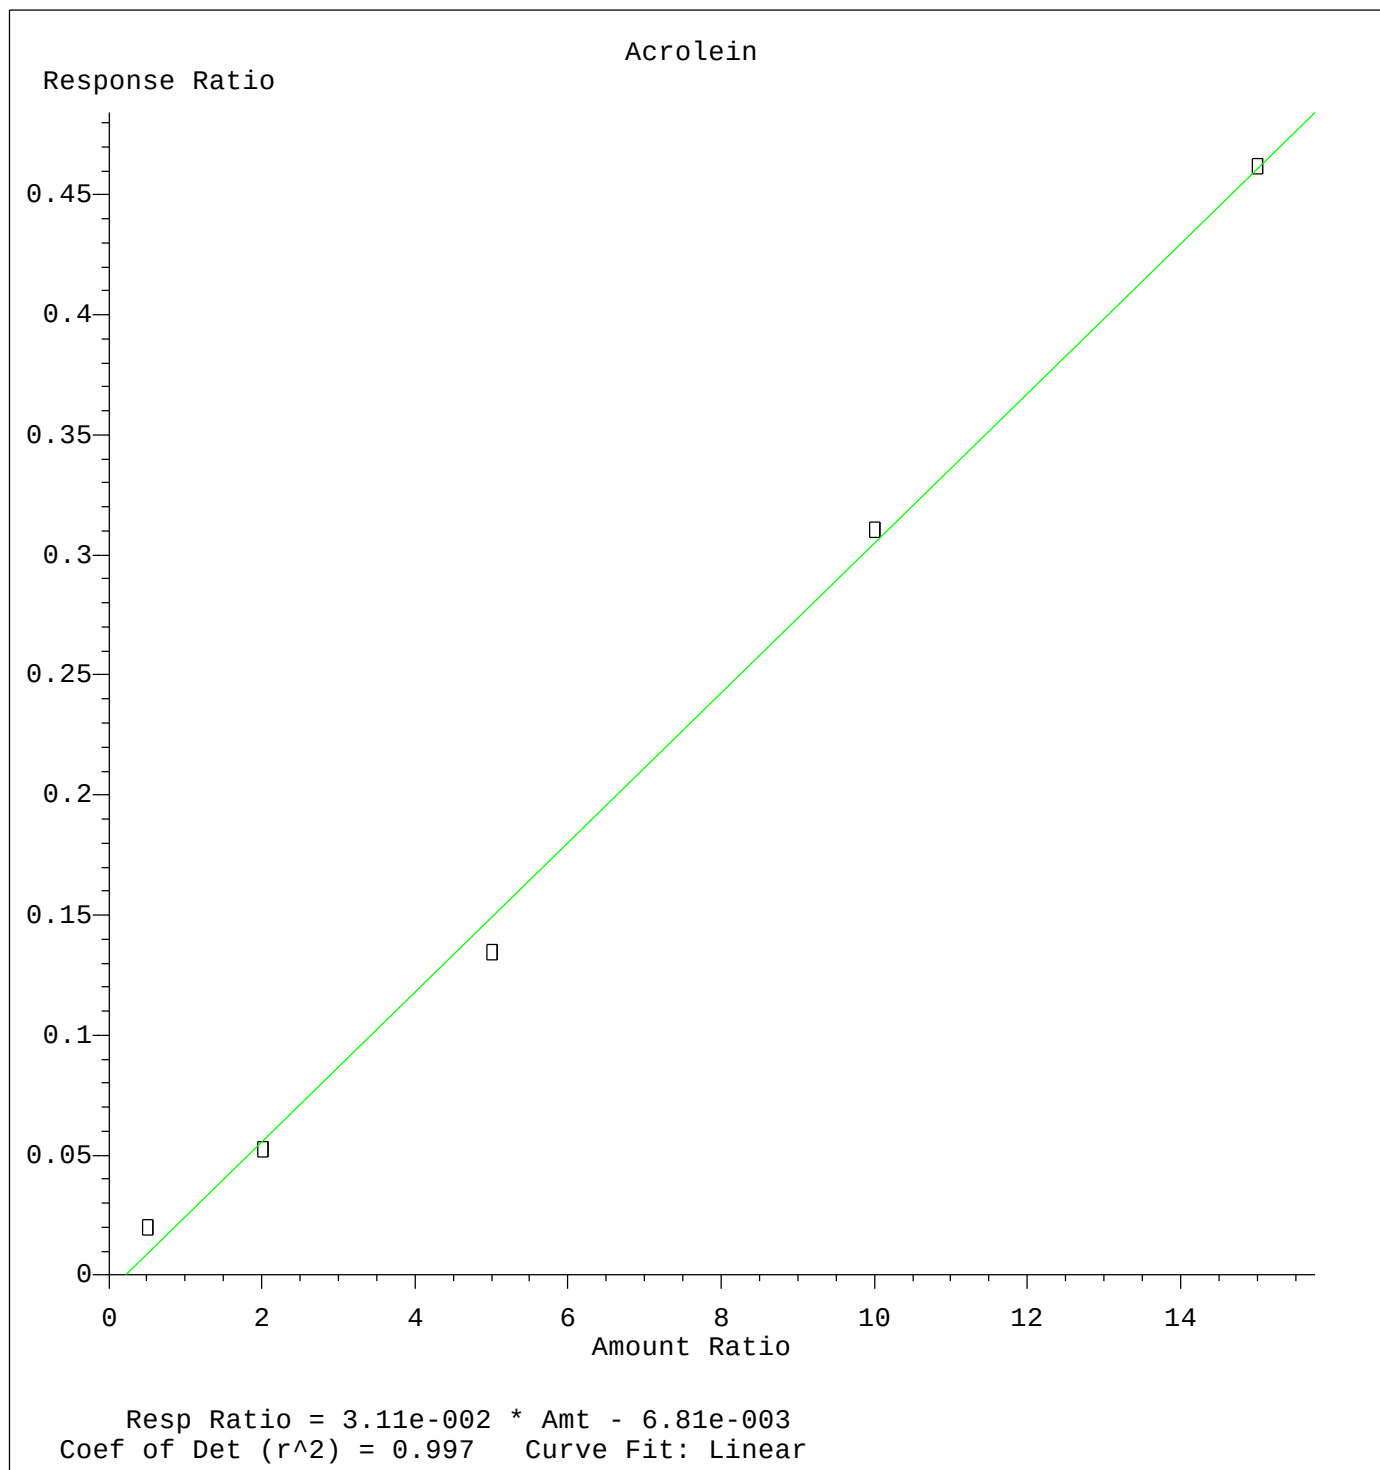

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X041918W.M
Calibration Table Last Updated: Fri Apr 20 14:48:32 2018