


Data Path : W:\HPCHEM1\MSVOA_X\DATA\VX042018\
 Data File : VX001000.D
 Acq On : 20 Apr 2018 09:14
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041918W.M
 Title : SW846 8260
 Last Update : Fri Apr 20 05:03:28 2018

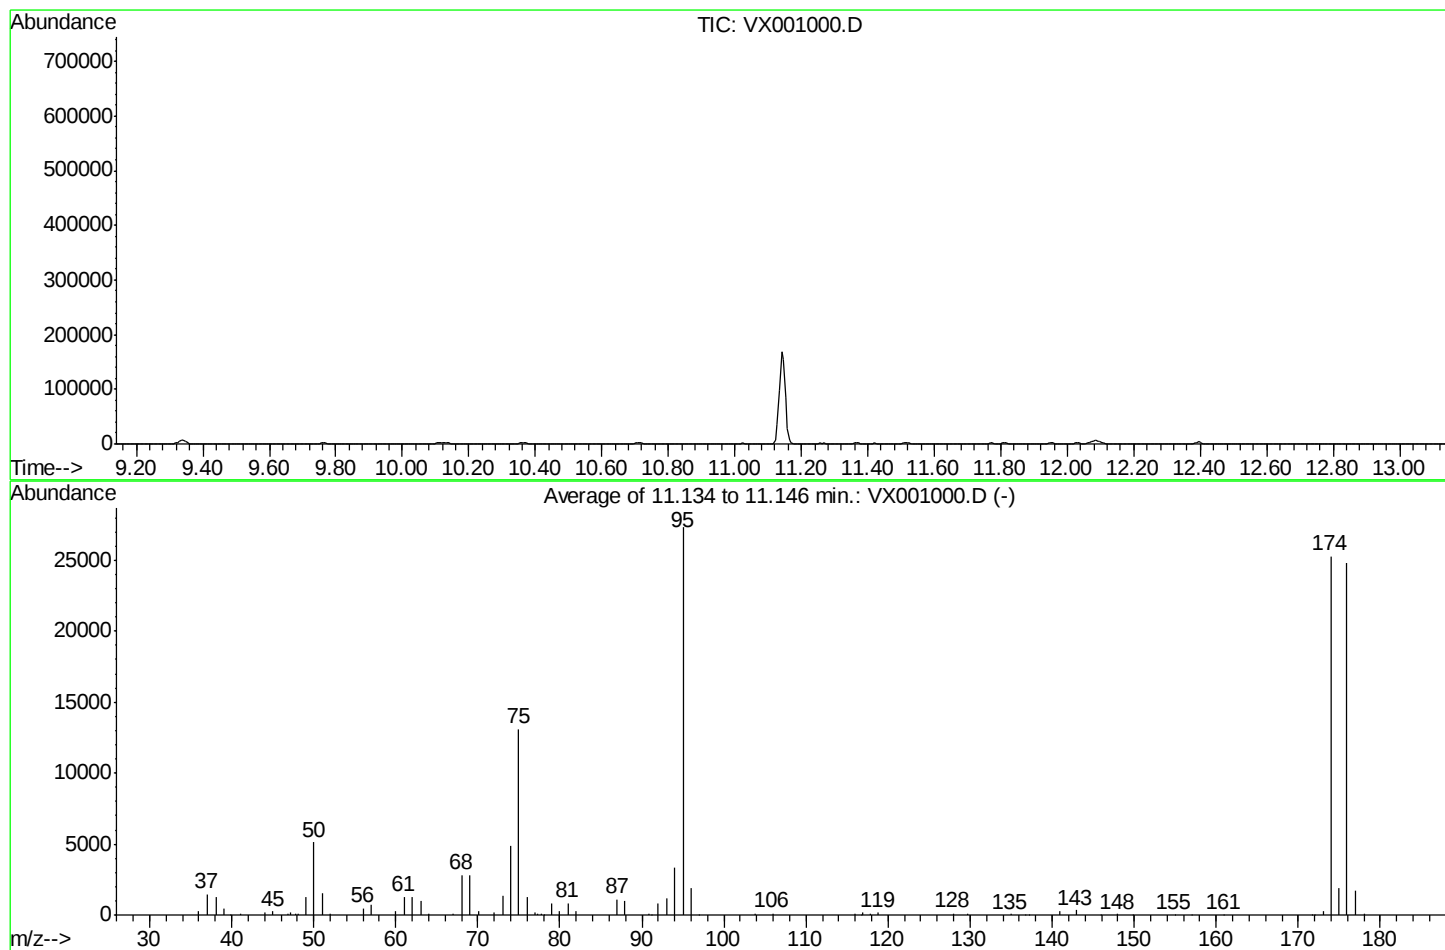

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	5135	PASS
75	95	30	60	48.0	13113	PASS
95	95	100	100	100.0	27317	PASS
96	95	5	9	7.0	1921	PASS
173	174	0.00	2	0.9	233	PASS
174	95	50	100	92.5	25256	PASS
175	174	5	9	7.6	1912	PASS
176	174	95	101	98.2	24792	PASS
177	176	5	9	6.8	1691	PASS