


Data Path : W:\HPCHEM1\MSVOA_X\DATA\VX042018\
Data File : VX001022.D
Acq On : 20 Apr 2018 21:23
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041918W.M
Title : SW846 8260
Last Update : Fri Apr 20 05:03:28 2018

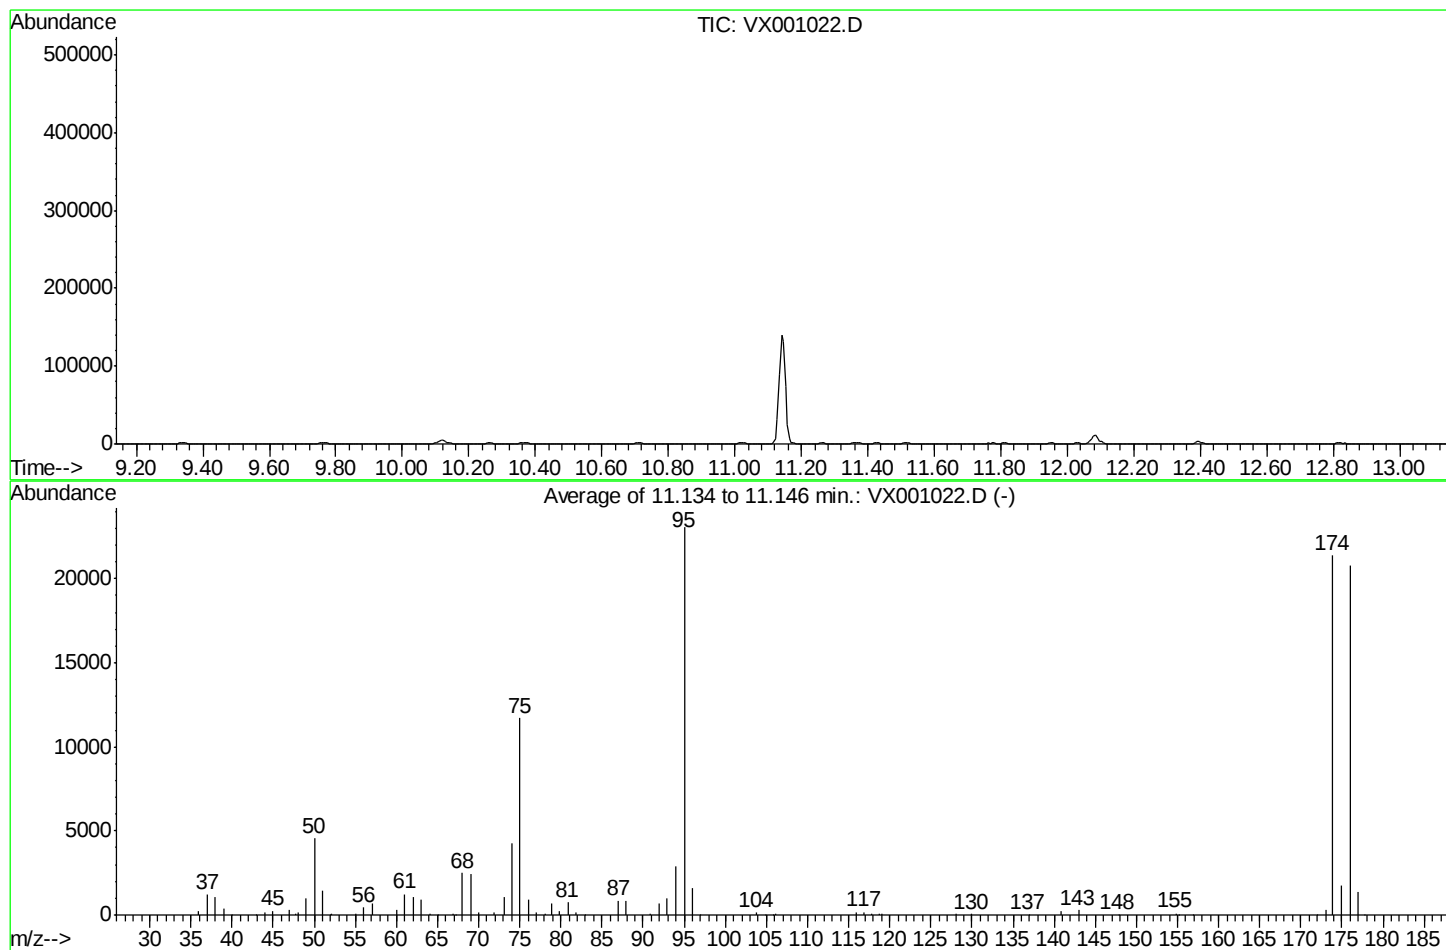

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	4550	PASS
75	95	30	60	50.8	11721	PASS
95	95	100	100	100.0	23058	PASS
96	95	5	9	6.8	1571	PASS
173	174	0.00	2	1.3	276	PASS
174	95	50	100	92.7	21367	PASS
175	174	5	9	8.1	1728	PASS
176	174	95	101	97.3	20791	PASS
177	176	5	9	6.5	1348	PASS