


Data Path : W:\HPCHEM1\MSVOA X\Data\VX042318\
 Data File : VX001047.D
 Acq On : 23 Apr 2018 09:38
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041918W.M
 Title : SW846 8260
 Last Update : Fri Apr 20 05:03:28 2018

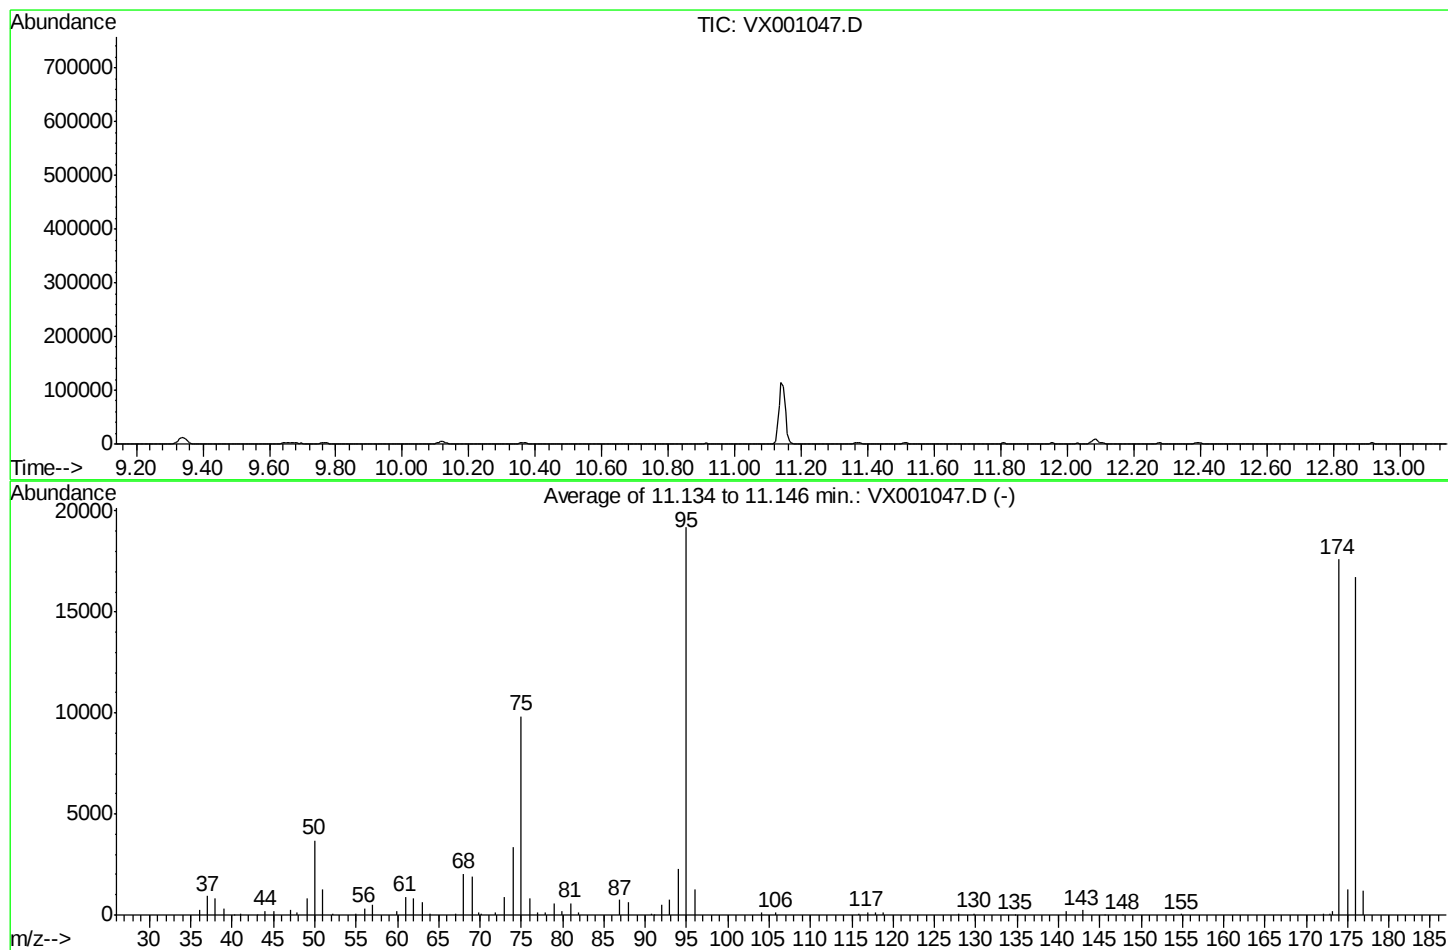

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	3695	PASS
75	95	30	60	51.3	9841	PASS
95	95	100	100	100.0	19193	PASS
96	95	5	9	6.7	1279	PASS
173	174	0.00	2	1.0	176	PASS
174	95	50	100	91.7	17592	PASS
175	174	5	9	7.4	1298	PASS
176	174	95	101	95.0	16713	PASS
177	176	5	9	7.1	1188	PASS