


Data Path : W:\HPCHEM1\MSVOA X\DATA\VX042518\
Data File : VX001112.D
Acq On : 25 Apr 2018 09:29
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041918W.M
Title : SW846 8260
Last Update : Fri Apr 20 05:03:28 2018

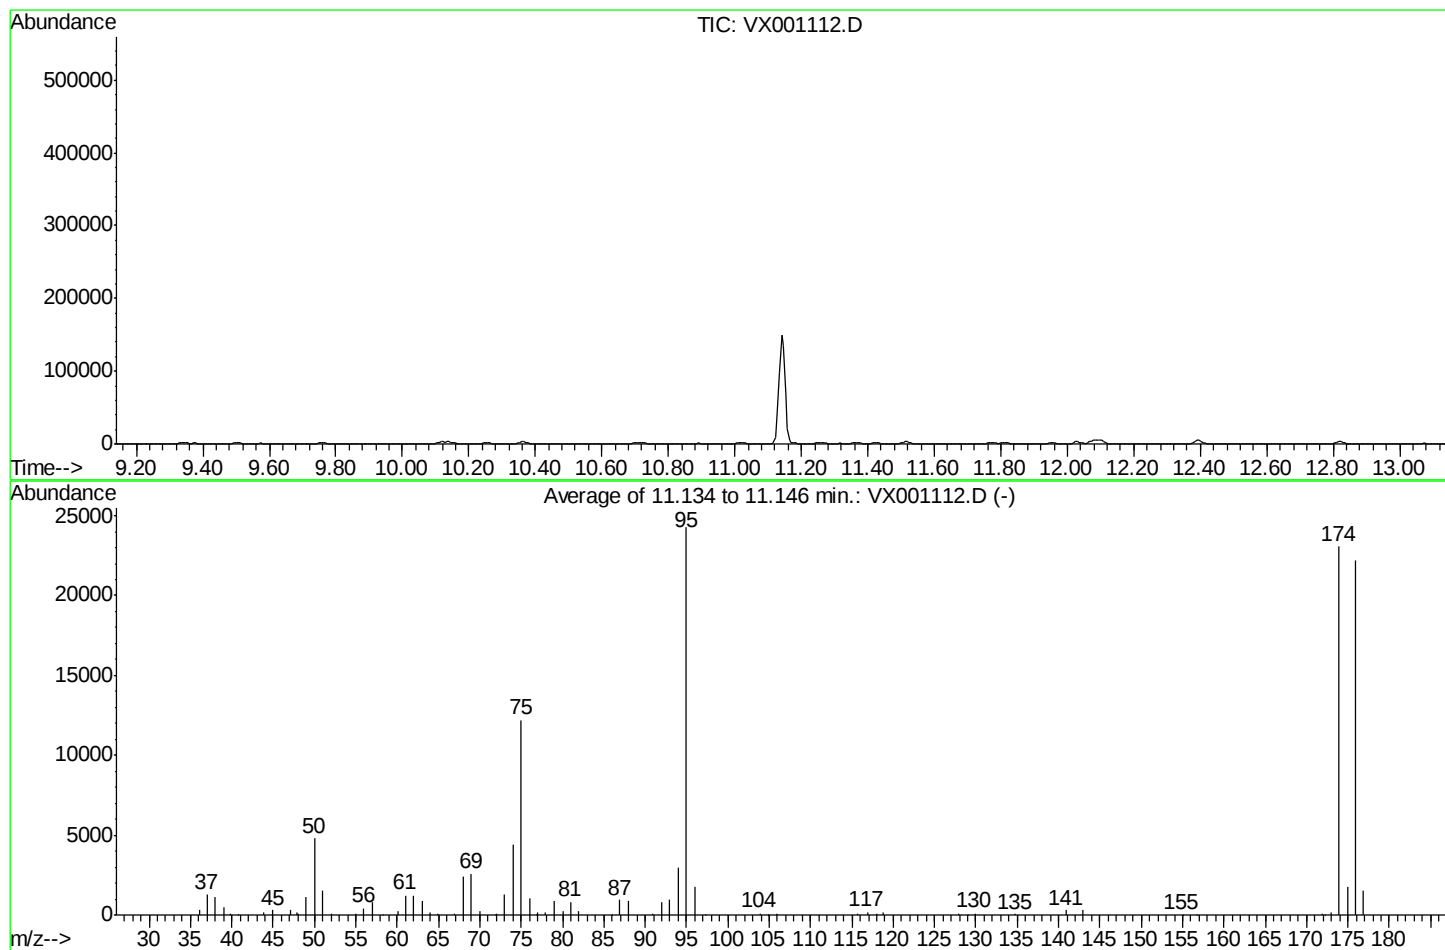

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	4801	PASS
75	95	30	60	50.3	12220	PASS
95	95	100	100	100.0	24272	PASS
96	95	5	9	7.3	1768	PASS
173	174	0.00	2	0.9	197	PASS
174	95	50	100	95.0	23065	PASS
175	174	5	9	7.7	1773	PASS
176	174	95	101	96.2	22193	PASS
177	176	5	9	6.8	1501	PASS