



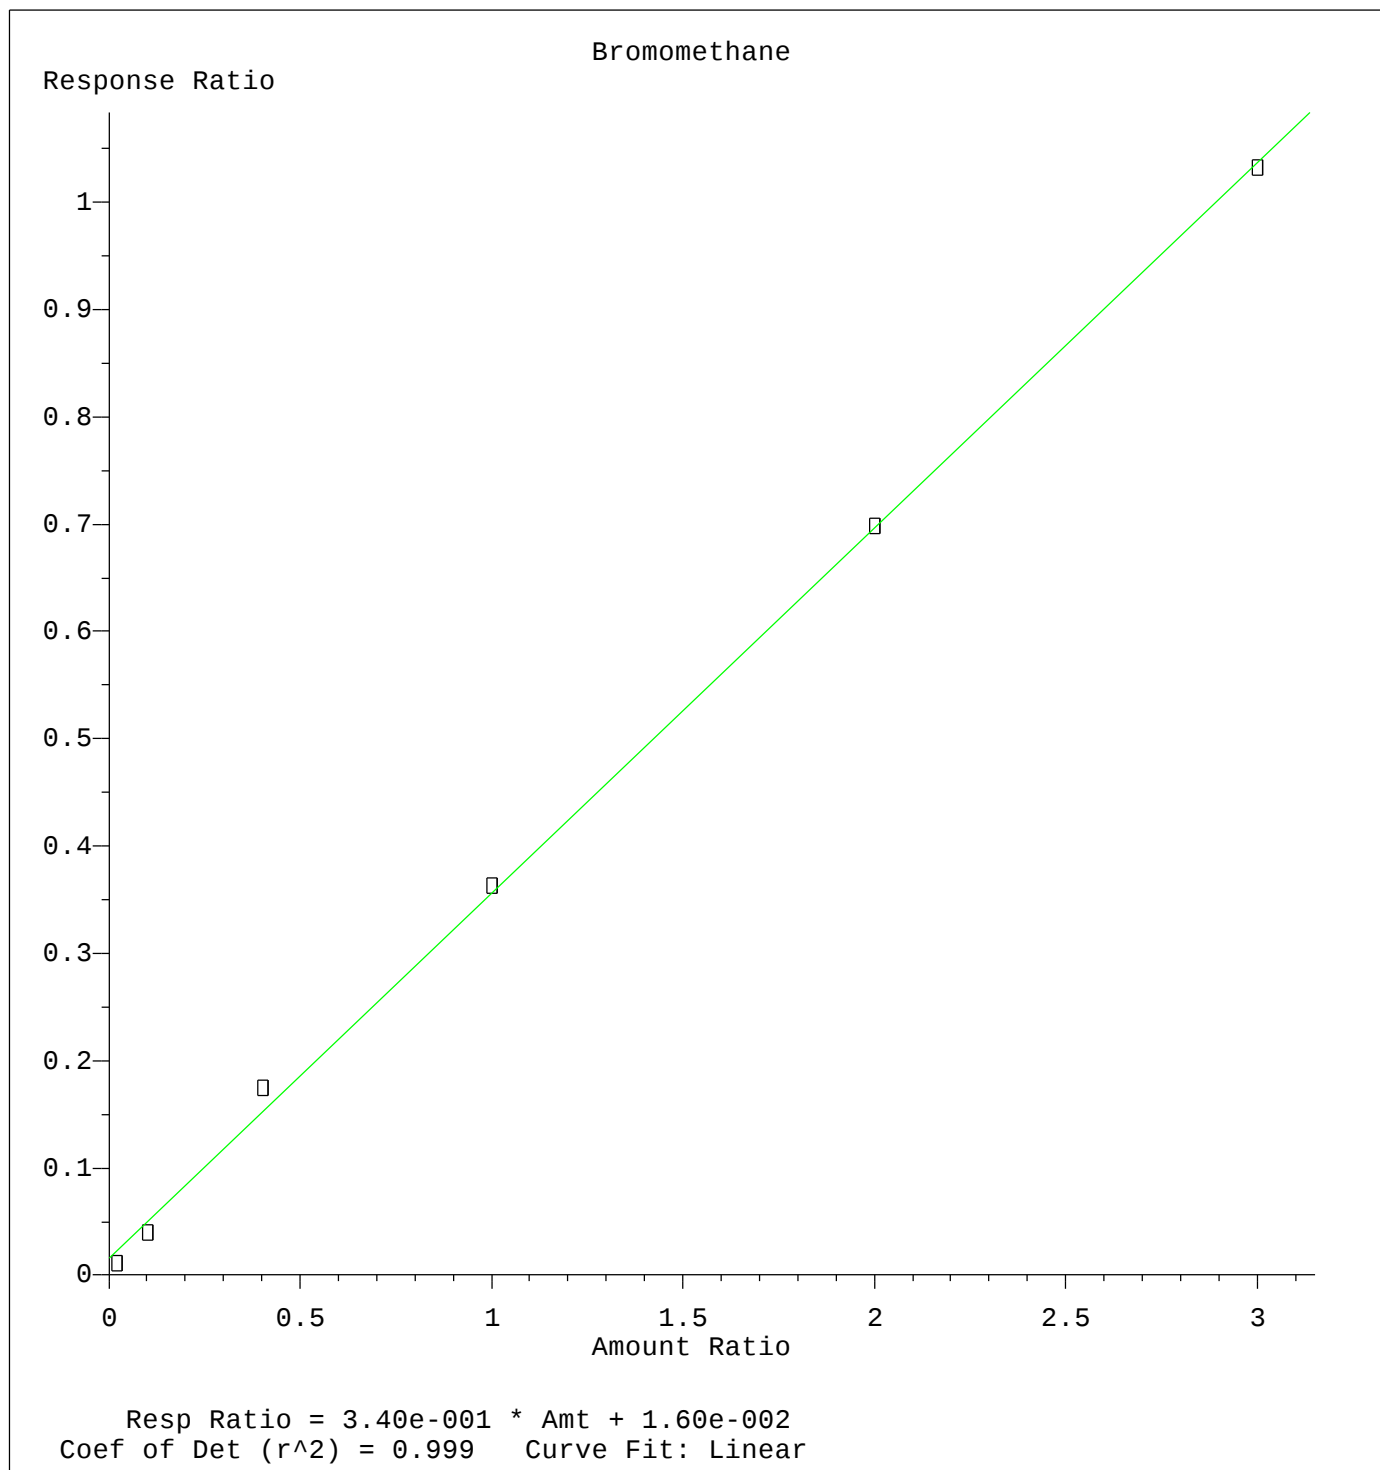


Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X042618W.M
Calibration Table Last Updated: Fri Apr 27 01:51:42 2018

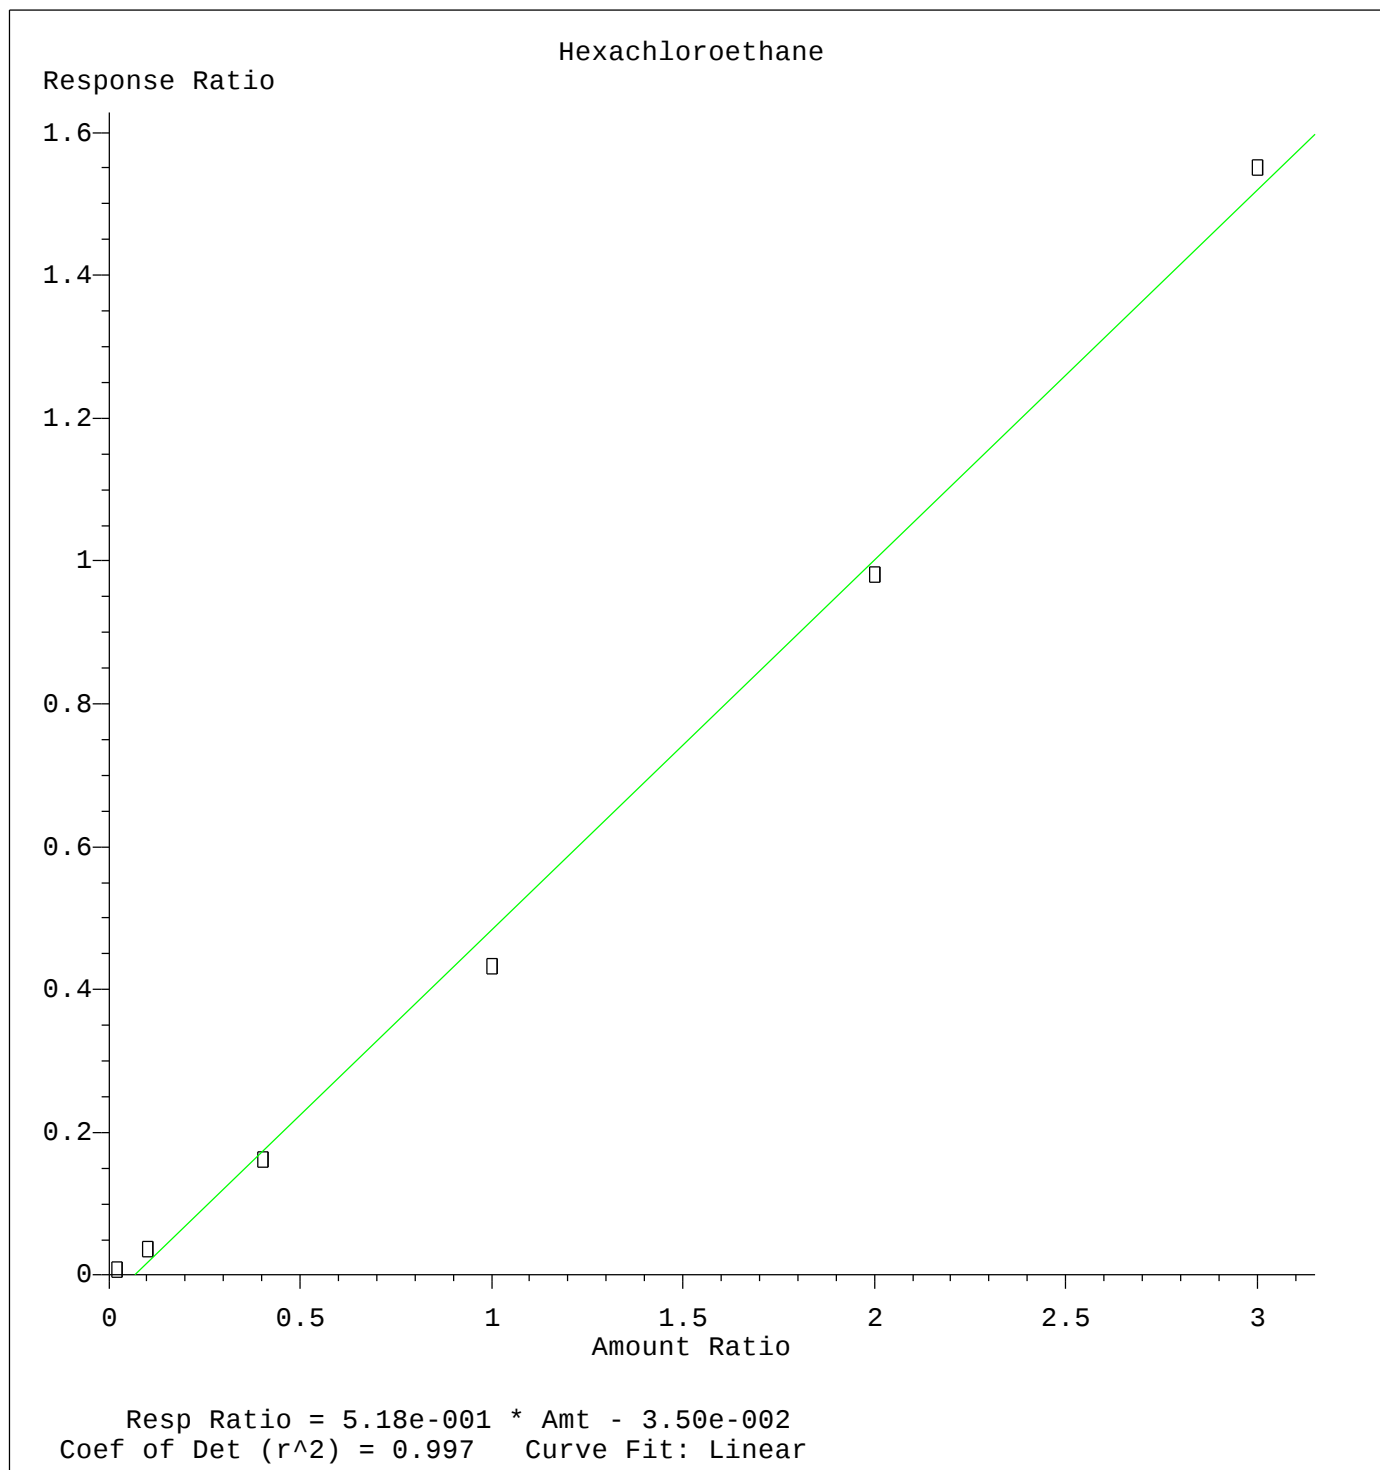

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X042618W.M
Calibration Table Last Updated: Fri Apr 27 01:51:42 2018


trans-1,4-Dichloro-2-butene

Response Ratio

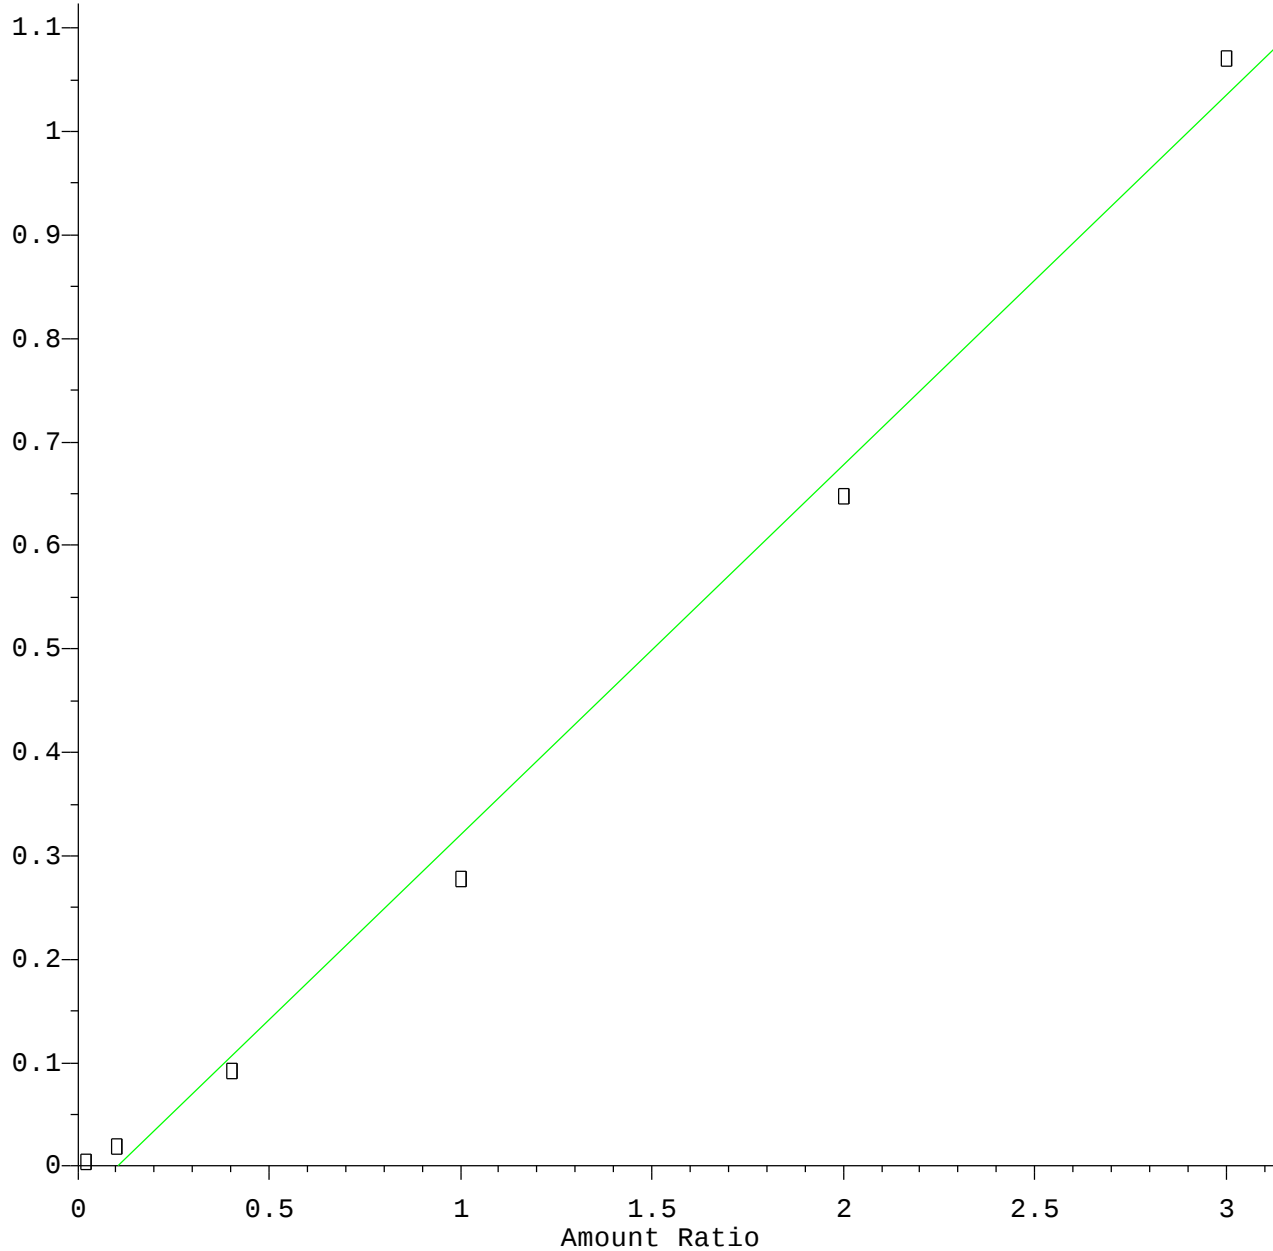

Resp Ratio = $3.57 \times 10^{-1} \times \text{Amt} - 3.68 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear


Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X042618W.M
Calibration Table Last Updated: Fri Apr 27 01:51:42 2018

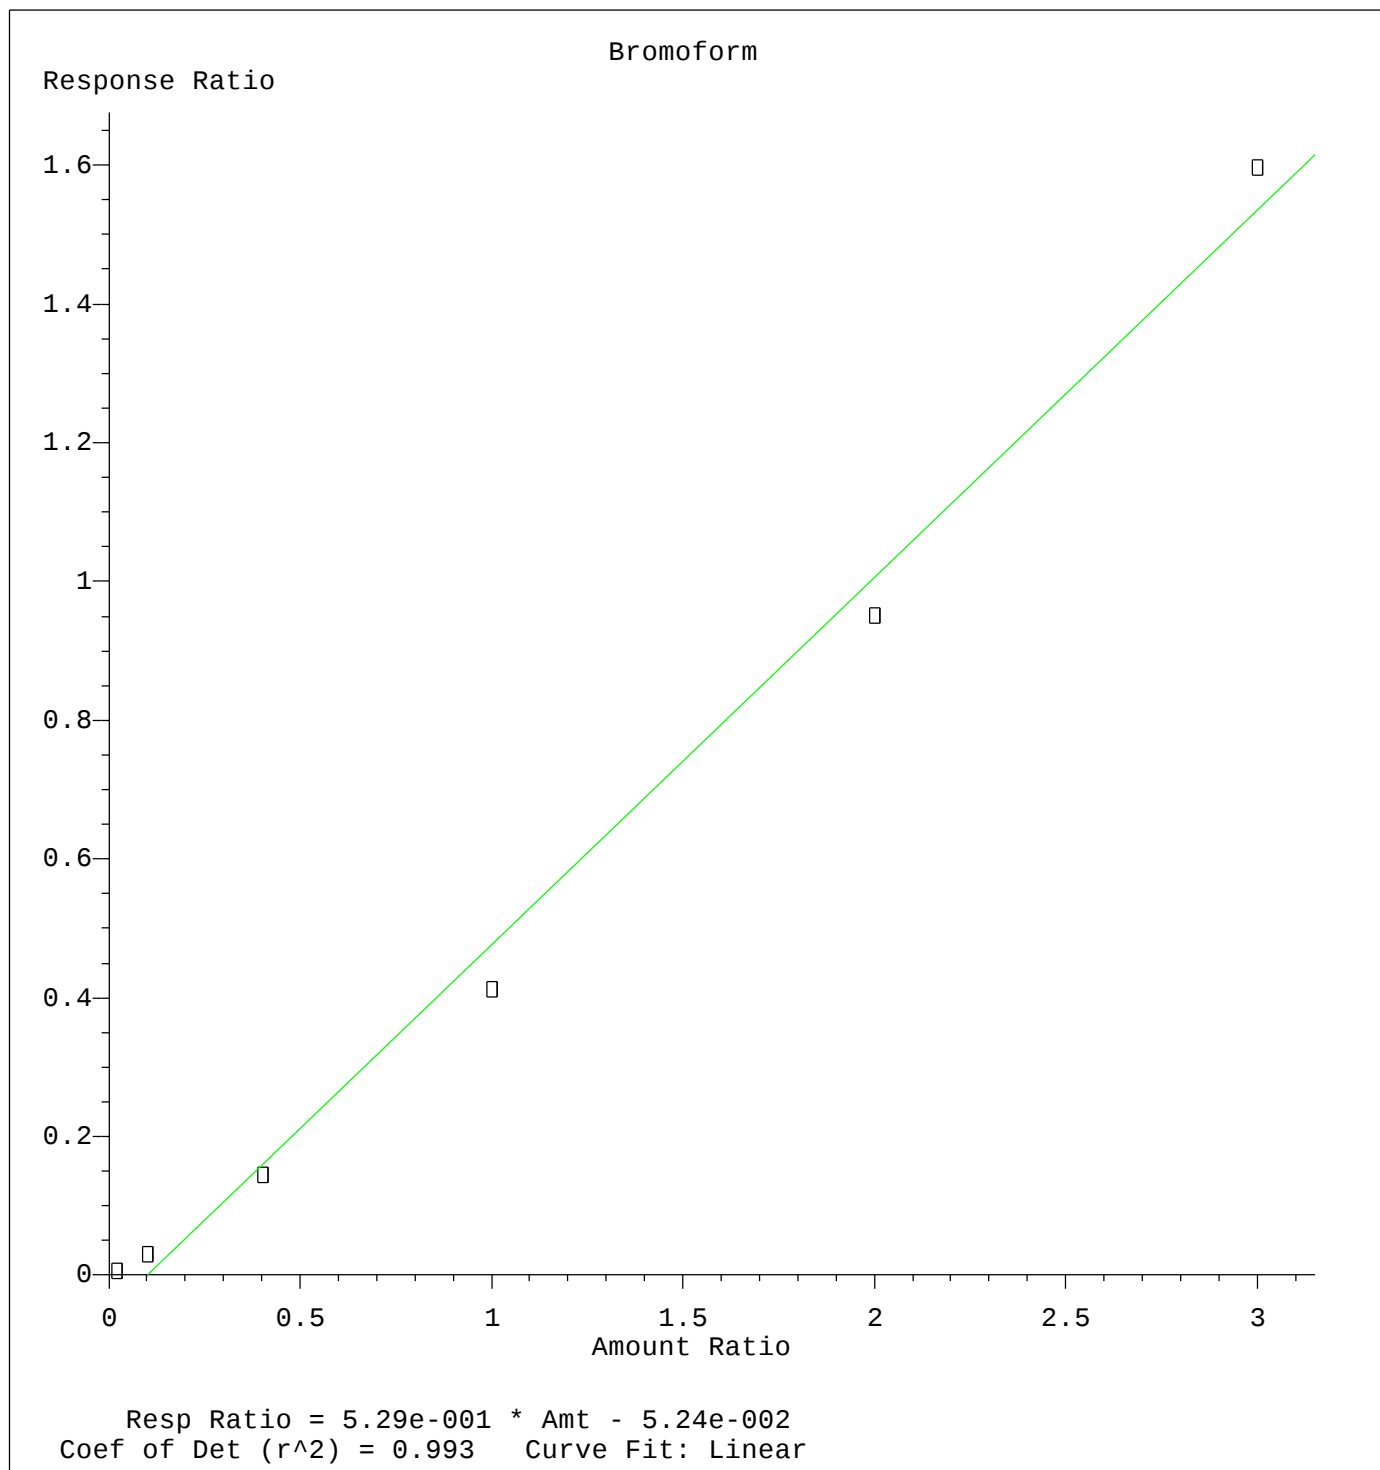

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X042618W.M
Calibration Table Last Updated: Fri Apr 27 01:51:42 2018

Dibromochloromethane

Response Ratio

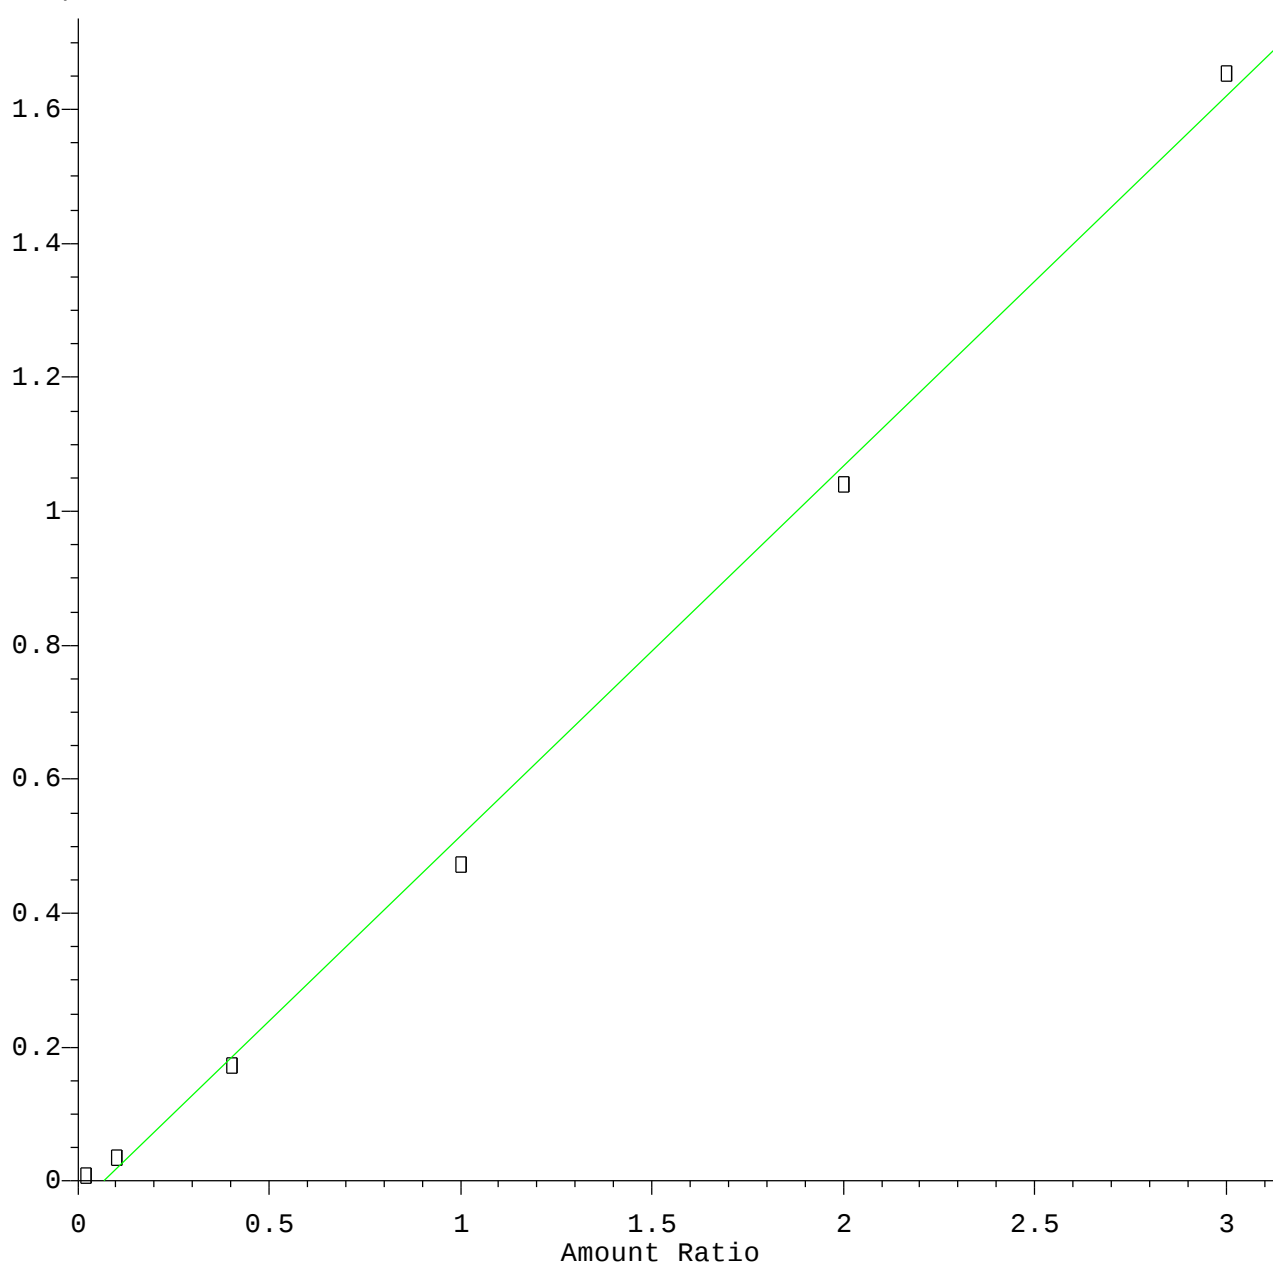


Resp Ratio = $5.52 \times 10^{-1} \times \text{Amt} - 3.69 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X042618W.M
Calibration Table Last Updated: Fri Apr 27 01:51:42 2018


cis-1,3-Dichloropropene

Response Ratio

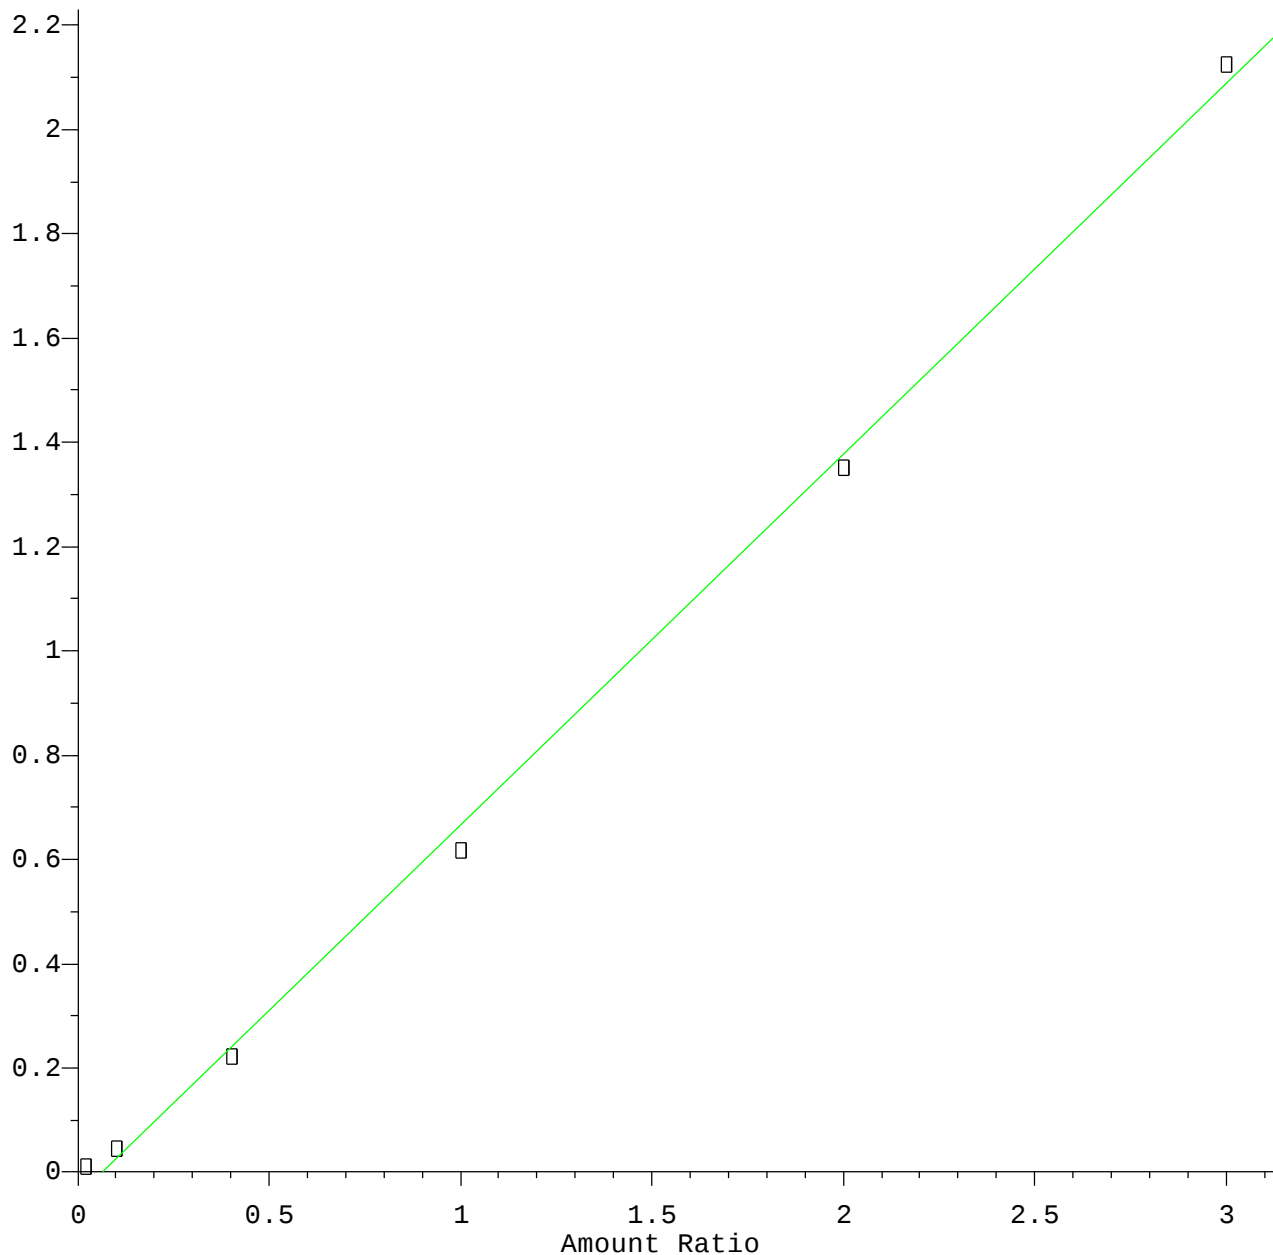

Resp Ratio = 7.11e-001 * Amt - 4.53e-002
Coef of Det (r²) = 0.998 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X042618W.M
Calibration Table Last Updated: Fri Apr 27 01:51:42 2018

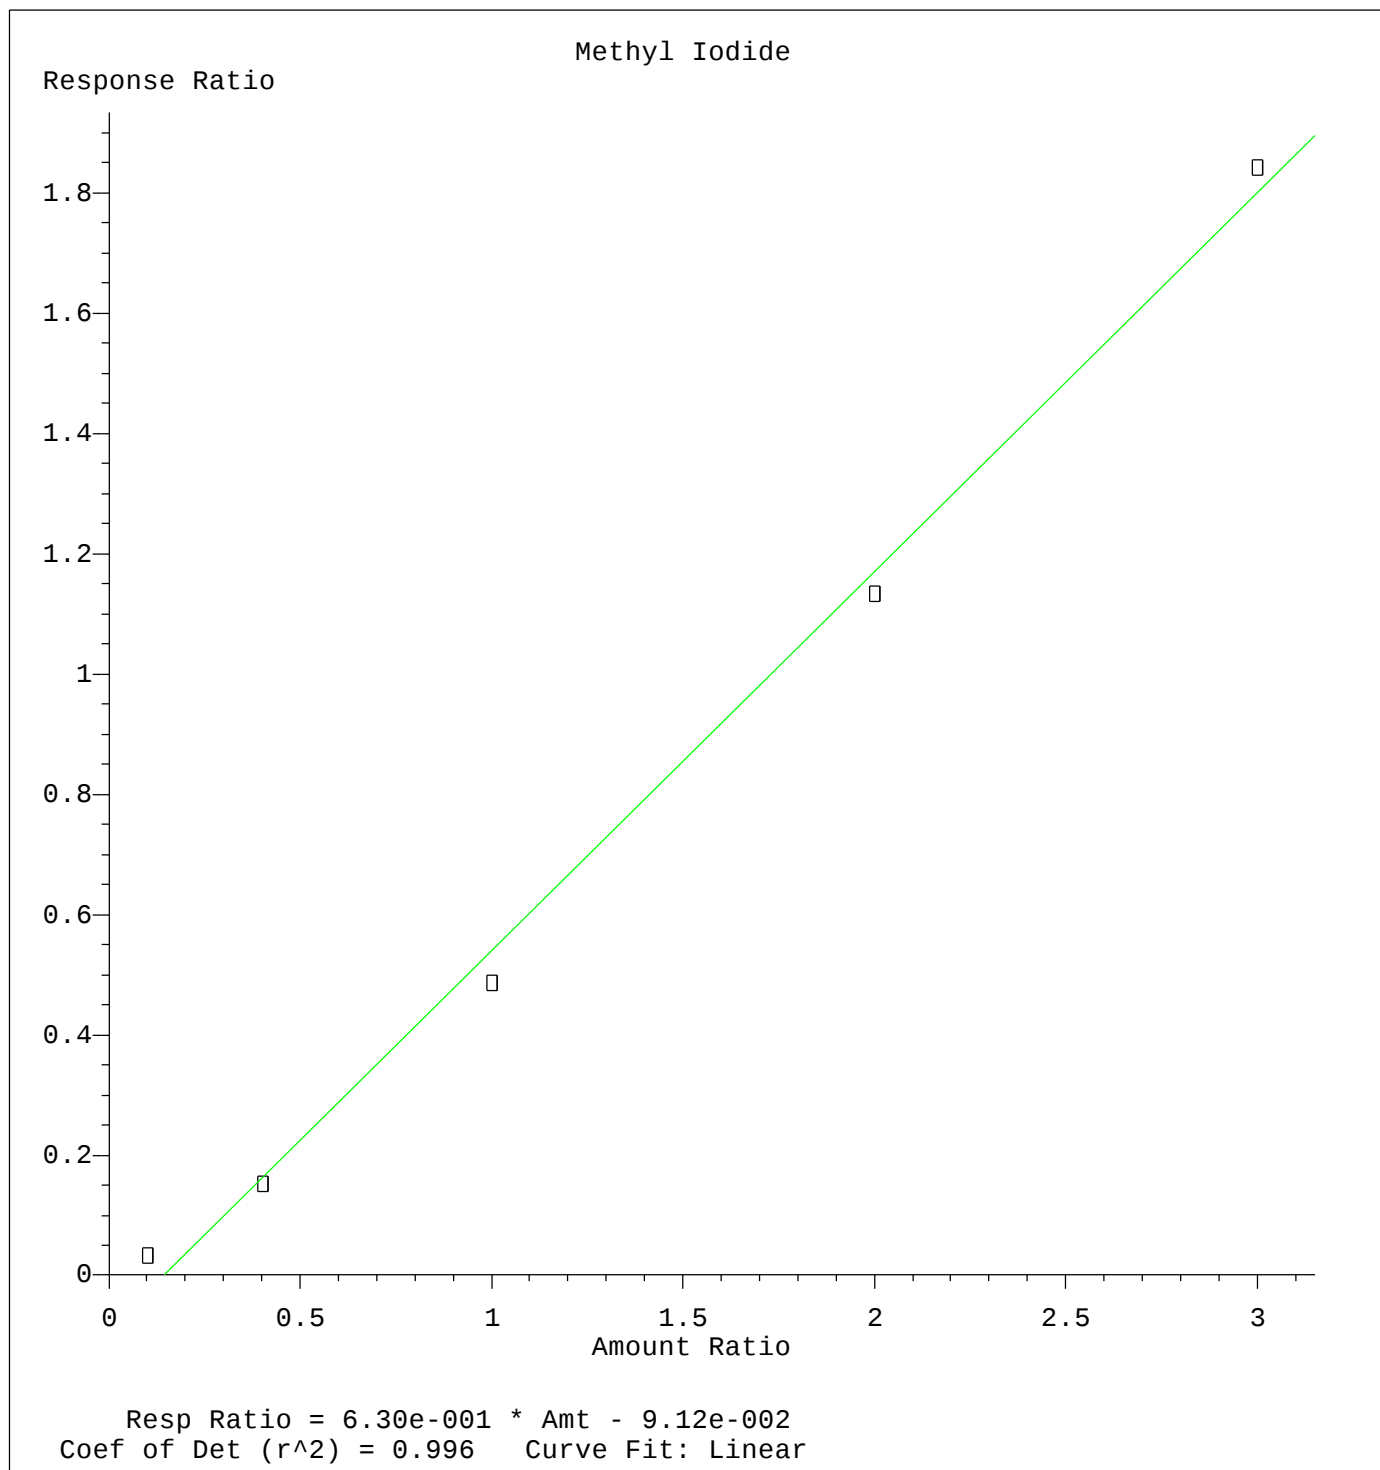

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X042618W.M
Calibration Table Last Updated: Fri Apr 27 01:51:42 2018