

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX042618\
 Data File : VX001154.D
 Acq On : 27 Apr 2018 05:23
 Operator : JC/MD
 Sample : PB108612ZHE#06 5X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB108612ZHE#06

Quant Time: Apr 27 08:11:38 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X042618W.M
 Quant Title : SW846 8260
 QLast Update : Fri Apr 27 01:51:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	208223	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	289331	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	257595	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	148364	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.08	65	136074	42.16	ug/l	0.00
Spiked Amount 50.000			Recovery	=	84.32%	
35) Dibromofluoromethane	5.51	113	105727	44.15	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.30%	
50) Toluene-d8	8.72	98	403533	44.65	ug/l	0.00
Spiked Amount 50.000			Recovery	=	89.30%	
62) 4-Bromofluorobenzene	11.14	95	139471	39.50	ug/l	0.00
Spiked Amount 50.000			Recovery	=	79.00%	
Target Compounds						
16) Acetone	2.45	43	3664	2.760	ug/l	98
18) Methyl Acetate	2.79	43	3807	1.146	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX042618\
Data File : VX001154.D
Acq On : 27 Apr 2018 05:23
Operator : JC/MD
Sample : PB108612ZHE#06 5X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB108612ZHE#06

Quant Time: Apr 27 08:11:38 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X042618W.M
Quant Title : SW846 8260
QLast Update : Fri Apr 27 01:51:42 2018
Response via : Initial Calibration

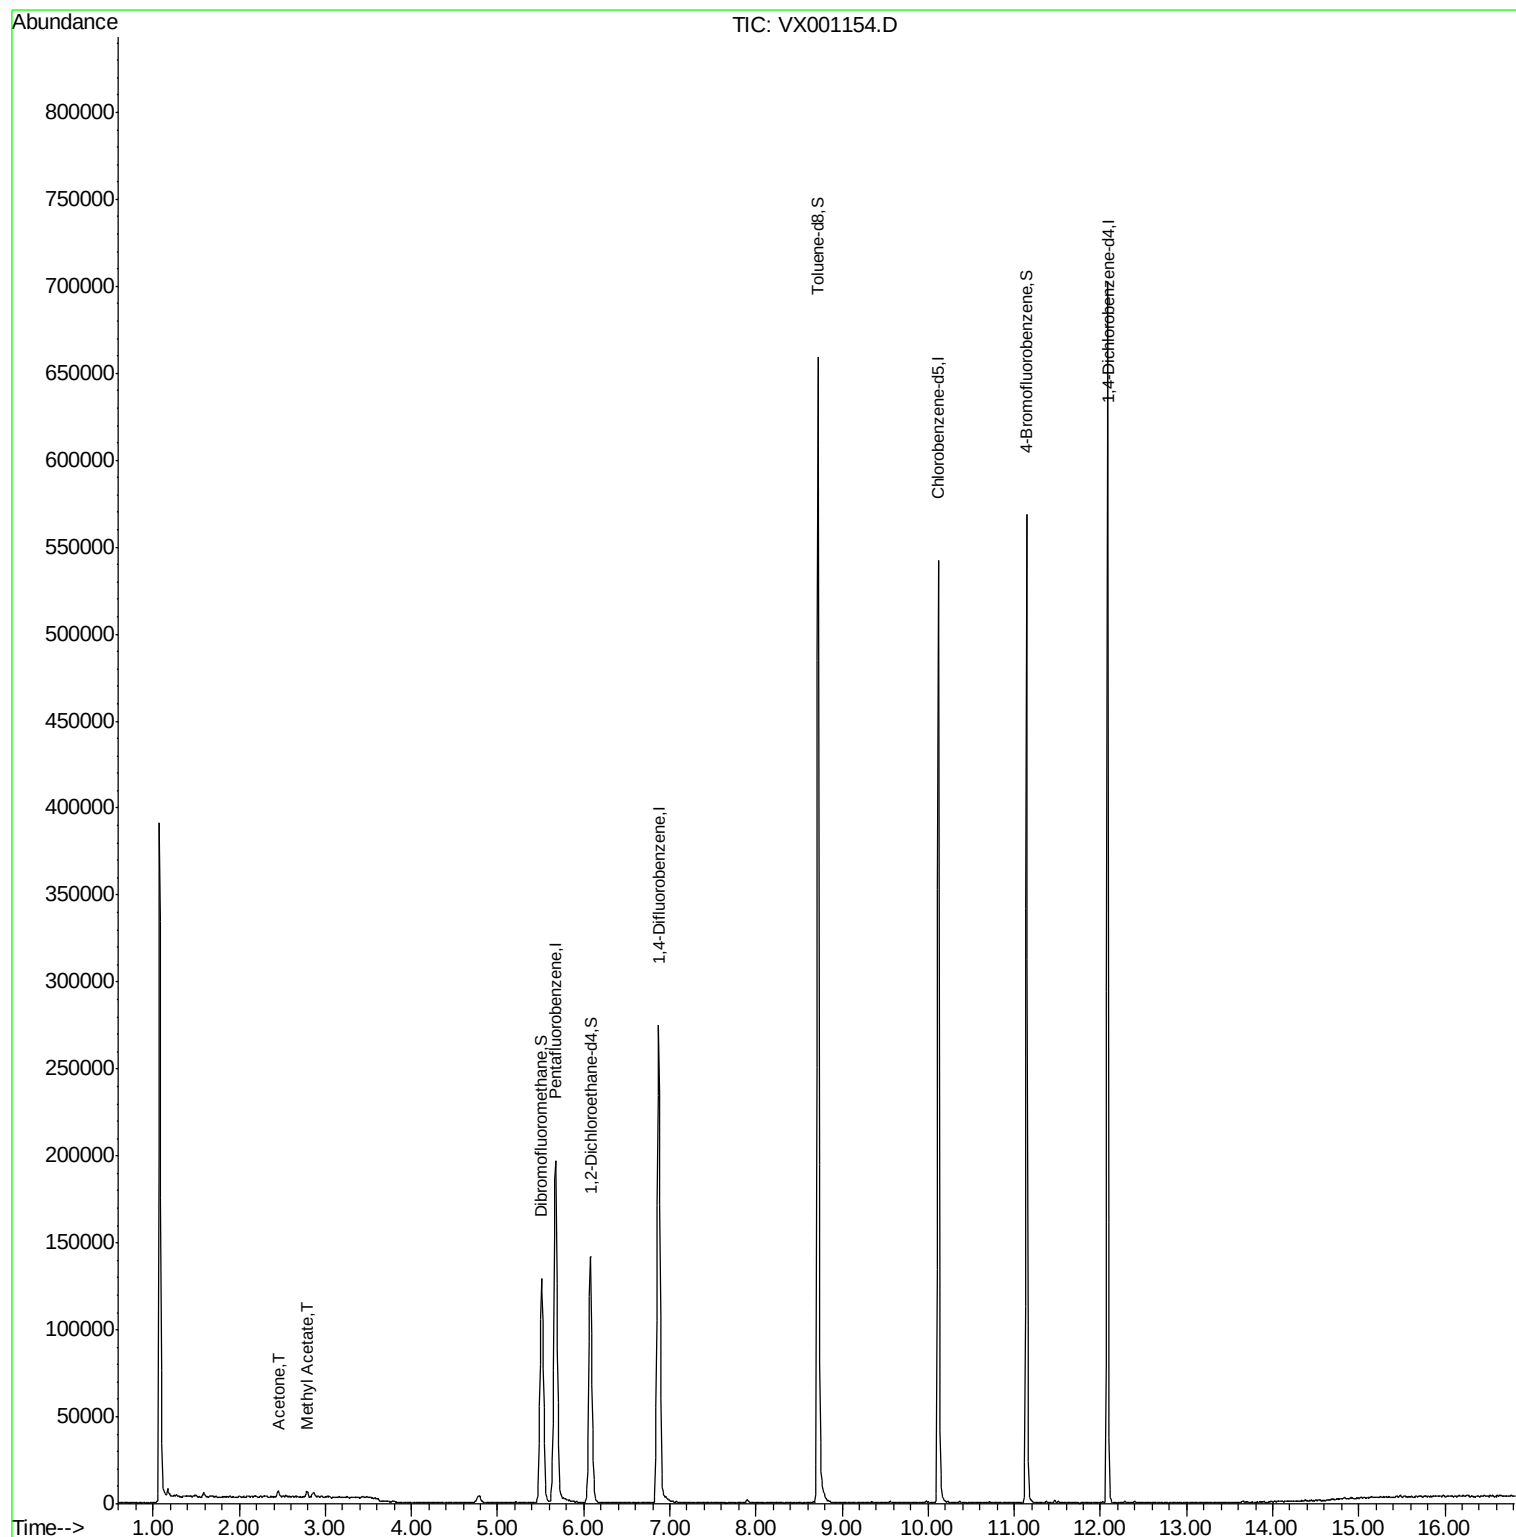

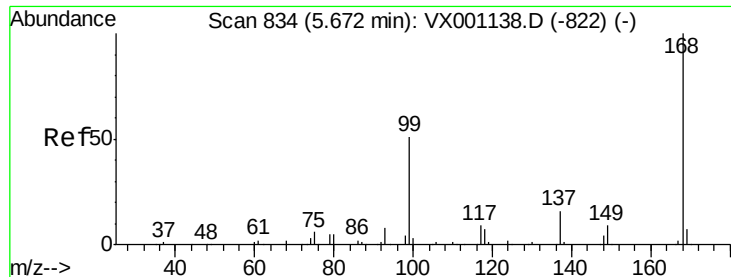

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.00 min

Lab File: VX001154.D

Acq: 27 Apr 2018 05:23

Instrument :

MSVOA_X

ClientSampleId :


PB108612ZHE#06

Tot Ion:168 Resp: 208223

Ion Ratio Lower Upper




168 100

99 48.7 40.6 60.8

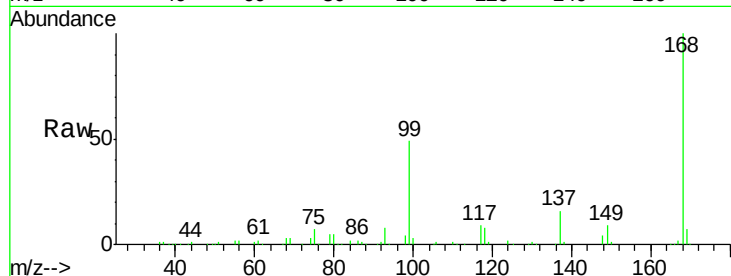

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

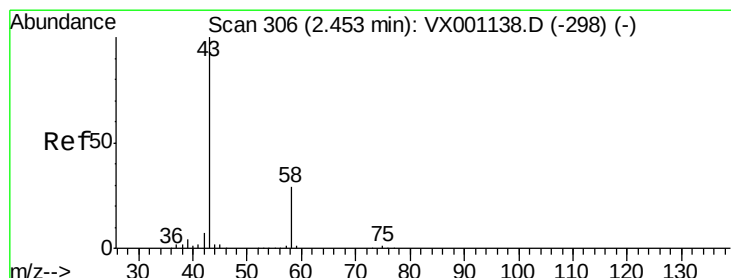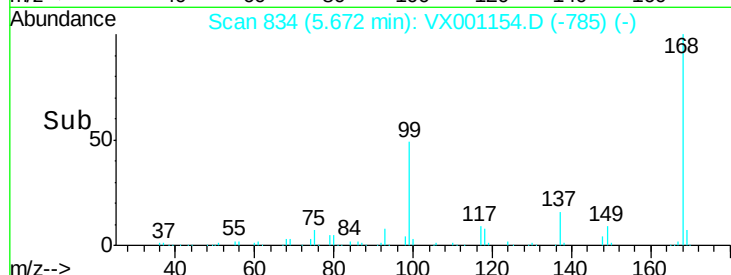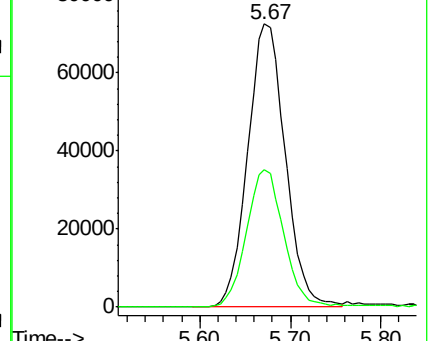

#16

Acetone

Concen: 2.760 ug/l

RT: 2.45 min Scan# 306

Delta R.T. -0.00 min

Lab File: VX001154.D


Acq: 27 Apr 2018 05:23

Tgt Ion: 43 Resp: 3664

Ion Ratio Lower Upper



43 100


58 27.8 23.0 34.6

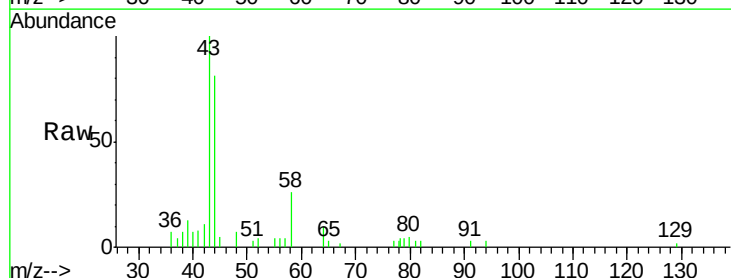

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0



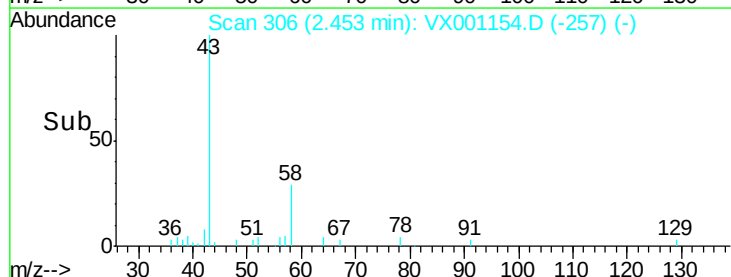
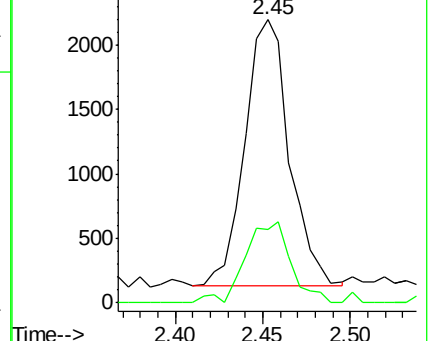


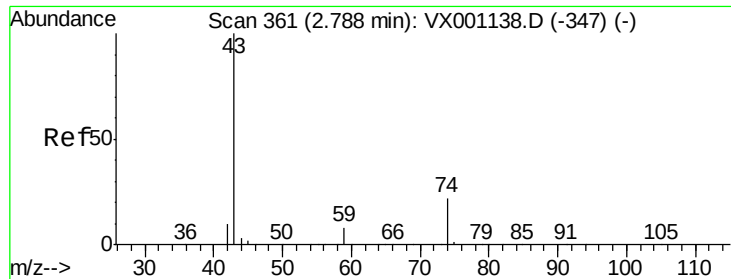

#18
Methyl Acetate
Concen: 1.146 ug/l
RT: 2.79 min Scan# 361
Delta R.T. -0.00 min
Lab File: VX001154.D
Acq: 27 Apr 2018 05:23




Instrument :
MSVOA_X
ClientSampleId :
PB108612ZHE#06


Tot Ion: 43 Resp: 3807
Ion Ratio Lower Upper
43 100
74 25.7 18.1 27.1

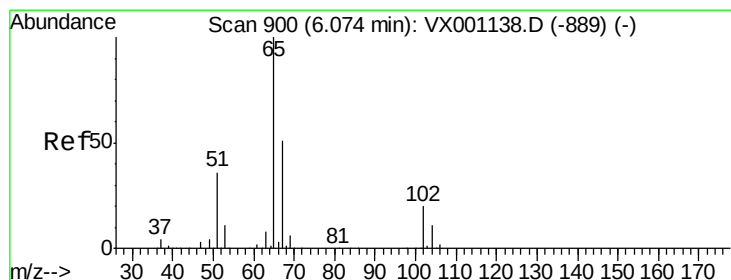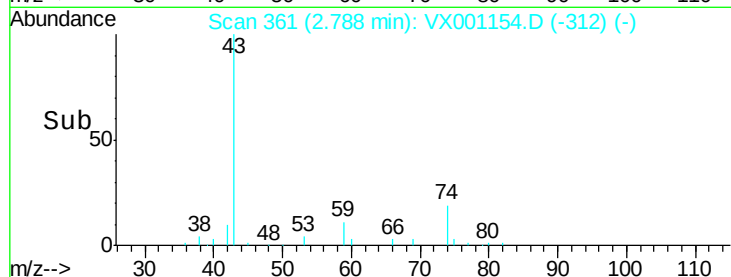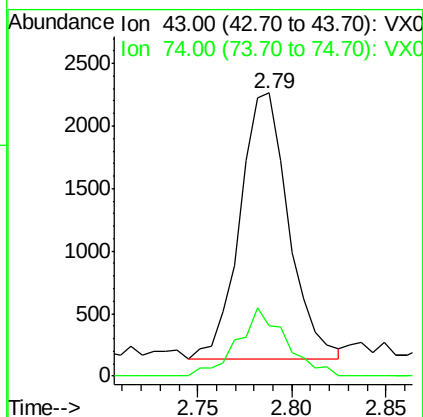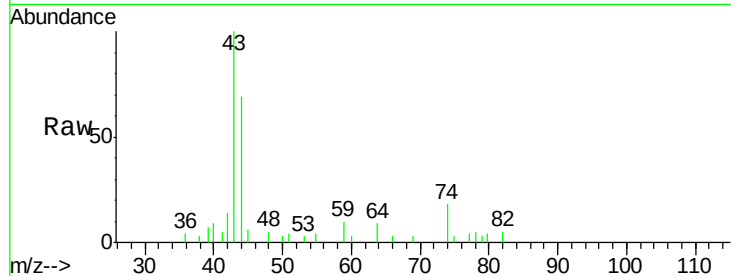

#33
1,2-Dichloroethane-d4
Concen: 42.158 ug/l
RT: 6.08 min Scan# 901
Delta R.T. 0.01 min
Lab File: VX001154.D
Acq: 27 Apr 2018 05:23

Tgt Ion: 65 Resp: 136074
Ion Ratio Lower Upper
65 100
67 50.8 0.0 102.2

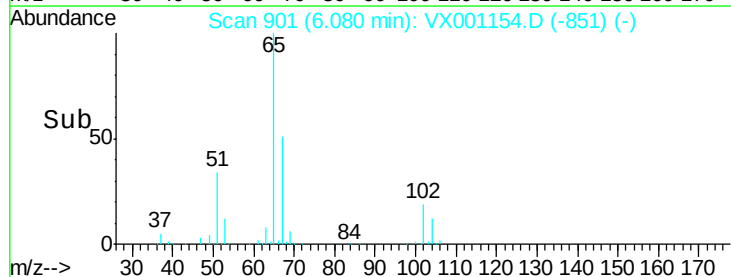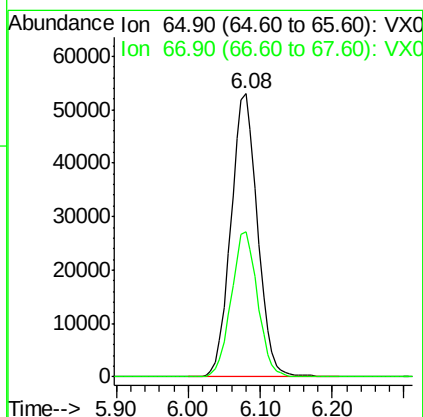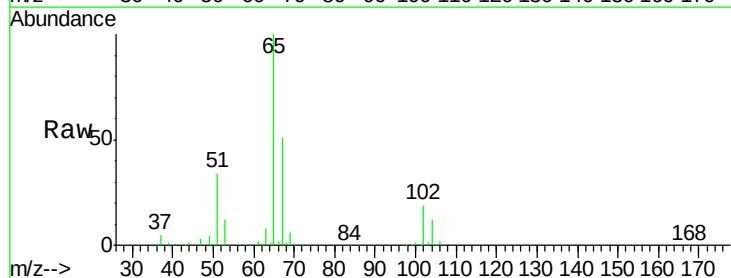

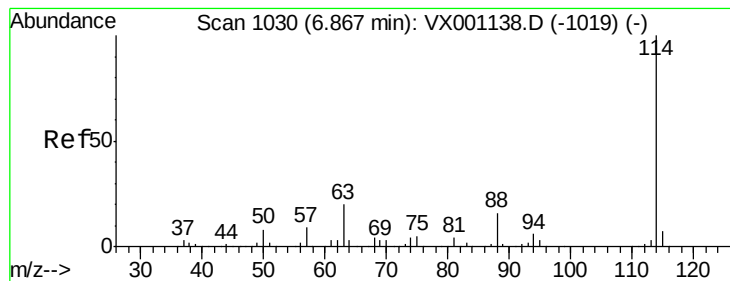

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.87 min Scan# 1031

Delta R.T. 0.01 min

Lab File: VX001154.D

Acq: 27 Apr 2018 05:23

Instrument :

MSVOA_X

ClientSampleId :

PB108612ZHE#06


Tot Ion:114 Resp: 289331

Ion Ratio Lower Upper

114 100

63 18.4 0.0 40.4

88 14.8 0.0 31.8

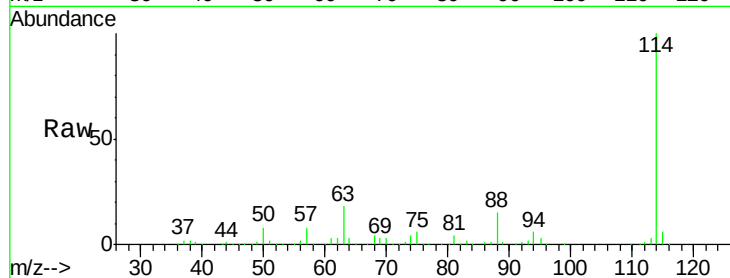

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

150000



100000

50000

0

6.87

6.70 6.80 6.90 7.00

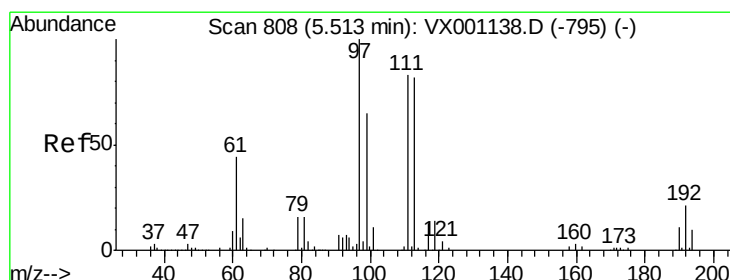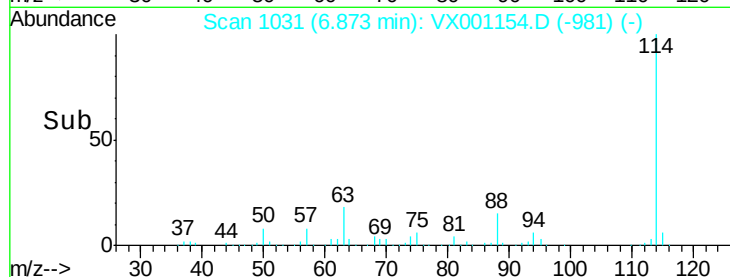

#35

Dibromofluoromethane

Concen: 44.149 ug/l

RT: 5.51 min Scan# 808

Delta R.T. -0.00 min

Lab File: VX001154.D

Acq: 27 Apr 2018 05:23


Tgt Ion:113 Resp: 105727

Ion Ratio Lower Upper

113 100

111 100.7 82.2 123.4

192 25.3 20.6 30.8

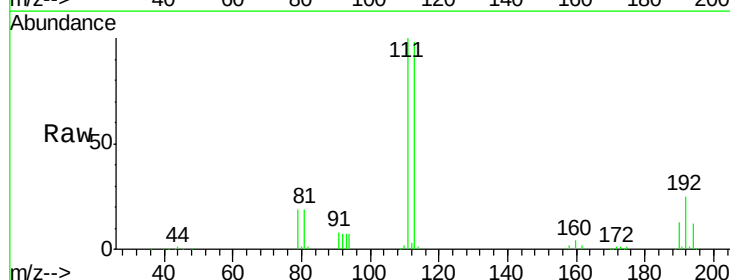

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

50000

40000

30000


20000


10000

0

5.51

5.40 5.50 5.60




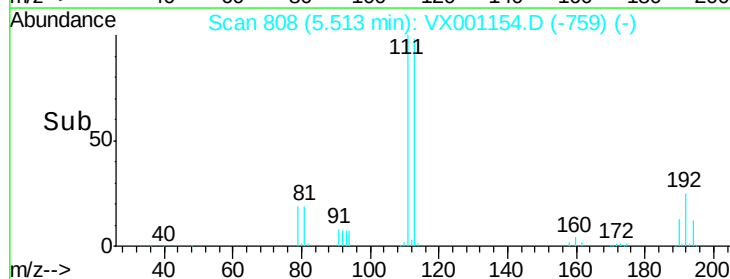


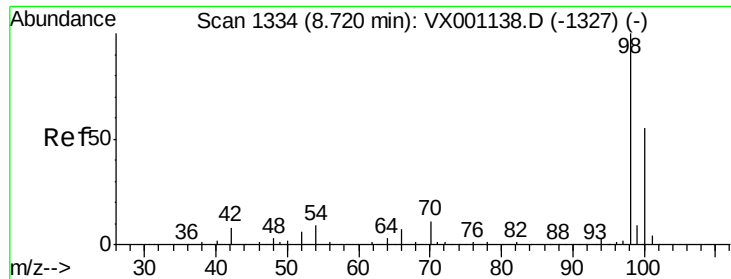

#50
Toluene-d8
Concen: 44.651 ug/l
RT: 8.72 min Scan# 1334
Delta R.T. -0.00 min
Lab File: VX001154.D
Acq: 27 Apr 2018 05:23




Instrument :
MSVOA_X
ClientSampleId :
PB108612ZHE#06


Tot Ion: 98 Resp: 403533
Ion Ratio Lower Upper
98 100
100 63.9 51.8 77.6

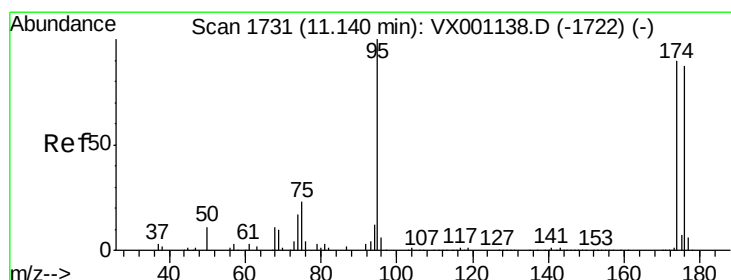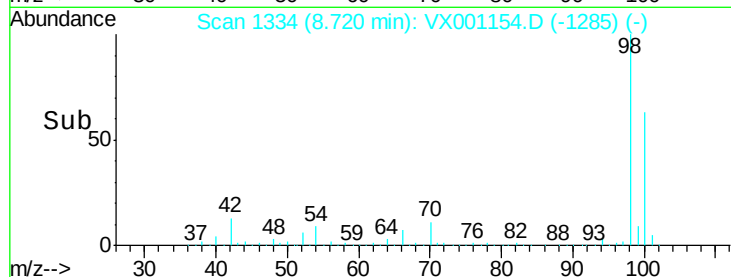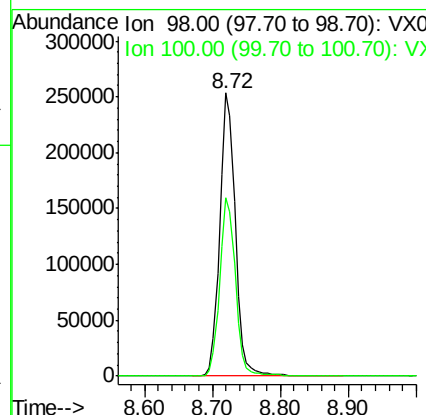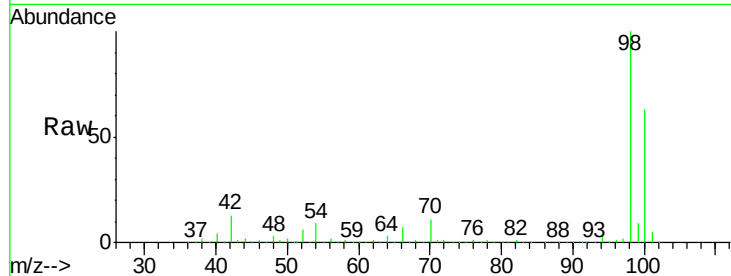

#62
4-Bromofluorobenzene
Concen: 39.505 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. -0.00 min
Lab File: VX001154.D
Acq: 27 Apr 2018 05:23

Tgt Ion: 95 Resp: 139471
Ion Ratio Lower Upper
95 100
174 100.7 0.0 194.4
176 98.1 0.0 190.2

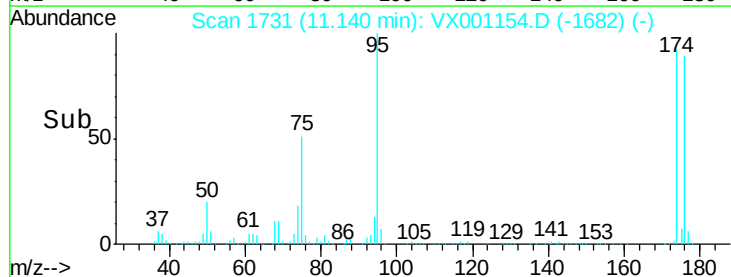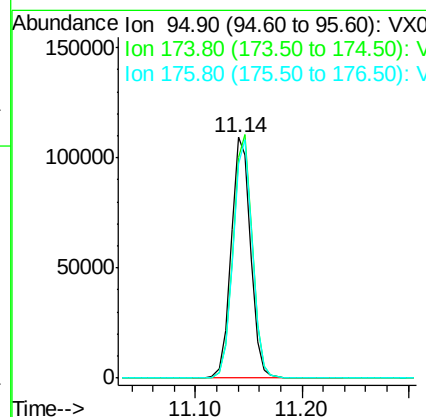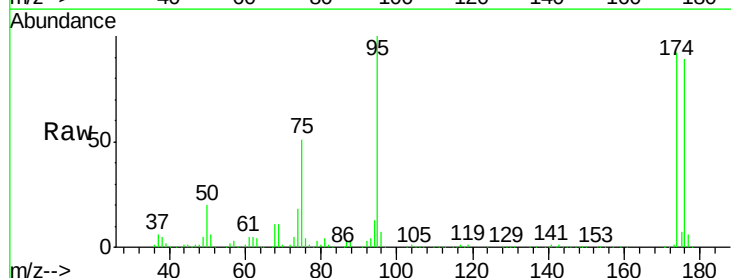


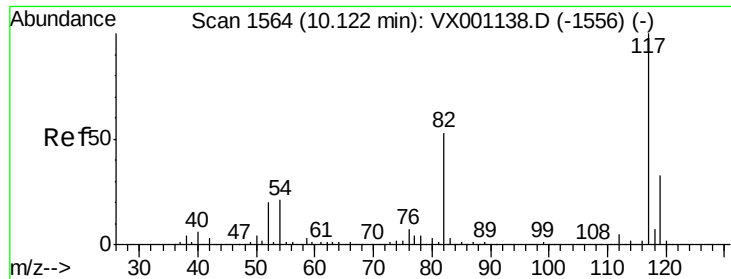




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1564
Delta R.T. -0.00 min
Lab File: VX001154.D
Acq: 27 Apr 2018 05:23

Instrument :
MSVOA_X
ClientSampleId :
PB108612ZHE#06

Tot Ion:117 Resp: 257595
Ion Ratio Lower Upper
117 100
82 50.8 42.1 63.1
119 32.4 26.1 39.1

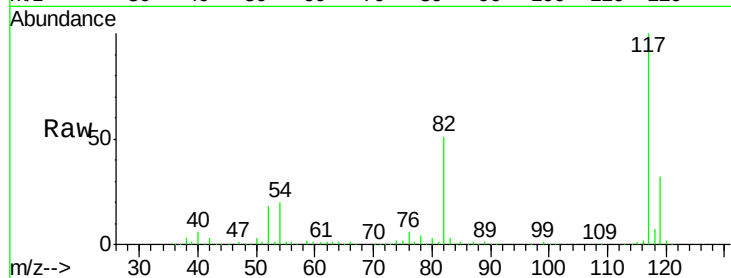


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

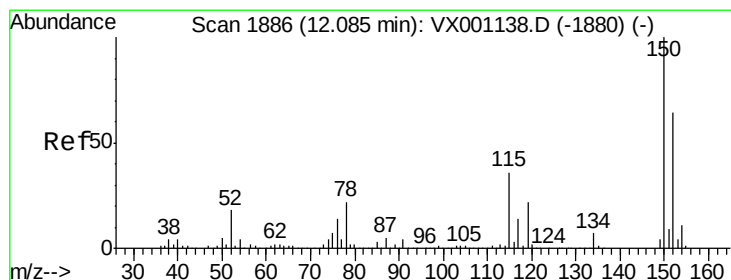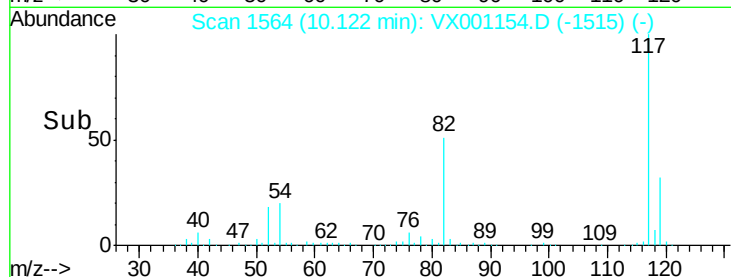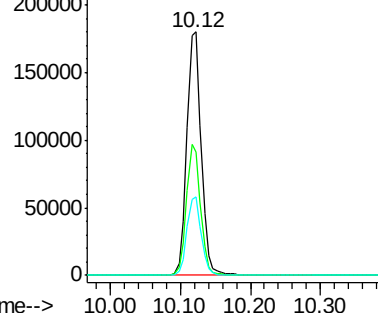

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.09 min Scan# 1886
Delta R.T. -0.00 min
Lab File: VX001154.D
Acq: 27 Apr 2018 05:23

Tgt Ion:152 Resp: 148364
Ion Ratio Lower Upper
152 100
115 52.7 38.0 114.0
150 154.1 0.0 349.6

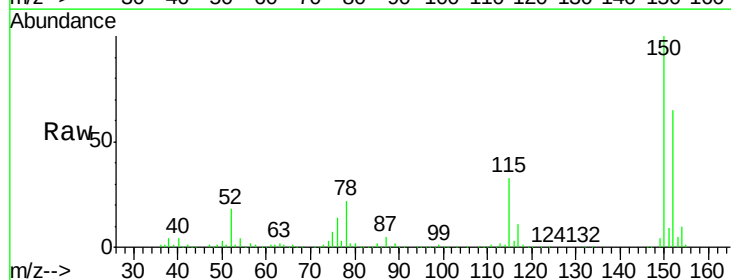

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

