


Data Path : W:\HPCHEM1\MSVOA X\DATA\VX042618\
Data File : VX001142.D
Acq On : 26 Apr 2018 20:54
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X042618W.M
Title : SW846 8260
Last Update : Fri Apr 27 01:51:42 2018

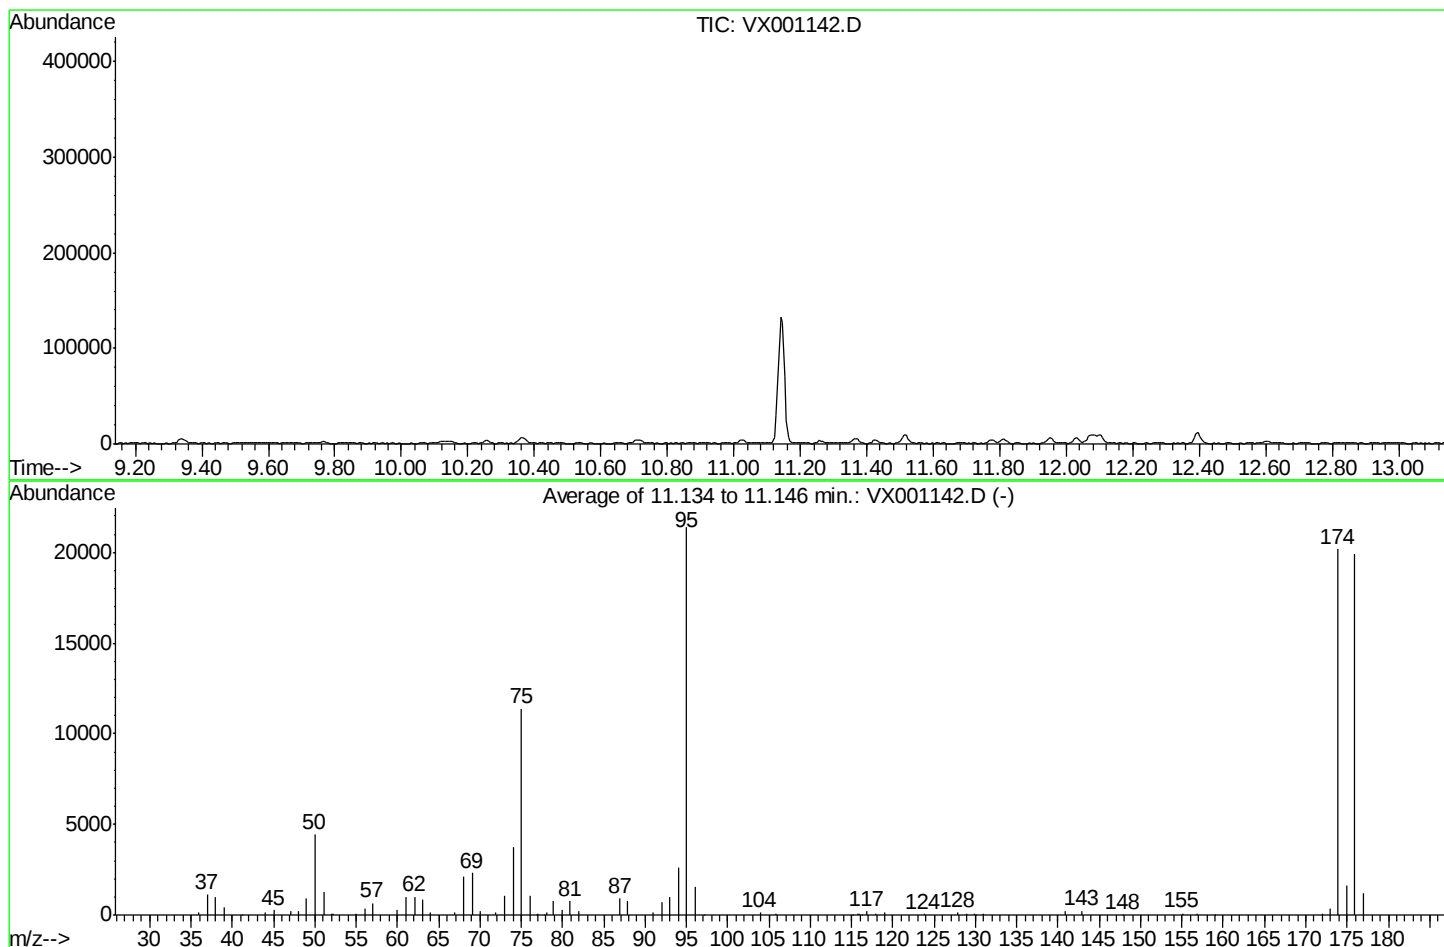

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	4446	PASS
75	95	30	60	53.2	11371	PASS
95	95	100	100	100.0	21383	PASS
96	95	5	9	7.3	1551	PASS
173	174	0.00	2	1.8	373	PASS
174	95	50	100	94.4	20181	PASS
175	174	5	9	8.0	1623	PASS
176	174	95	101	98.5	19878	PASS
177	176	5	9	6.2	1230	PASS