


Data Path : W:\HPCHEM1\MSVOA X\DATA\VX042718\
 Data File : VX001185.D
 Acq On : 27 Apr 2018 22:01
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X042618W.M
 Title : SW846 8260
 Last Update : Fri Apr 27 01:51:42 2018

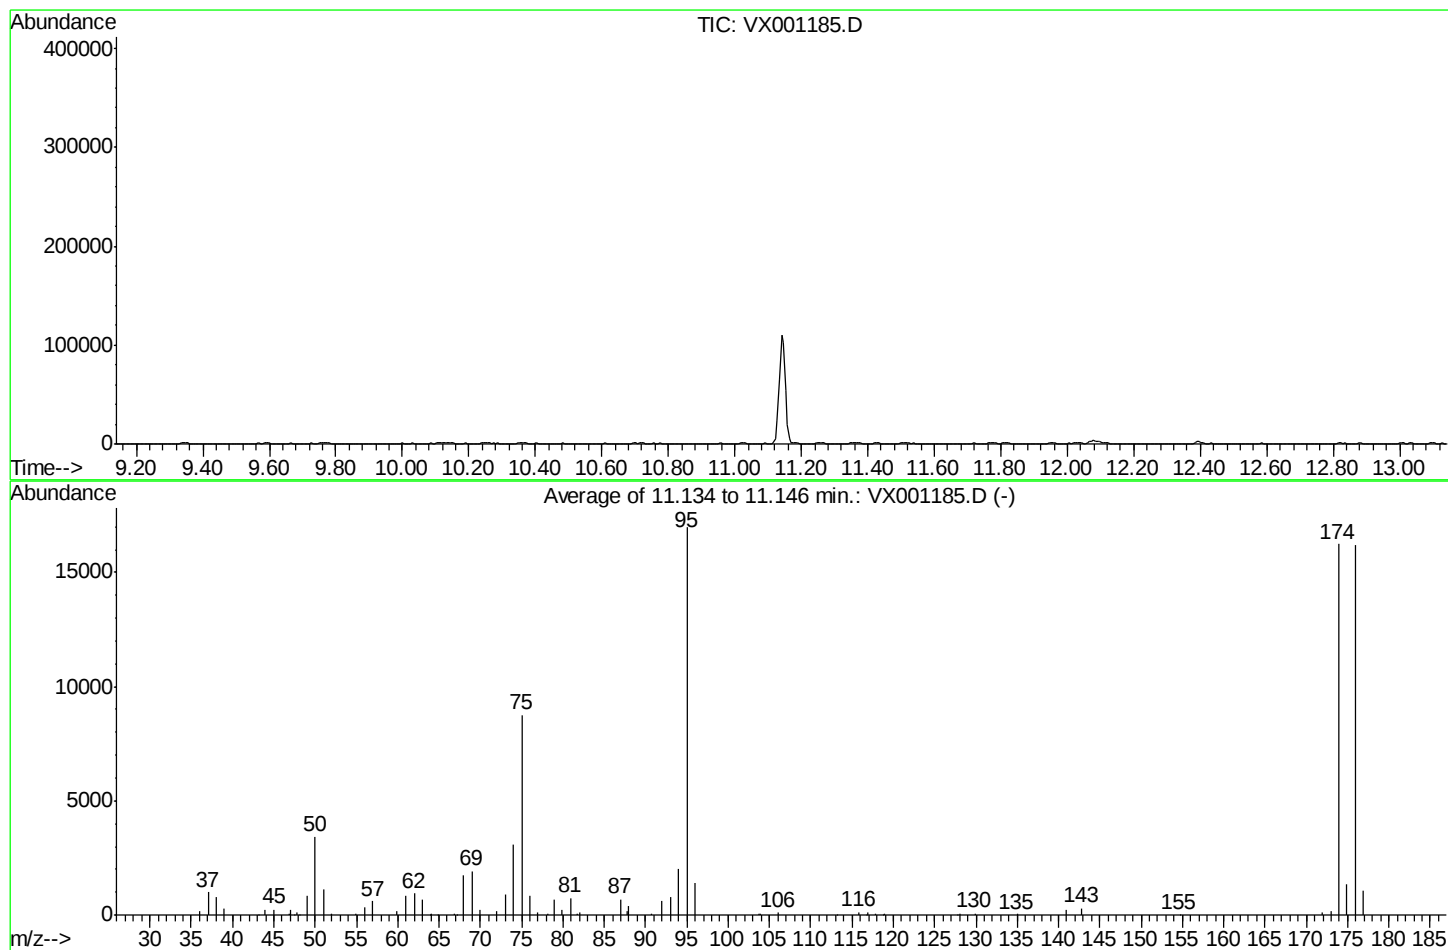

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	3443	PASS
75	95	30	60	51.7	8774	PASS
95	95	100	100	100.0	16978	PASS
96	95	5	9	8.4	1418	PASS
173	174	0.00	2	1.1	179	PASS
174	95	50	100	95.6	16237	PASS
175	174	5	9	8.3	1354	PASS
176	174	95	101	100.0	16231	PASS
177	176	5	9	6.5	1058	PASS