


Data Path : W:\HPCHEM1\MSVOA X\Data\VX042818\
Data File : VX001228.D
Acq On : 28 Apr 2018 21:55
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X042618W.M
Title : SW846 8260
Last Update : Fri Apr 27 01:51:42 2018

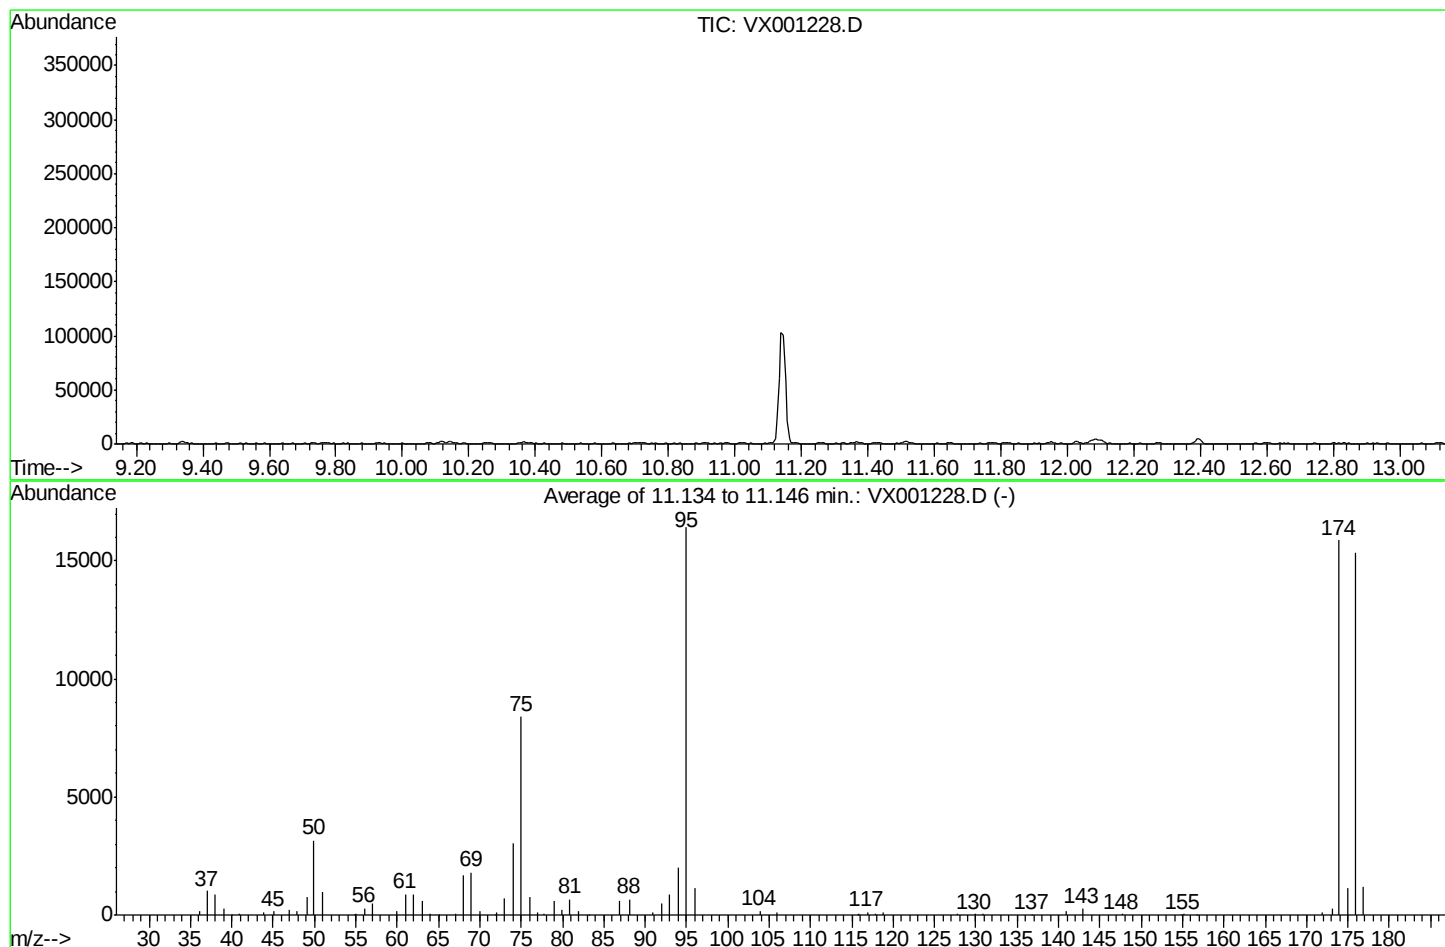

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	3155	PASS
75	95	30	60	51.0	8380	PASS
95	95	100	100	100.0	16422	PASS
96	95	5	9	6.8	1120	PASS
173	174	0.00	2	1.6	248	PASS
174	95	50	100	96.6	15864	PASS
175	174	5	9	7.2	1140	PASS
176	174	95	101	96.7	15340	PASS
177	176	5	9	7.7	1179	PASS