


Data Path : W:\HPCHEM1\MSVOA X\Data\VX043018\
Data File : VX001254.D
Acq On : 30 Apr 2018 09:31
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\624X043018W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue May 01 09:17:40 2018

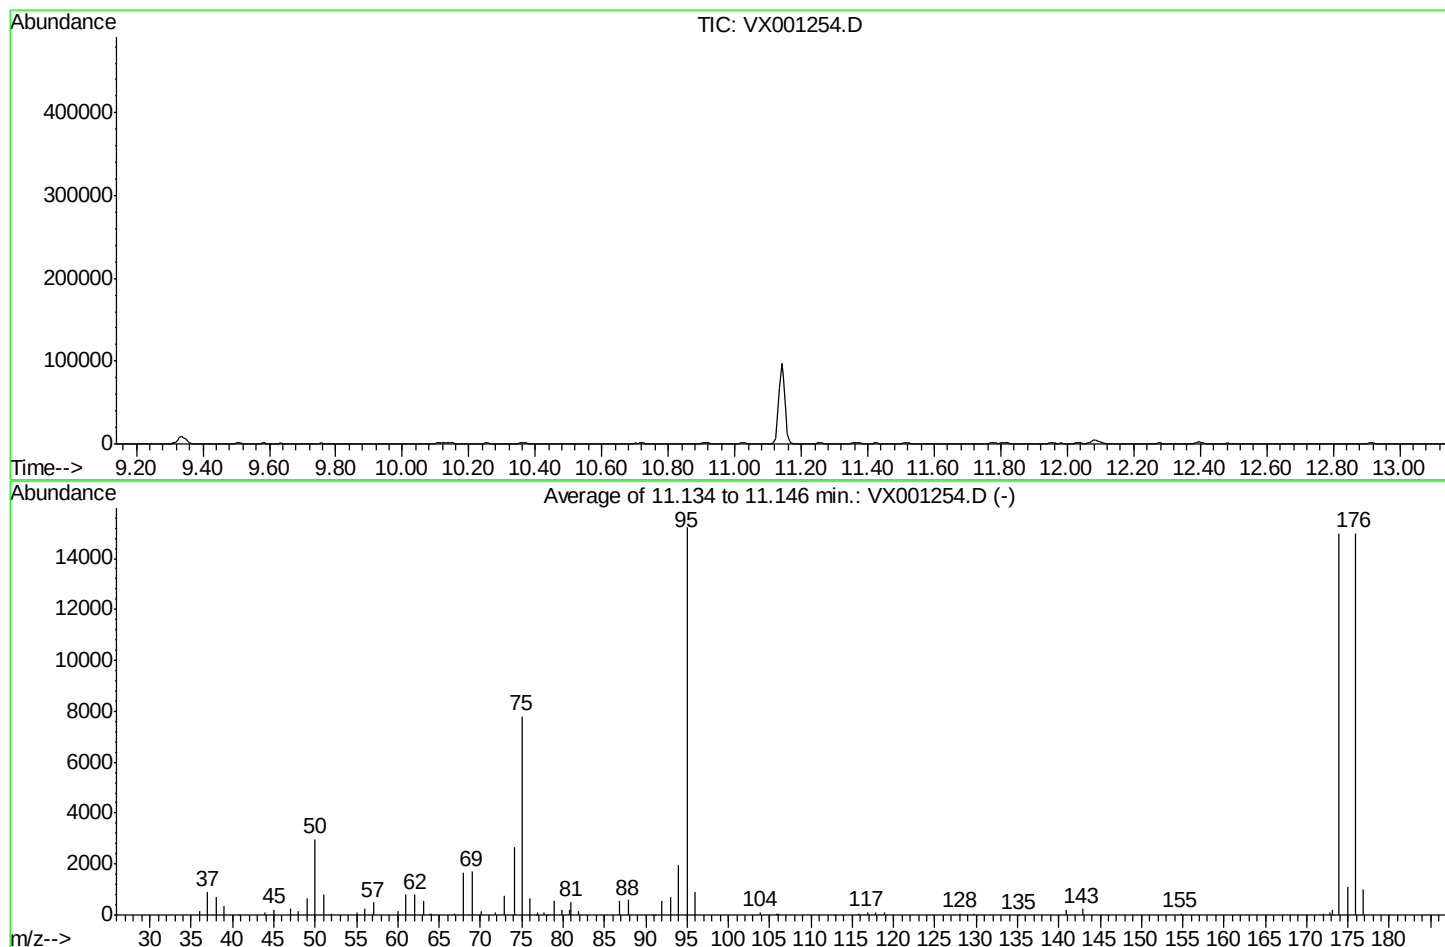

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	2991	PASS
75	95	30	60	51.3	7810	PASS
95	95	100	100	100.0	15223	PASS
96	95	5	9	6.1	923	PASS
173	174	0.00	2	1.2	187	PASS
174	95	50	100	98.4	14979	PASS
175	174	5	9	7.5	1118	PASS
176	174	95	101	100.1	14993	PASS
177	176	5	9	6.8	1022	PASS