



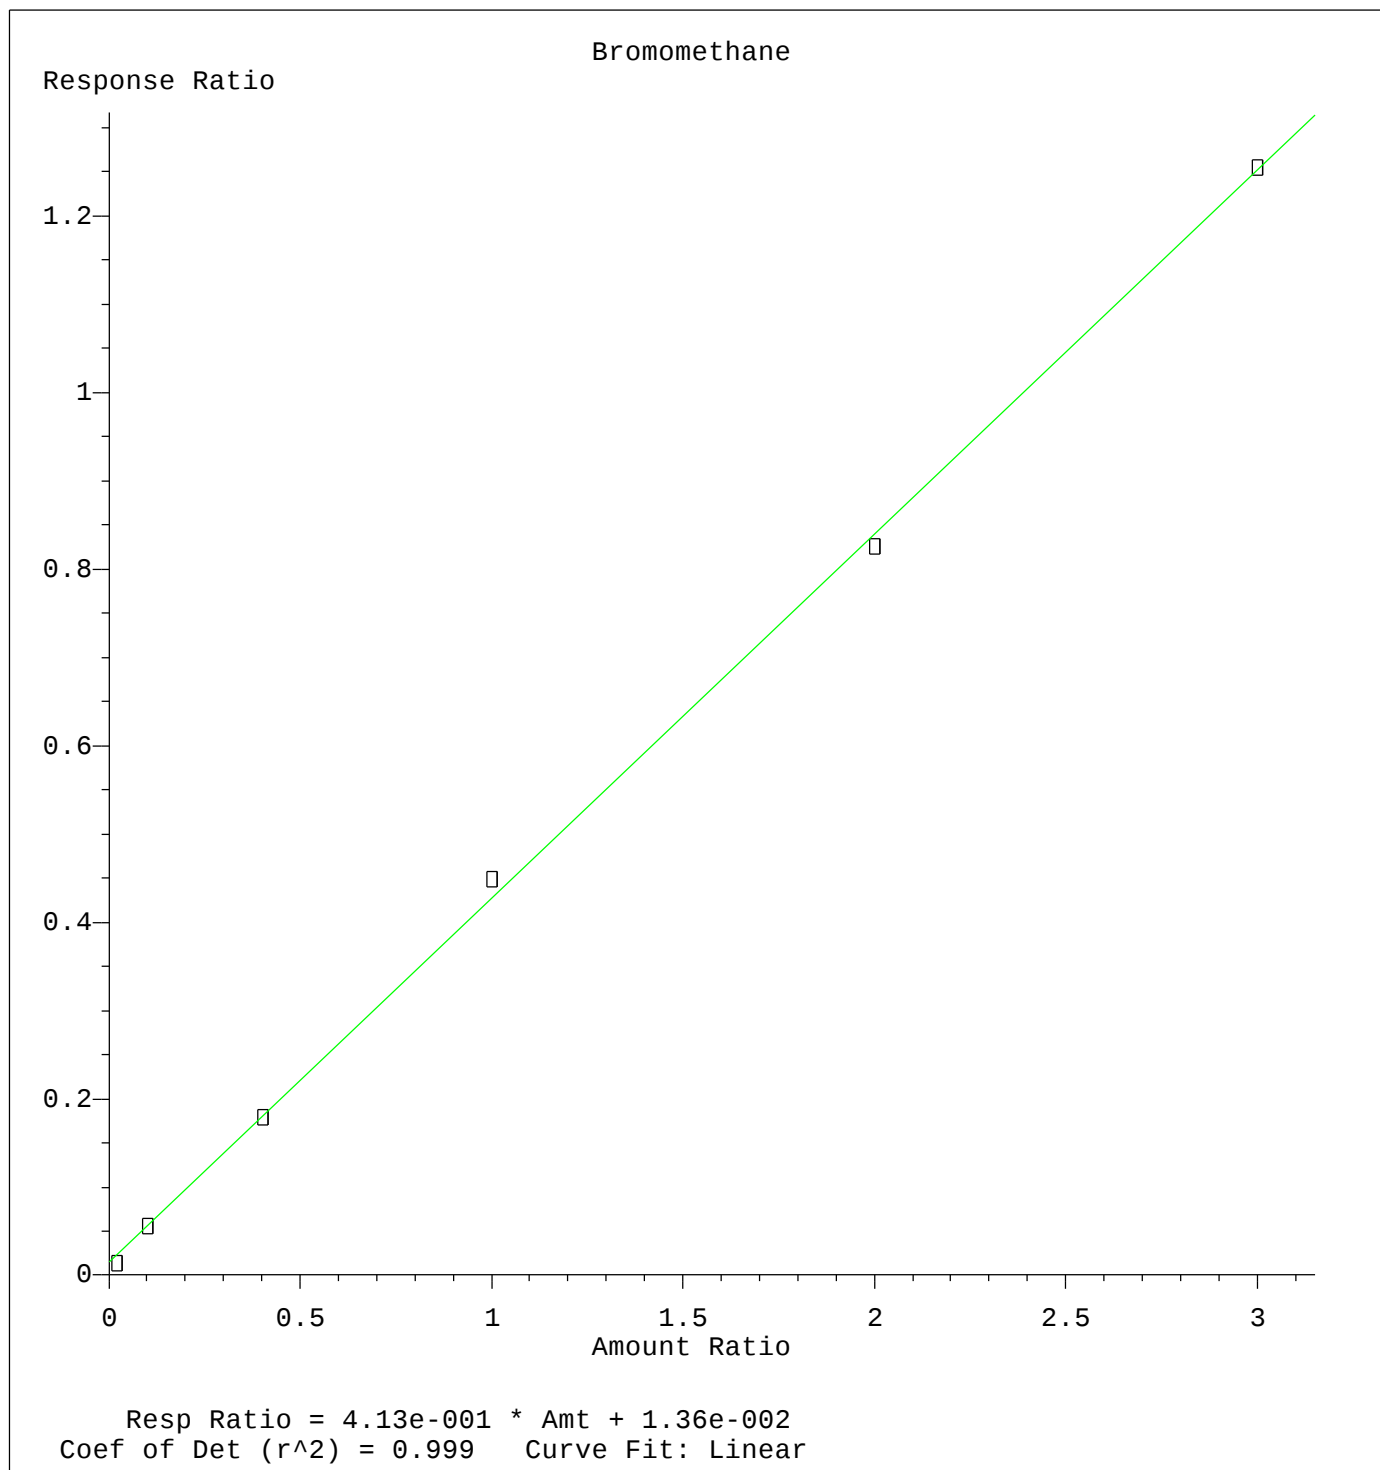

Method Name: W:\HPCHEM1\MSVOA\_X\METHOD\82X050118W.M  
Calibration Table Last Updated: Wed May 02 16:53:20 2018


trans-1,4-Dichloro-2-butene

Response Ratio

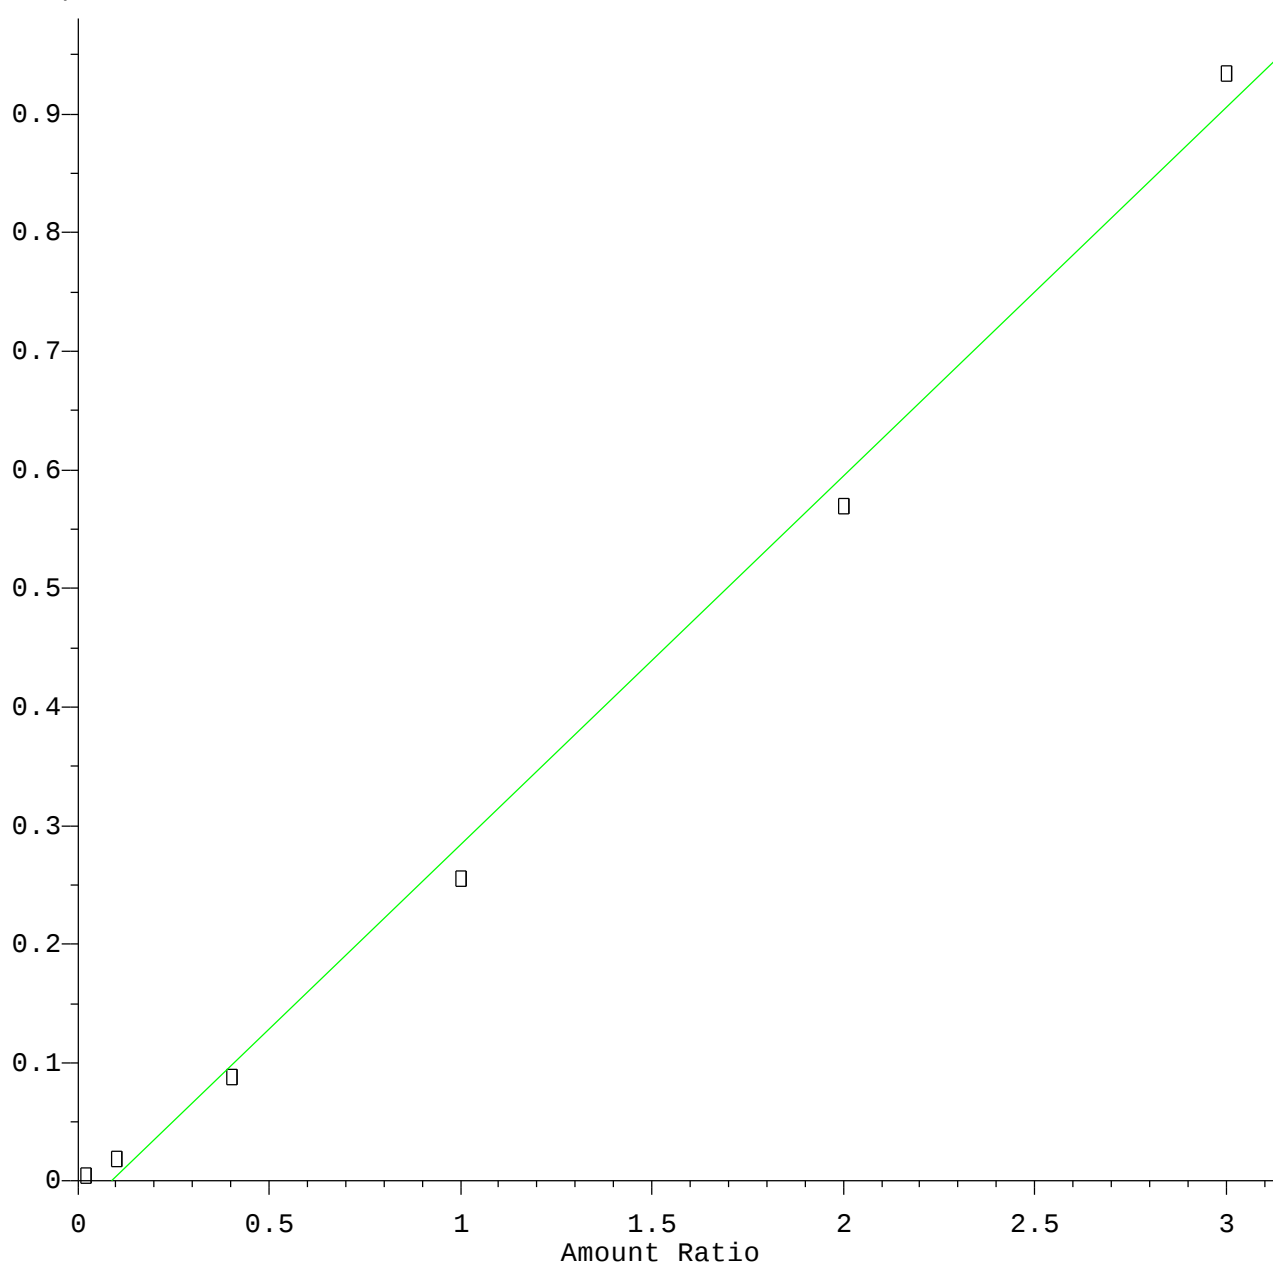

Resp Ratio =  $3.11 \times 10^{-1} \times \text{Amt} - 2.66 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.995    Curve Fit: Linear


Method Name: W:\HPCHEM1\MSVOA\_X\METHOD\82X050118W.M  
Calibration Table Last Updated: Wed May 02 16:53:20 2018

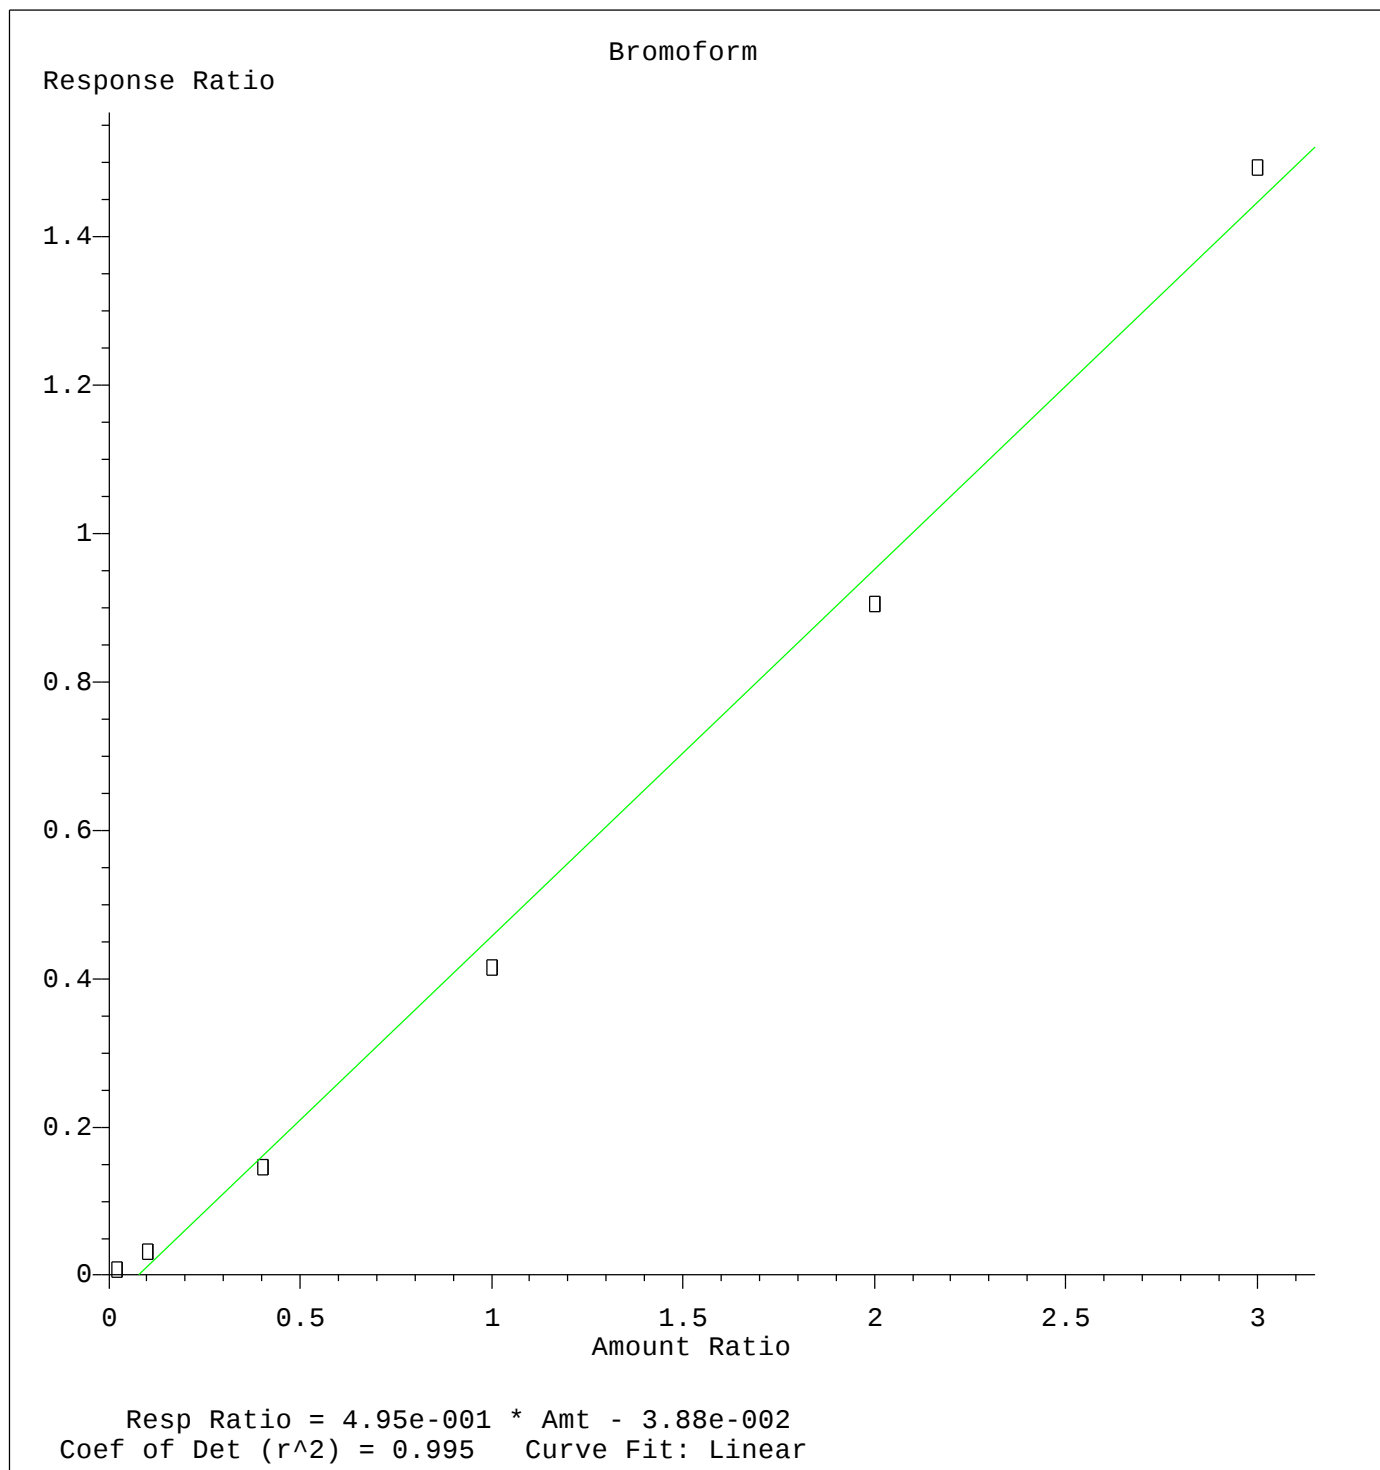

Method Name: W:\HPCHEM1\MSVOA\_X\METHOD\82X050118W.M  
Calibration Table Last Updated: Wed May 02 16:53:20 2018


# Methylene Chloride

Response Ratio

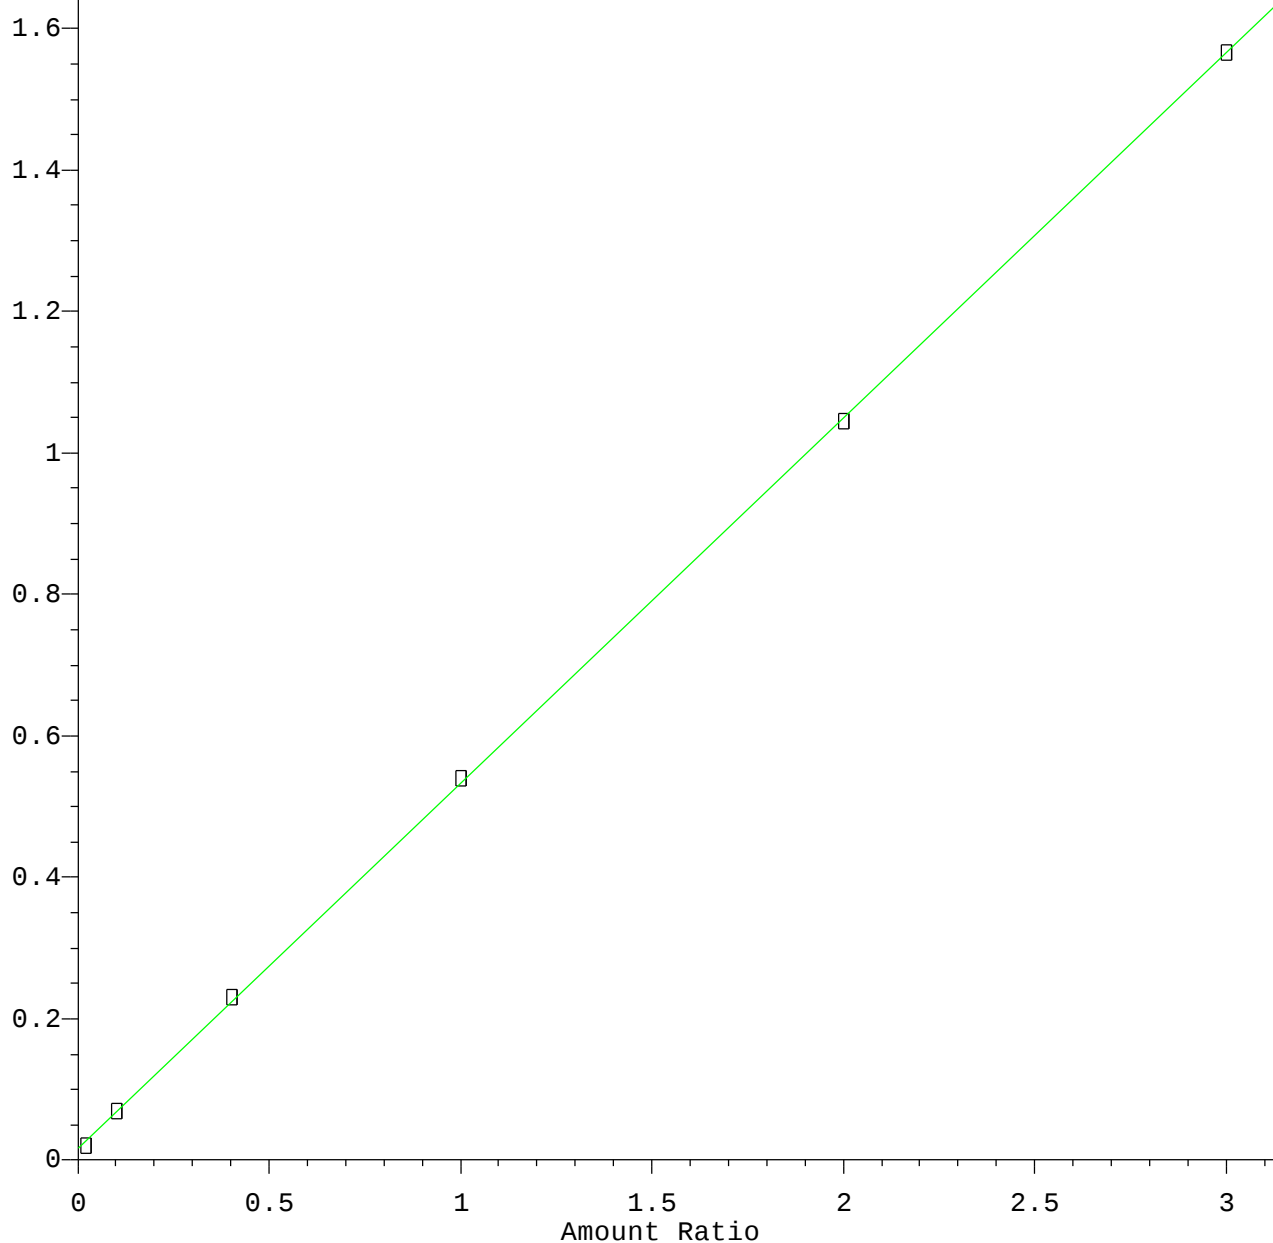

Resp Ratio =  $5.16 \times 10^{-1} \times \text{Amt} + 1.70 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 1.000 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA\_X\METHOD\82X050118W.M  
Calibration Table Last Updated: Wed May 02 16:53:20 2018

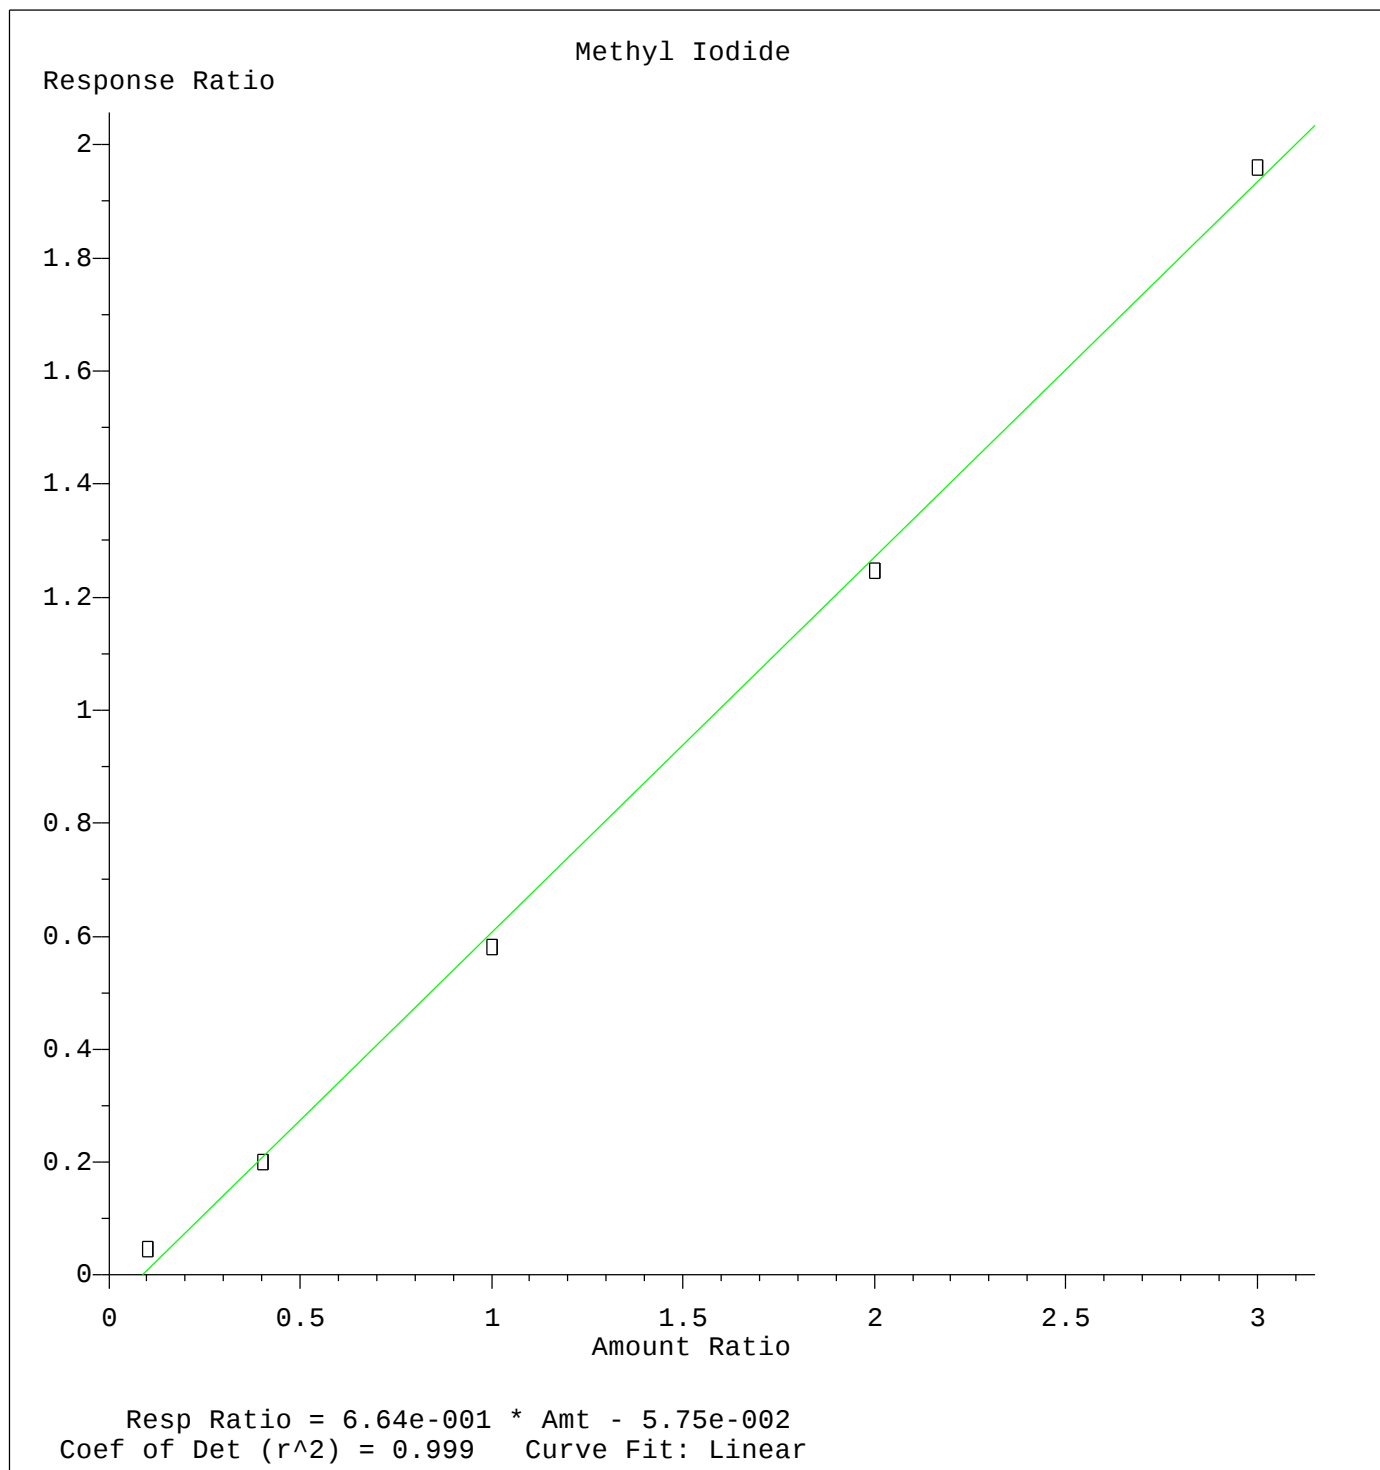

Method Name: W:\HPCHEM1\MSVOA\_X\METHOD\82X050118W.M  
Calibration Table Last Updated: Wed May 02 16:53:20 2018