

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX050218\
 Data File : VX001326.D
 Acq On : 02 May 2018 19:21
 Operator : JC/MD
 Sample : PB108794ZHE#11
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB108794ZHE#11

Quant Time: May 03 05:43:42 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X050118W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 02 01:48:25 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	147381	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	194837	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	167815	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	86377	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.08	65	88924	43.59	ug/l	0.00
Spiked Amount 50.000			Recovery	=	87.18%	
35) Dibromofluoromethane	5.52	113	74714	44.51	ug/l	0.00
Spiked Amount 50.000			Recovery	=	89.02%	
50) Toluene-d8	8.72	98	270936	45.18	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.36%	
62) 4-Bromofluorobenzene	11.14	95	81815	34.11	ug/l	0.00
Spiked Amount 50.000			Recovery	=	68.22%	
Target Compounds						
16) Acetone	2.45	43	11762	13.51	ug/l	95
18) Methyl Acetate	2.79	43	15051	7.32	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX050218\
Data File : VX001326.D
Acq On : 02 May 2018 19:21
Operator : JC/MD
Sample : PB108794ZHE#11
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB108794ZHE#11

Quant Time: May 03 05:43:42 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X050118W.M
Quant Title : SW846 8260
QLast Update : Wed May 02 01:48:25 2018
Response via : Initial Calibration

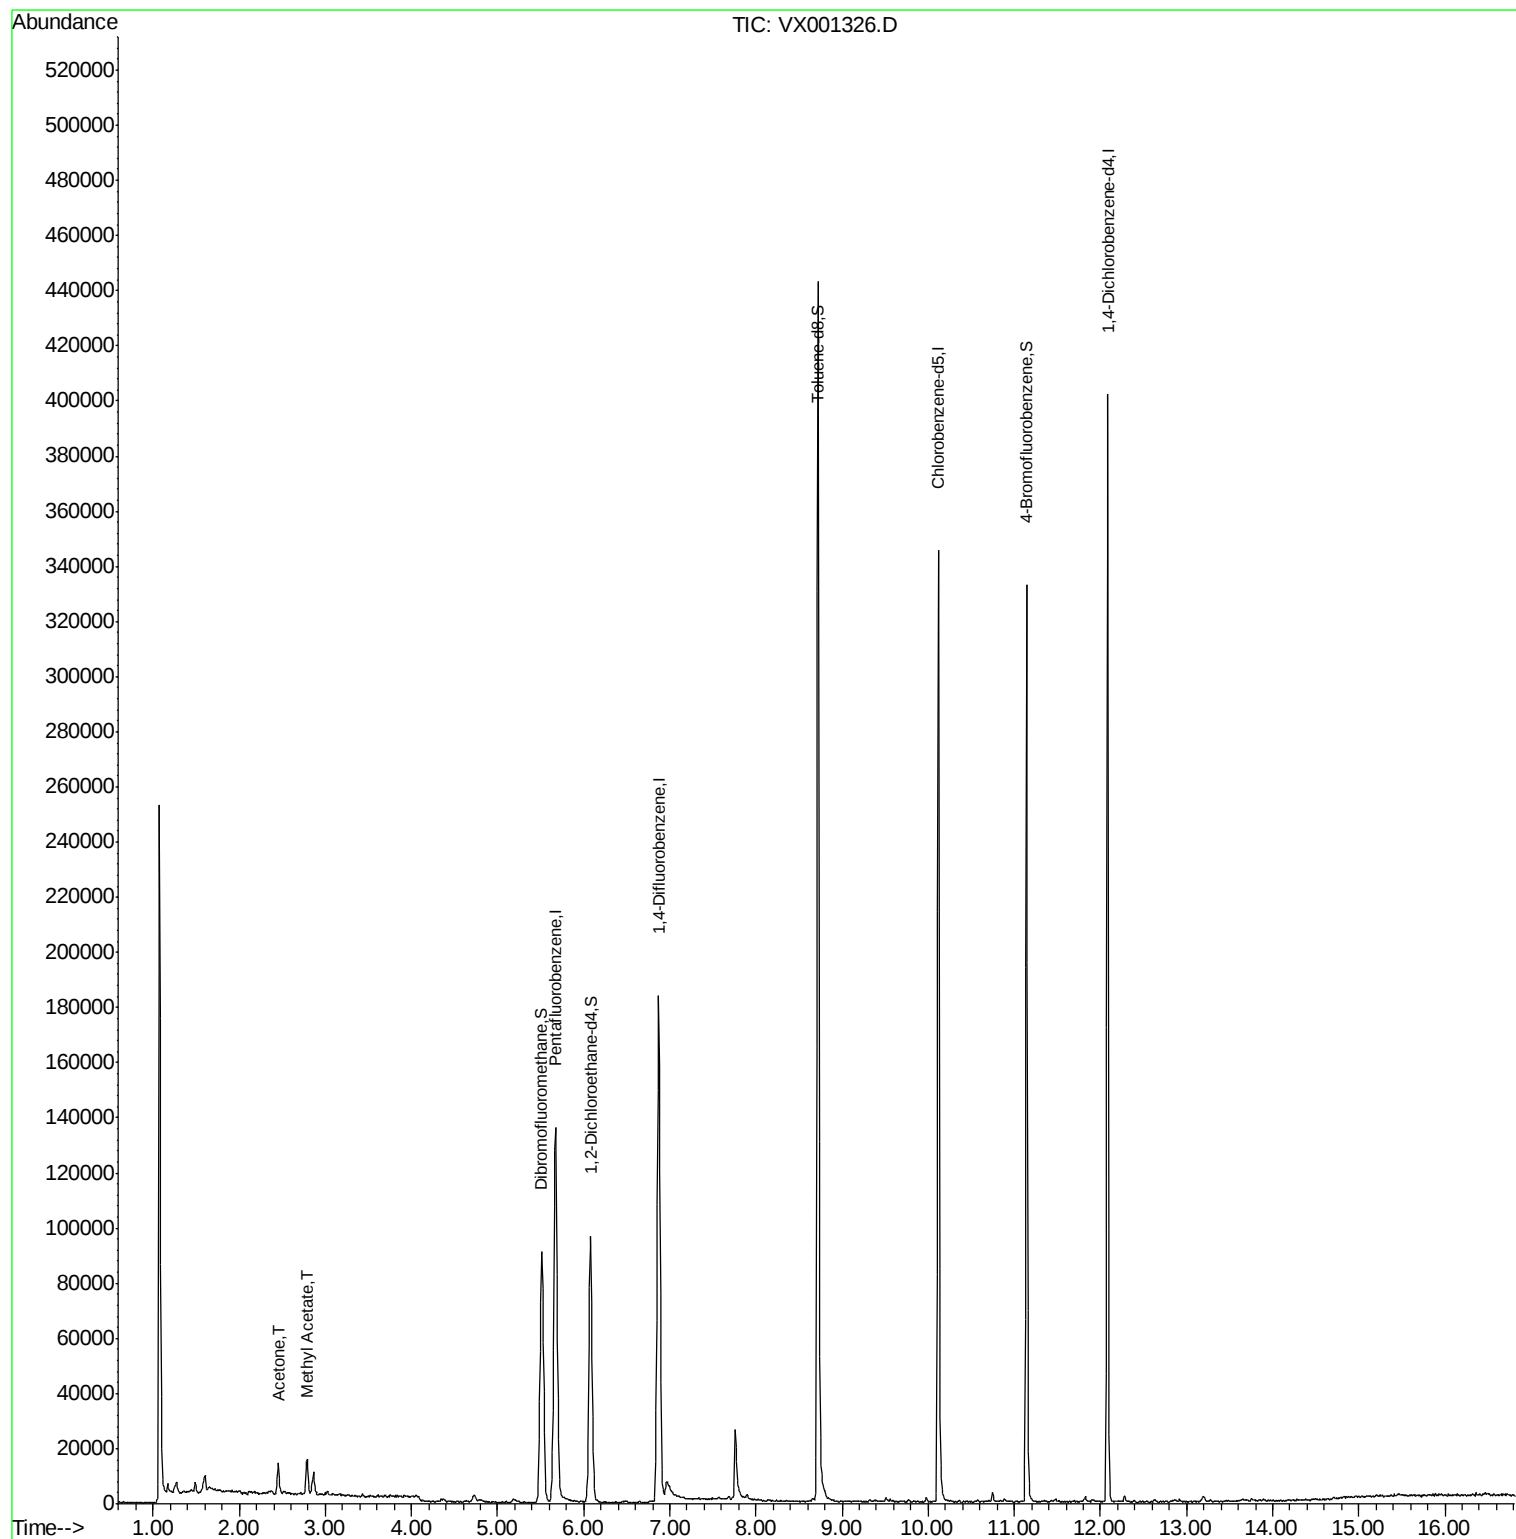

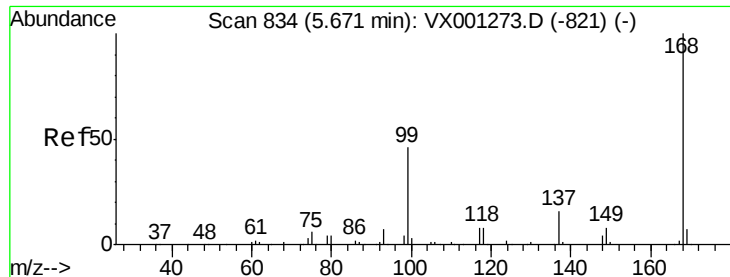

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. 0.00 min

Lab File: VX001326.D

Acq: 02 May 2018 19:21

Instrument :

MSVOA_X

ClientSampleId :


PB108794ZHE#11

Tot Ion:168 Resp: 147381

Ion Ratio Lower Upper

168 100

99 46.1 36.5 54.7

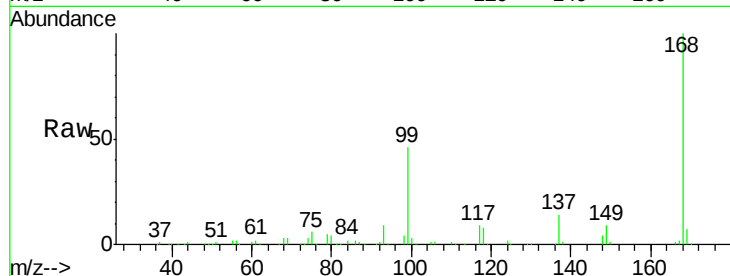

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

60000

50000

40000



30000

20000

10000

0

Time--> 5.50 5.60 5.70 5.80

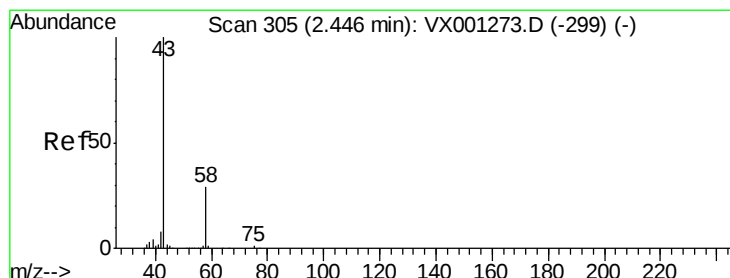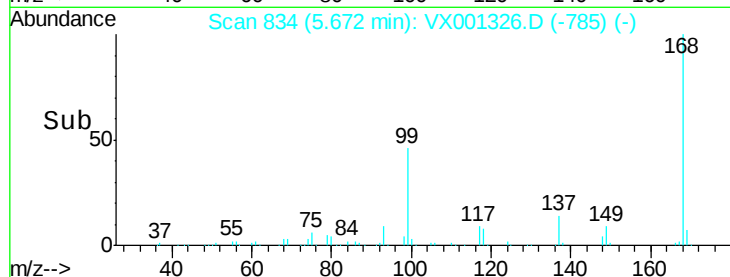

#16

Acetone

Concen: 13.51 ug/l

RT: 2.45 min Scan# 306

Delta R.T. 0.01 min

Lab File: VX001326.D


Acq: 02 May 2018 19:21

Tgt Ion: 43 Resp: 11762

Ion Ratio Lower Upper

43 100

58 25.8 22.8 34.2

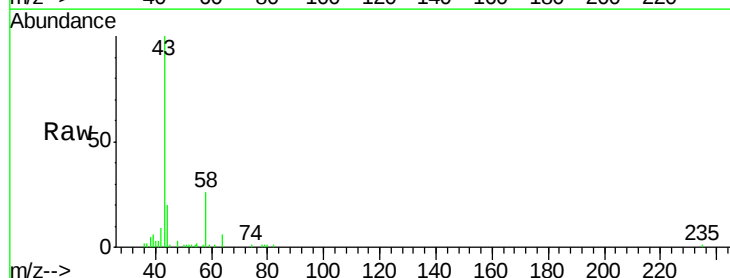

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.45

8000


6000


4000

2000

0

Time--> 2.40 2.45 2.50 2.55




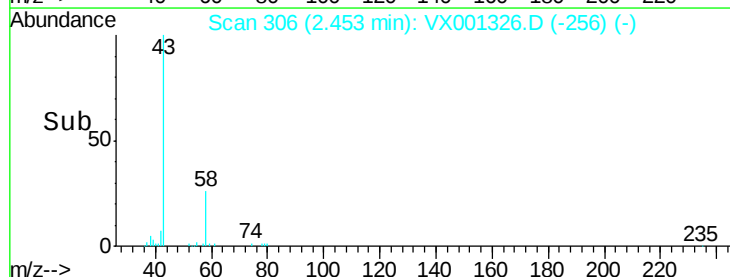


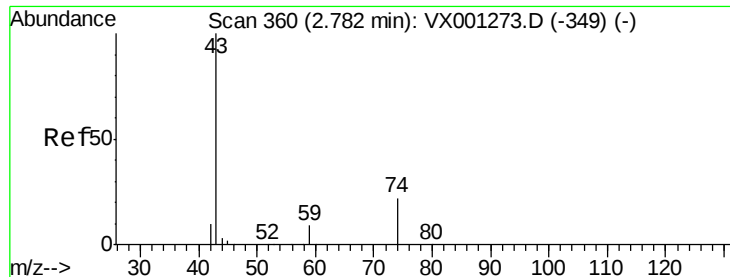

#18
Methvl Acetate
Concen: 7.32 ug/l
RT: 2.79 min Scan# 361
Delta R.T. 0.01 min
Lab File: VX001326.D
Acq: 02 May 2018 19:21




Instrument :
MSVOA_X
ClientSampleId :
PB108794ZHE#11


Tot Ion: 43 Resp: 15051
Ion Ratio Lower Upper
43 100
74 23.6 17.8 26.6

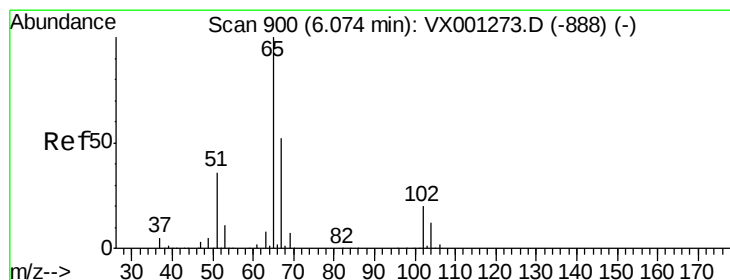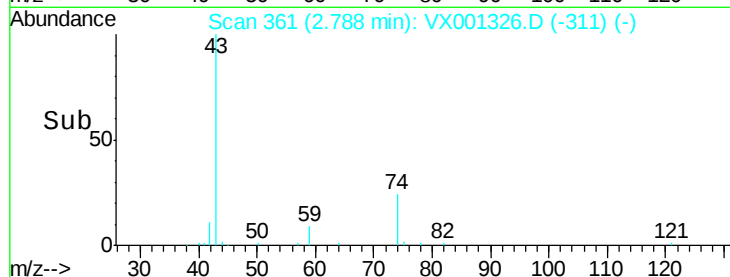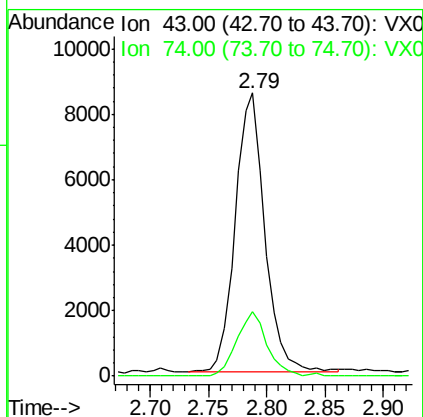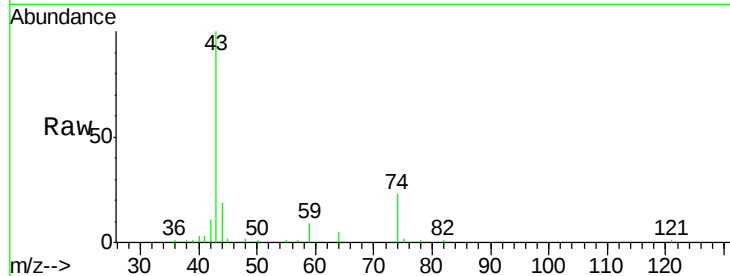

#33
1,2-Dichloroethane-d4
Concen: 43.59 ug/l
RT: 6.08 min Scan# 901
Delta R.T. 0.01 min
Lab File: VX001326.D
Acq: 02 May 2018 19:21

Tgt Ion: 65 Resp: 88924
Ion Ratio Lower Upper
65 100
67 52.1 0.0 102.8

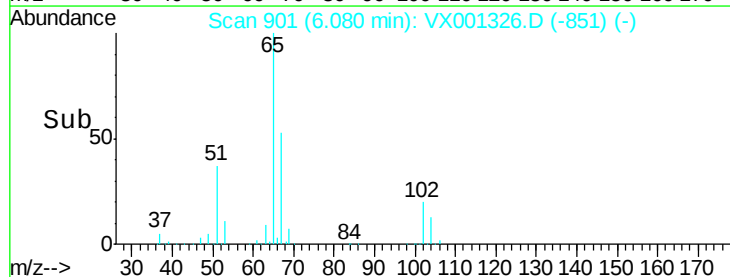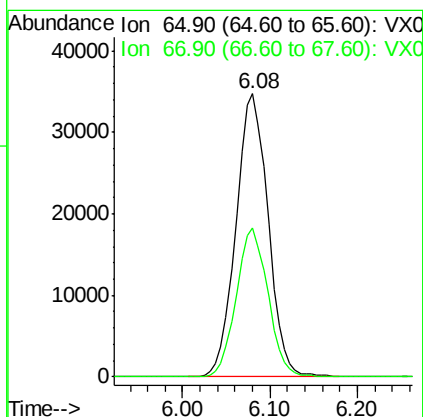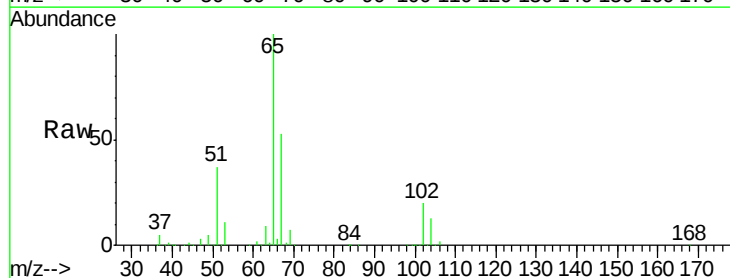

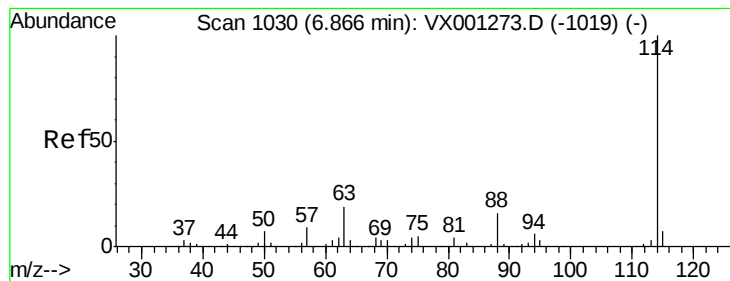

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1031

Delta R.T. 0.01 min

Lab File: VX001326.D

Acq: 02 May 2018 19:21

Instrument :

MSVOA_X

ClientSampleId :

PB108794ZHE#11


Tot Ion:114 Resp: 194837

Ion Ratio Lower Upper

114 100

63 18.2 0.0 38.8




88 15.7 0.0 32.2

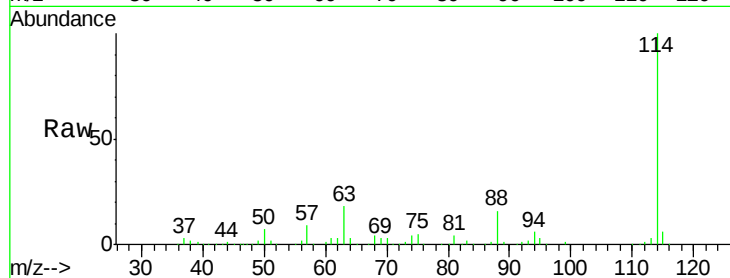

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

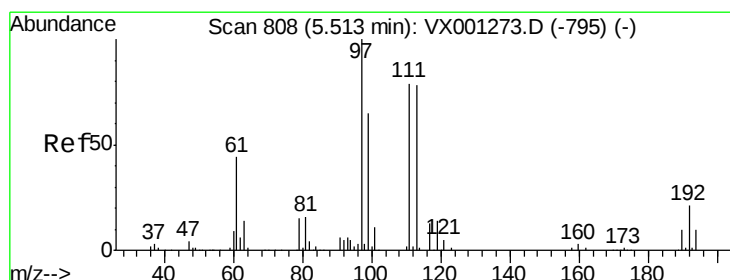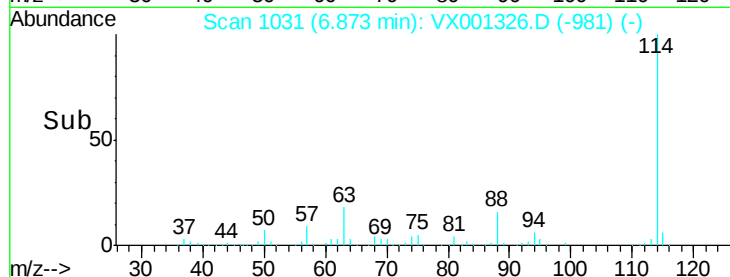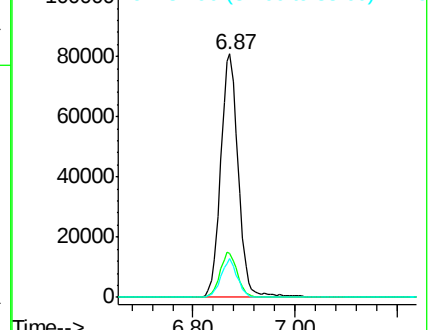

#35

Dibromofluoromethane

Concen: 44.51 ug/l

RT: 5.52 min Scan# 809

Delta R.T. 0.01 min

Lab File: VX001326.D

Acq: 02 May 2018 19:21


Tgt Ion:113 Resp: 74714

Ion Ratio Lower Upper

113 100

111 101.6 81.2 121.8



192 25.4 20.7 31.1

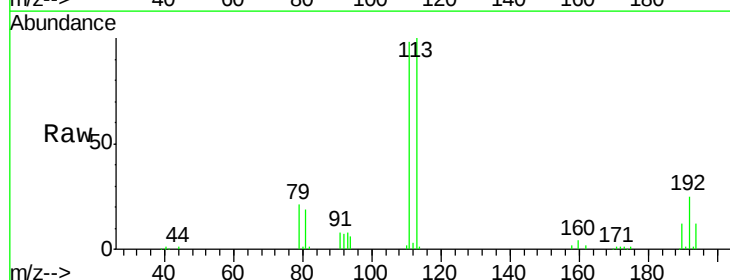


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



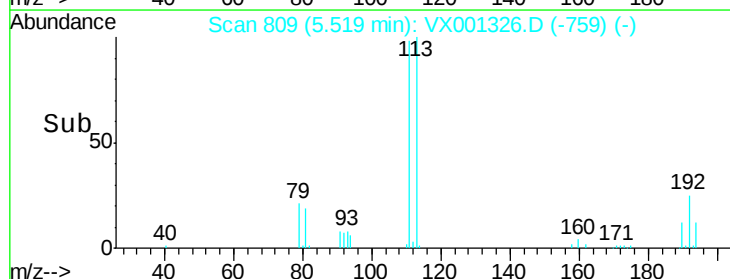
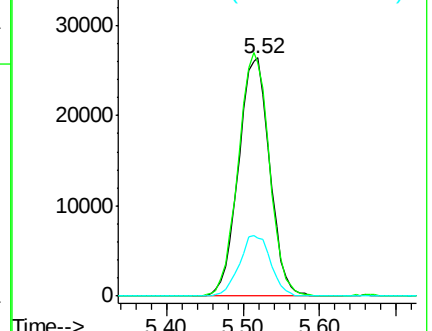


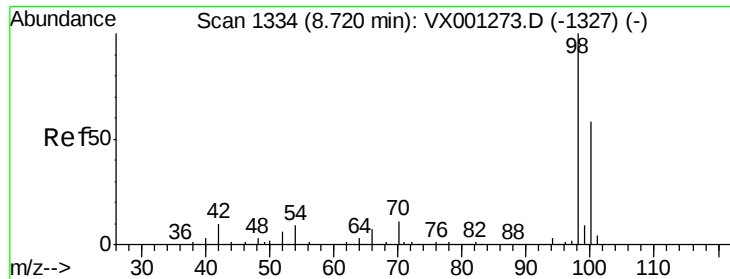

#50
Toluene-d8
Concen: 45.18 ug/l
RT: 8.72 min Scan# 1334
Delta R.T. 0.00 min
Lab File: VX001326.D
Acq: 02 May 2018 19:21




Instrument :
MSVOA_X
ClientSampleId :
PB108794ZHE#11


Tot Ion: 98 Resp: 270936
Ion Ratio Lower Upper
98 100
100 63.7 51.0 76.4

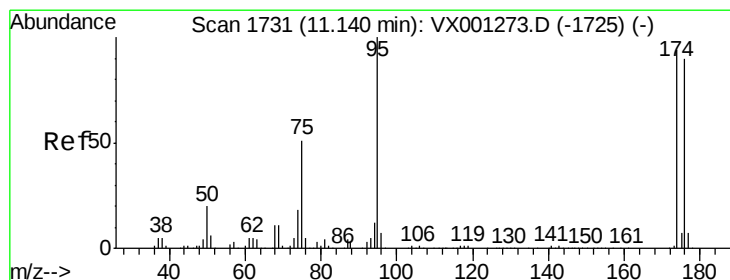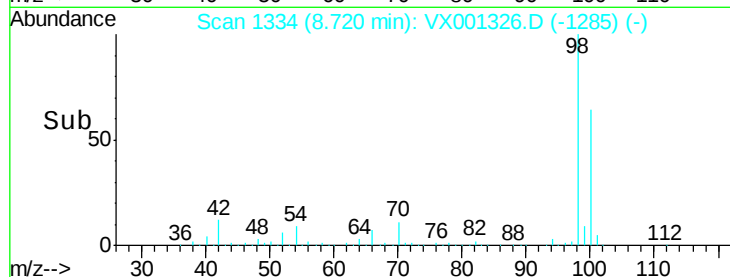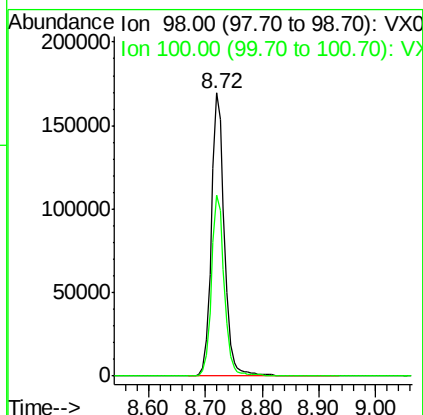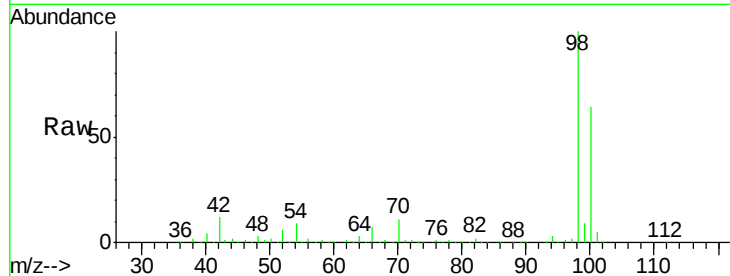

#62
4-Bromofluorobenzene
Concen: 34.11 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. 0.00 min
Lab File: VX001326.D
Acq: 02 May 2018 19:21

Tgt Ion: 95 Resp: 81815
Ion Ratio Lower Upper
95 100
174 104.6 0.0 201.8
176 100.7 0.0 197.2

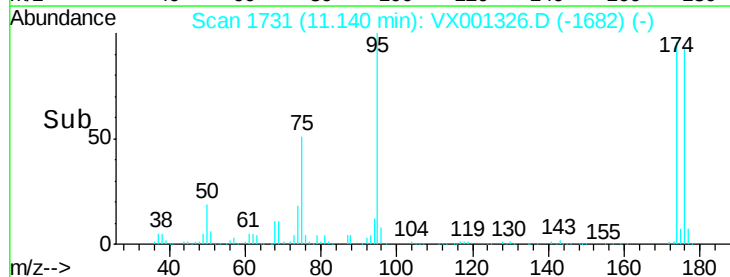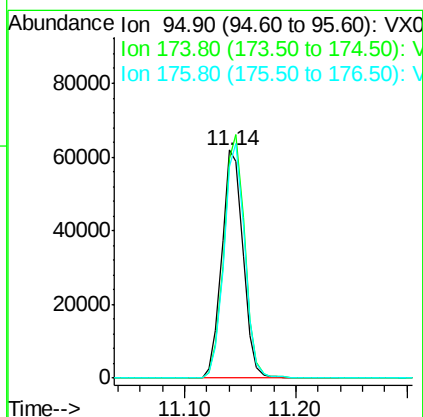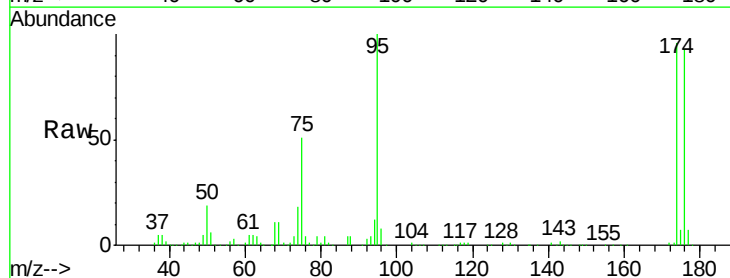


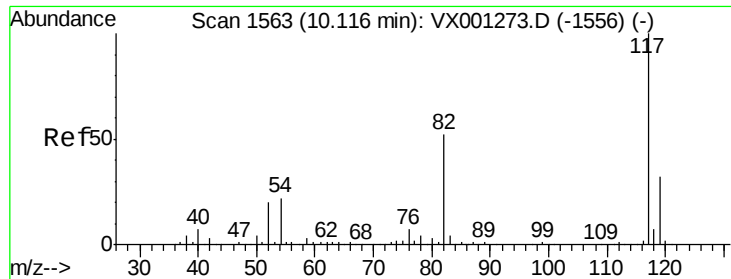




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1564
Delta R.T. 0.01 min
Lab File: VX001326.D
Acq: 02 May 2018 19:21

Instrument :
MSVOA_X
ClientSampleId :
PB108794ZHE#11

Tot Ion:117 Resp: 167815
Ion Ratio Lower Upper
117 100
82 51.0 41.4 62.0
119 32.4 25.5 38.3

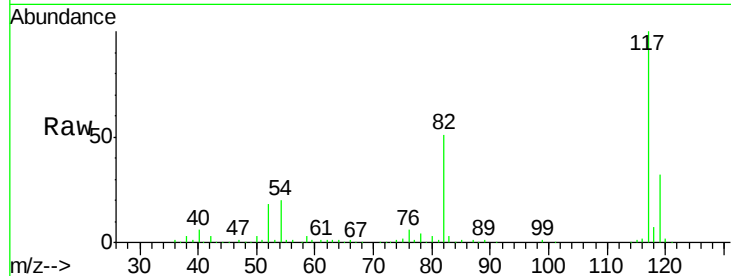


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

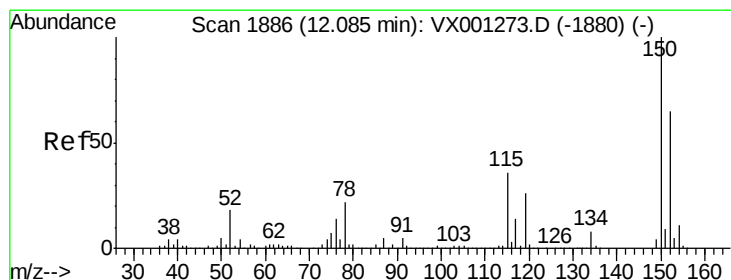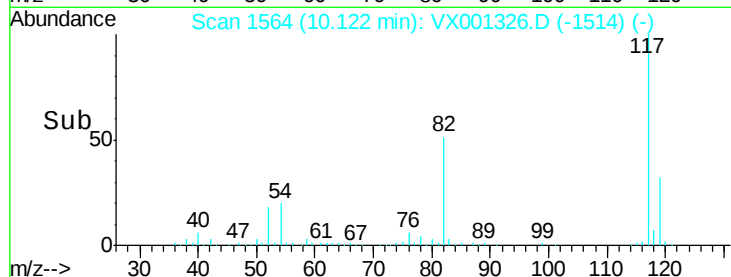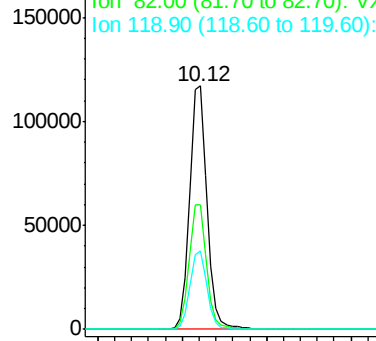

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.09 min Scan# 1886
Delta R.T. 0.00 min
Lab File: VX001326.D
Acq: 02 May 2018 19:21

Tgt Ion:152 Resp: 86377
Ion Ratio Lower Upper
152 100
115 51.0 38.6 115.7
150 154.6 0.0 349.2

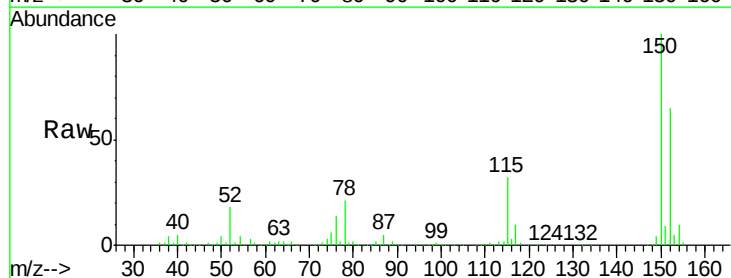

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

