


Data Path : W:\HPCHEM1\MSVOA X\DATA\VX050218\
Data File : VX001330.D
Acq On : 02 May 2018 21:09
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\624X043018W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue May 01 09:17:40 2018

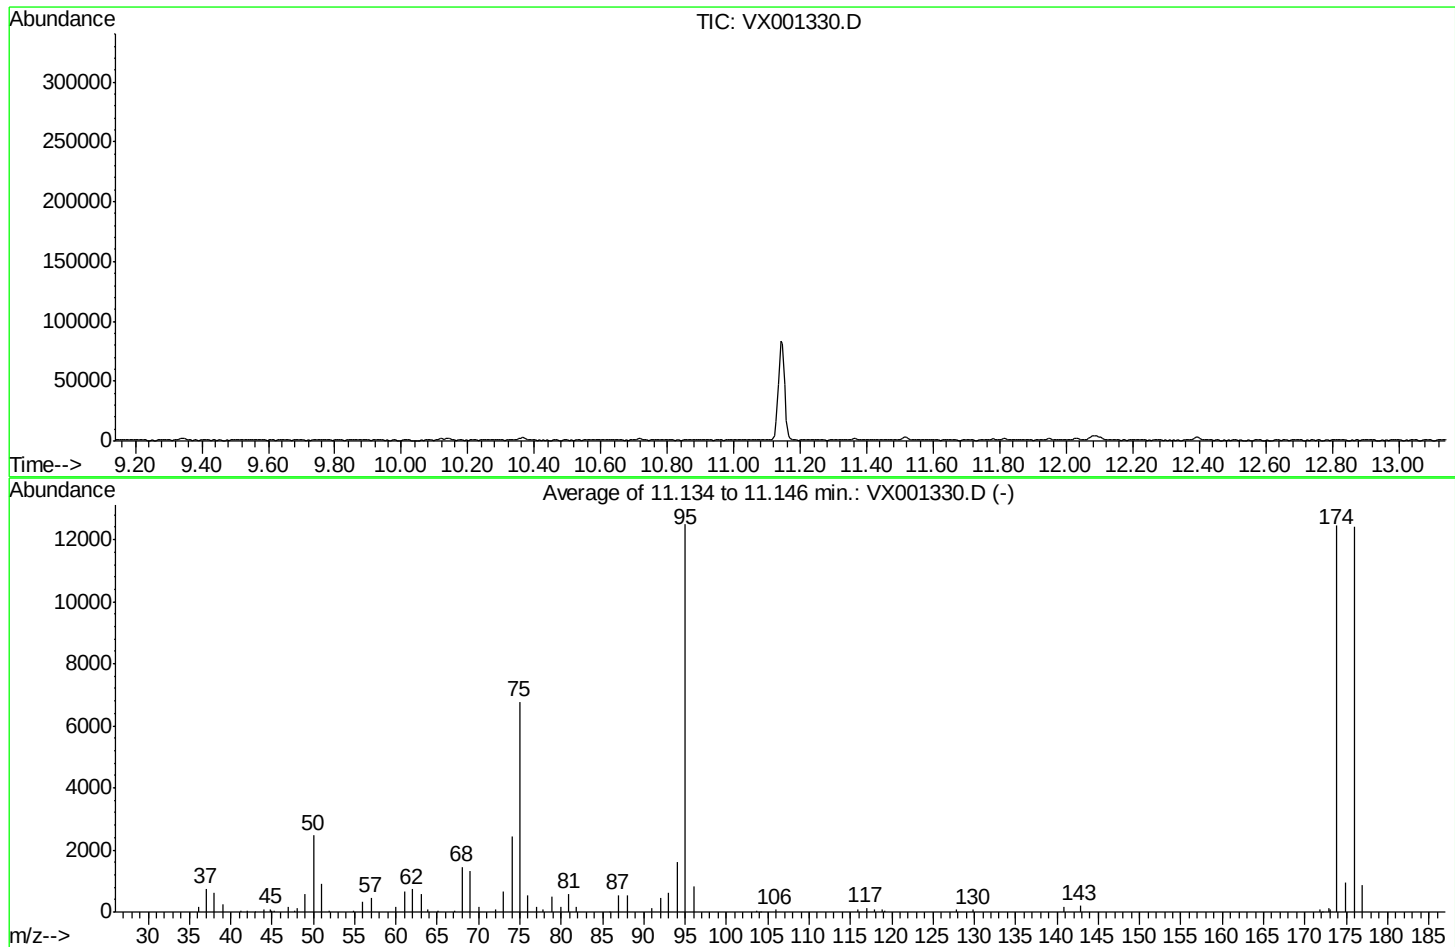

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	2462	PASS
75	95	30	60	54.3	6779	PASS
95	95	100	100	100.0	12493	PASS
96	95	5	9	6.7	835	PASS
173	174	0.00	2	1.0	125	PASS
174	95	50	100	99.6	12447	PASS
175	174	5	9	7.8	967	PASS
176	174	95	101	99.9	12435	PASS
177	176	5	9	7.0	867	PASS