

Data File : VX001371.D

Acq On : 03 May 2018 20:39

Operator : JC/MD

Sample : J2686-04 5X

Misc : 5.0mL/MSVOA_X/WATER

ALS Vial : 20 Sample Multiplier: 1

Instrument :

MSVOA_X

ClientSampleId :

GS-2-PAINT-CHIP-WIPES

Quant Time: May 04 07:16:58 2018

Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X050118W.M

Quant Title : SW846 8260

QLast Update : Wed May 02 01:48:25 2018

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	153709	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	215188	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	197891	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	102680	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.08	65	80604	37.88	ug/l	0.00
Spiked Amount	50.000		Recovery	=	75.76%	
35) Dibromofluoromethane	5.51	113	67566	36.45	ug/l	0.00
Spiked Amount	50.000		Recovery	=	72.90%	
50) Toluene-d8	8.72	98	254874	38.48	ug/l	0.00
Spiked Amount	50.000		Recovery	=	76.96%	
62) 4-Bromofluorobenzene	11.15	95	85970	32.46	ug/l	0.00
Spiked Amount	50.000		Recovery	=	64.92%	

Target Compounds

						Qvalue
5) Bromomethane	1.64	94	658	Below Cal	#	80
6) Chloroethane	1.73	64	277	0.25	ug/l	91
10) Methyl Iodide	2.53	142	782	4.71	ug/l #	80
11) Tert butyl alcohol	3.09	59	1089	2.97	ug/l #	54
12) 1,1-Dichloroethene	2.38	96	315	0.20	ug/l #	77
13) Acrolein	2.31	56	438	2.08	ug/l	93
16) Acetone	2.45	43	16025	17.64	ug/l	93
18) Methyl Acetate	2.78	43	4928	2.30	ug/l	98
20) Methylene Chloride	2.86	84	65614	39.71	ug/l	99
24) 1,1-Dichloroethane	3.71	63	2111	0.73	ug/l #	85
25) 2-Butanone	4.73	43	3612	2.94	ug/l	98
29) Tetrahydrofuran	5.19	42	784	1.04	ug/l #	64
31) Cyclohexane	5.67	56	2639	1.01	ug/l #	1
32) 1,1,1-Trichloroethane	5.51	97	1609	0.60	ug/l #	42
36) 1,1-Dichloropropene	5.68	75	9616	3.87	ug/l #	48
38) Carbon Tetrachloride	5.67	117	13318	5.12	ug/l #	18
44) Trichloroethene	7.22	130	50584	23.13	ug/l	97
51) 4-Methyl-2-Pentanone	8.66	43	1219	0.47	ug/l	98
52) Toluene	8.79	92	1508	0.32	ug/l	95
59) 2-Hexanone	9.51	43	1425	0.70	ug/l	99
67) Ethyl Benzene	10.26	91	7322	0.83	ug/l #	88
68) m/p-Xylenes	10.37	106	13543	3.88	ug/l	95
69) o-Xylene	10.71	106	6387	1.89	ug/l	99
76) 1,2,3-Trichloropropane	11.15	75	43911	23.13	ug/l #	40
81) trans-1,4-Dichloro-2-buten	11.15	75	43911	73.08	ug/l #	6
95) Naphthalene	13.84	128	82950	11.04	ug/l	100

(#)=qualifier out of range (m)=manual integration (+)=signals summed

Data File : VX001371.D

Acq On : 03 May 2018 20:39

Operator : JC/MD

Sample : J2686-04 5X

Misc : 5.0mL/MSVOA_X/WATER

ALS Vial : 20 Sample Multiplier: 1

Instrument :

MSVOA_X

ClientSampleId :

GS-2-PAINT-CHIP-WIPES


Quant Time: May 04 07:16:58 2018

Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X050118W.M

Quant Title : SW846 8260

QLast Update : Wed May 02 01:48:25 2018

Response via : Initial Calibration

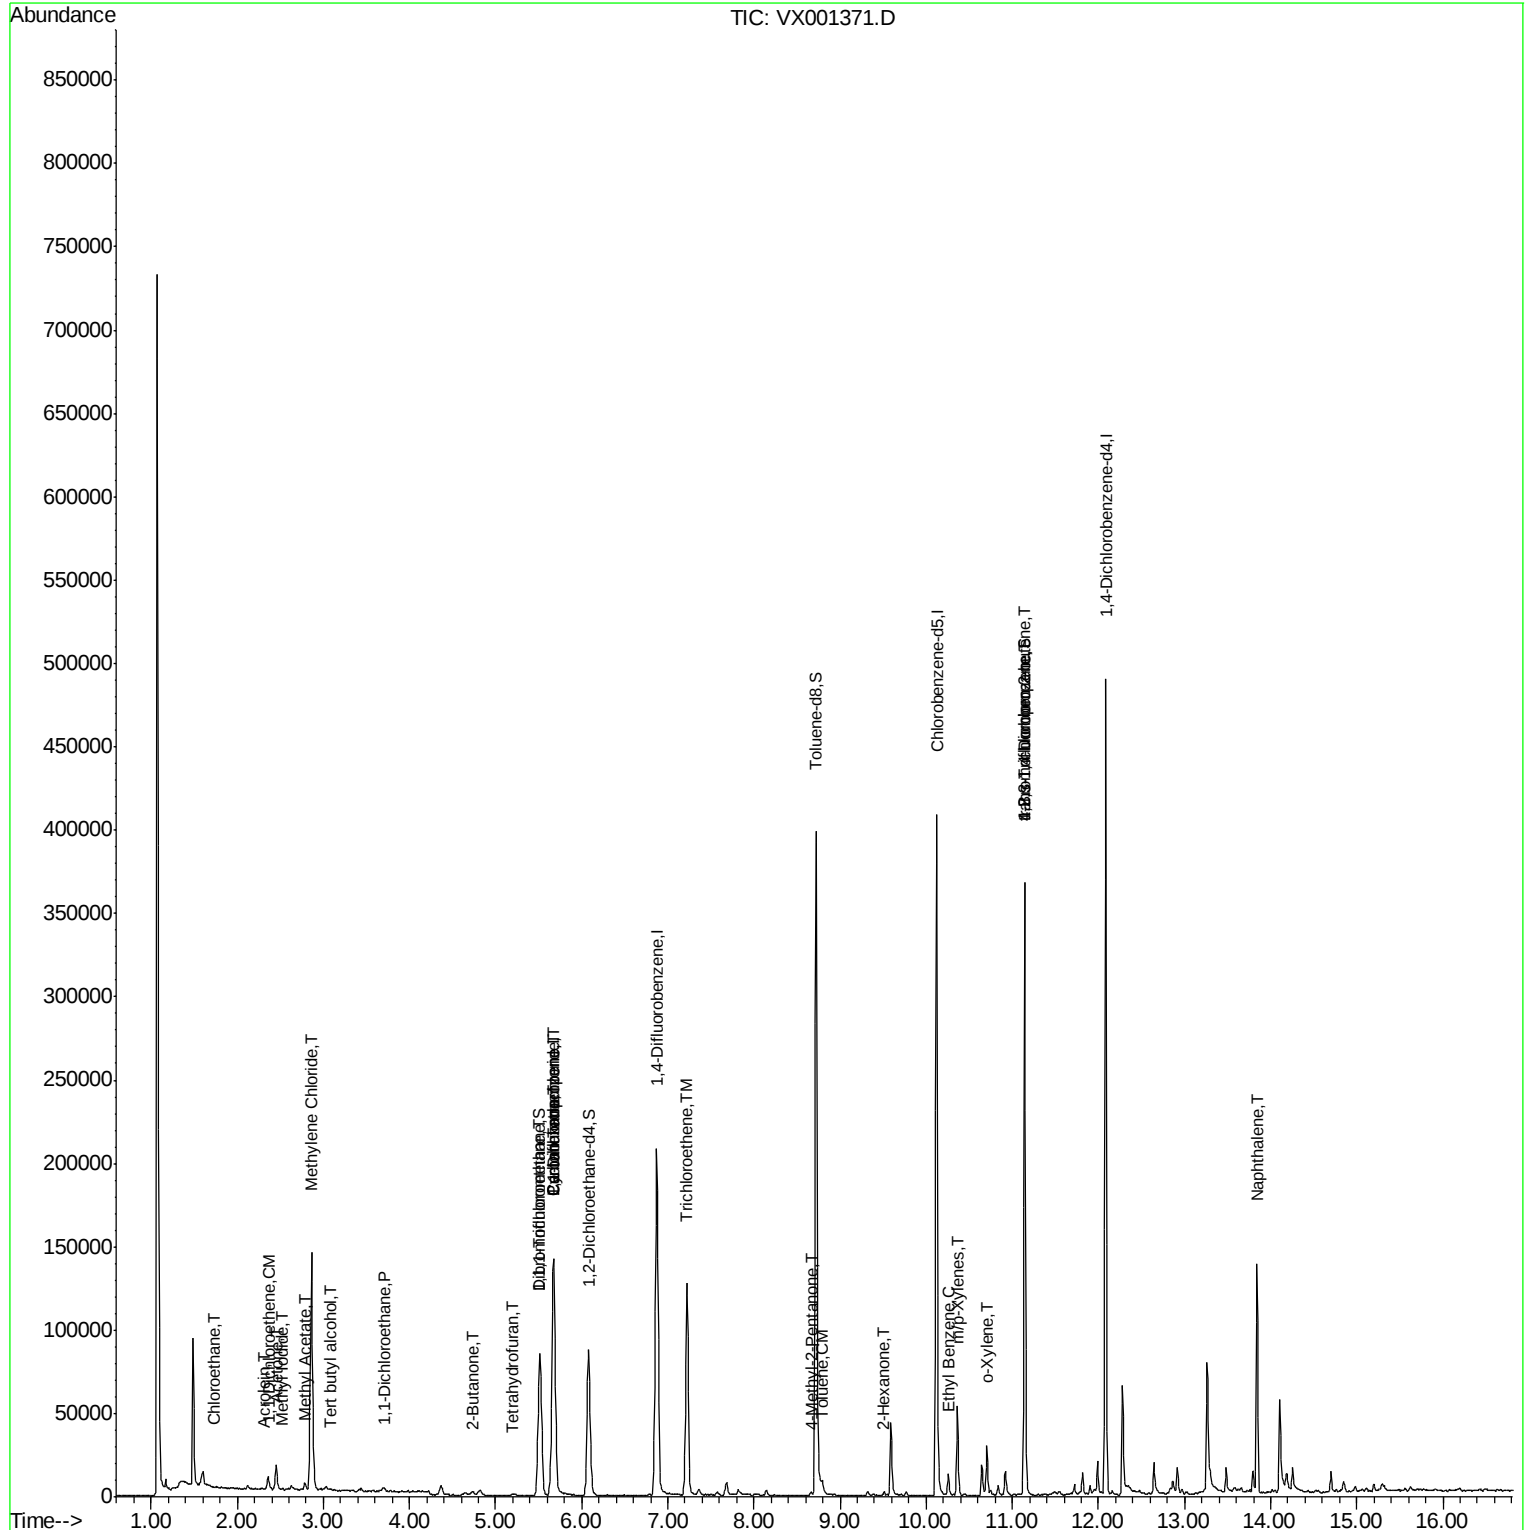



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. 0.00 min

Lab File: VX001371.D

Acq: 03 May 2018 20:39

Instrument :

MSVOA_X

ClientSampleId :


GS-2-PAINT-CHIP-WIPES

Tgt Ion:168 Resp: 153709

Ion Ratio Lower Upper

168 100

99 45.5 36.5 54.7

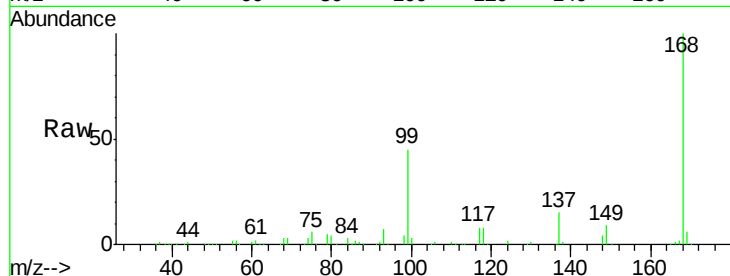

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

60000

50000

40000



30000

20000

10000

0

Time--> 5.50 5.60 5.70 5.80



#5

Bromomethane

Concen: Below Cal

RT: 1.64 min Scan# 173

Delta R.T. 0.01 min

Lab File: VX001371.D


Acq: 03 May 2018 20:39

Tgt Ion: 94 Resp: 658

Ion Ratio Lower Upper

94 100

96 75.1 75.6 113.4#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1.64


300


200

100

0

Time--> 1.60 1.65 1.70





#6

Chloroethane

Concen: 0.25 ug/l

RT: 1.73 min Scan# 187

Delta R.T. 0.01 min

Lab File: VX001371.D

Acq: 03 May 2018 20:39

Instrument :

MSVOA_X

ClientSampleId :


GS-2-PAINT-CHIP-WIPES

Tgt Ion: 64 Resp: 277

Ion Ratio Lower Upper

64 100

66 36.9 25.7 38.5



Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0

250

200

150

100



50

0

1.70 1.75

1.73

Time-->



#10

Methyl Iodide

Concen: 4.71 ug/l

RT: 2.53 min Scan# 318

Delta R.T. 0.01 min

Lab File: VX001371.D

Acq: 03 May 2018 20:39


Tgt Ion: 142 Resp: 782

Ion Ratio Lower Upper

142 100

127 57.5 35.7 53.5#

141 6.0 11.4 17.0#



Abundance Ion 141.80 (141.50 to 142.50): V

Ion 126.80 (126.50 to 127.50): V

Ion 140.80 (140.50 to 141.50): V

500

400

300

200


100


0

2.50 2.55

2.53

Time-->







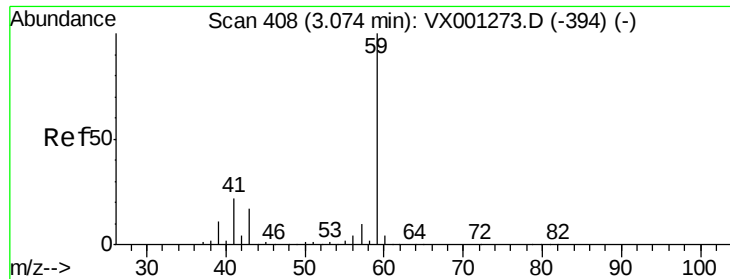

#11
Tert butyl alcohol
Concen: 2.97 ug/l
RT: 3.09 min Scan# 410
Delta R.T. 0.01 min
Lab File: VX001371.D
Acq: 03 May 2018 20:39




Instrument :
MSVOA_X
ClientSampleId :
GS-2-PAINT-CHIP-WIPES


Tgt Ion: 59 Resp: 1089
Ion Ratio Lower Upper
59 100
57 28.1 8.6 12.8#

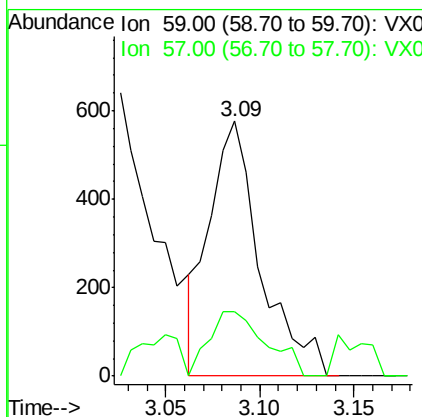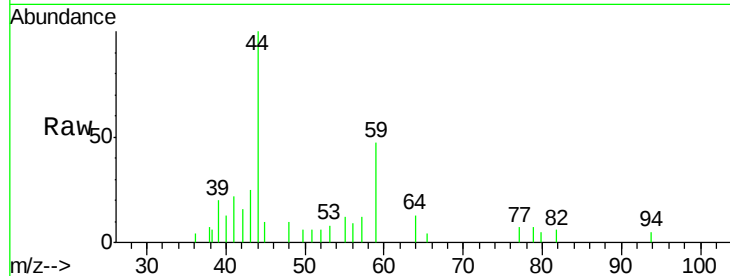

#12
1,1-Dichloroethene
Concen: 0.20 ug/l
RT: 2.38 min Scan# 294
Delta R.T. 0.01 min
Lab File: VX001371.D
Acq: 03 May 2018 20:39

Tgt Ion: 96 Resp: 315
Ion Ratio Lower Upper
96 100
61 129.9 130.1 195.1#
98 47.5 50.3 75.5#



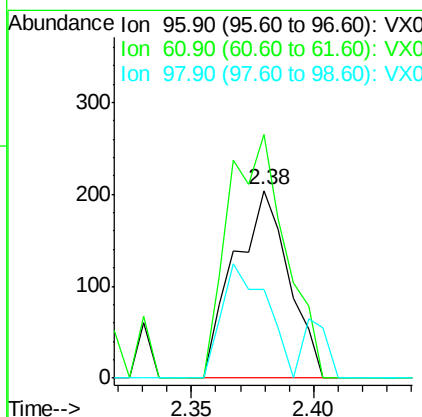





#13
Acrolein
Concen: 2.08 ug/l
RT: 2.31 min Scan# 282
Delta R.T. 0.01 min
Lab File: VX001371.D
Acq: 03 May 2018 20:39




Instrument :
MSVOA_X
ClientSampleId :
GS-2-PAINT-CHIP-WIPES


Tgt Ion: 56 Resp: 438
Ion Ratio Lower Upper
56 100
55 65.5 57.2 85.8

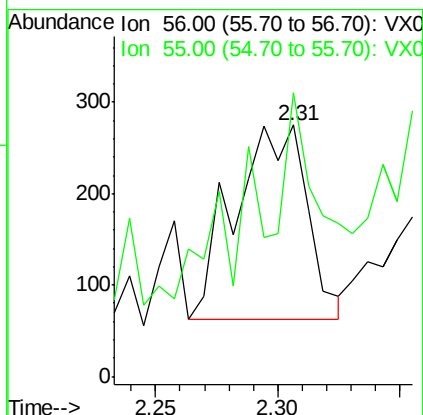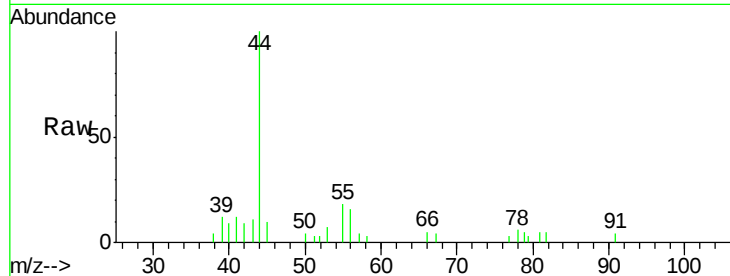

#16
Acetone
Concen: 17.64 ug/l
RT: 2.45 min Scan# 306
Delta R.T. 0.01 min
Lab File: VX001371.D
Acq: 03 May 2018 20:39

Tgt Ion: 43 Resp: 16025
Ion Ratio Lower Upper
43 100
58 25.0 22.8 34.2



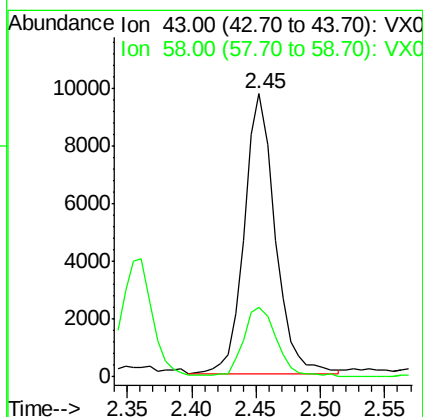
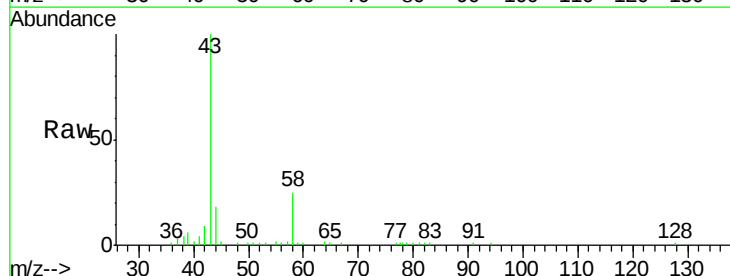


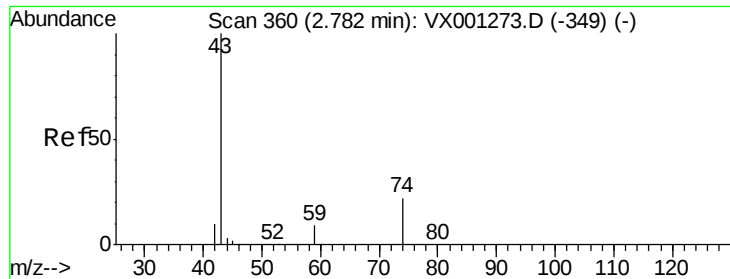

#18
Methyl Acetate
Concen: 2.30 ug/l
RT: 2.78 min Scan# 360
Delta R.T. 0.00 min
Lab File: VX001371.D
Acq: 03 May 2018 20:39




Instrument :
MSVOA_X
ClientSampleId :
GS-2-PAINT-CHIP-WIPES


Tgt Ion: 43 Resp: 4928
Ion Ratio Lower Upper
43 100
74 23.3 17.8 26.6

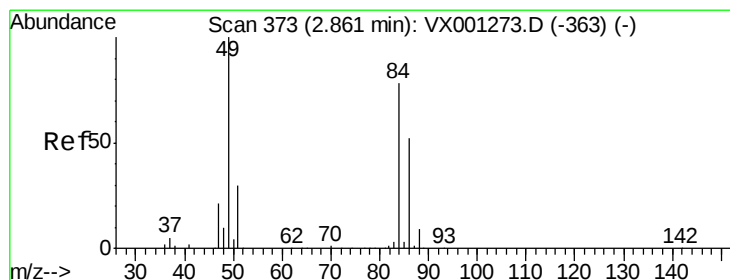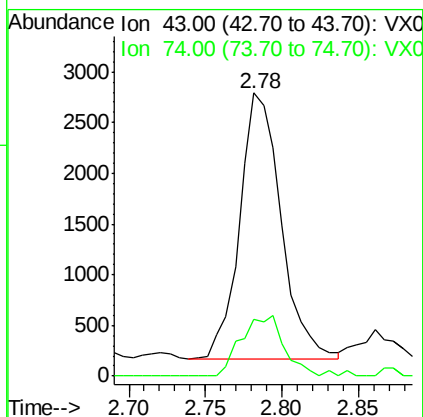

#20
Methylene Chloride
Concen: 39.71 ug/l
RT: 2.86 min Scan# 373
Delta R.T. 0.00 min
Lab File: VX001371.D
Acq: 03 May 2018 20:39

Tgt Ion: 84 Resp: 65614
Ion Ratio Lower Upper
84 100
49 127.4 102.8 154.2
51 39.7 30.9 46.3
86 67.2 53.0 79.4

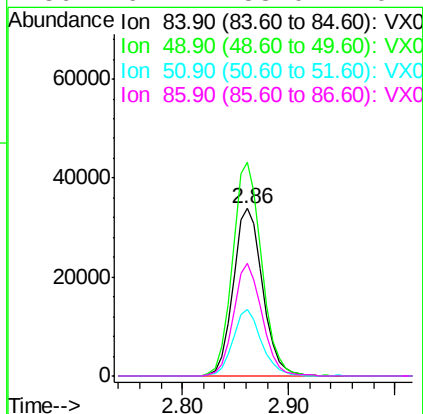



#24

1,1-Dichloroethane

Concen: 0.73 ug/l

RT: 3.71 min Scan# 512

Delta R.T. 0.01 min

Lab File: VX001371.D

Acq: 03 May 2018 20:39

Instrument :

MSVOA_X

ClientSampleId :

GS-2-PAINT-CHIP-WIPES





Tgt Ion: 63 Resp: 2111

Ion Ratio Lower Upper

63 100

98 0.0 3.5 10.5#

100 6.7 2.3 6.8

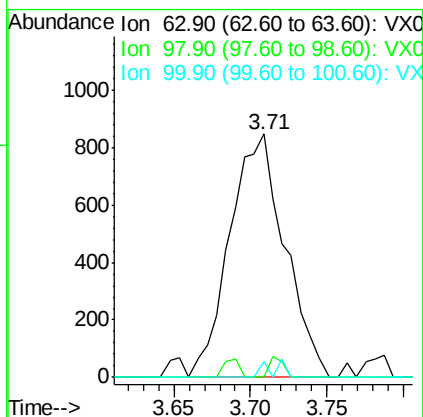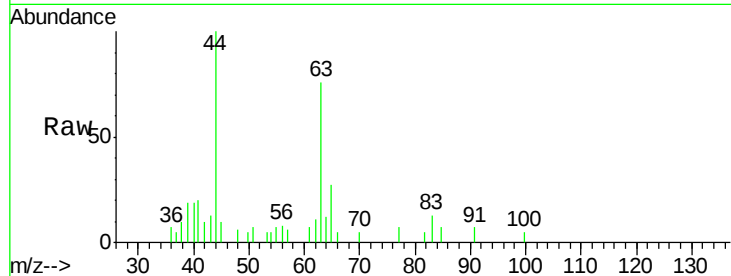

#25

2-Butanone

Concen: 2.94 ug/l

RT: 4.73 min Scan# 680

Delta R.T. 0.02 min

Lab File: VX001371.D




Acq: 03 May 2018 20:39


Tgt Ion: 43 Resp: 3612

Ion Ratio Lower Upper

43 100

72 24.8 20.5 30.7

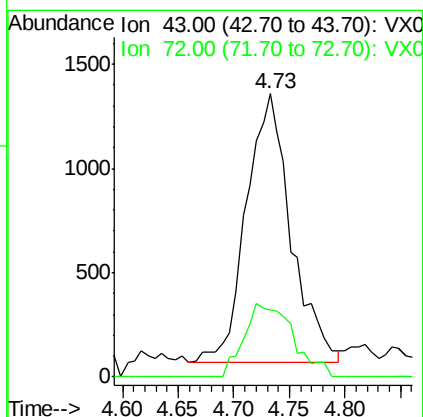



#29

Tetrahydrofuran

Concen: 1.04 ug/l

RT: 5.19 min Scan# 755

Delta R.T. 0.02 min

Lab File: VX001371.D

Acq: 03 May 2018 20:39

Instrument :

MSVOA_X

ClientSampleId :

GS-2-PAINT-CHIP-WIPES





Tgt Ion: 42 Resp: 784

Ion Ratio Lower Upper

42 100

72 34.9 34.6 52.0

71 3.4 32.7 49.1#

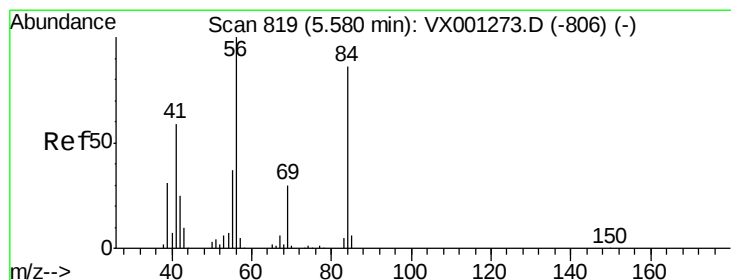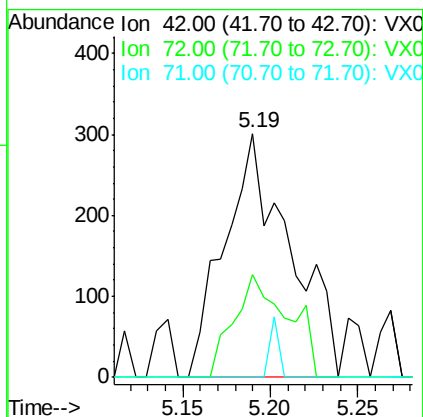

#31

Cyclohexane

Concen: 1.01 ug/l

RT: 5.67 min Scan# 834

Delta R.T. 0.09 min

Lab File: VX001371.D

Acq: 03 May 2018 20:39




Tgt Ion: 56 Resp: 2639


Ion Ratio Lower Upper

56 100

69 150.3 24.0 36.0#

84 145.9 69.0 103.4#

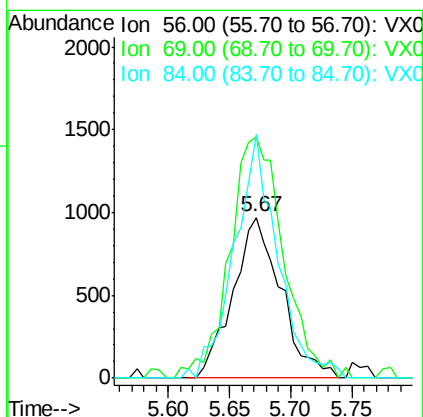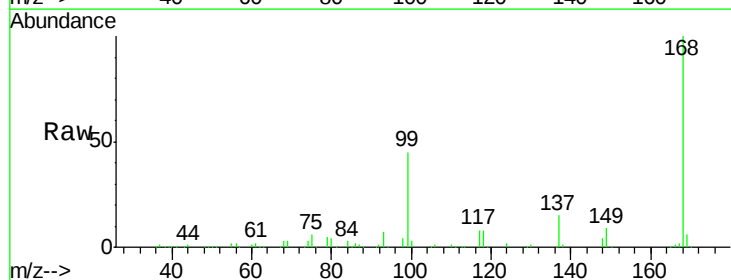



#32

1,1,1-Trichloroethane

Concen: 0.60 ug/l

RT: 5.51 min Scan# 807

Delta R.T. 0.00 min

Lab File: VX001371.D

Acq: 03 May 2018 20:39

Instrument :

MSVOA_X

ClientSampleId :

GS-2-PAINT-CHIP-WIPES


Tgt Ion: 97 Resp: 1609

Ion Ratio Lower Upper

97 100

99 0.0 51.8 77.6#




61 29.6 35.4 53.2#

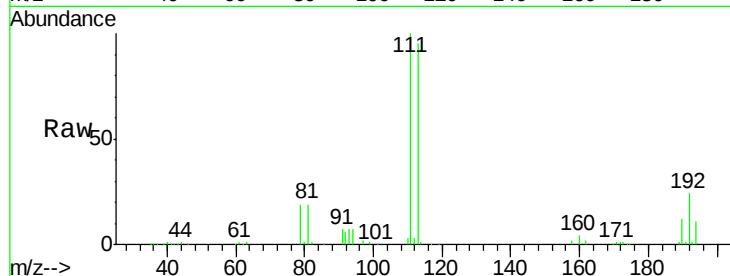

Abundance Ion 96.90 (96.60 to 97.60): VX0

Ion 98.90 (98.60 to 99.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

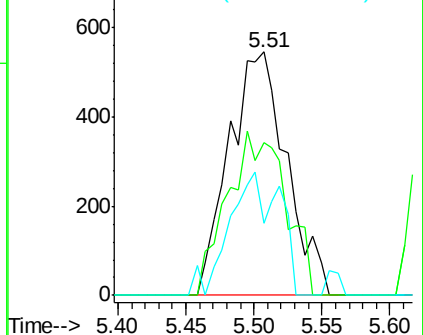

#33

1,2-Dichloroethane-d4

Concen: 37.88 ug/l

RT: 6.08 min Scan# 901

Delta R.T. 0.01 min

Lab File: VX001371.D


Acq: 03 May 2018 20:39

Tgt Ion: 65 Resp: 80604

Ion Ratio Lower Upper



65 100


67 52.3 0.0 102.8



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0




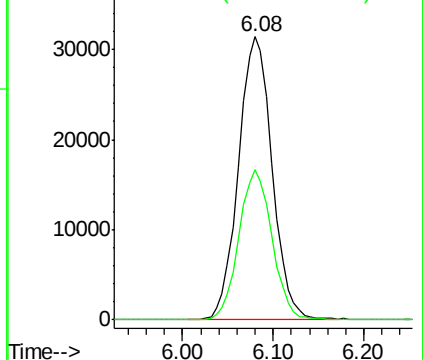




#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.87 min Scan# 1031
 Delta R.T. 0.01 min
 Lab File: VX001371.D
 Acq: 03 May 2018 20:39




Instrument :
 MSVOA_X
 ClientSampleId :
 GS-2-PAINT-CHIP-WIPES


Tgt Ion:114 Resp: 215188
 Ion Ratio Lower Upper
 114 100
 63 19.1 0.0 38.8
 88 14.6 0.0 32.2

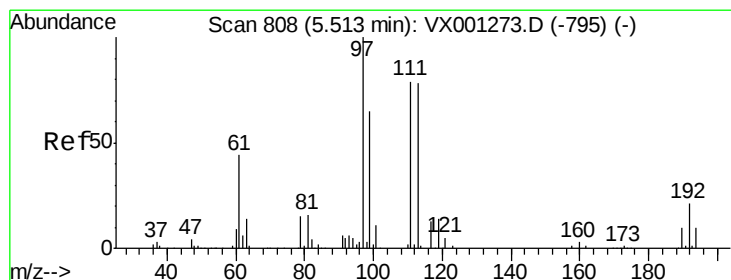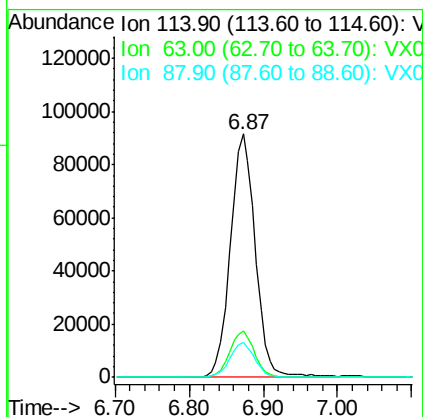

#35
 Dibromofluoromethane
 Concen: 36.45 ug/l
 RT: 5.51 min Scan# 808
 Delta R.T. 0.00 min
 Lab File: VX001371.D
 Acq: 03 May 2018 20:39

Tgt Ion:113 Resp: 67566
 Ion Ratio Lower Upper
 113 100
 111 102.7 81.2 121.8
 192 25.9 20.7 31.1

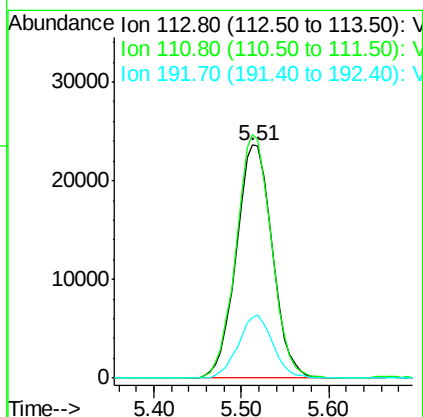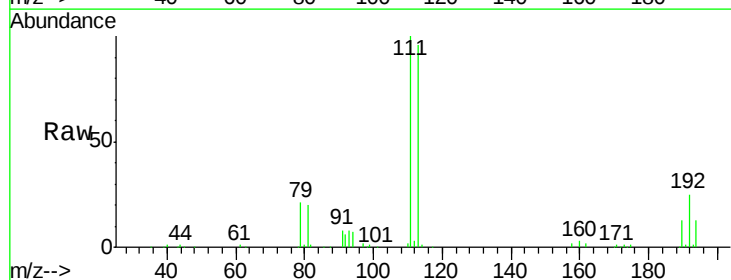

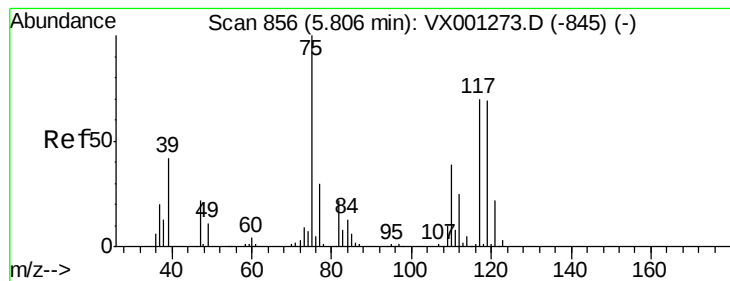

#36

1,1-Dichloropropene

Concen: 3.87 ug/l

RT: 5.68 min Scan# 835

Delta R.T. -0.13 min

Lab File: VX001371.D

Acq: 03 May 2018 20:39

Instrument :

MSVOA_X

ClientSampleId :

GS-2-PAINT-CHIP-WIPES


Tgt Ion: 75 Resp: 9616

Ion Ratio Lower Upper

75 100

110 8.5 18.9 56.9#




77 0.0 24.2 36.2#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

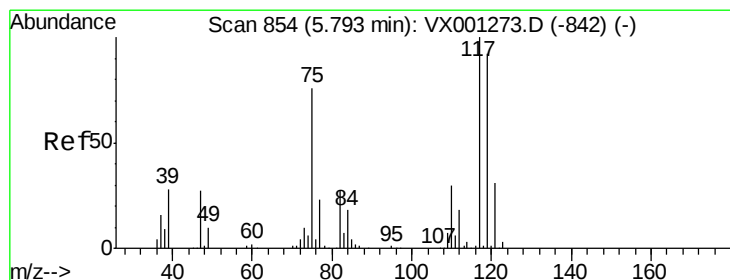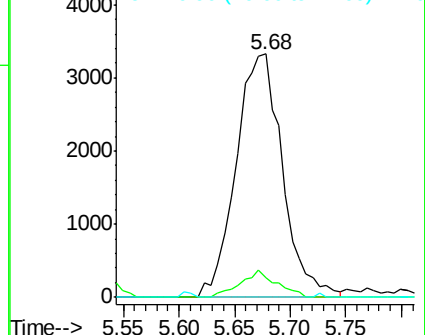

#38

Carbon Tetrachloride

Concen: 5.12 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.13 min

Lab File: VX001371.D

Acq: 03 May 2018 20:39


Tgt Ion: 117 Resp: 13318

Ion Ratio Lower Upper

117 100

119 5.0 73.4 110.2#



121 0.0 25.0 37.4#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

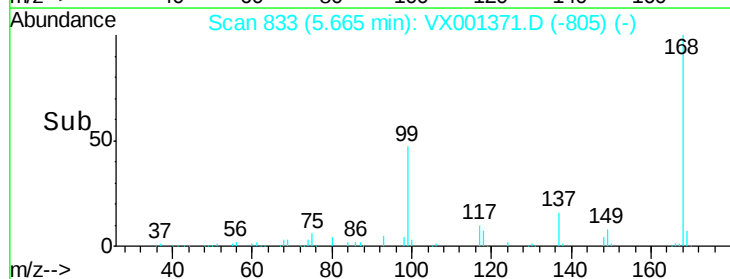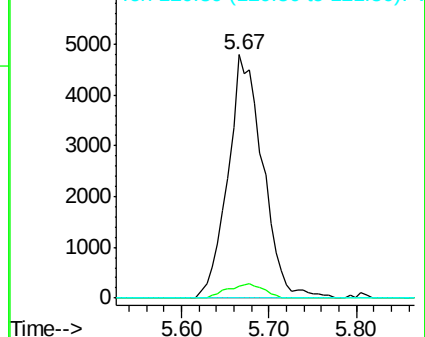



#44

Trichloroethene

Concen: 23.13 ug/l

RT: 7.22 min Scan# 1088

Delta R.T. 0.00 min

Lab File: VX001371.D

Acq: 03 May 2018 20:39

Instrument :

MSVOA_X

ClientSampleId :


GS-2-PAINT-CHIP-WIPES

Tgt Ion:130 Resp: 50584

Ion Ratio Lower Upper




130 100

95 85.3 0.0 176.0

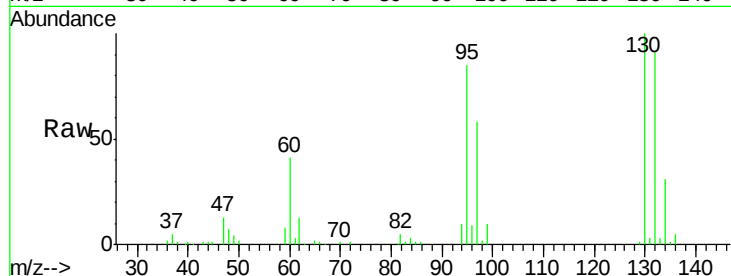

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

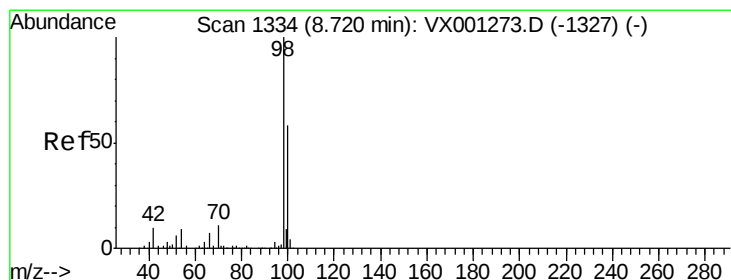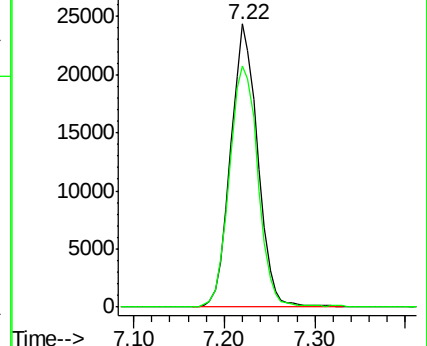

#50

Toluene-d8

Concen: 38.48 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. 0.00 min

Lab File: VX001371.D


Acq: 03 May 2018 20:39

Tgt Ion: 98 Resp: 254874

Ion Ratio Lower Upper



98 100


100 62.9 51.0 76.4



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

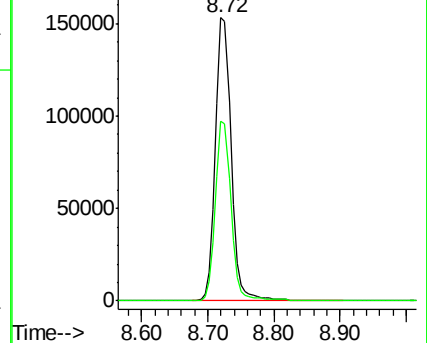



#51

4-Methyl-2-Pentanone

Concen: 0.47 ug/l

RT: 8.66 min Scan# 1325

Delta R.T. 0.01 min

Lab File: VX001371.D

Acq: 03 May 2018 20:39

Instrument :

MSVOA_X

ClientSampleId :


GS-2-PAINT-CHIP-WIPES

Tgt Ion: 43 Resp: 1219

Ion Ratio Lower Upper


43 100

58 35.2 29.0 43.6


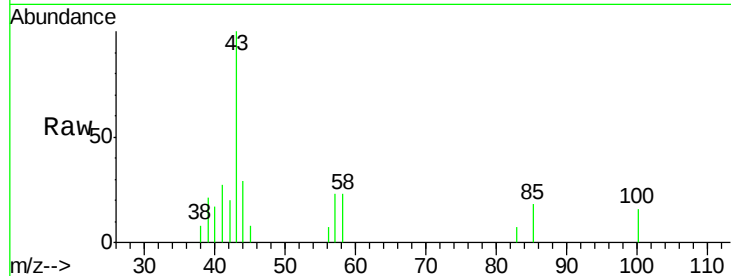


Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

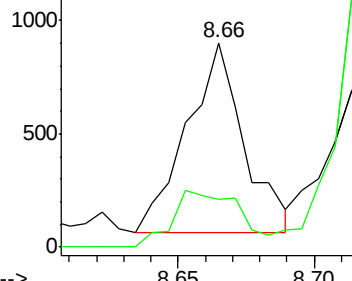

Time-->



#52

Toluene

Concen: 0.32 ug/l

RT: 8.79 min Scan# 1346

Delta R.T. 0.00 min

Lab File: VX001371.D


Acq: 03 May 2018 20:39

Tgt Ion: 92 Resp: 1508

Ion Ratio Lower Upper


92 100

91 166.5 139.0 208.6





Abundance Ion 92.00 (91.70 to 92.70): VX0

Ion 91.00 (90.70 to 91.70): VX0

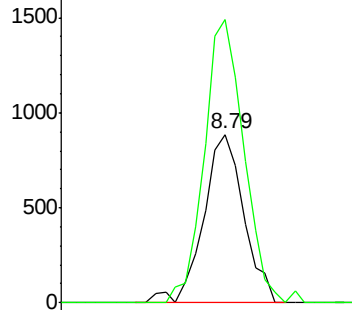

Time-->









#59
2-Hexanone
Concen: 0.70 ug/l
RT: 9.51 min Scan# 1464
Delta R.T. 0.01 min
Lab File: VX001371.D
Acq: 03 May 2018 20:39




Instrument :
MSVOA_X
ClientSampleId :
GS-2-PAINT-CHIP-WIPES


Tgt Ion: 43 Resp: 1425
Ion Ratio Lower Upper
43 100
58 51.8 25.7 77.0

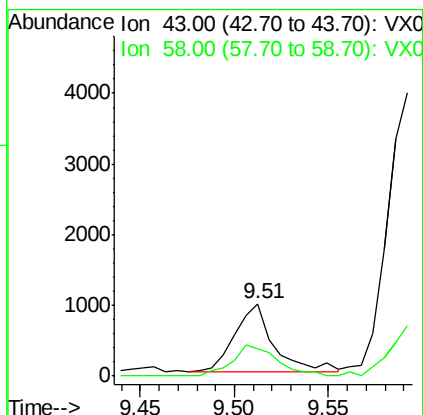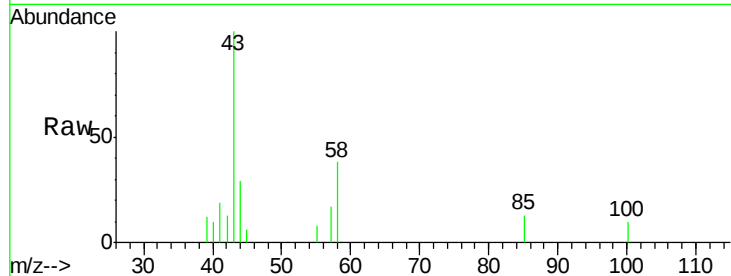

#62
4-Bromofluorobenzene
Concen: 32.46 ug/l
RT: 11.15 min Scan# 1732
Delta R.T. 0.01 min
Lab File: VX001371.D
Acq: 03 May 2018 20:39

Tgt Ion: 95 Resp: 85970
Ion Ratio Lower Upper
95 100
174 105.0 0.0 201.8
176 101.2 0.0 197.2

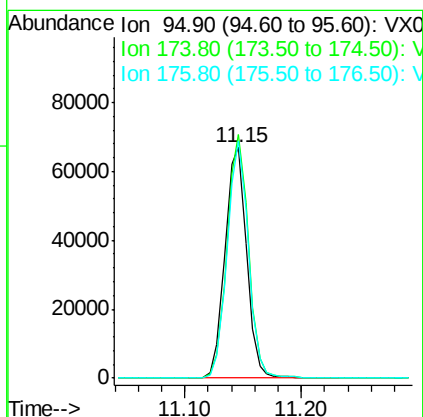







#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1564
Delta R.T. 0.01 min
Lab File: VX001371.D
Acq: 03 May 2018 20:39

Instrument :
MSVOA_X
ClientSampleId :
GS-2-PAINT-CHIP-WIPES

Tgt Ion: 117 Resp: 197891
Ion Ratio Lower Upper
117 100
82 50.2 41.4 62.0
119 31.9 25.5 38.3

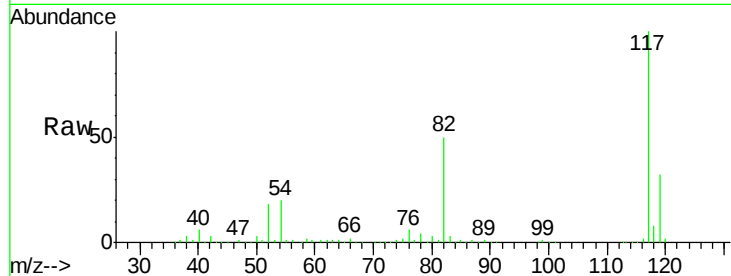


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V


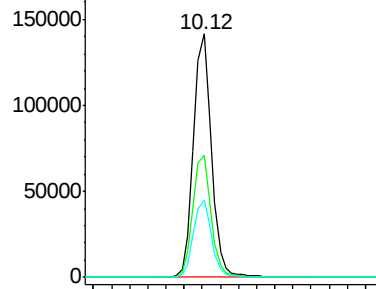



#67
Ethyl Benzene
Concen: 0.83 ug/l
RT: 10.26 min Scan# 1586
Delta R.T. 0.00 min
Lab File: VX001371.D
Acq: 03 May 2018 20:39

Tgt Ion: 91 Resp: 7322
Ion Ratio Lower Upper
91 100
106 37.8 24.9 37.3#



Abundance Ion 91.00 (90.70 to 91.70): VX0
Ion 106.00 (105.70 to 106.70): V

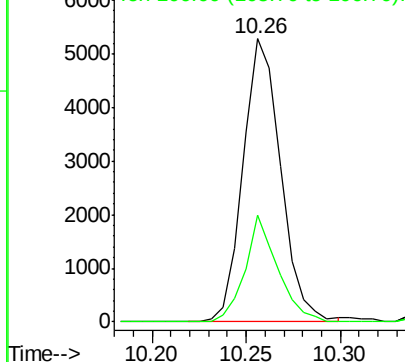







#68
m/p-Xylenes
Concen: 3.88 ug/l
RT: 10.37 min Scan# 1604
Delta R.T. 0.00 min
Lab File: VX001371.D
Acq: 03 May 2018 20:39

Instrument :
MSVOA_X
ClientSampleId :
GS-2-PAINT-CHIP-WIPES

Tgt Ion:106 Resp: 13543
Ion Ratio Lower Upper
106 100
91 191.5 159.4 239.2

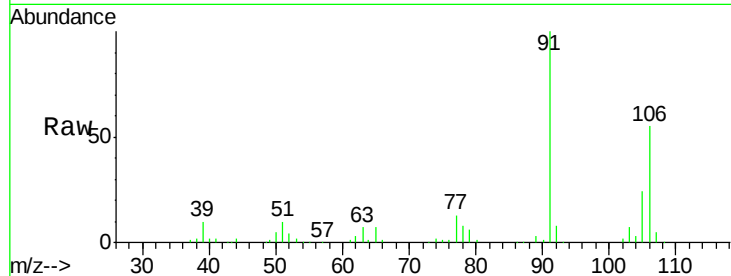


Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VX0


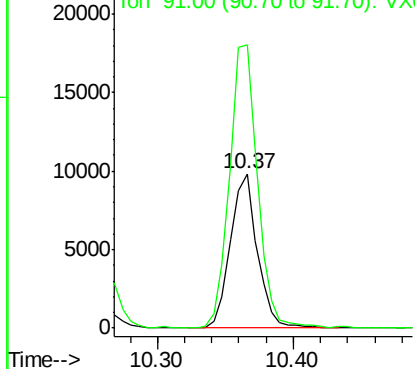



#69
o-Xylene
Concen: 1.89 ug/l
RT: 10.71 min Scan# 1660
Delta R.T. 0.01 min
Lab File: VX001371.D
Acq: 03 May 2018 20:39

Tgt Ion:106 Resp: 6387
Ion Ratio Lower Upper
106 100
91 213.7 106.3 319.0



Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VX0

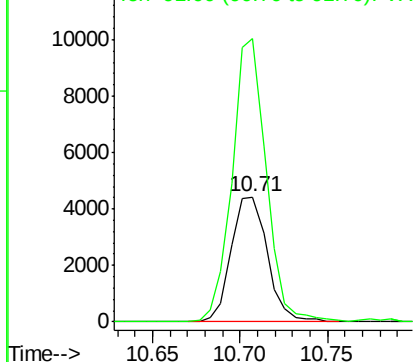

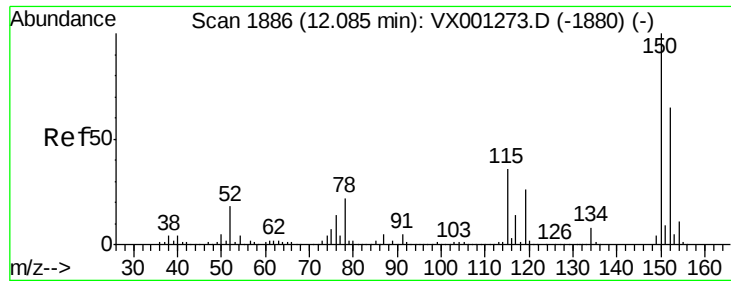

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.09 min Scan# 1886

Delta R.T. 0.00 min

Lab File: VX001371.D

Acq: 03 May 2018 20:39

Instrument :

MSVOA_X

ClientSampleId :

GS-2-PAINT-CHIP-WIPES


Tgt Ion:152 Resp: 102680

Ion Ratio Lower Upper

152 100

115 51.8 38.6 115.7




150 154.0 0.0 349.2

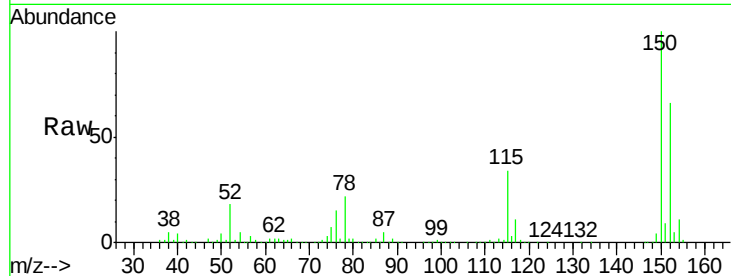

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

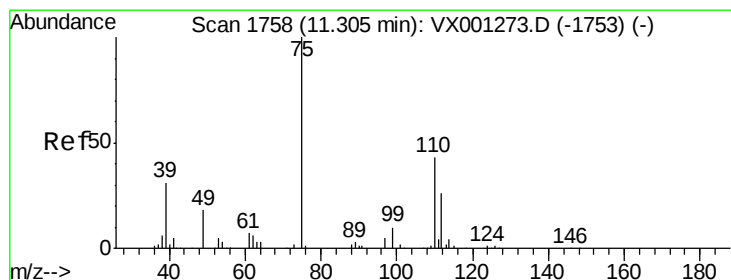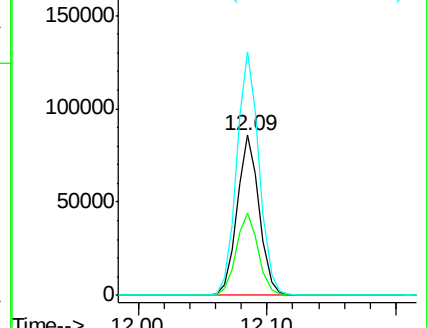

#76

1,2,3-Trichloropropane

Concen: 23.13 ug/l

RT: 11.15 min Scan# 1732

Delta R.T. -0.16 min

Lab File: VX001371.D


Acq: 03 May 2018 20:39

Tgt Ion: 75 Resp: 43911

Ion Ratio Lower Upper



75 100


77 1.7 18.9 56.5#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0




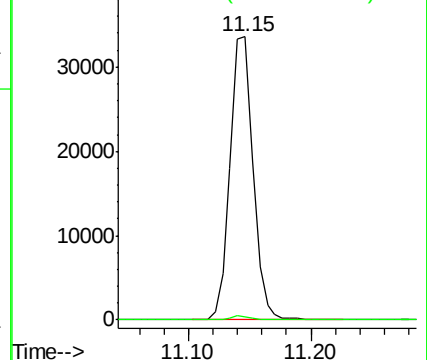




#81
 trans-1,4-Dichloro-2-butene
 Concen: 73.08 ug/l
 RT: 11.15 min Scan# 1732
 Delta R.T. 0.07 min
 Lab File: VX001371.D
 Acq: 03 May 2018 20:39

Instrument :
 MSVOA_X
 ClientSampleId :
 GS-2-PAINT-CHIP-WIPES

Tgt Ion: 75 Resp: 43911
 Ion Ratio Lower Upper
 75 100
 53 0.0 87.1 130.7#
 89 0.0 38.9 58.3#

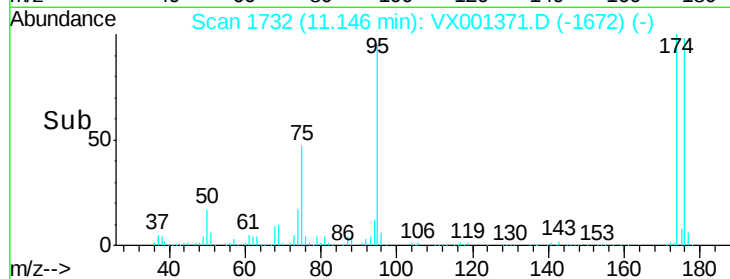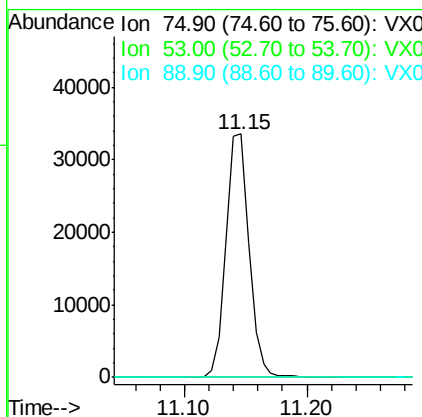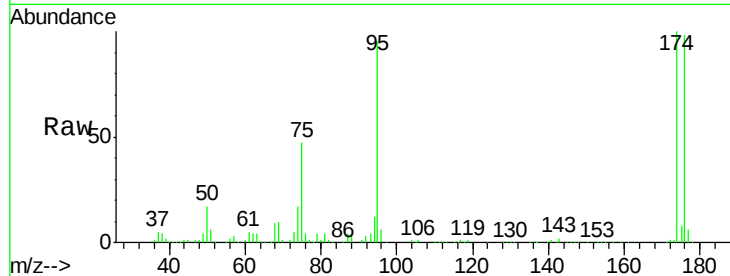

#95
 Naphthalene
 Concen: 11.04 ug/l
 RT: 13.84 min Scan# 2174
 Delta R.T. 0.00 min
 Lab File: VX001371.D
 Acq: 03 May 2018 20:39

Tgt Ion: 128 Resp: 82950
 Ion Ratio Lower Upper
 128 100
 127 13.0 10.5 15.7
 129 11.1 8.7 13.1

