


Data Path : W:\HPCHEM1\MSVOA X\DATA\VX050418\
 Data File : VX001389.D
 Acq On : 04 May 2018 09:57
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X050118W.M
 Title : SW846 8260
 Last Update : Wed May 02 01:48:25 2018

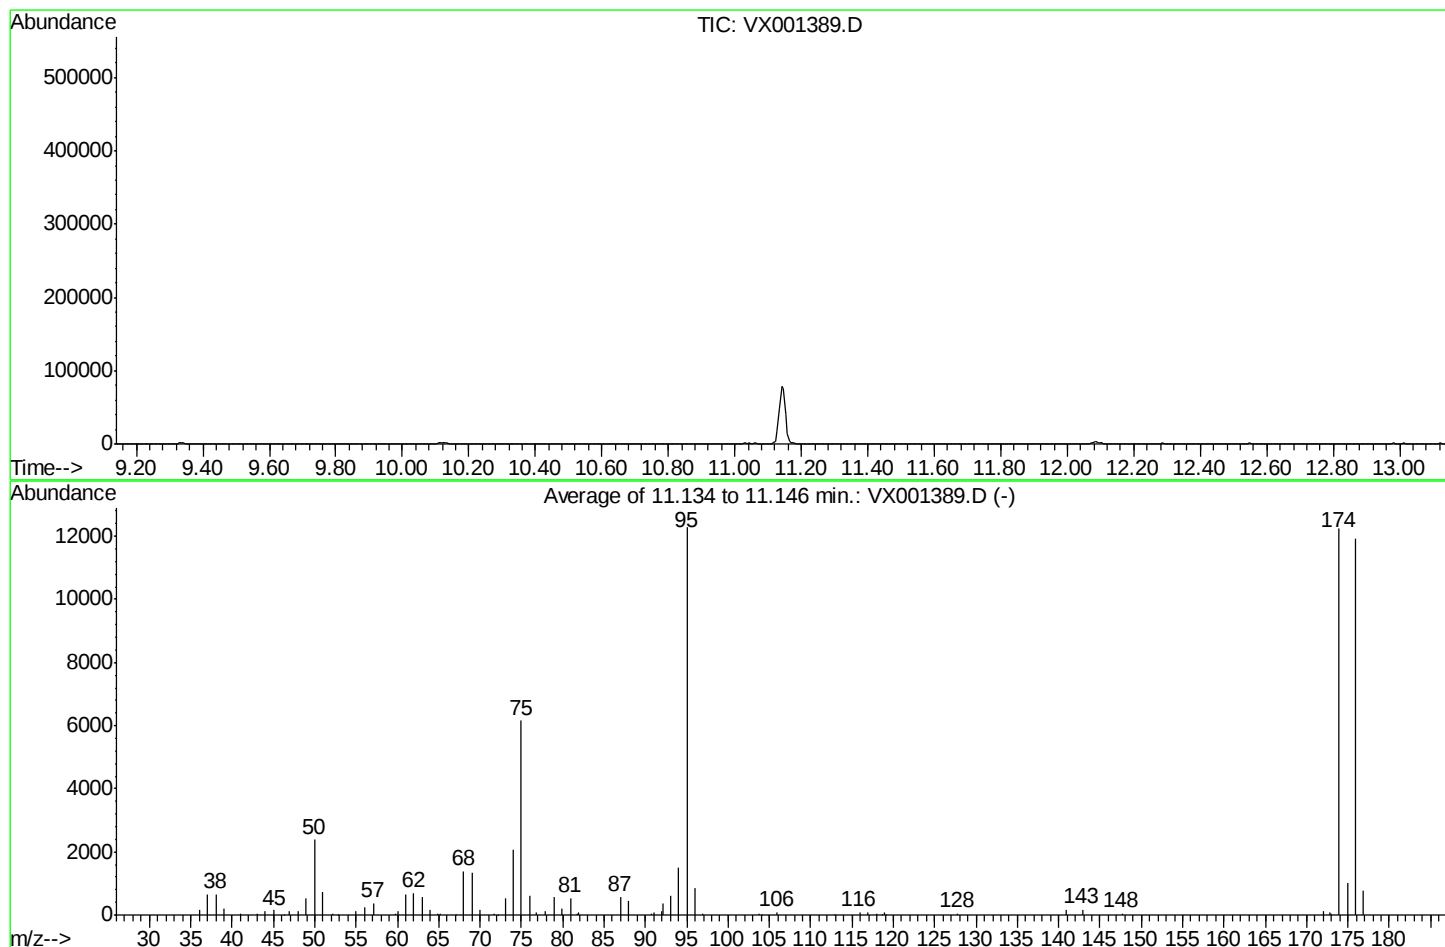

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	2377	PASS
75	95	30	60	50.1	6151	PASS
95	95	100	100	100.0	12284	PASS
96	95	5	9	7.0	858	PASS
173	174	0.00	2	0.8	97	PASS
174	95	50	100	99.8	12260	PASS
175	174	5	9	8.4	1029	PASS
176	174	95	101	97.1	11907	PASS
177	176	5	9	6.6	780	PASS