

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX050818\
 Data File : VX001534.D
 Acq On : 09 May 2018 01:08
 Operator : JC/MD
 Sample : J2671-04 5X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 AU-02-050718-B

Quant Time: May 09 07:52:10 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X050518W.M
 Quant Title : SW846 8260
 QLast Update : Sun May 06 07:59:25 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	244543	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	335810	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	294541	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	164790	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	166375	47.33	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.66%	
35) Dibromofluoromethane	5.51	113	128274	42.94	ug/l	0.00
Spiked Amount 50.000			Recovery	=	85.88%	
50) Toluene-d8	8.72	98	457616	41.97	ug/l	0.00
Spiked Amount 50.000			Recovery	=	83.94%	
62) 4-Bromofluorobenzene	11.14	95	151008	36.08	ug/l	0.00
Spiked Amount 50.000			Recovery	=	72.16%	
Target Compounds						
16) Acetone	2.45	43	6404	4.01	ug/l	98
18) Methyl Acetate	2.78	43	5892	1.41	ug/l	91
20) Methylene Chloride	2.86	84	3348	1.06	ug/l #	90
95) Naphthalene	13.84	128	117472	9.62	ug/l	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX050818\
Data File : VX001534.D
Acq On : 09 May 2018 01:08
Operator : JC/MD
Sample : J2671-04 5X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AU-02-050718-B

Quant Time: May 09 07:52:10 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X050518W.M
Quant Title : SW846 8260
QLast Update : Sun May 06 07:59:25 2018
Response via : Initial Calibration

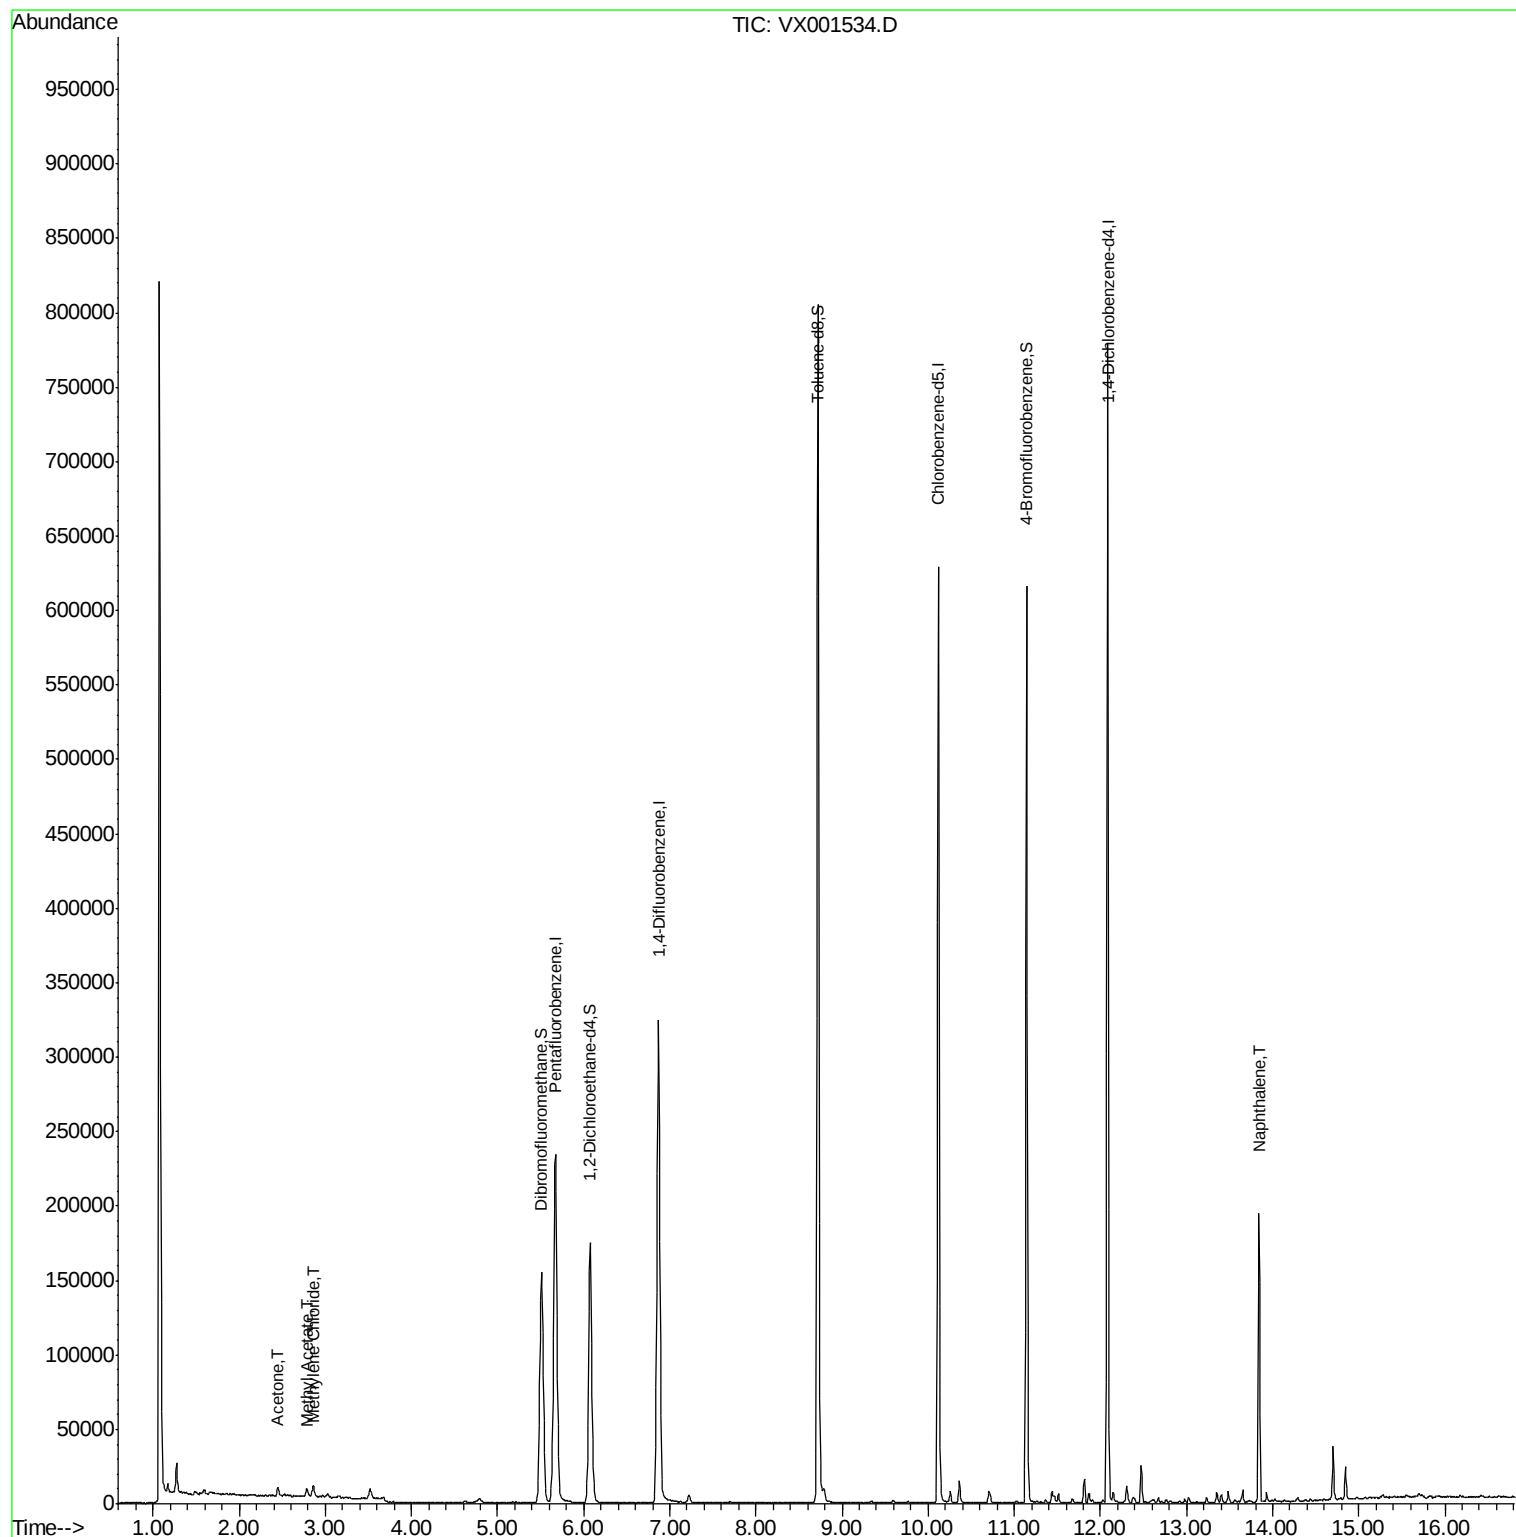



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. 0.00 min

Lab File: VX001534.D

Acq: 09 May 2018 01:08

Instrument :

MSVOA_X

ClientSampleId :


AU-02-050718-B

Tot Ion:168 Resp: 244543

Ion Ratio Lower Upper




168 100

99 46.9 36.6 54.8

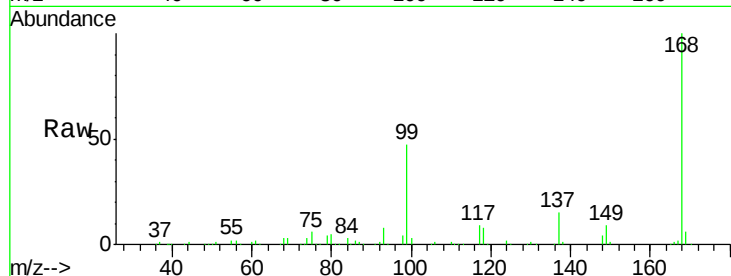

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

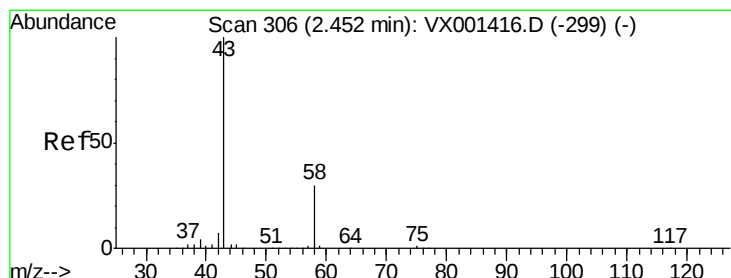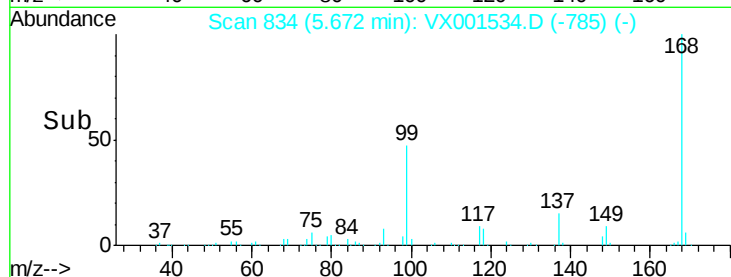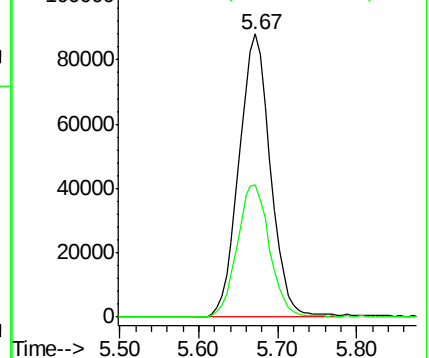

#16

Acetone

Concen: 4.01 ug/l

RT: 2.45 min Scan# 306

Delta R.T. 0.00 min

Lab File: VX001534.D


Acq: 09 May 2018 01:08

Tgt Ion: 43 Resp: 6404

Ion Ratio Lower Upper



43 100


58 28.5 23.8 35.8

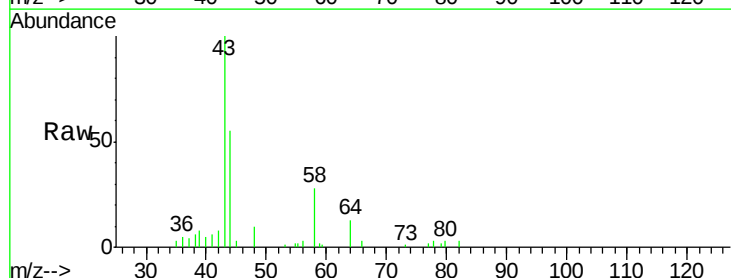

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0



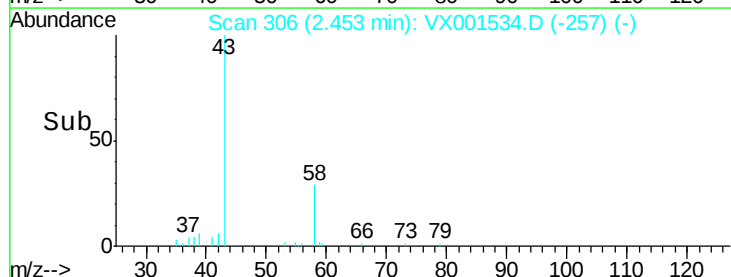
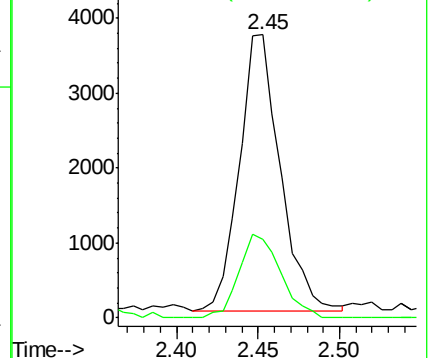


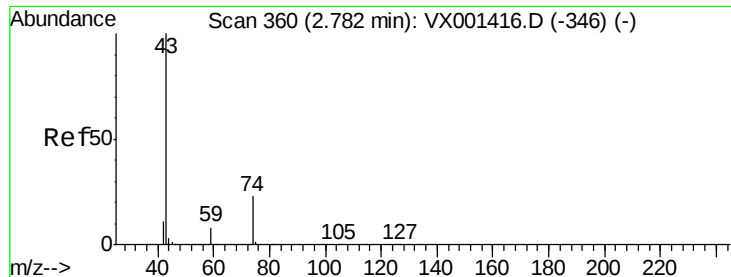

#18
Methvl Acetate
Concen: 1.41 ug/l
RT: 2.78 min Scan# 360
Delta R.T. 0.00 min
Lab File: VX001534.D
Acq: 09 May 2018 01:08




Instrument :
MSVOA_X
ClientSampleId :
AU-02-050718-B


Tot Ion: 43 Resp: 5892
Ion Ratio Lower Upper
43 100
74 27.6 18.6 27.8

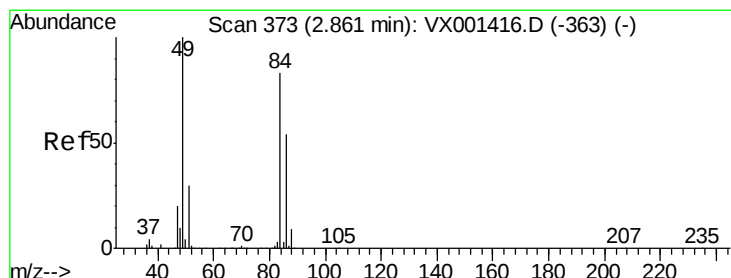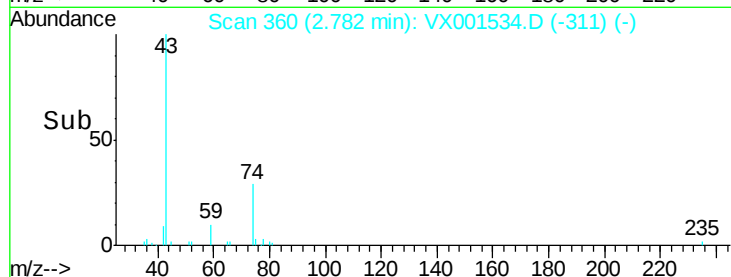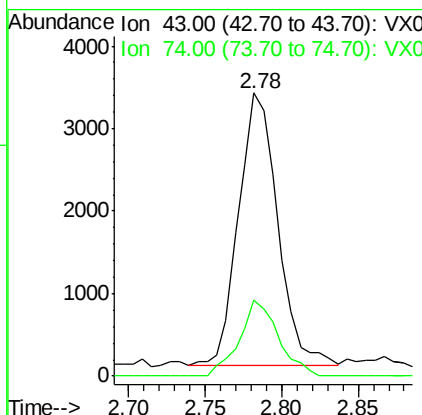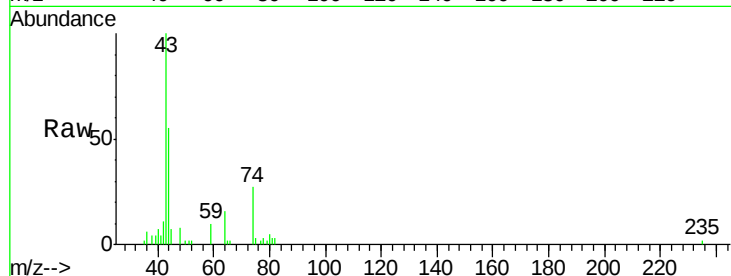

#20
Methylene Chloride
Concen: 1.06 ug/l
RT: 2.86 min Scan# 372
Delta R.T. -0.01 min
Lab File: VX001534.D
Acq: 09 May 2018 01:08

Tgt Ion: 84 Resp: 3348
Ion Ratio Lower Upper
84 100
49 112.1 96.6 144.8
51 43.8 29.0 43.4#
86 55.0 52.2 78.4

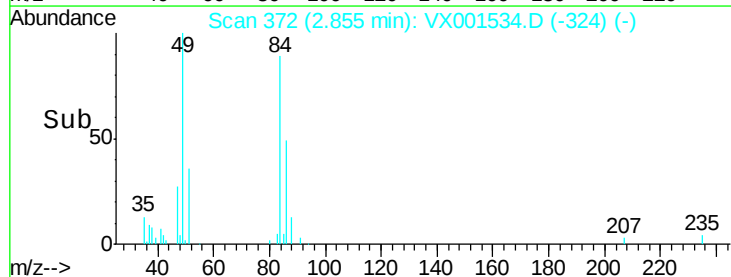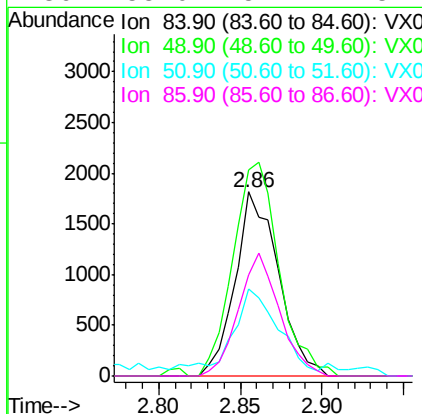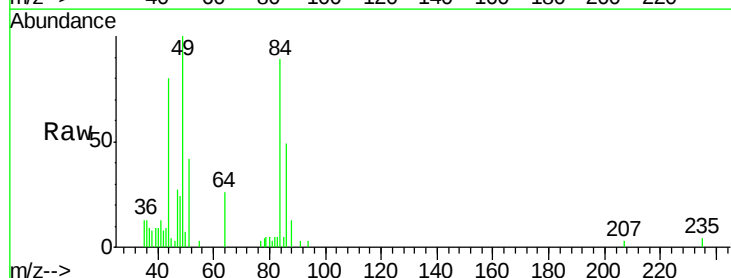

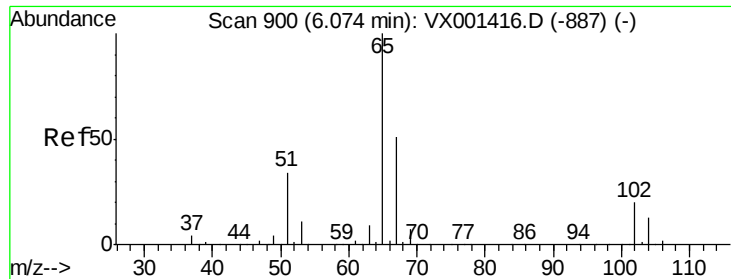

#33

1,2-Dichloroethane-d4

Concen: 47.33 ug/l

RT: 6.07 min Scan# 900

Delta R.T. 0.00 min

Lab File: VX001534.D

Acq: 09 May 2018 01:08

Instrument :

MSVOA_X

ClientSampleId :


AU-02-050718-B

Tot Ion: 65 Resp: 166375

Ion Ratio Lower Upper




65 100

67 50.4 0.0 101.8

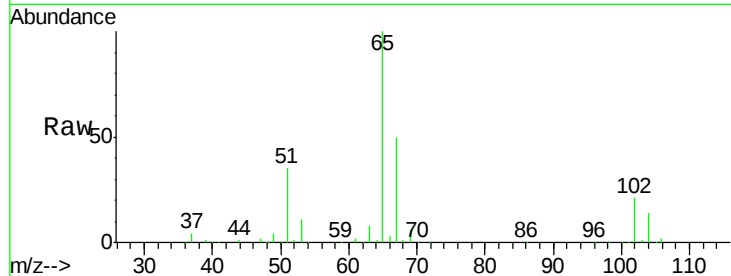

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

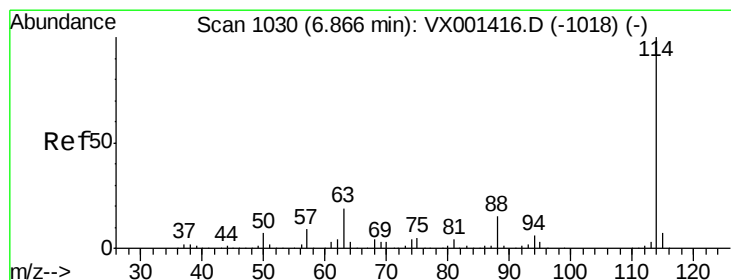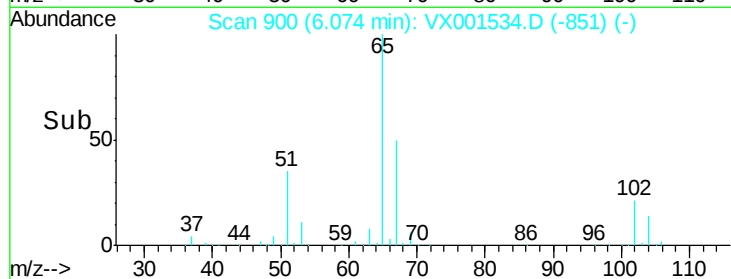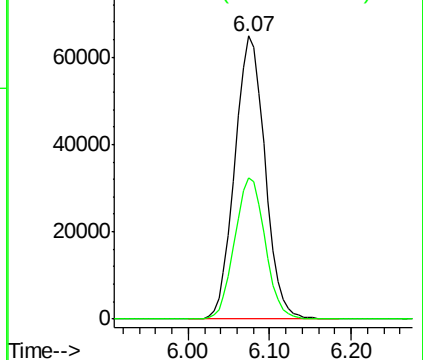

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. 0.00 min

Lab File: VX001534.D

Acq: 09 May 2018 01:08


Tgt Ion: 114 Resp: 335810

Ion Ratio Lower Upper

114 100

63 19.5 0.0 38.6



88 14.9 0.0 30.8

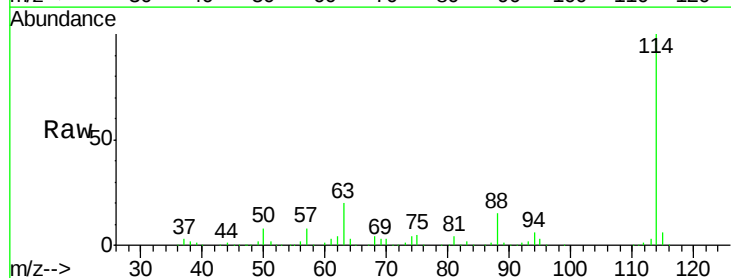


Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0



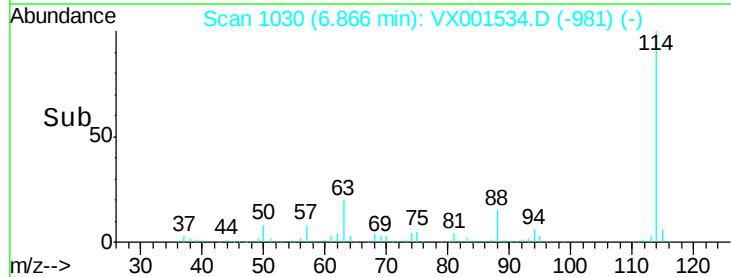
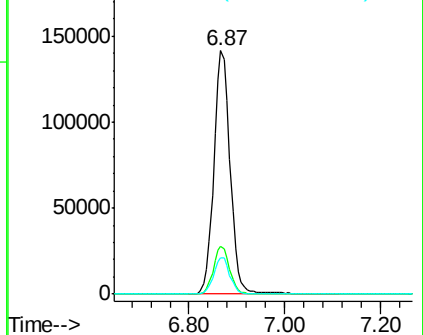


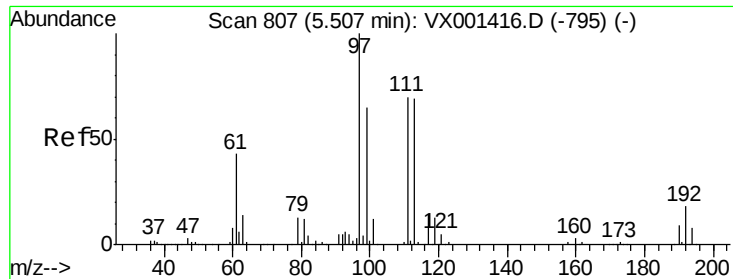

#35
 Dibromofluoromethane
 Concen: 42.94 ug/l
 RT: 5.51 min Scan# 807
 Delta R.T. 0.00 min
 Lab File: VX001534.D
 Acq: 09 May 2018 01:08




Instrument :
 MSVOA_X
 ClientSampleId :
 AU-02-050718-B


Tot Ion:113 Resp: 128274
 Ion Ratio Lower Upper
 113 100
 111 101.5 82.2 123.2
 192 26.4 21.4 32.0

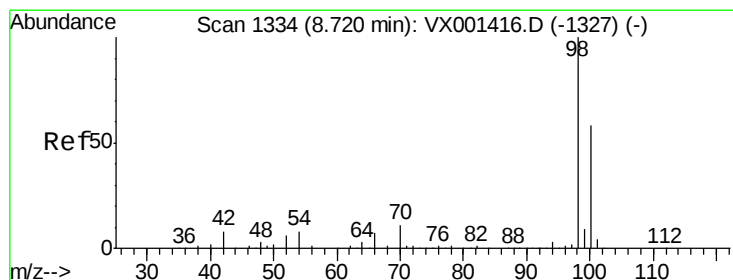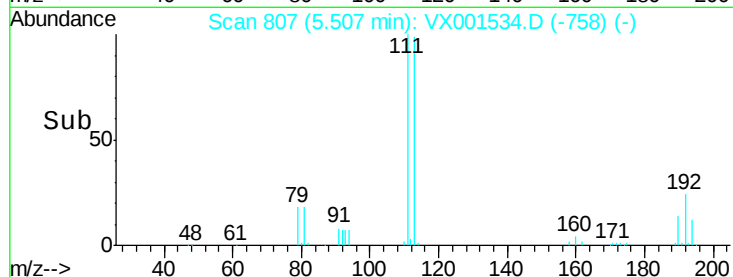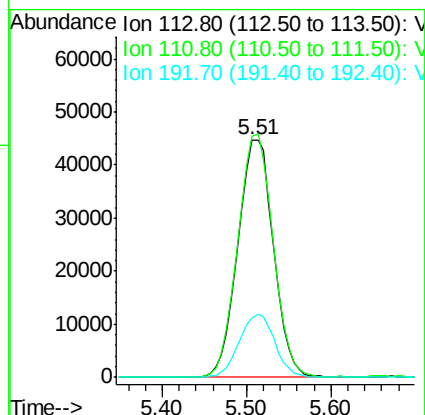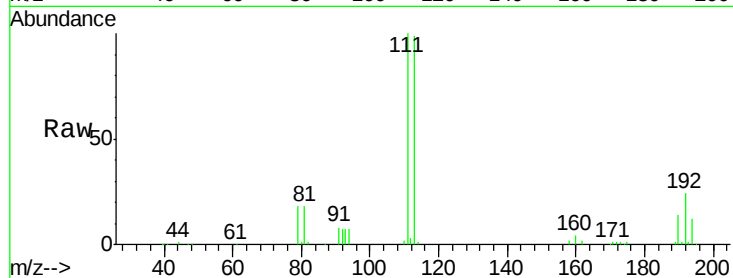

#50
 Toluene-d8
 Concen: 41.97 ug/l
 RT: 8.72 min Scan# 1334
 Delta R.T. 0.00 min
 Lab File: VX001534.D
 Acq: 09 May 2018 01:08

Tgt Ion: 98 Resp: 457616
 Ion Ratio Lower Upper
 98 100
 100 66.5 54.0 81.0


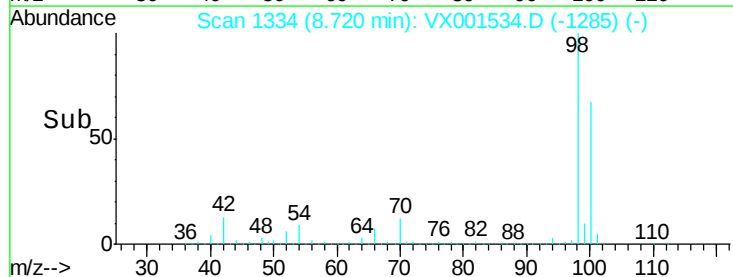
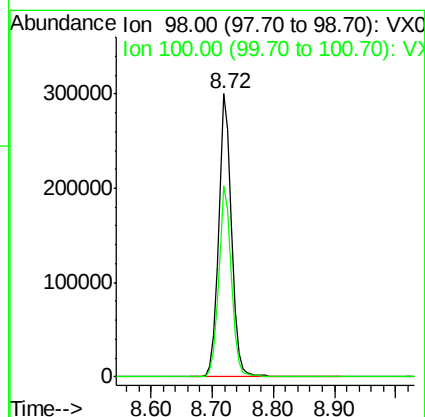
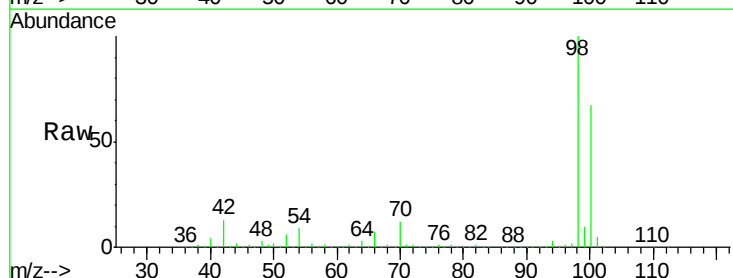


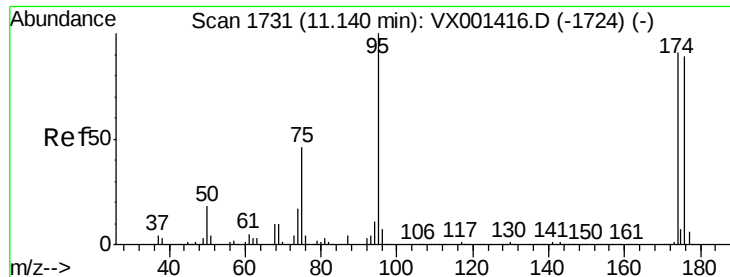

#62
4-Bromofluorobenzene
Concen: 36.08 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. 0.00 min
Lab File: VX001534.D
Acq: 09 May 2018 01:08




Instrument :
MSVOA_X
ClientSampleId :
AU-02-050718-B


Tot Ion: 95 Resp: 151008
Ion Ratio Lower Upper
95 100
174 102.3 0.0 202.0
176 98.5 0.0 197.4

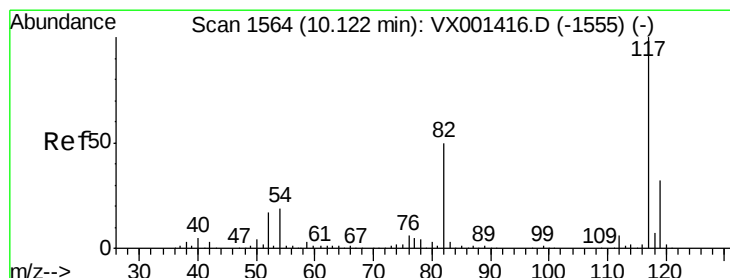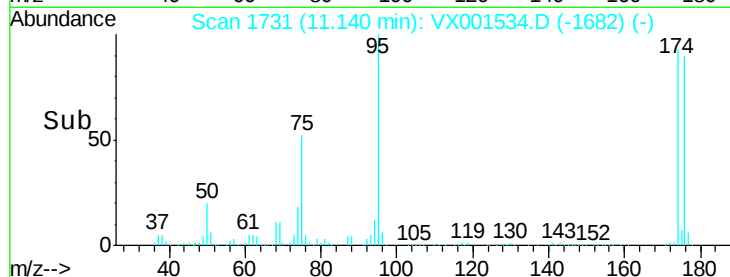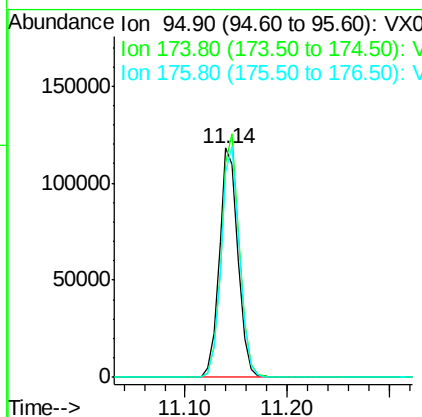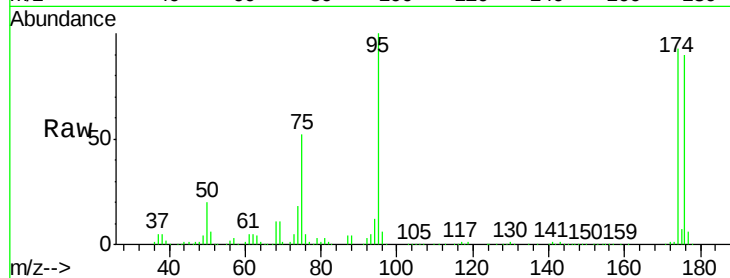

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. -0.01 min
Lab File: VX001534.D
Acq: 09 May 2018 01:08

Tgt Ion: 117 Resp: 294541
Ion Ratio Lower Upper
117 100
82 53.2 40.0 60.0
119 31.5 25.8 38.8

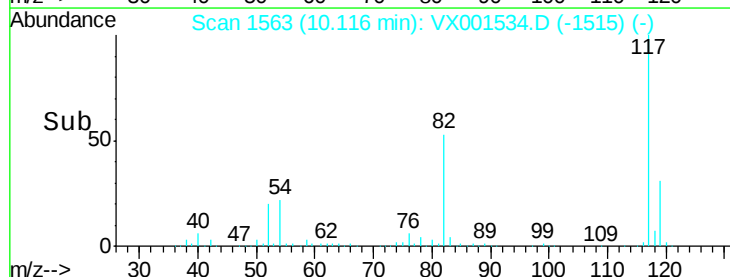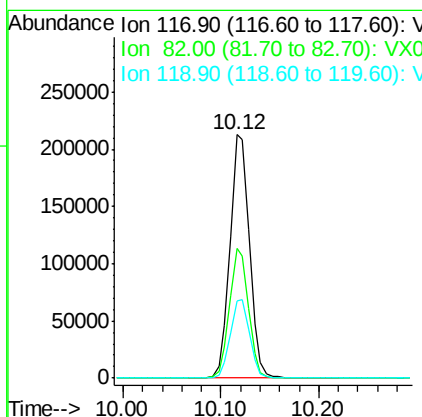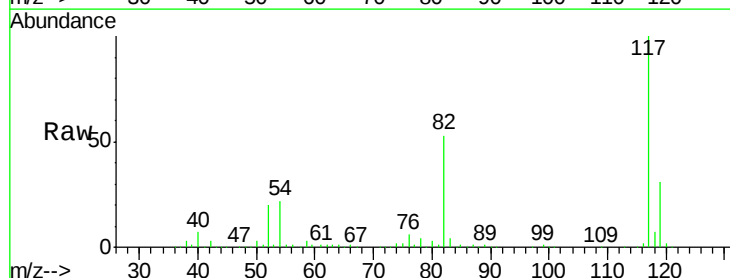

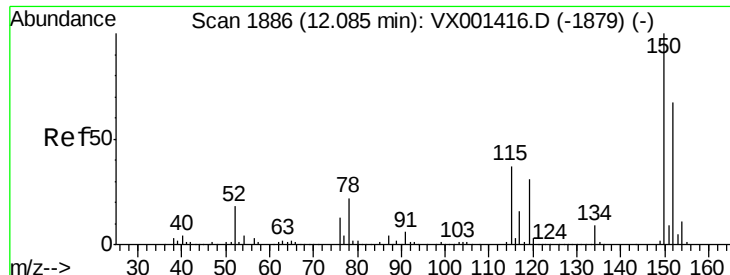

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.09 min Scan# 1886

Delta R.T. 0.00 min

Lab File: VX001534.D

Acq: 09 May 2018 01:08

Instrument :

MSVOA_X

ClientSampleId :

AU-02-050718-B


Tot Ion:152 Resp: 164790

Ion Ratio Lower Upper

152 100

115 53.0 37.7 113.1




150 156.4 0.0 349.4

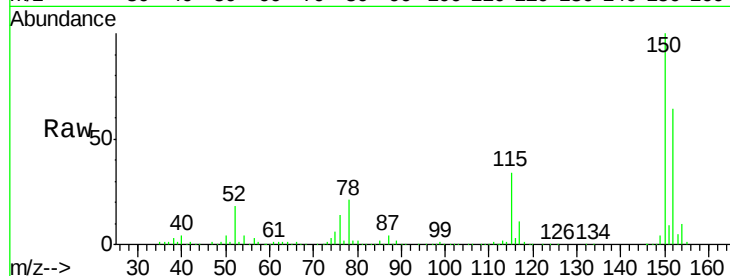

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

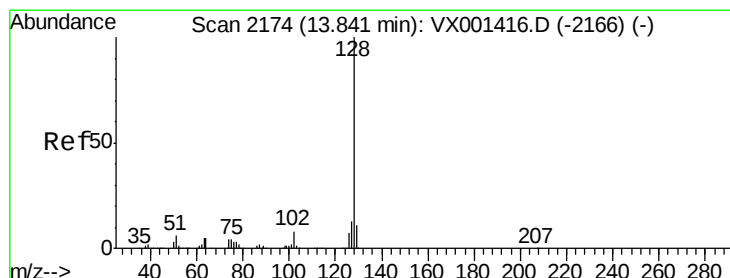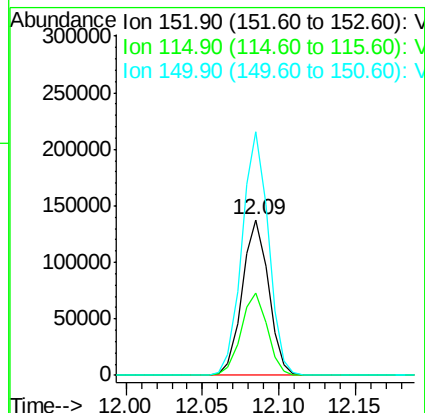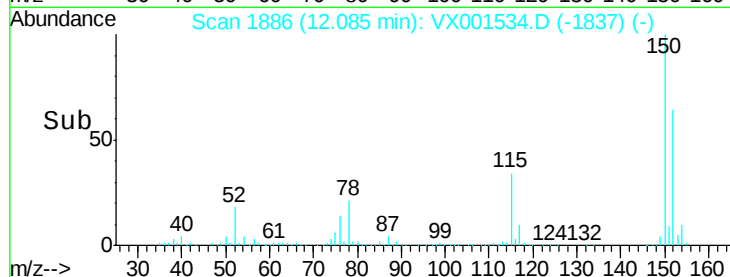

#95

Naphthalene

Concen: 9.62 ug/l

RT: 13.84 min Scan# 2174

Delta R.T. 0.00 min

Lab File: VX001534.D

Acq: 09 May 2018 01:08


Tgt Ion:128 Resp: 117472

Ion Ratio Lower Upper

128 100

127 13.1 10.4 15.6

129 11.0 8.7 13.1

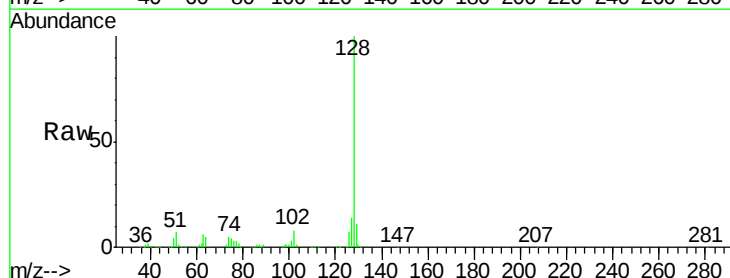

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

