


Data Path : W:\HPCHEM1\MSVOA X\Data\VX050818\
 Data File : VX001503.D
 Acq On : 08 May 2018 09:41
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X050518W.M
 Title : SW846 8260
 Last Update : Sun May 06 07:59:25 2018

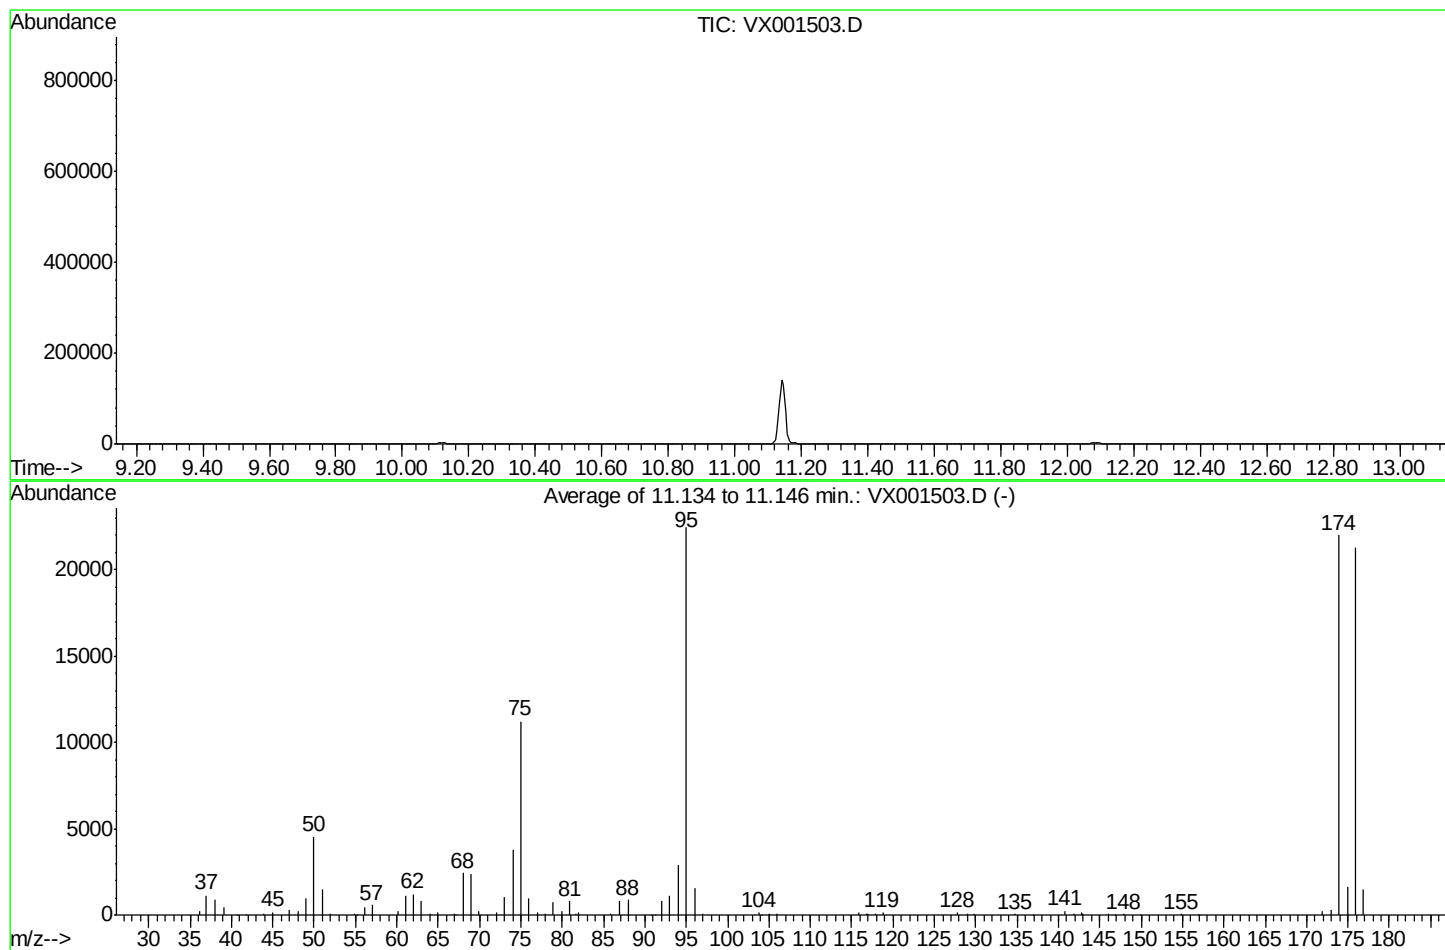

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	4547	PASS
75	95	30	60	49.9	11217	PASS
95	95	100	100	100.0	22458	PASS
96	95	5	9	6.8	1525	PASS
173	174	0.00	2	1.5	334	PASS
174	95	50	100	98.0	21999	PASS
175	174	5	9	7.6	1664	PASS
176	174	95	101	96.6	21251	PASS
177	176	5	9	7.1	1502	PASS