


Data Path : W:\HPCHEM1\MSVOA X\Data\VX050818\
Data File : VX001528.D
Acq On : 08 May 2018 22:01
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X050518W.M
Title : SW846 8260
Last Update : Sun May 06 07:59:25 2018

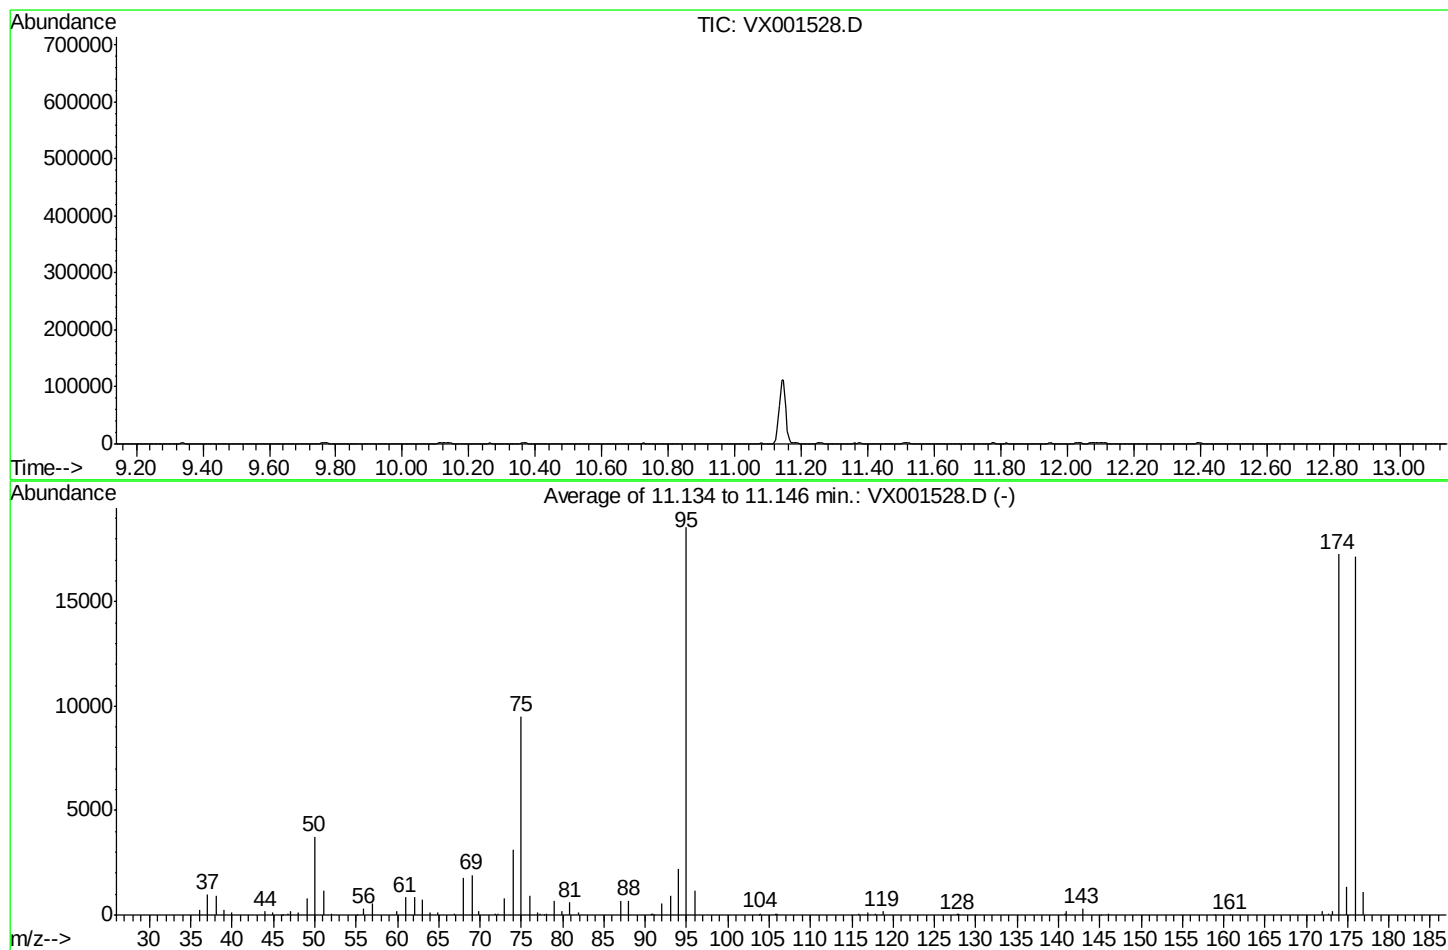

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	3742	PASS
75	95	30	60	51.1	9477	PASS
95	95	100	100	100.0	18558	PASS
96	95	5	9	6.4	1183	PASS
173	174	0.00	2	1.2	200	PASS
174	95	50	100	93.1	17271	PASS
175	174	5	9	7.9	1367	PASS
176	174	95	101	99.5	17184	PASS
177	176	5	9	6.4	1100	PASS