

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX050918\
 Data File : VX001583.D
 Acq On : 10 May 2018 04:14
 Operator : JC/MD
 Sample : J2649-06
 Misc : 5.61g/5mL/100ul/5mL/MSVOA_X/MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-3

Quant Time: May 10 05:41:39 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X050518W.M
 Quant Title : SW846 8260
 QLast Update : Sun May 06 07:59:25 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	239756	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	331116	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	301223	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	177906	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	158513	46.00	ug/l	0.00
Spiked Amount			Recovery	=	92.00%	
35) Dibromofluoromethane	5.51	113	118967	40.39	ug/l	0.00
Spiked Amount			Recovery	=	80.78%	
50) Toluene-d8	8.72	98	462257	43.00	ug/l	0.00
Spiked Amount			Recovery	=	86.00%	
62) 4-Bromofluorobenzene	11.15	95	159406	38.63	ug/l	0.00
Spiked Amount			Recovery	=	77.26%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
64) Tetrachloroethene	9.34	164	5235	1.25	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX050918\
Data File : VX001583.D
Acq On : 10 May 2018 04:14
Operator : JC/MD
Sample : J2649-06
Misc : 5.61q/5mL/100ul/5mL/MSVOA_X/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-3

Quant Time: May 10 05:41:39 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X050518W.M
Quant Title : SW846 8260
QLast Update : Sun May 06 07:59:25 2018
Response via : Initial Calibration

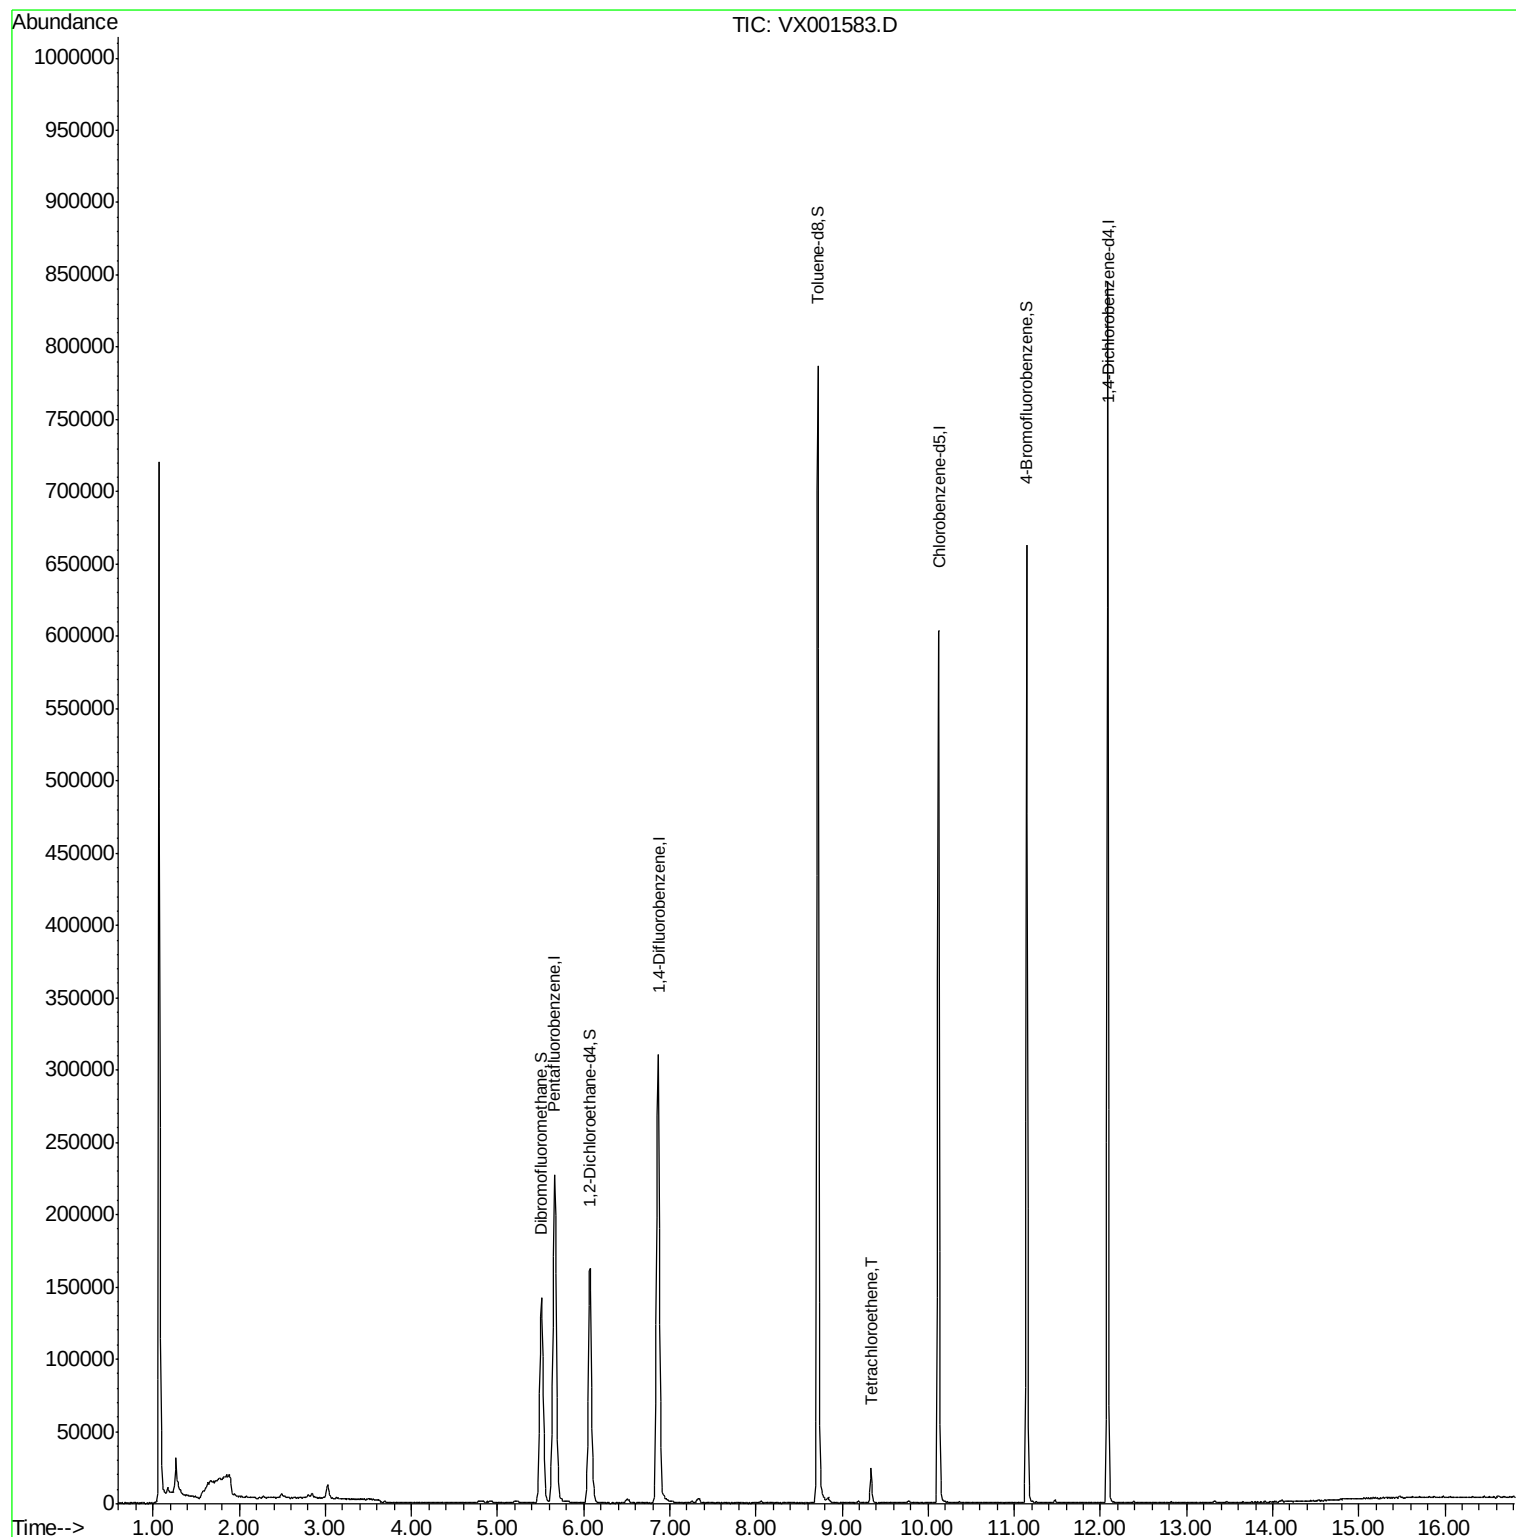

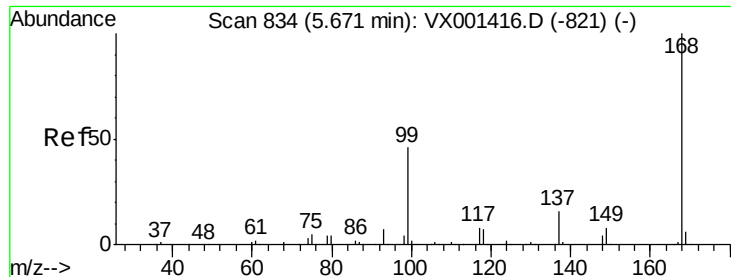

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.01 min

Lab File: VX001583.D

Acq: 10 May 2018 04:14

Instrument :

MSVOA_X

ClientSampled :


SB-3

Tot Ion:168 Resp: 239756

Ion Ratio Lower Upper

168 100

99 47.6 36.6 54.8

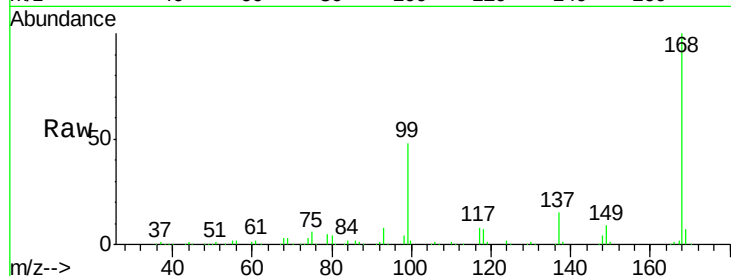

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

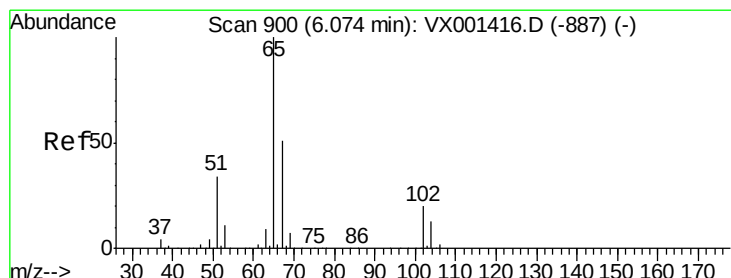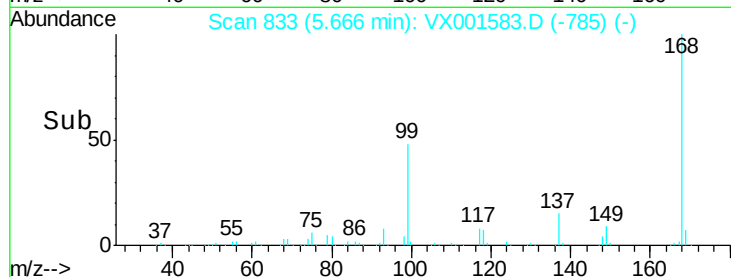

#33

1,2-Dichloroethane-d4

Concen: 46.00 ug/l

RT: 6.07 min Scan# 899

Delta R.T. -0.01 min

Lab File: VX001583.D


Acq: 10 May 2018 04:14

Tgt Ion: 65 Resp: 158513

Ion Ratio Lower Upper

65 100

67 50.8 0.0 101.8

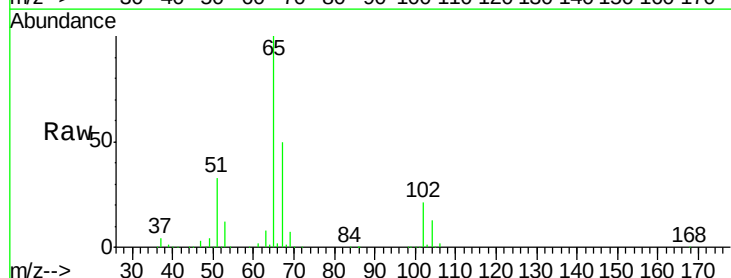

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07


60000


40000

20000

0

Time--> 5.90 6.00 6.10 6.20

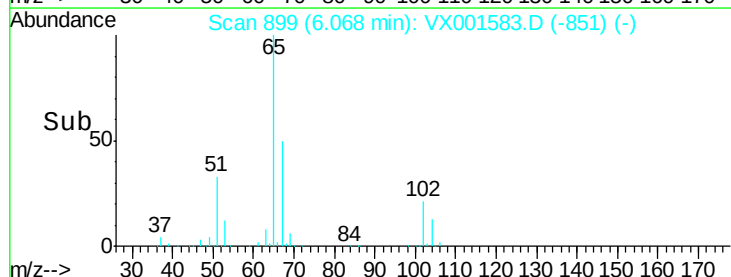

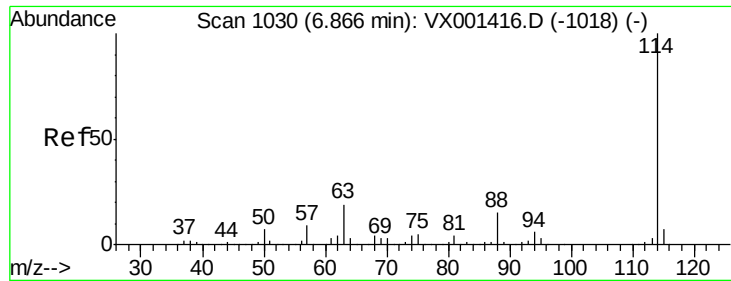

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. 0.00 min

Lab File: VX001583.D

Acq: 10 May 2018 04:14

Instrument :

MSVOA_X

ClientSampleId :

SB-3


Tot Ion:114 Resp: 331116

Ion Ratio Lower Upper

114 100

63 19.2 0.0 38.6




88 14.9 0.0 30.8

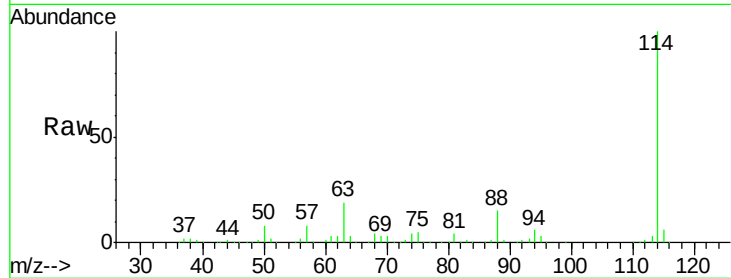

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

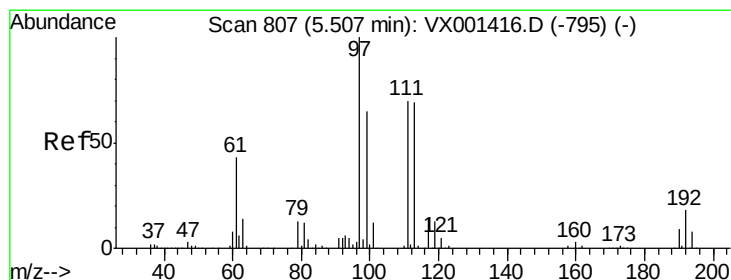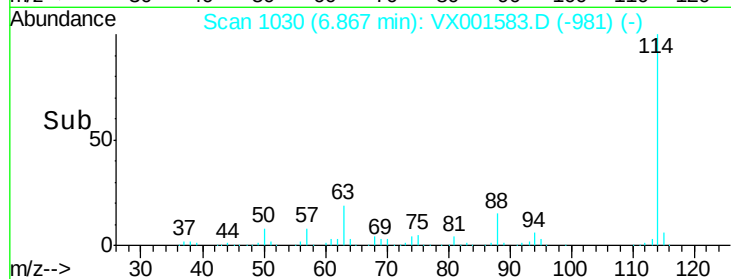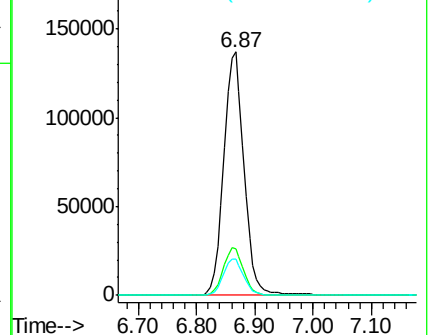

#35

Dibromofluoromethane

Concen: 40.39 ug/l

RT: 5.51 min Scan# 807

Delta R.T. 0.00 min

Lab File: VX001583.D

Acq: 10 May 2018 04:14


Tgt Ion:113 Resp: 118967

Ion Ratio Lower Upper

113 100

111 101.5 82.2 123.2



192 26.0 21.4 32.0

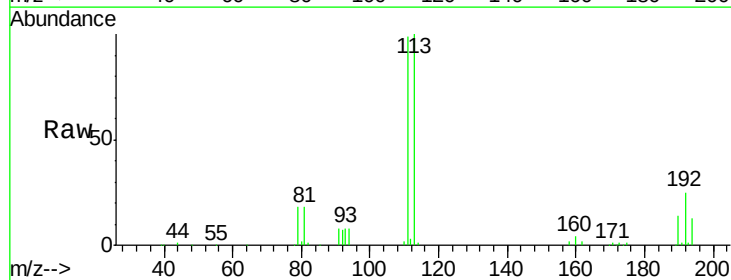


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

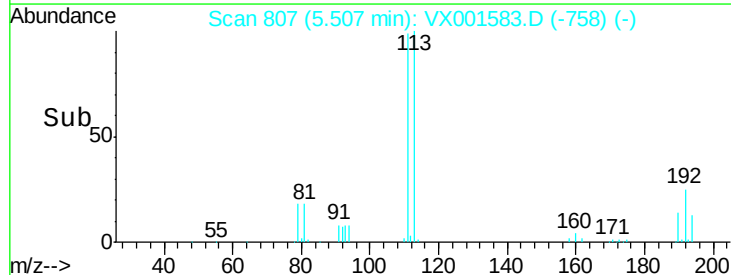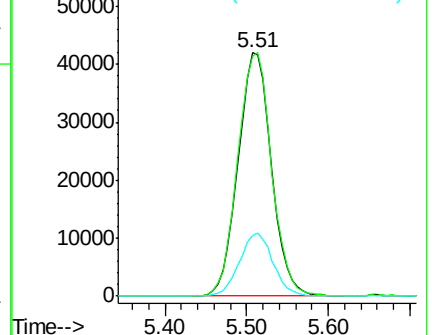

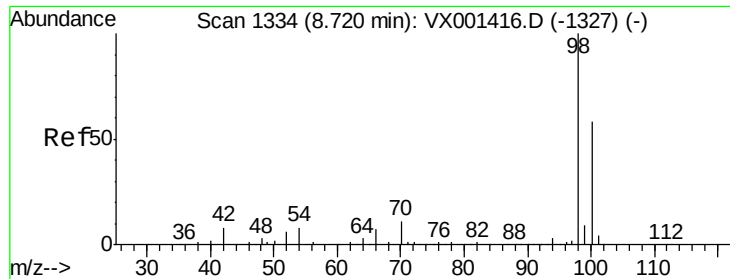

#50

Toluene-d8

Concen: 43.00 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. 0.00 min

Lab File: VX001583.D

Acq: 10 May 2018 04:14

Instrument :

MSVOA_X

ClientSampleId :


SB-3

Tot Ion: 98 Resp: 462257

Ion Ratio Lower Upper




98 100

100 65.4 54.0 81.0

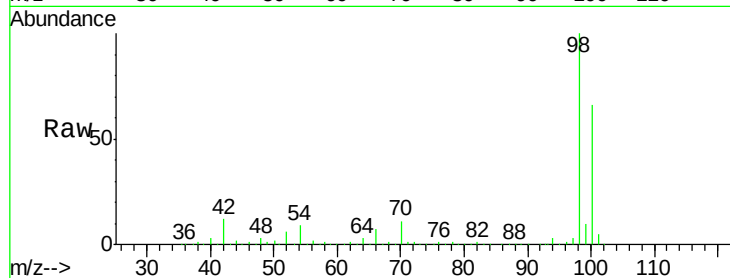

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

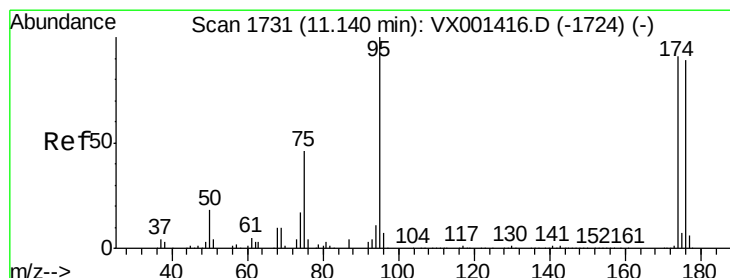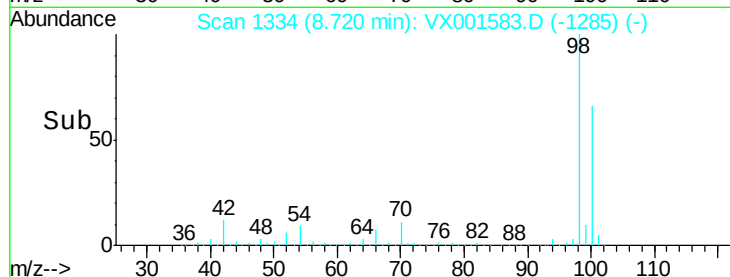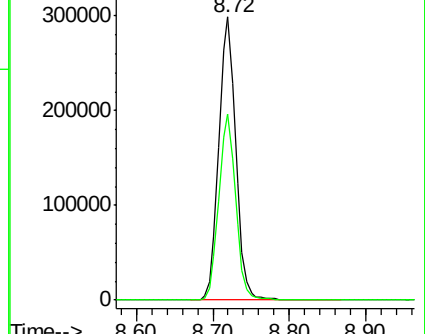

#62

4-Bromofluorobenzene

Concen: 38.63 ug/l

RT: 11.15 min Scan# 1732

Delta R.T. 0.01 min

Lab File: VX001583.D

Acq: 10 May 2018 04:14


Tgt Ion: 95 Resp: 159406

Ion Ratio Lower Upper

95 100

174 100.0 0.0 202.0



176 98.8 0.0 197.4

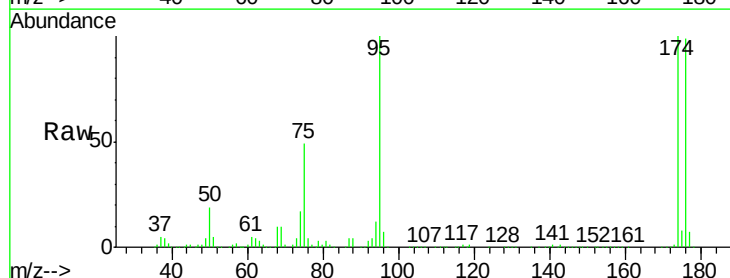


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

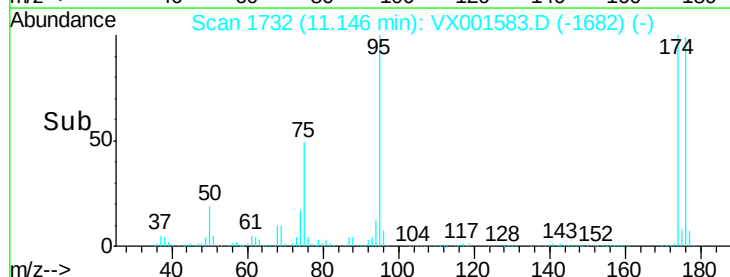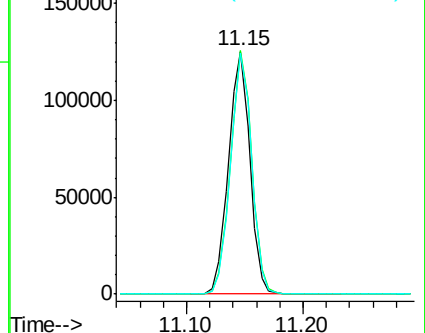


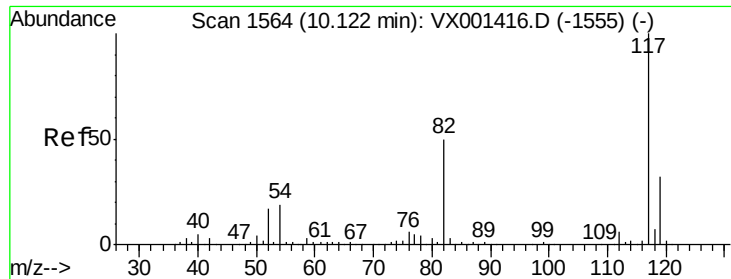




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1564
Delta R.T. 0.00 min
Lab File: VX001583.D
Acq: 10 May 2018 04:14

Instrument :
MSVOA_X
ClientSampled :
SB-3

Tot Ion:117 Resp: 301223
Ion Ratio Lower Upper
117 100
82 50.9 40.0 60.0
119 31.9 25.8 38.8

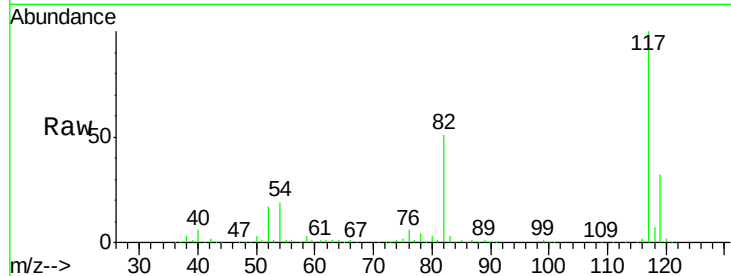


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

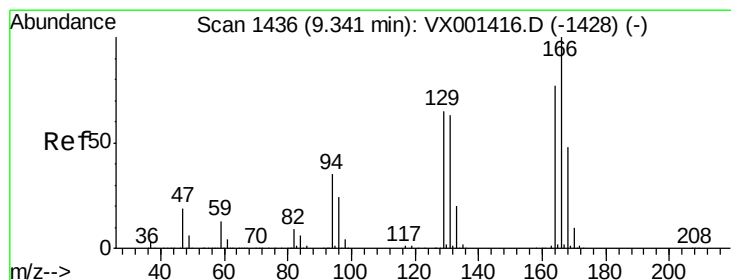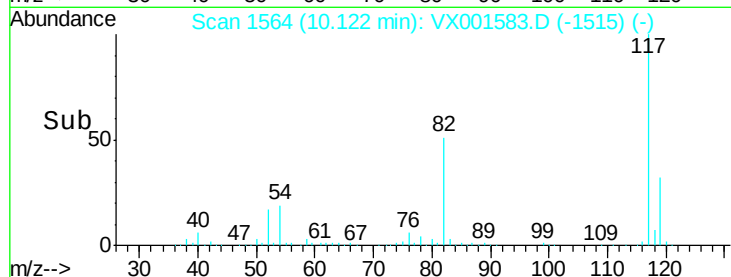
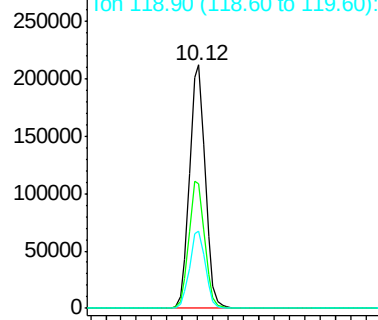



#64
Tetrachloroethene
Concen: 1.25 ug/l
RT: 9.34 min Scan# 1435
Delta R.T. -0.01 min
Lab File: VX001583.D
Acq: 10 May 2018 04:14

Tgt Ion:164 Resp: 5235
Ion Ratio Lower Upper
164 100
166 135.8 103.5 155.3
129 77.2 66.7 100.1
131 82.7 64.9 97.3

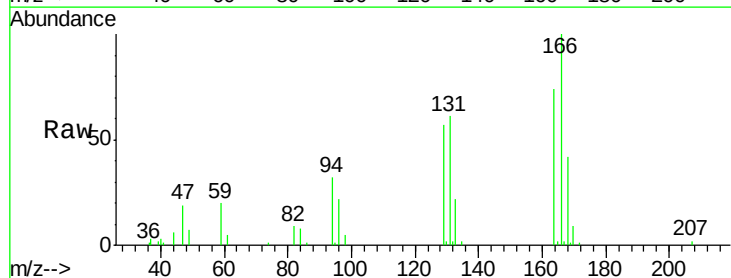

Abundance Ion 163.80 (163.50 to 164.50): V
Ion 165.80 (165.50 to 166.50): V
Ion 128.80 (128.50 to 129.50): V
Ion 130.80 (130.50 to 131.50): V

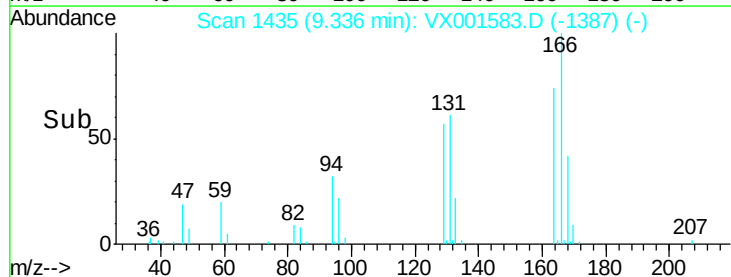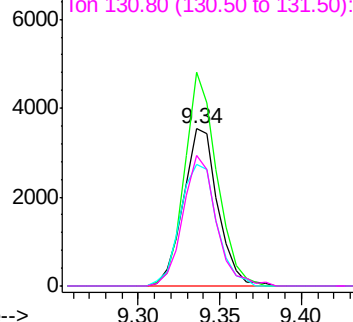

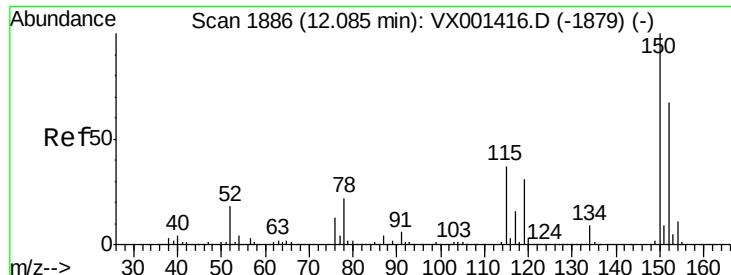

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.00 ug/l
 RT: 12.09 min Scan# 1886
 Delta R.T. 0.00 min
 Lab File: VX001583.D
 Acq: 10 May 2018 04:14

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-3

Tot Ion	Ratio	Lower	Upper
152	100		
115	52.8	37.7	113.1
150	154.9	0.0	349.4

