


Data Path : W:\HPCHEM1\MSVOA X\Data\VX050918\
 Data File : VX001552.D
 Acq On : 09 May 2018 12:29
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\624X043018W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue May 01 09:17:40 2018

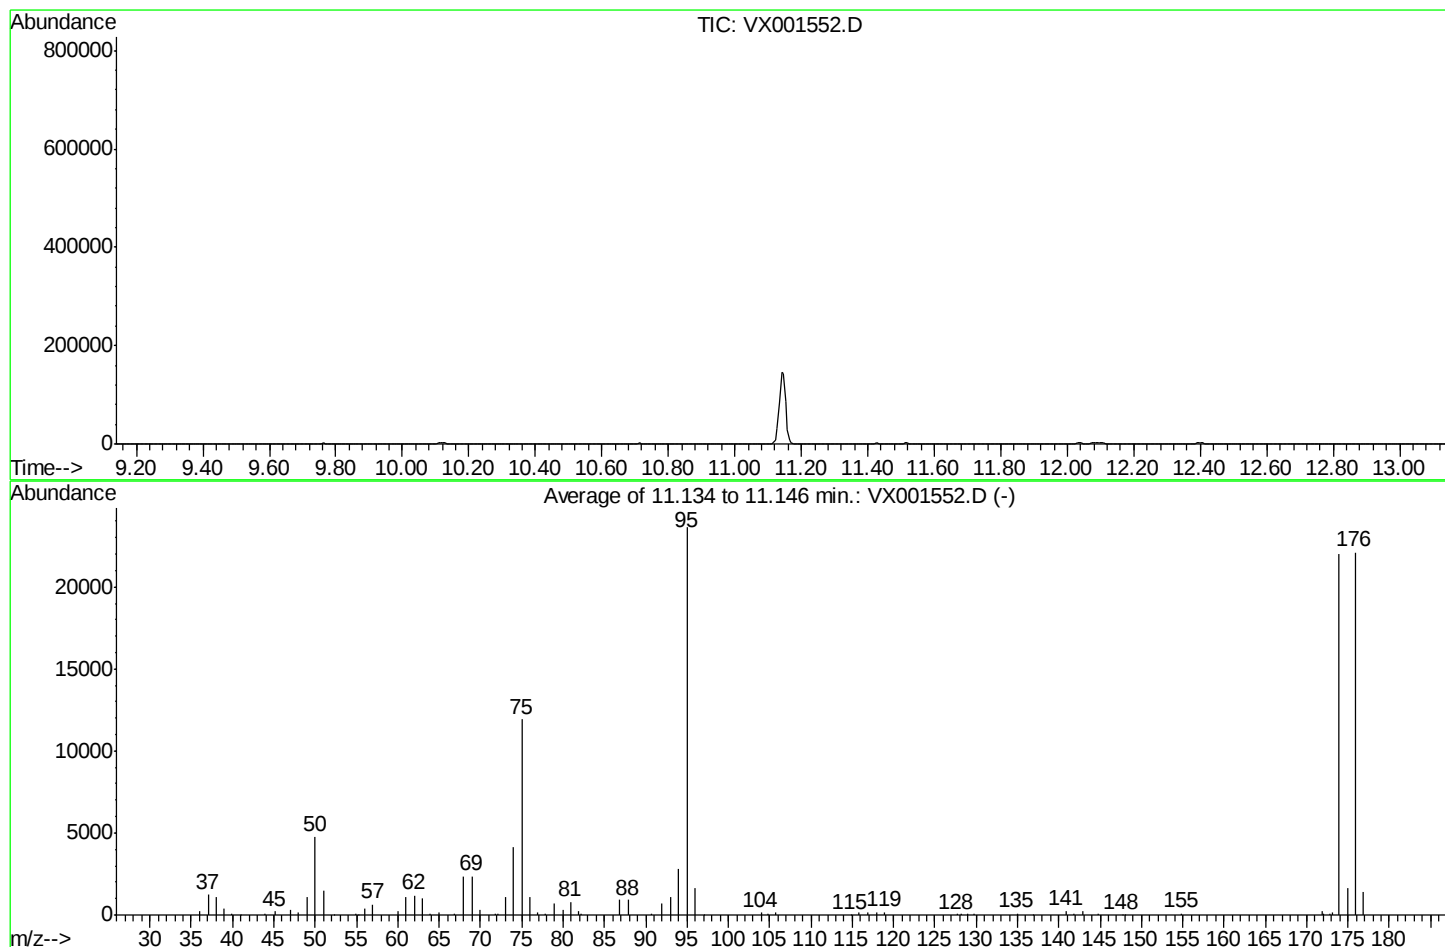

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	4762	PASS
75	95	30	60	50.5	11925	PASS
95	95	100	100	100.0	23629	PASS
96	95	5	9	7.0	1652	PASS
173	174	0.00	2	0.9	197	PASS
174	95	50	100	93.1	21989	PASS
175	174	5	9	7.5	1654	PASS
176	174	95	101	100.4	22081	PASS
177	176	5	9	6.2	1377	PASS