


Data Path : W:\HPCHEM1\MSVOA X\DATA\VX050918\
Data File : VX001572.D
Acq On : 09 May 2018 23:20
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X050518W.M
Title : SW846 8260
Last Update : Sun May 06 07:59:25 2018

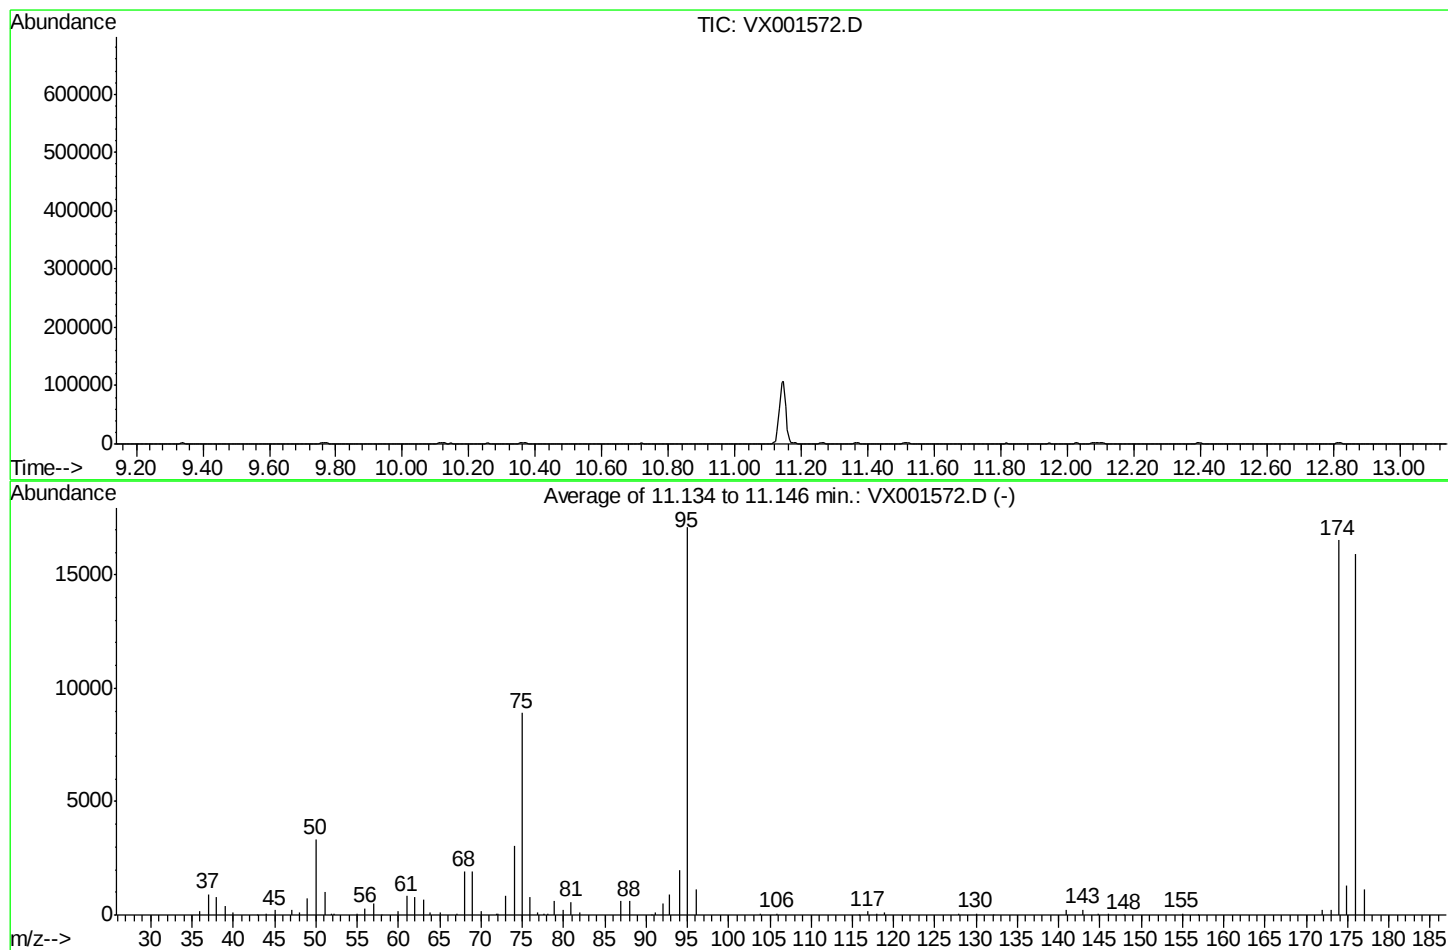

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	3327	PASS
75	95	30	60	52.1	8905	PASS
95	95	100	100	100.0	17098	PASS
96	95	5	9	6.5	1114	PASS
173	174	0.00	2	1.4	232	PASS
174	95	50	100	96.7	16526	PASS
175	174	5	9	7.8	1287	PASS
176	174	95	101	96.4	15939	PASS
177	176	5	9	7.1	1124	PASS