


Data Path : W:\HPCHEM1\MSVOA X\Data\VX051118\
Data File : VX001617.D
Acq On : 10 May 2018 22:09
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\624X051118W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri May 11 07:16:13 2018

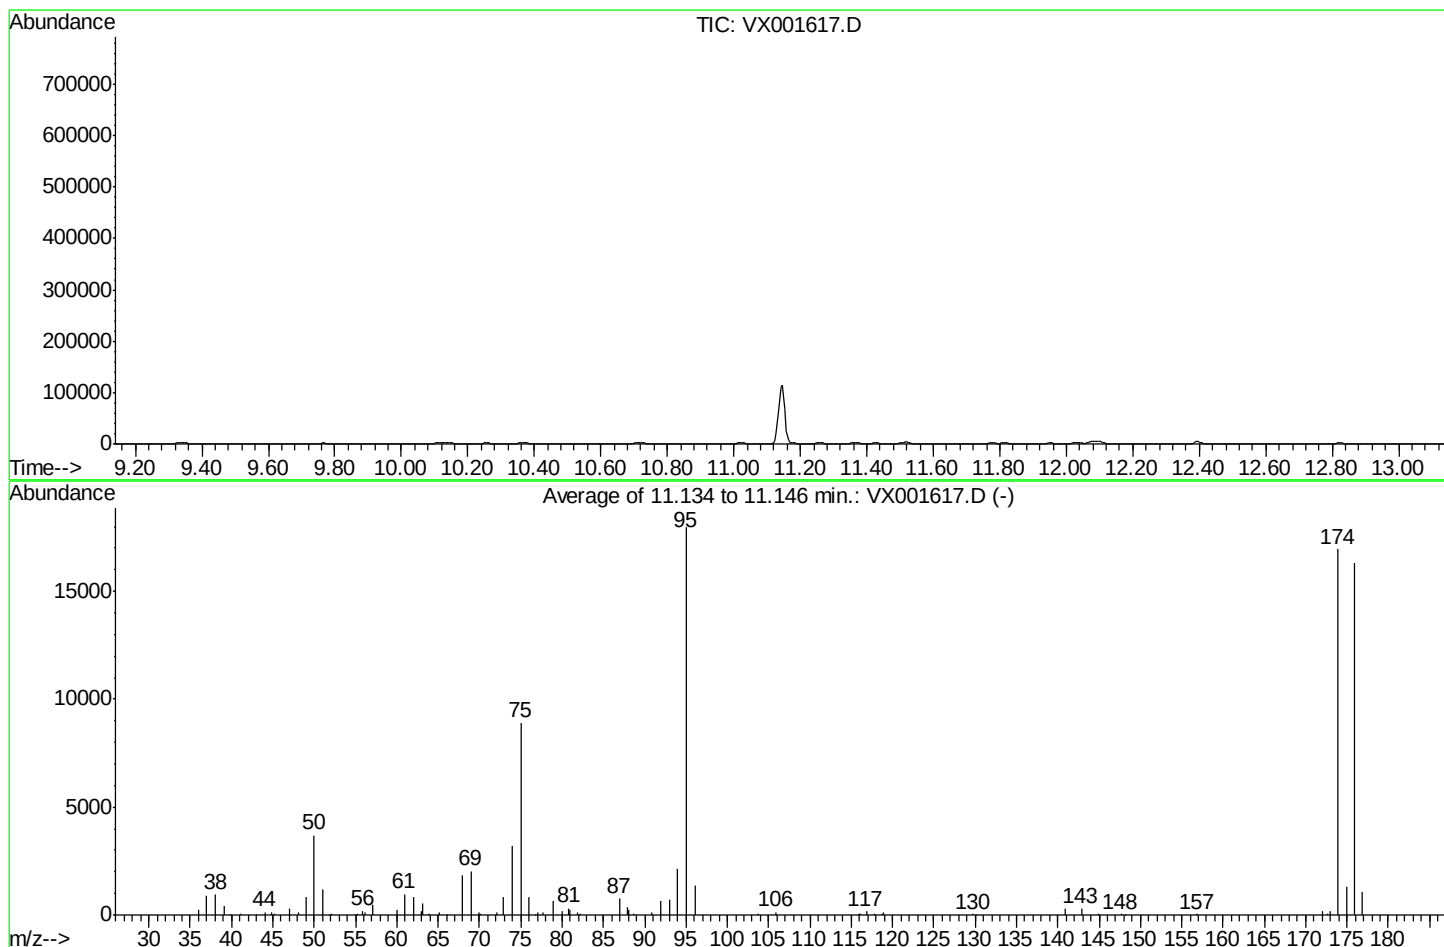

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	3686	PASS
75	95	30	60	49.6	8904	PASS
95	95	100	100	100.0	17962	PASS
96	95	5	9	7.7	1386	PASS
173	174	0.00	2	1.2	201	PASS
174	95	50	100	94.4	16952	PASS
175	174	5	9	7.7	1304	PASS
176	174	95	101	96.3	16319	PASS
177	176	5	9	6.7	1087	PASS