

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX051218\
 Data File : VX001694.D
 Acq On : 13 May 2018 03:47
 Operator : JC/MD
 Sample : PB109200ZHE#10
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB109200ZHE#10

Quant Time: May 14 07:52:21 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X050518W.M
 Quant Title : SW846 8260
 QLast Update : Sun May 06 07:59:25 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	267237	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	365802	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	317061	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	171097	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	176450	45.94	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.88%	
35) Dibromofluoromethane	5.51	113	142944	43.93	ug/l	0.00
Spiked Amount 50.000			Recovery	=	87.86%	
50) Toluene-d8	8.72	98	506800	42.67	ug/l	0.00
Spiked Amount 50.000			Recovery	=	85.34%	
62) 4-Bromofluorobenzene	11.14	95	158595	34.79	ug/l	0.00
Spiked Amount 50.000			Recovery	=	69.58%	
Target Compounds						
16) Acetone	2.45	43	7727	4.43	ug/l	95
18) Methyl Acetate	2.78	43	22668	4.95	ug/l	100
20) Methylene Chloride	2.86	84	2659	0.77	ug/l	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX051218\
Data File : VX001694.D
Acq On : 13 May 2018 03:47
Operator : JC/MD
Sample : PB109200ZHE#10
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB109200ZHE#10

Quant Time: May 14 07:52:21 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X050518W.M
Quant Title : SW846 8260
QLast Update : Sun May 06 07:59:25 2018
Response via : Initial Calibration

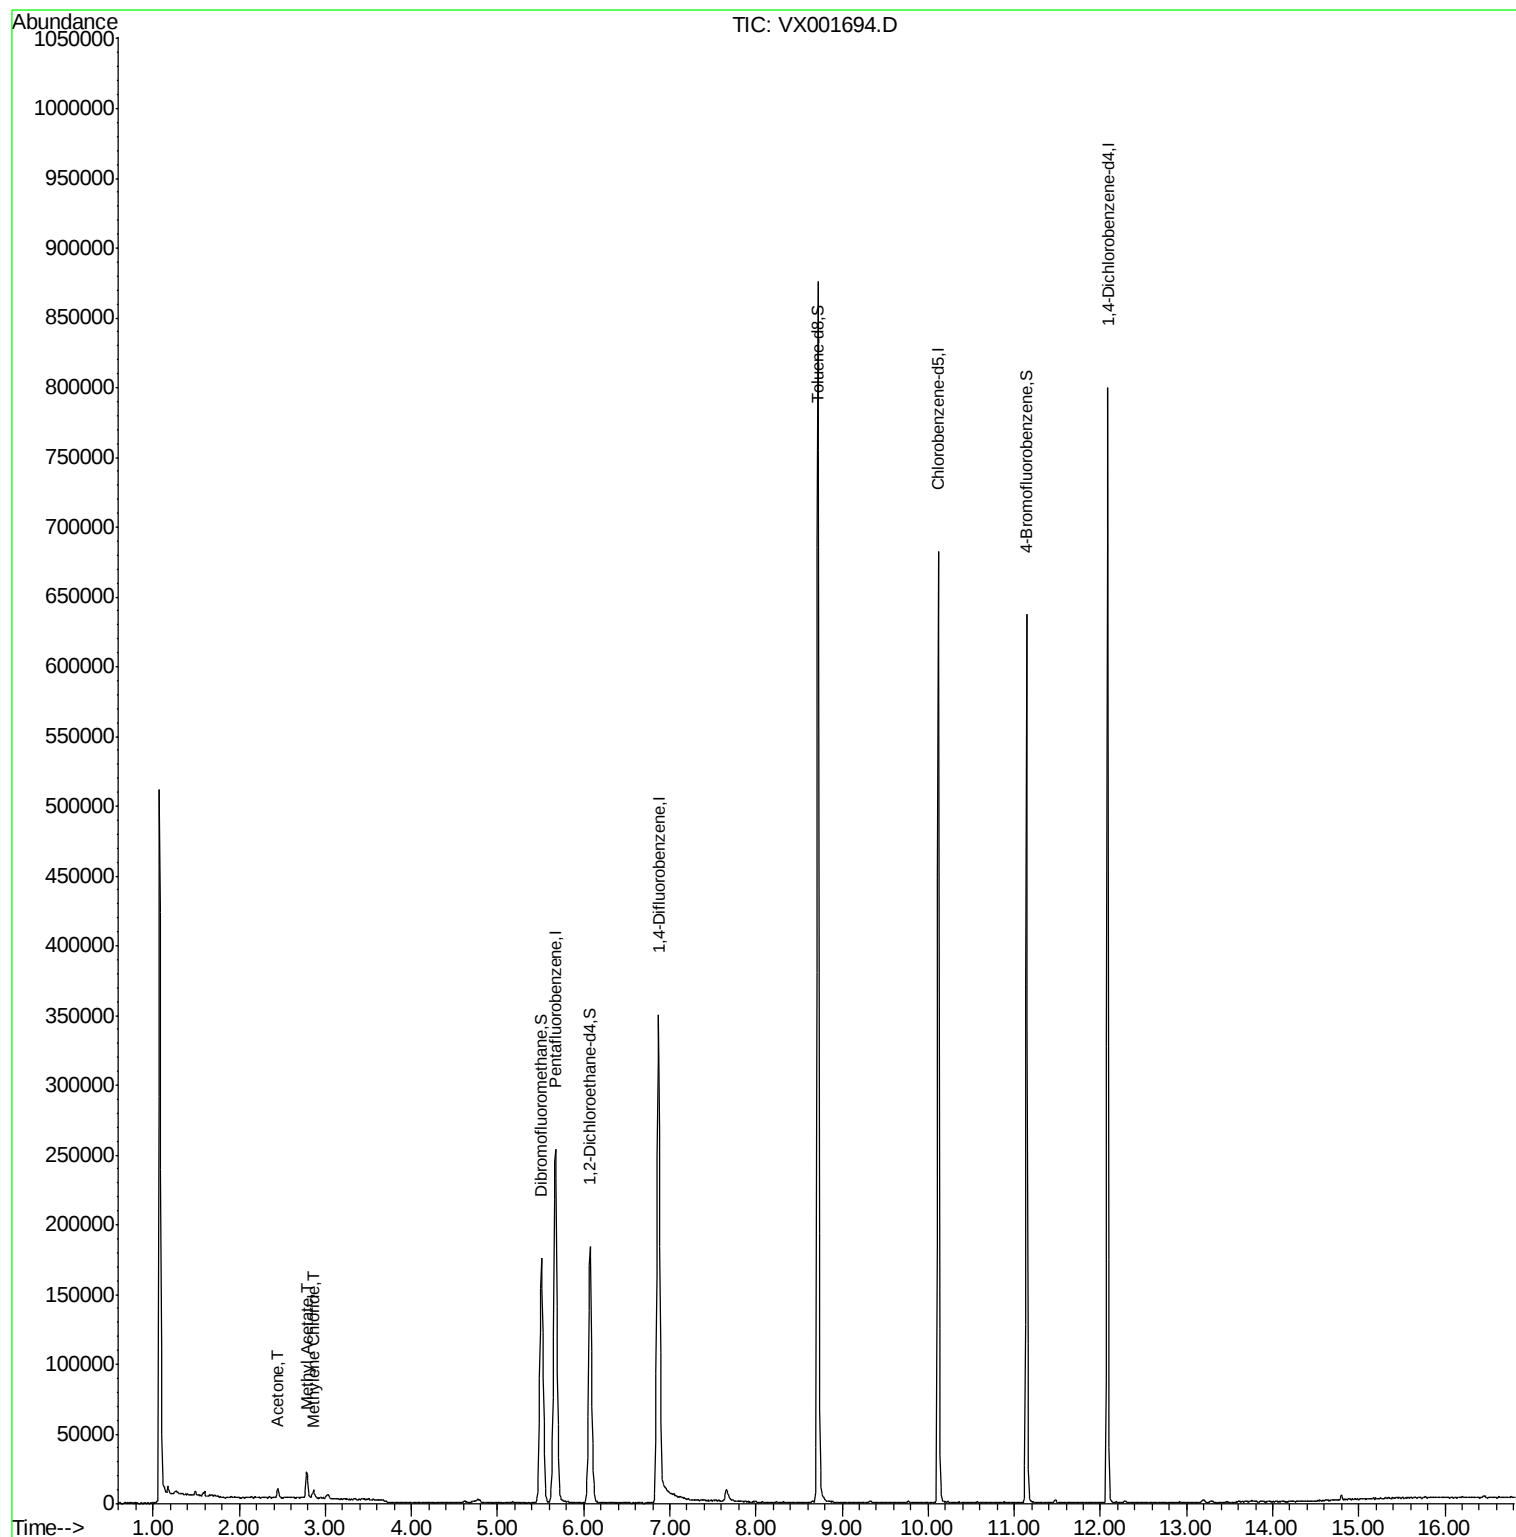



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. 0.00 min

Lab File: VX001694.D

Acq: 13 May 2018 03:47

Instrument :

MSVOA_X

ClientSampleId :


PB109200ZHE#10

Tot Ion:168 Resp: 267237

Ion Ratio Lower Upper




168 100

99 47.8 36.6 54.8

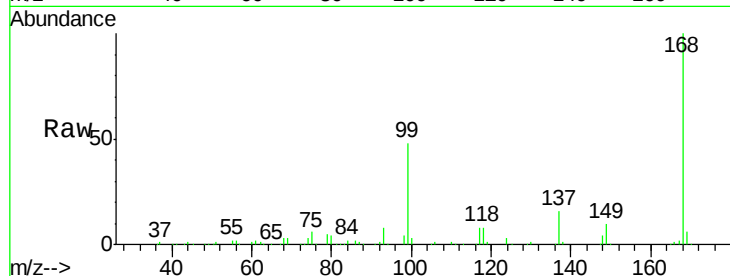

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

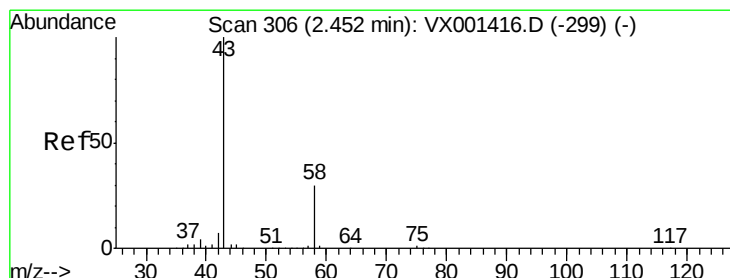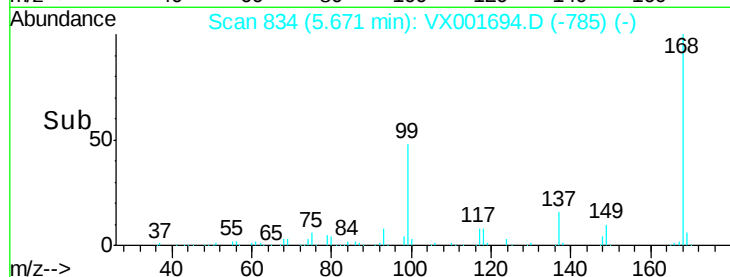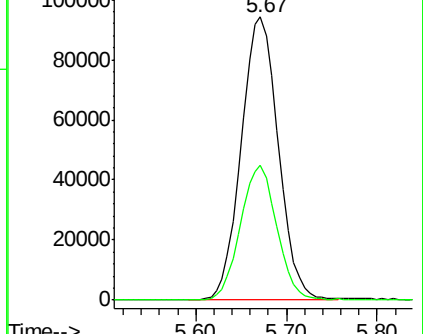

#16

Acetone

Concen: 4.43 ug/l

RT: 2.45 min Scan# 305

Delta R.T. -0.01 min

Lab File: VX001694.D


Acq: 13 May 2018 03:47

Tgt Ion: 43 Resp: 7727

Ion Ratio Lower Upper



43 100


58 32.3 23.8 35.8

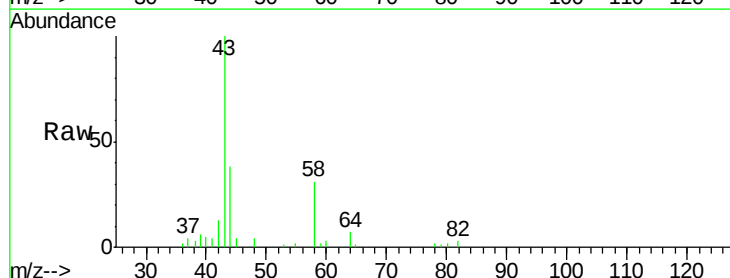

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0



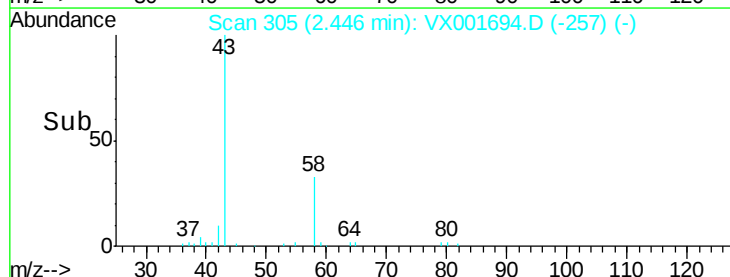
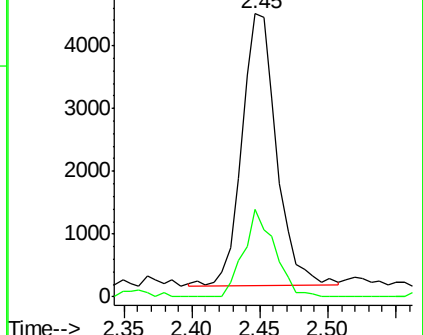


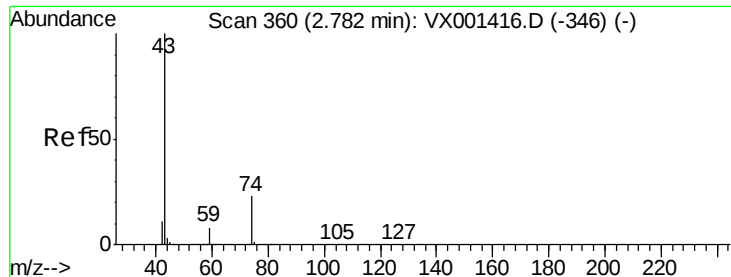

#18
Methvl Acetate
Concen: 4.95 ug/l
RT: 2.78 min Scan# 360
Delta R.T. 0.00 min
Lab File: VX001694.D
Acq: 13 May 2018 03:47




Instrument :
MSVOA_X
ClientSampleId :
PB109200ZHE#10


Tot Ion: 43 Resp: 22668
Ion Ratio Lower Upper
43 100
74 23.4 18.6 27.8

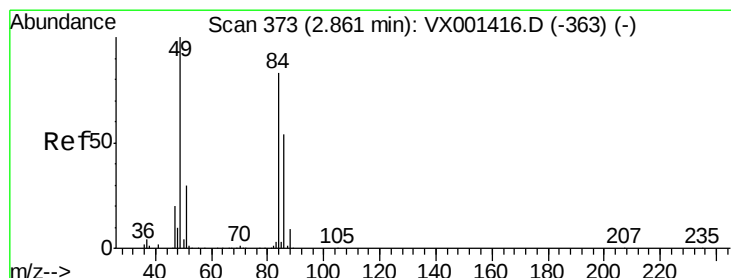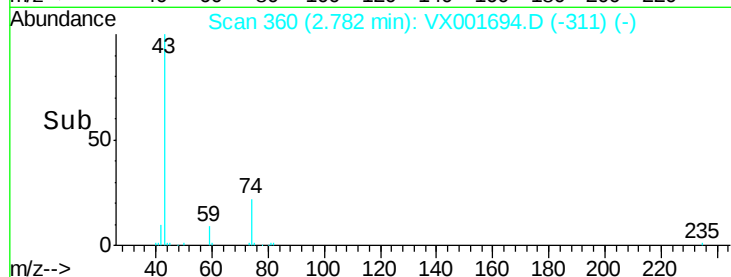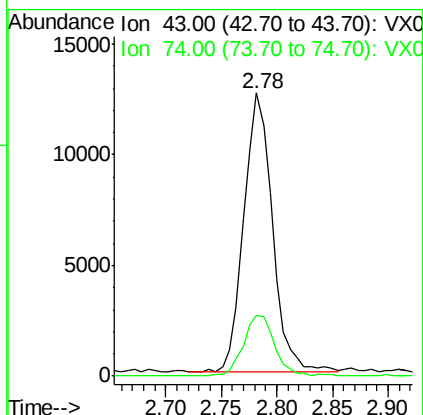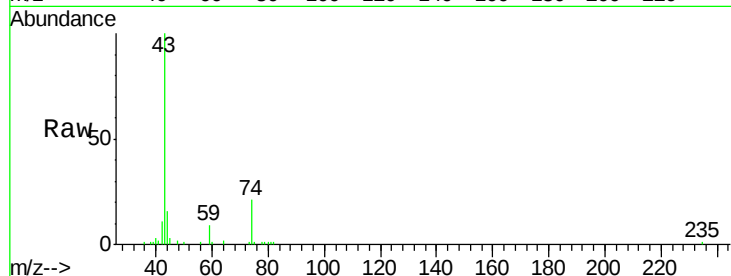

#20
Methylene Chloride
Concen: 0.77 ug/l
RT: 2.86 min Scan# 373
Delta R.T. 0.00 min
Lab File: VX001694.D
Acq: 13 May 2018 03:47

Tgt Ion: 84 Resp: 2659
Ion Ratio Lower Upper
84 100
49 105.8 96.6 144.8
51 37.3 29.0 43.4
86 67.7 52.2 78.4

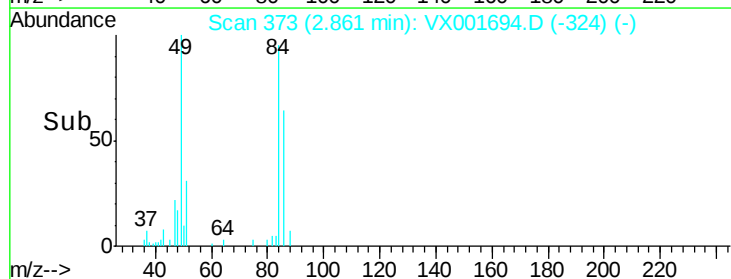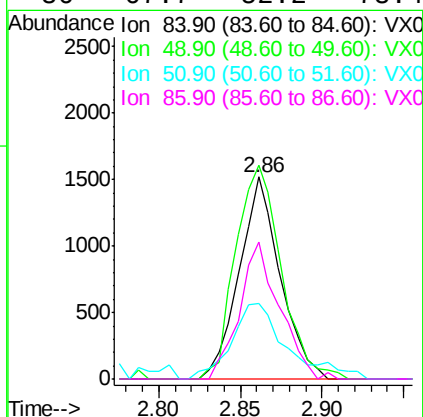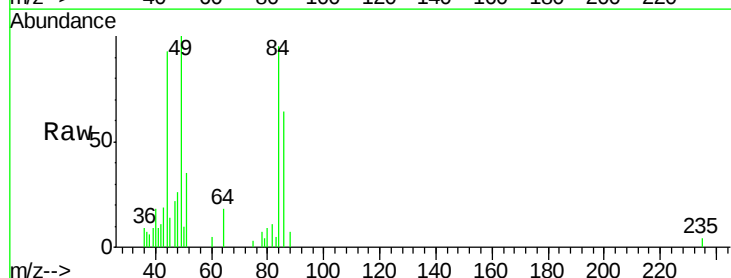

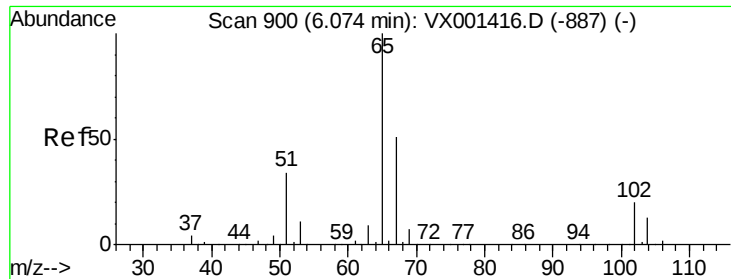

#33

1,2-Dichloroethane-d4

Concen: 45.94 ug/l

RT: 6.07 min Scan# 900

Delta R.T. 0.00 min

Lab File: VX001694.D

Acq: 13 May 2018 03:47

Instrument :

MSVOA_X

ClientSampleId :


PB109200ZHE#10

Tot Ion: 65 Resp: 176450

Ion Ratio Lower Upper




65 100

67 50.6 0.0 101.8

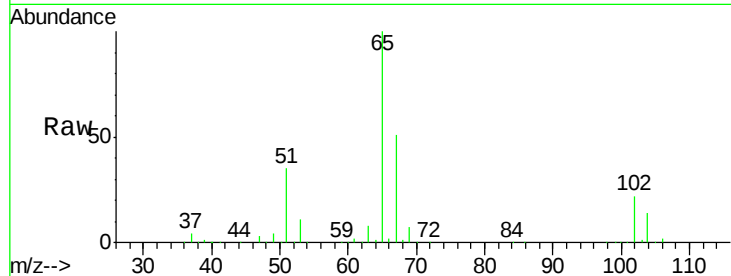

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

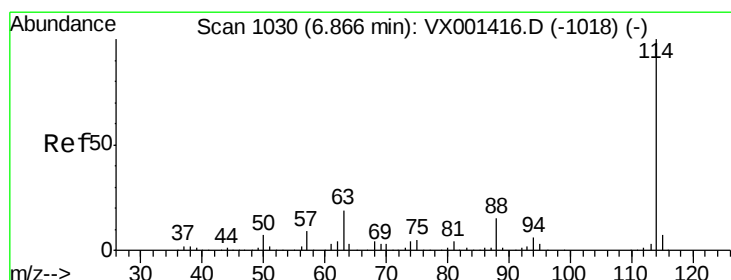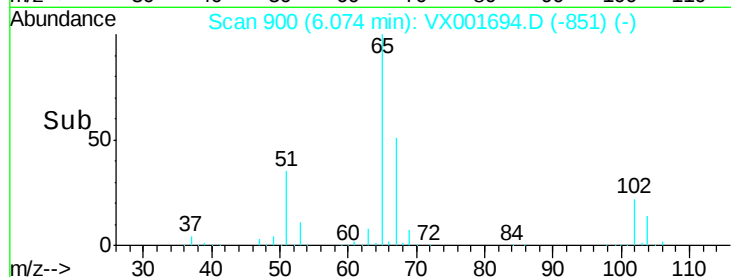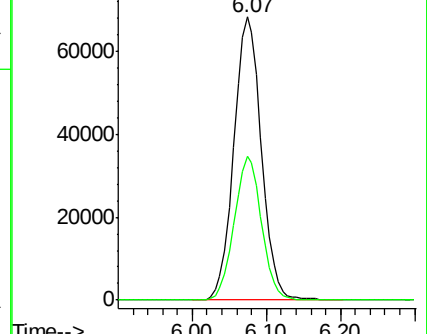

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. 0.00 min

Lab File: VX001694.D

Acq: 13 May 2018 03:47


Tgt Ion: 114 Resp: 365802

Ion Ratio Lower Upper

114 100

63 19.6 0.0 38.6



88 14.5 0.0 30.8

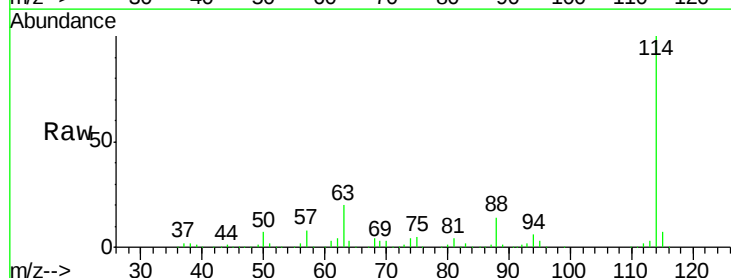


Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0



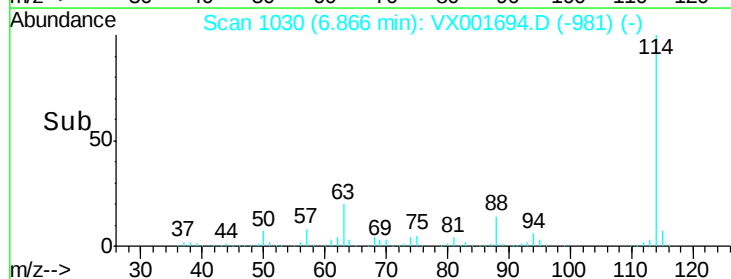
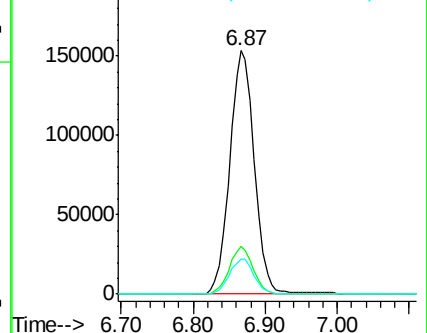


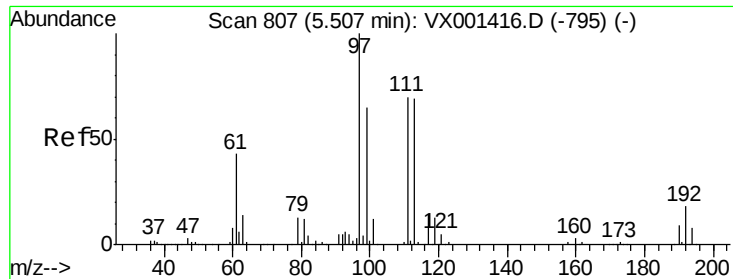

#35
 Dibromofluoromethane
 Concen: 43.93 ug/l
 RT: 5.51 min Scan# 808
 Delta R.T. 0.01 min
 Lab File: VX001694.D
 Acq: 13 May 2018 03:47




Instrument :
 MSVOA_X
 ClientSampleId :
 PB109200ZHE#10


Tot Ion:113 Resp: 142944
 Ion Ratio Lower Upper
 113 100
 111 101.0 82.2 123.2
 192 26.5 21.4 32.0

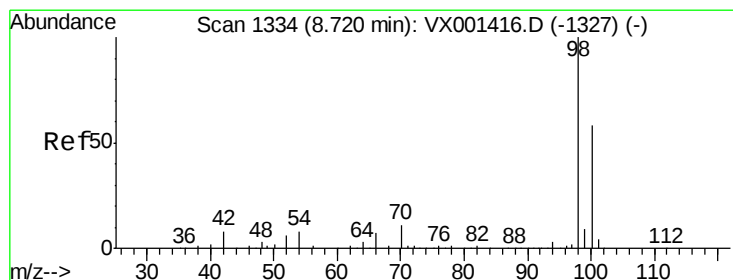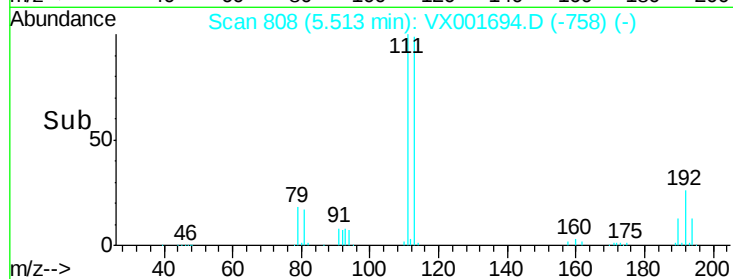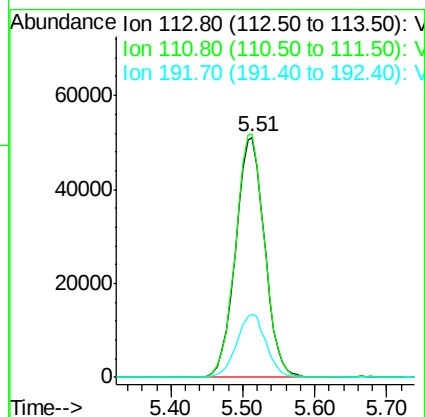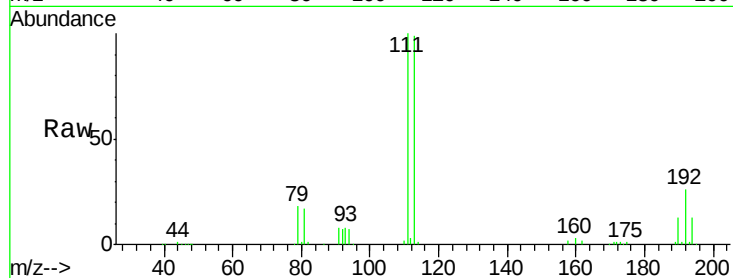

#50
 Toluene-d8
 Concen: 42.67 ug/l
 RT: 8.72 min Scan# 1334
 Delta R.T. 0.00 min
 Lab File: VX001694.D
 Acq: 13 May 2018 03:47

Tgt Ion: 98 Resp: 506800
 Ion Ratio Lower Upper
 98 100
 100 66.0 54.0 81.0


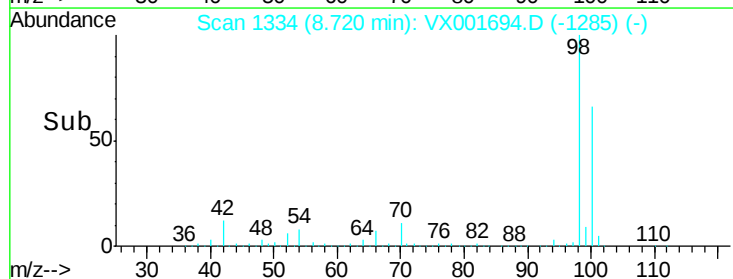
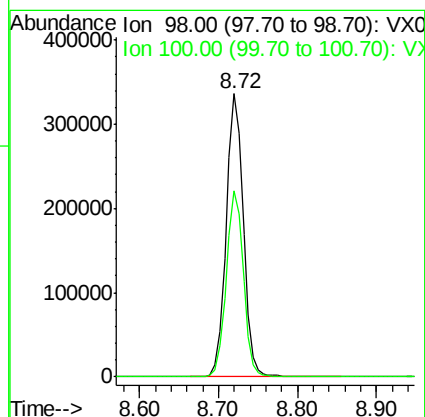
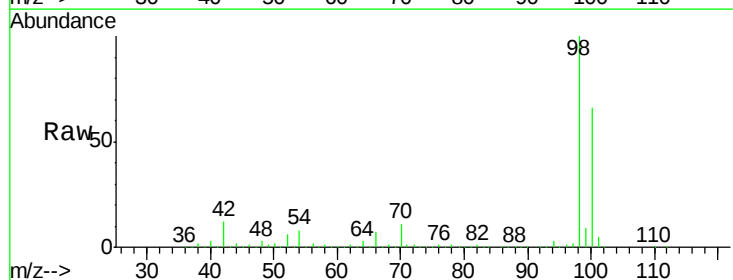


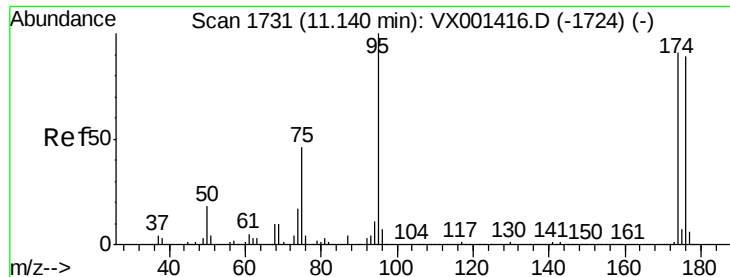

#62
4-Bromofluorobenzene
Concen: 34.79 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. 0.00 min
Lab File: VX001694.D
Acq: 13 May 2018 03:47




Instrument :
MSVOA_X
ClientSampleId :
PB109200ZHE#10


Tot Ion: 95 Resp: 158595
Ion Ratio Lower Upper
95 100
174 102.2 0.0 202.0
176 99.7 0.0 197.4

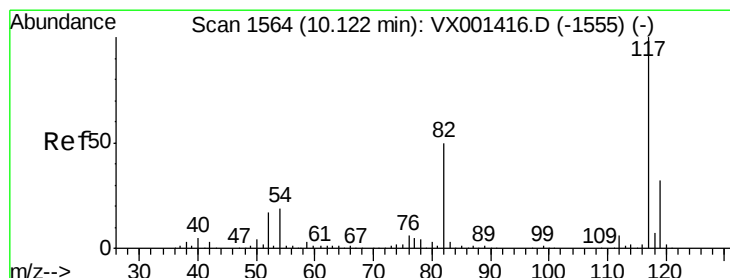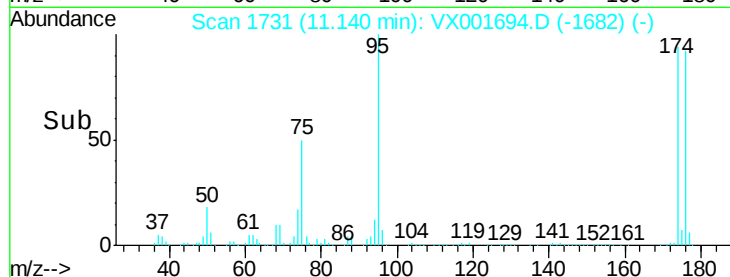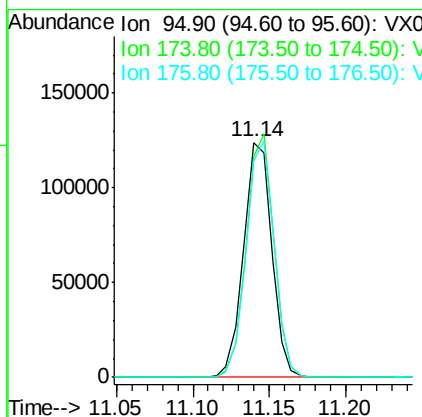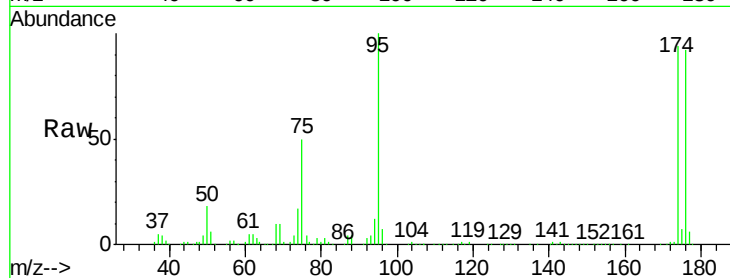

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. -0.01 min
Lab File: VX001694.D
Acq: 13 May 2018 03:47

Tgt Ion: 117 Resp: 317061
Ion Ratio Lower Upper
117 100
82 52.1 40.0 60.0
119 31.7 25.8 38.8

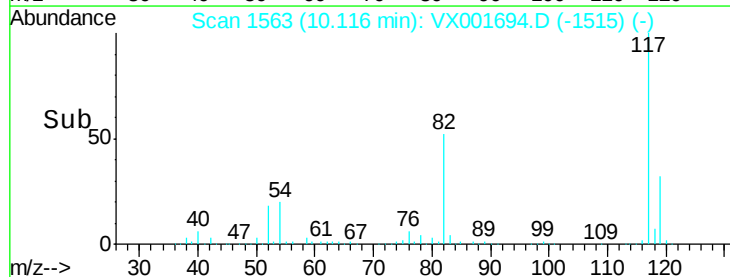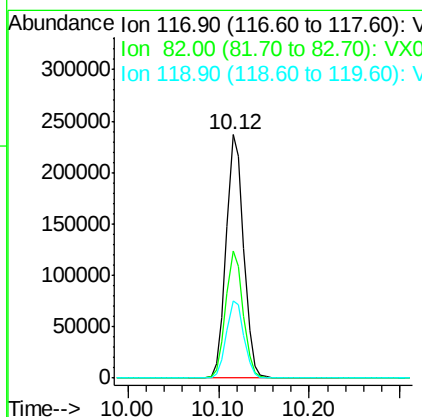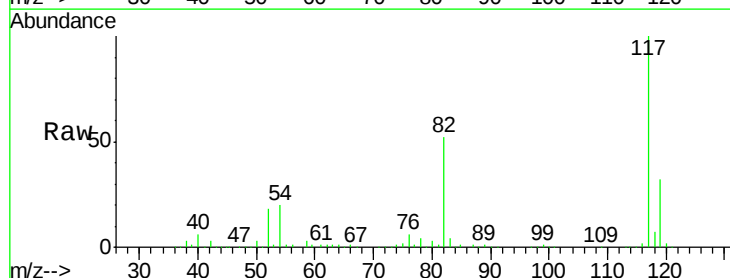

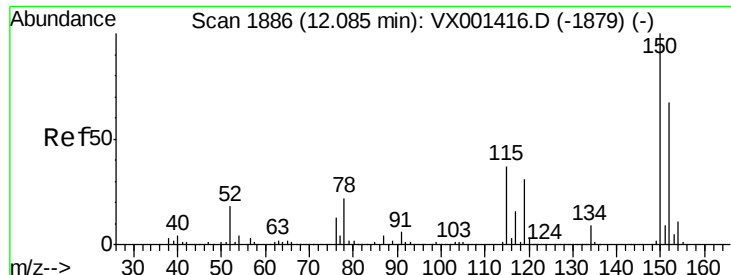

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.08 min Scan# 1886

Delta R.T. 0.00 min

Lab File: VX001694.D


Acq: 13 May 2018 03:47

Instrument :

MSVOA_X

ClientSampleId :

PB109200ZHE#10

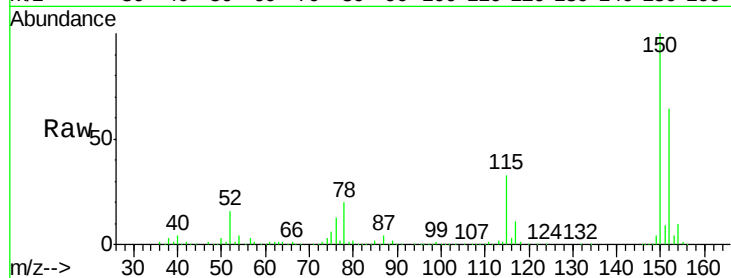

Tot Ion:152 Resp: 171097

Ion Ratio Lower Upper

152 100

115 52.4 37.7 113.1

150 156.9 0.0 349.4

