


Data Path : W:\HPCHEM1\MSVOA X\DATA\VX051218\
Data File : VX001679.D
Acq On : 12 May 2018 21:09
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X050518W.M
Title : SW846 8260
Last Update : Sun May 06 07:59:25 2018

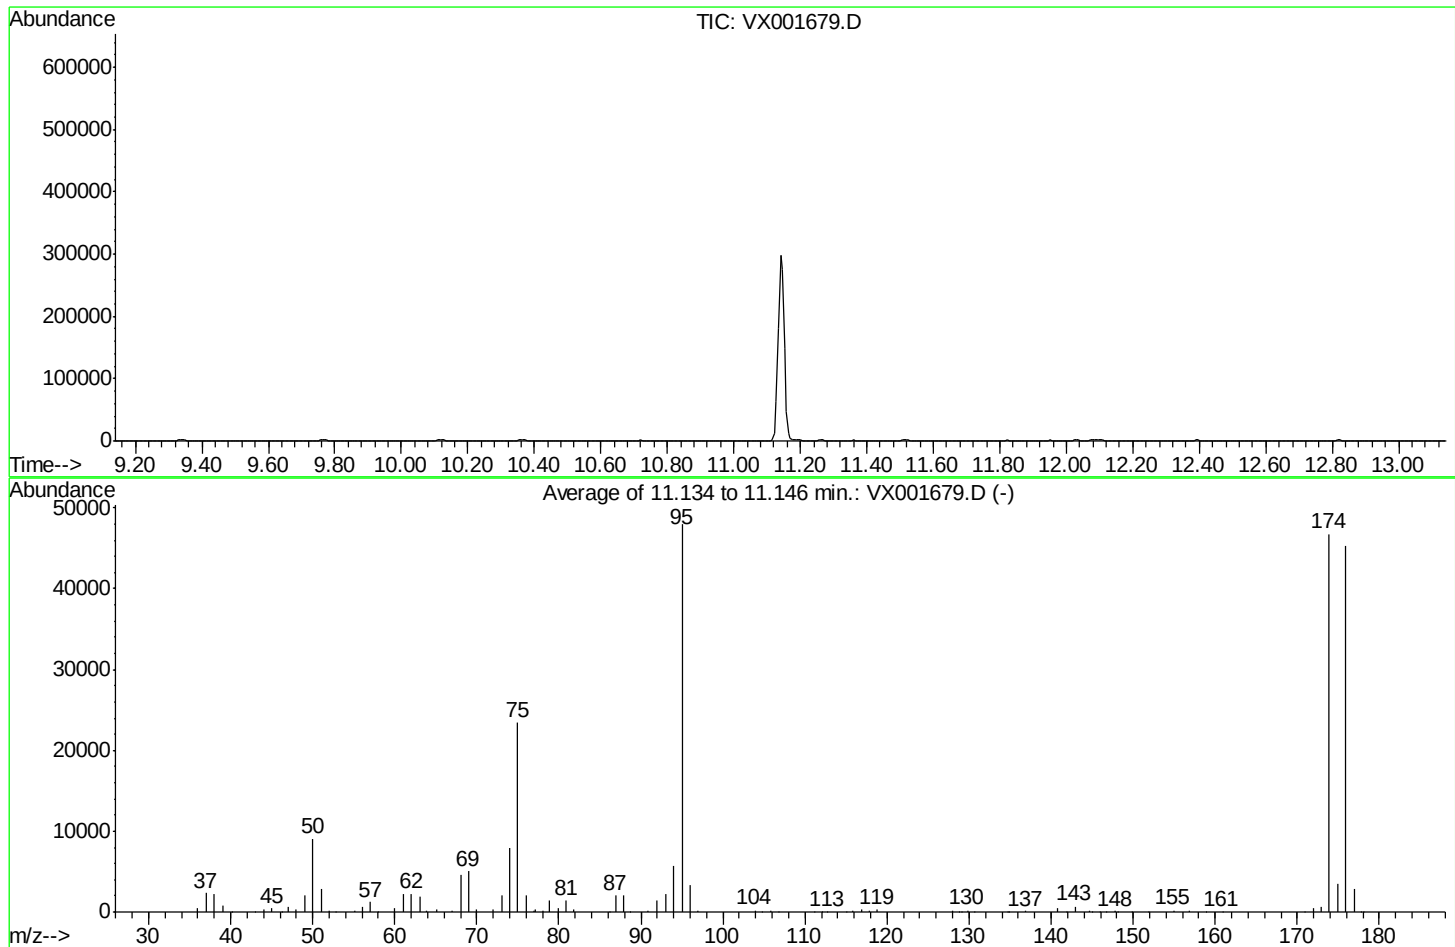

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	9062	PASS
75	95	30	60	48.7	23373	PASS
95	95	100	100	100.0	47968	PASS
96	95	5	9	7.1	3404	PASS
173	174	0.00	2	1.3	593	PASS
174	95	50	100	97.4	46741	PASS
175	174	5	9	7.6	3529	PASS
176	174	95	101	96.9	45280	PASS
177	176	5	9	6.4	2880	PASS