


Data Path : W:\HPCHEM1\MSVOA X\Data\VX051418\  
 Data File : VX001705.D  
 Acq On : 14 May 2018 09:35  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT3.P

Method : W:\HPCHEM1\MSVOA\_X\METHOD\624X051118W.M  
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
 Last Update : Fri May 11 07:16:13 2018

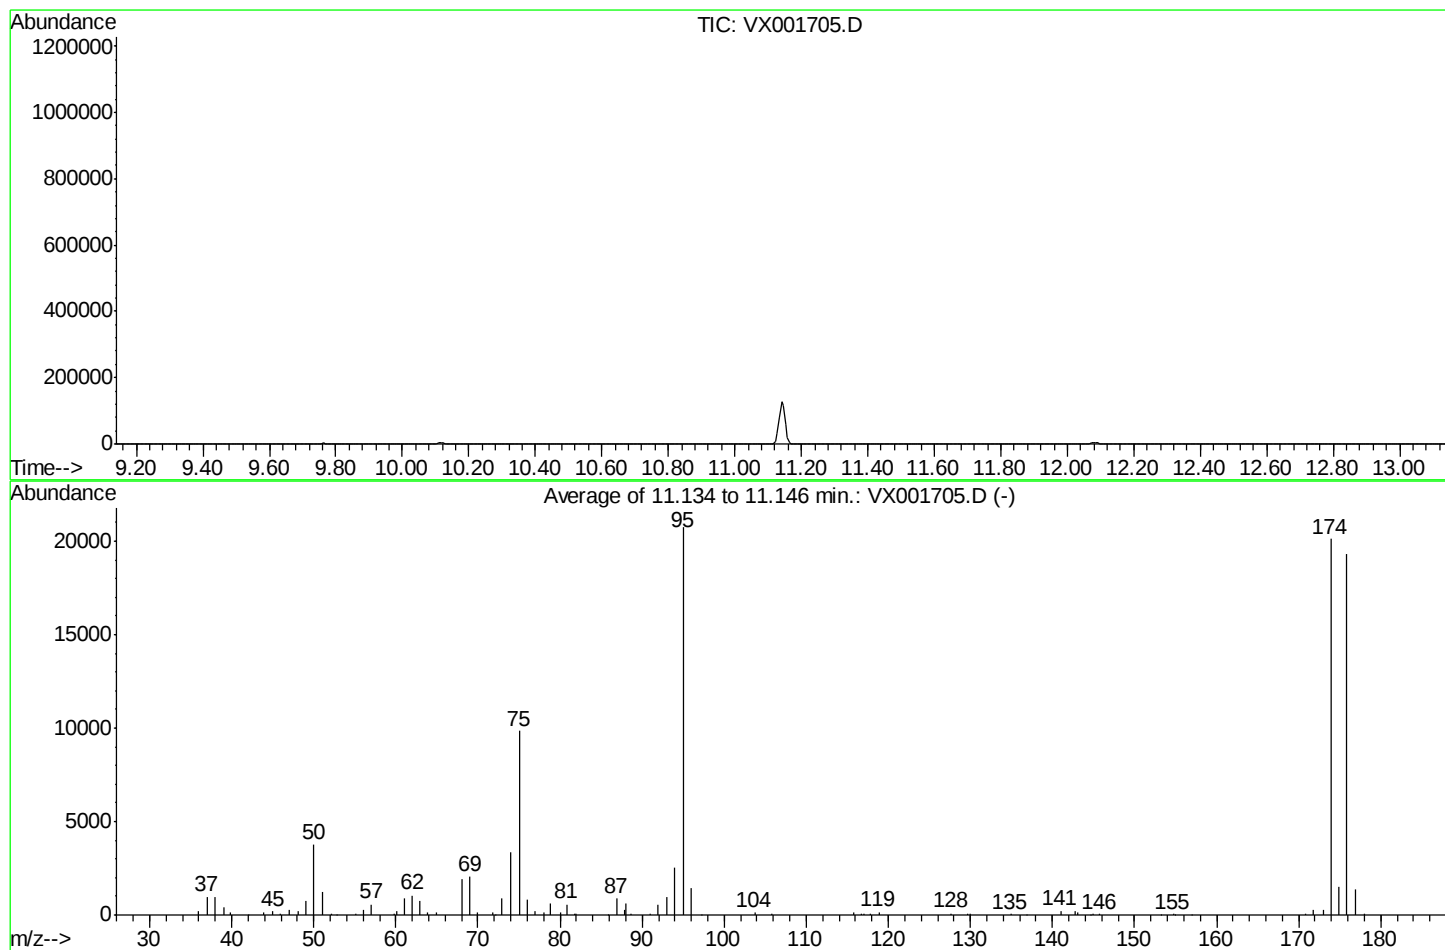

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1725

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 18.1      | 3753    | PASS             |
| 75          | 95           | 30           | 60           | 47.4      | 9844    | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 20747   | PASS             |
| 96          | 95           | 5            | 9            | 7.0       | 1445    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.3       | 257     | PASS             |
| 174         | 95           | 50           | 100          | 96.9      | 20110   | PASS             |
| 175         | 174          | 5            | 9            | 7.4       | 1479    | PASS             |
| 176         | 174          | 95           | 101          | 96.1      | 19325   | PASS             |
| 177         | 176          | 5            | 9            | 6.9       | 1341    | PASS             |