

Data File : VX001723.D

Acq On : 14 May 2018 21:50

Operator : JC/MD

Sample : J2833-05

Misc : 5.0mL/MSVOA_X/WATER

ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB050918

Quant Time: May 15 05:39:29 2018

Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X051518W.M

Quant Title : SW846 8260

QLast Update : Tue May 15 01:36:22 2018

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	294426	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	396397	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	342880	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	190051	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.07	65	176463	44.71	ug/l	0.00
Spiked Amount	50.000		Recovery	=	89.42%	
35) Dibromofluoromethane	5.51	113	143474	42.89	ug/l	0.00
Spiked Amount	50.000		Recovery	=	85.78%	
50) Toluene-d8	8.72	98	543643	45.38	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.76%	
62) 4-Bromofluorobenzene	11.14	95	176494	40.91	ug/l	0.00
Spiked Amount	50.000		Recovery	=	81.82%	

Target Compounds

						Qvalue
5) Bromomethane	1.65	94	1177	Below Cal	#	68
10) Methyl Iodide	2.53	142	1168	0.42	ug/l #	68
11) Tert butyl alcohol	3.08	59	451	0.64	ug/l #	72
13) Acrolein	2.50	56	30018	60.41	ug/l #	1
14) Allyl chloride	2.50	41	2526331	469.66	ug/l #	1
15) Acrylonitrile	3.16	53	793	0.45	ug/l #	83
17) Carbon Disulfide	2.56	76	2472	0.33	ug/l	95
20) Methylene Chloride	2.86	84	60886	18.35	ug/l	98
25) 2-Butanone	4.73	43	9232	3.89	ug/l	98
29) Tetrahydrofuran	5.17	42	1163	0.75	ug/l #	67
36) 1,1-Dichloropropene	5.81	75	960	0.21	ug/l #	61
37) Ethyl Acetate	4.73	43	9232	1.94	ug/l #	68
38) Carbon Tetrachloride	5.67	117	24554	5.14	ug/l #	16
68) m/p-Xylenes	10.37	106	2341	0.39	ug/l	91
71) Bromoform	10.85	173	51	2.94	ug/l #	29
76) 1,2,3-Trichloropropane	11.14	75	84085	23.27	ug/l #	39
78) n-propylbenzene	11.37	91	2972	0.21	ug/l	99
80) 1,3,5-Trimethylbenzene	11.51	105	2210	0.22	ug/l	94
81) trans-1,4-Dichloro-2-buten	11.14	75	84085	68.06	ug/l #	10
82) 4-Chlorotoluene	11.51	91	2120	0.21	ug/l	98
84) 1,2,4-Trimethylbenzene	11.81	105	4188	0.39	ug/l	96
87) 1,3-Dichlorobenzene	12.03	146	1903	0.28	ug/l	93
88) 1,4-Dichlorobenzene	12.03	146	1903	0.27	ug/l	92
89) n-Butylbenzene	12.40	91	3107	0.31	ug/l	87
93) 1,2,4-Trichlorobenzene	13.65	180	2124	0.39	ug/l	99
94) Hexachlorobutadiene	13.79	225	904	0.31	ug/l	86
96) 1,2,3-Trichlorobenzene	14.02	180	1255	0.23	ug/l	98

(#)=qualifier out of range (m)=manual integration (+)=signals summed

Data File : VX001723.D

Acq On : 14 May 2018 21:50

Operator : JC/MD

Sample : J2833-05

Misc : 5.0mL/MSVOA_X/WATER

ALS Vial : 20 Sample Multiplier: 1

Instrument :

MSVOA_X

ClientSampleId :

FB050918


Quant Time: May 15 05:39:29 2018

Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X051518W.M

Quant Title : SW846 8260

QLast Update : Tue May 15 01:36:22 2018

Response via : Initial Calibration

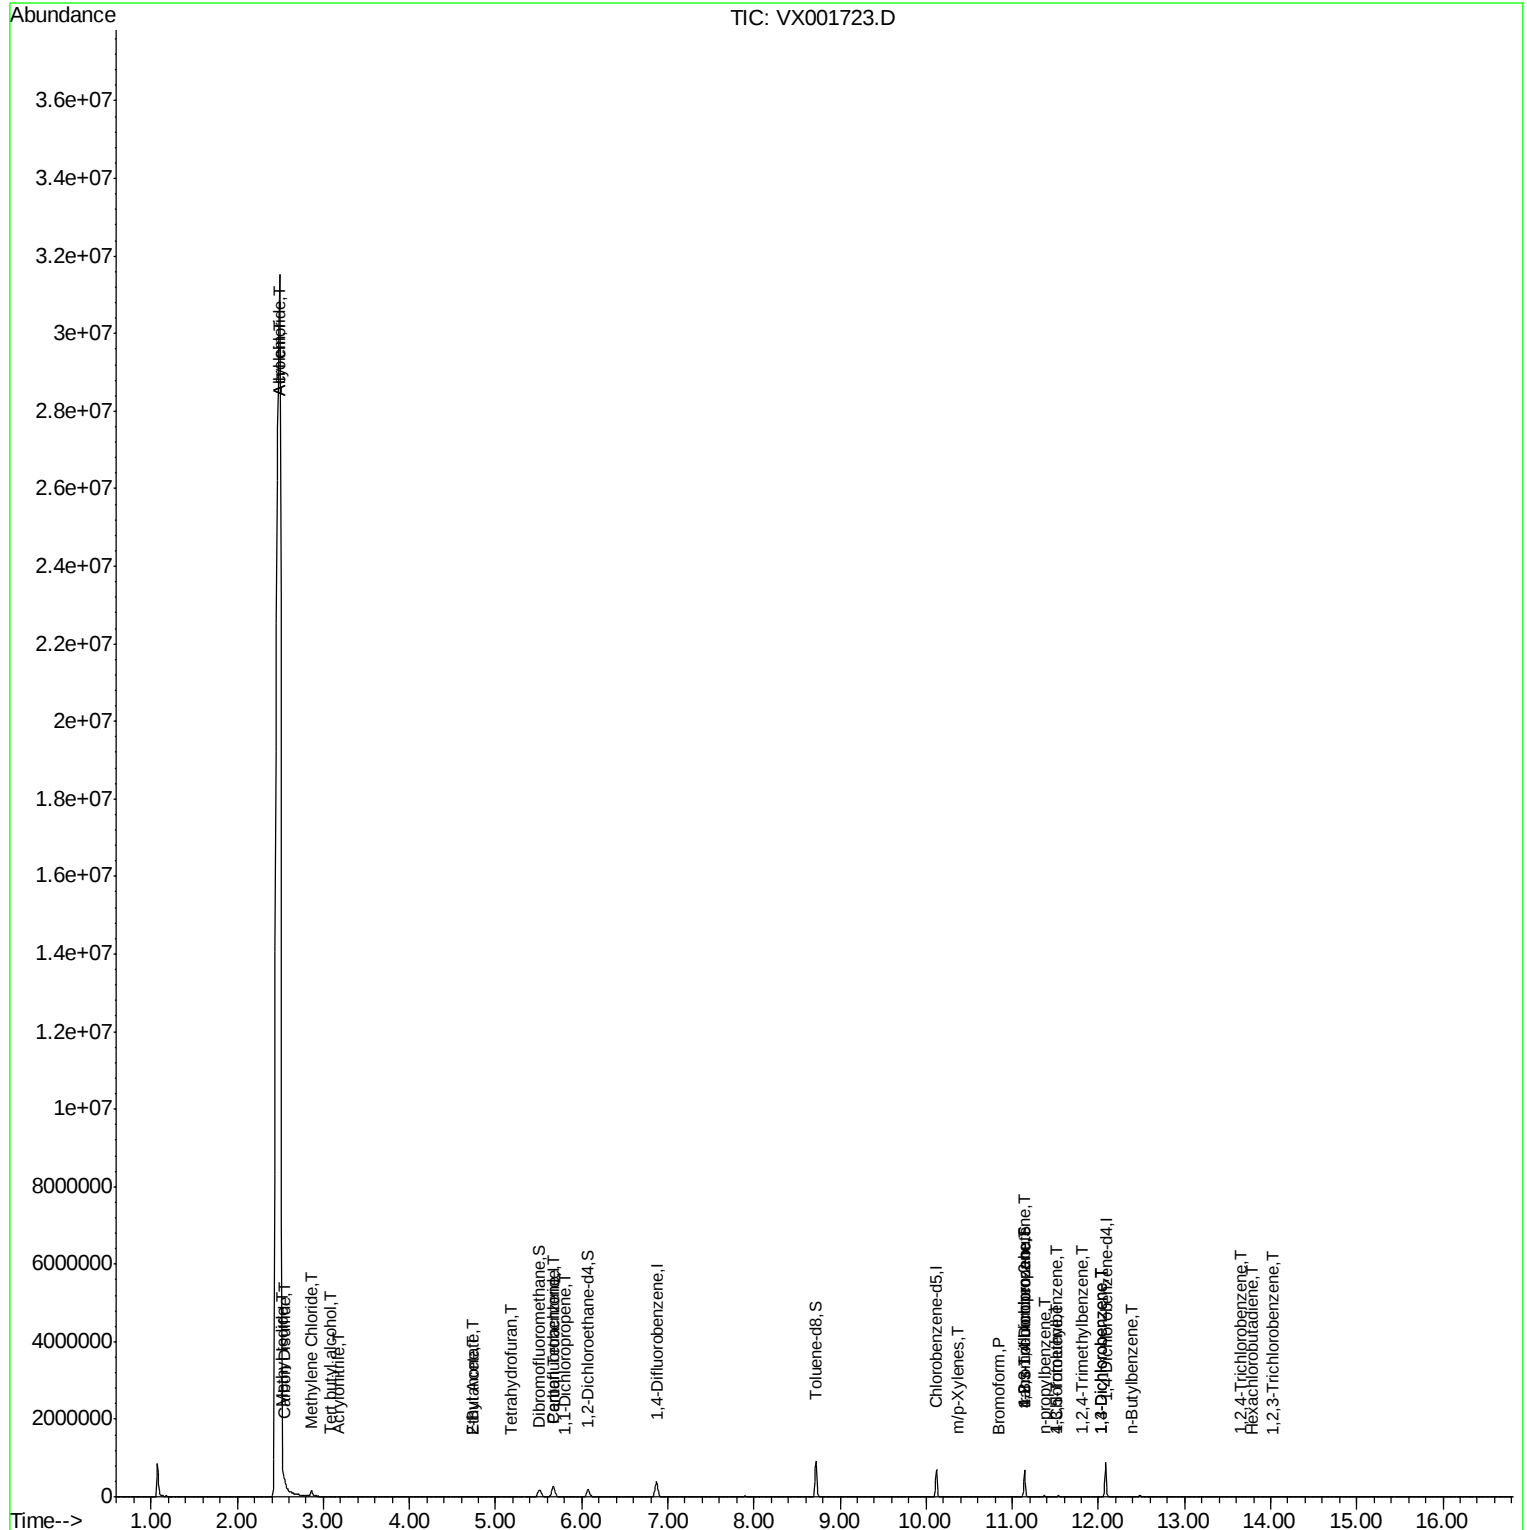



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.00 min

Lab File: VX001723.D

Acq: 14 May 2018 21:50

Instrument :

MSVOA_X

ClientSampleId :


FB050918

Tgt Ion:168 Resp: 294426

Ion Ratio Lower Upper

168 100

99 46.6 35.0 52.4

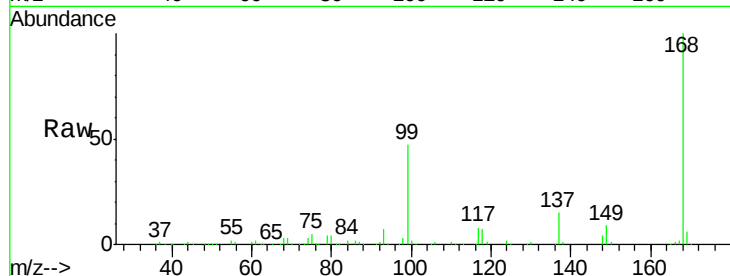

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

120000

100000

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80



#5

Bromomethane

Concen: Below Cal

RT: 1.65 min Scan# 175

Delta R.T. 0.02 min

Lab File: VX001723.D


Acq: 14 May 2018 21:50

Tgt Ion: 94 Resp: 1177

Ion Ratio Lower Upper

94 100

96 65.3 77.4 116.0#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1.65

600

500

400


300


200

100

0

Time--> 1.60 1.65 1.70 1.75









#10
Methyl Iodide
Concen: 0.42 ug/l
RT: 2.53 min Scan# 319
Delta R.T. 0.02 min
Lab File: VX001723.D
Acq: 14 May 2018 21:50




Instrument :
MSVOA_X
ClientSampleId :
FB050918


Tgt Ion: 142 Resp: 1168
Ion Ratio Lower Upper
142 100
127 21.5 32.5 48.7#
141 0.0 11.4 17.0#

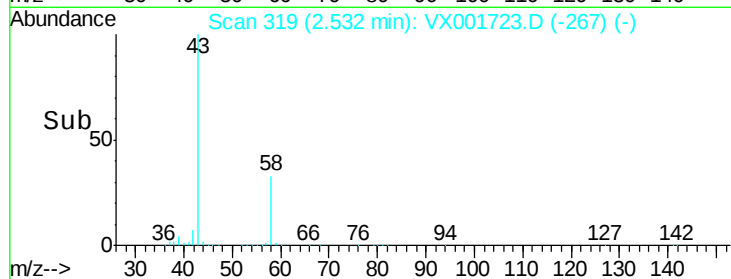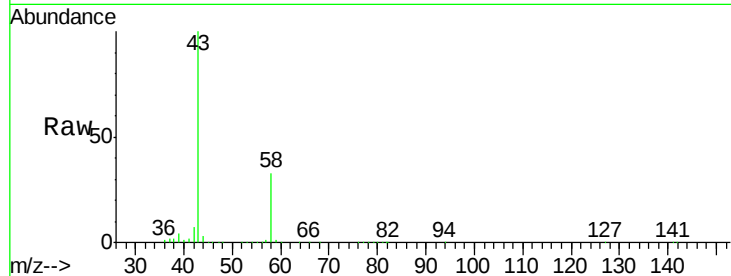

#11
Tert butyl alcohol
Concen: 0.64 ug/l
RT: 3.08 min Scan# 409
Delta R.T. -0.00 min
Lab File: VX001723.D
Acq: 14 May 2018 21:50

Tgt Ion: 59 Resp: 451
Ion Ratio Lower Upper
59 100
57 0.0 8.5 12.7#

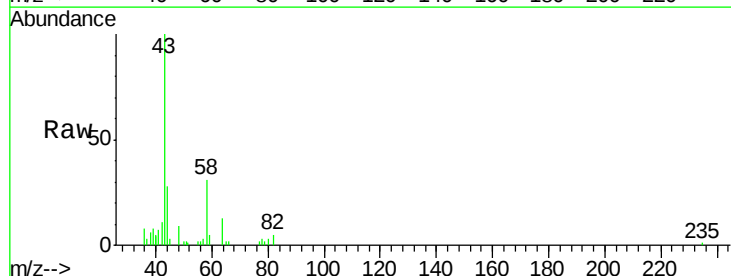



#13

Acrolein

Concen: 60.41 ug/l

RT: 2.50 min Scan# 313

Delta R.T. 0.20 min

Lab File: VX001723.D

Acq: 14 May 2018 21:50

Instrument :

MSVOA_X

ClientSampled :





FB050918

Tgt Ion: 56 Resp: 30018

Ion Ratio Lower Upper

56 100

55 1431.9 56.2 84.2#

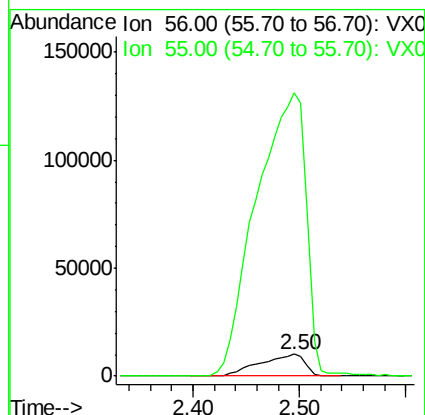

#14

Allyl chloride

Concen: 469.66 ug/l

RT: 2.50 min Scan# 313

Delta R.T. -0.23 min

Lab File: VX001723.D

Acq: 14 May 2018 21:50




Tgt Ion: 41 Resp: 2526331


Ion Ratio Lower Upper

41 100

39 181.7 49.8 74.6#

76 0.0 25.8 38.8#

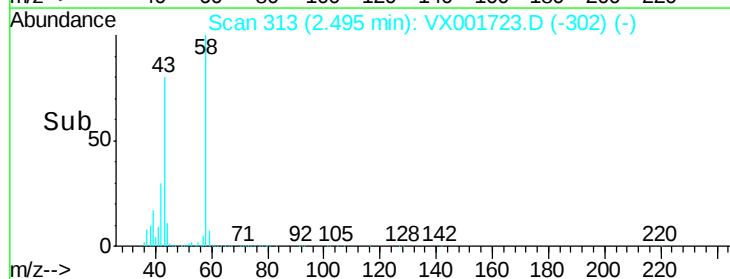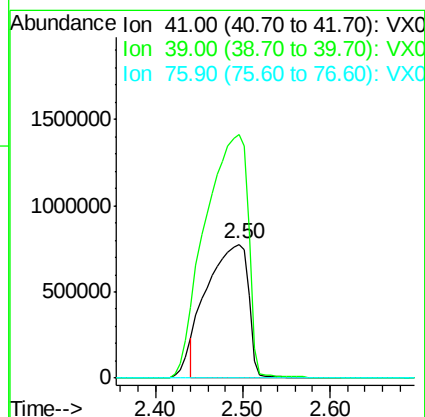



#15

Acrylonitrile

Concen: 0.45 ug/l

RT: 3.16 min Scan# 422

Delta R.T. 0.01 min

Lab File: VX001723.D

Acq: 14 May 2018 21:50





Instrument :

MSVOA_X

ClientSampled :

FB050918

Tgt Ion:	53	Resp:	793
Ion	Ratio	Lower	Upper
53	100		
52	75.2	65.6	98.4
51	57.5	28.1	42.1#

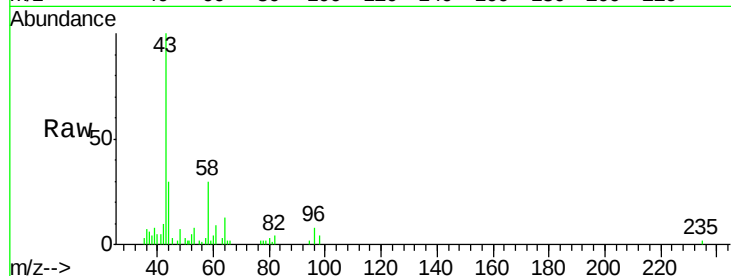

#17

Carbon Disulfide

Concen: 0.33 ug/l




RT: 2.56 min Scan# 323


Delta R.T. -0.01 min

Lab File: VX001723.D

Acq: 14 May 2018 21:50

Tgt Ion:	76	Resp:	2472
Ion	Ratio	Lower	Upper
76	100		
78	11.2	7.6	11.4







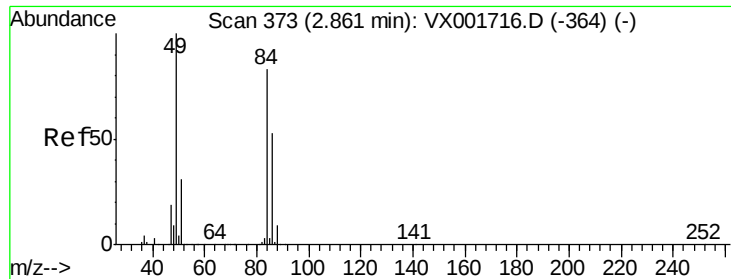

#20
Methylene Chloride
Concen: 18.35 ug/l
RT: 2.86 min Scan# 373
Delta R.T. -0.00 min
Lab File: VX001723.D
Acq: 14 May 2018 21:50




Instrument :
MSVOA_X
ClientSampleId :
FB050918


Tgt Ion:	84	Resp:	60886
Ion	Ratio	Lower	Upper
84	100		
49	122.0	96.3	144.5
51	35.8	29.8	44.6
86	66.1	51.0	76.6

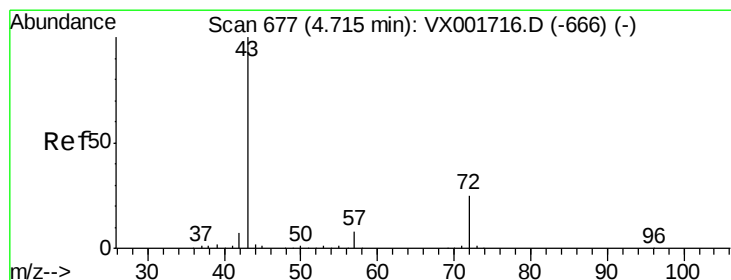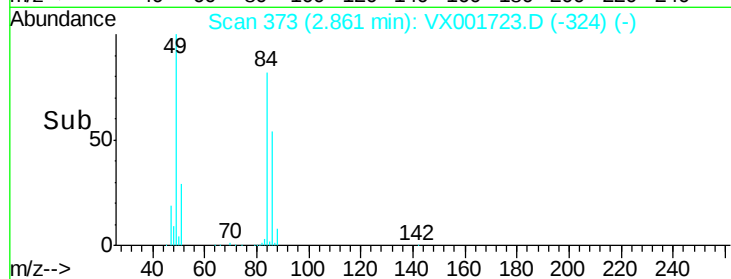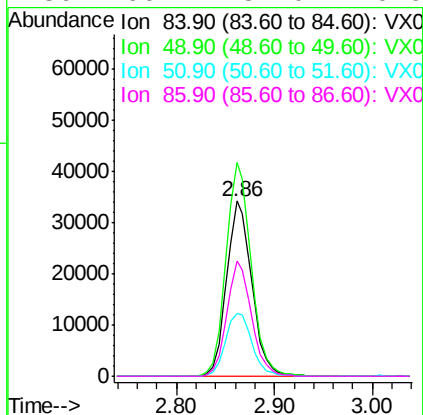

#25
2-Butanone
Concen: 3.89 ug/l
RT: 4.73 min Scan# 679
Delta R.T. 0.01 min
Lab File: VX001723.D
Acq: 14 May 2018 21:50

Tgt Ion:	43	Resp:	9232
Ion	Ratio	Lower	Upper
43	100		
72	23.7	19.8	29.6


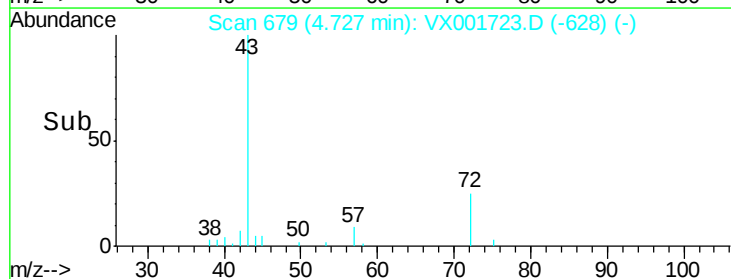

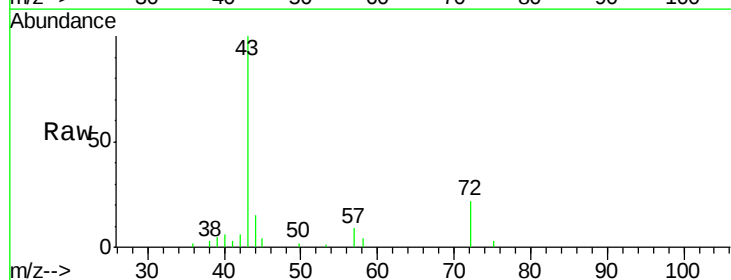




#29
Tetrahydrofuran
Concen: 0.75 ug/l
RT: 5.17 min Scan# 752
Delta R.T. -0.00 min
Lab File: VX001723.D
Acq: 14 May 2018 21:50




Instrument :
MSVOA_X
ClientSampleId :
FB050918


Tgt Ion: 42 Resp: 1163
Ion Ratio Lower Upper
42 100
72 8.7 35.4 53.2#
71 35.6 33.2 49.8

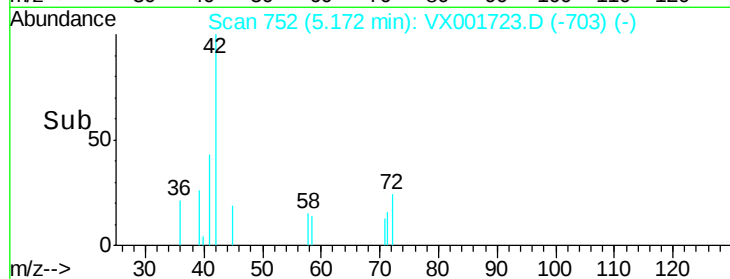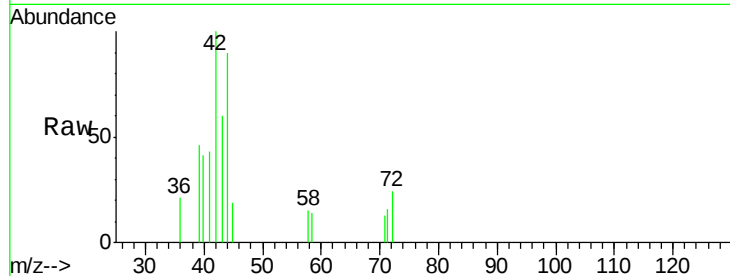

#33
1,2-Dichloroethane-d4
Concen: 44.71 ug/l
RT: 6.07 min Scan# 900
Delta R.T. -0.00 min
Lab File: VX001723.D
Acq: 14 May 2018 21:50

Tgt Ion: 65 Resp: 176463
Ion Ratio Lower Upper
65 100
67 51.7 0.0 102.8

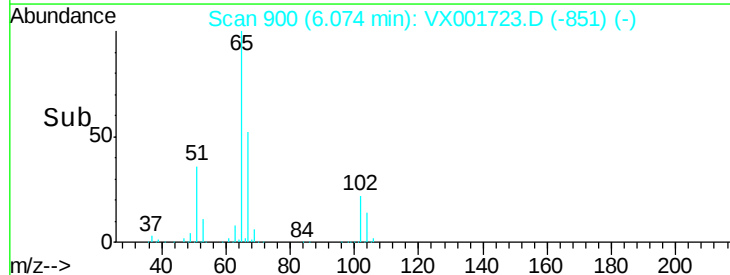

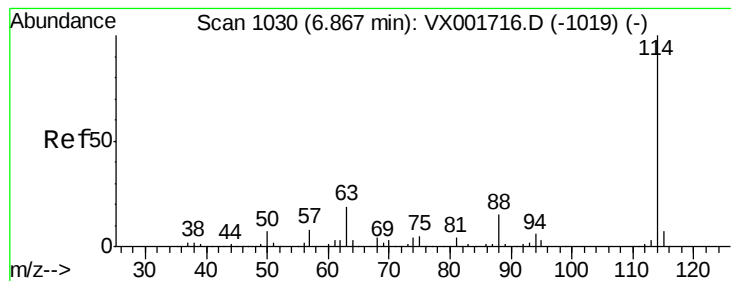

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. -0.00 min

Lab File: VX001723.D

Acq: 14 May 2018 21:50

Instrument :

MSVOA_X

ClientSampleId :

FB050918


Tgt Ion:114 Resp: 396397

Ion Ratio Lower Upper

114 100

63 18.5 0.0 37.0




88 14.6 0.0 29.8



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

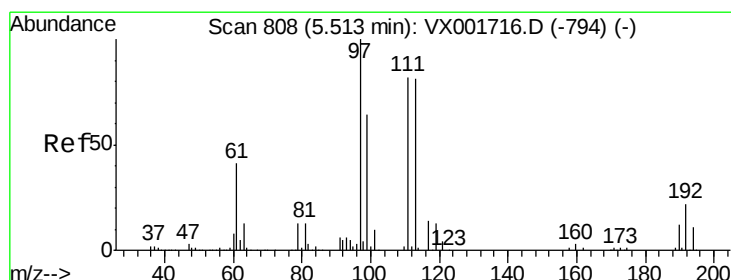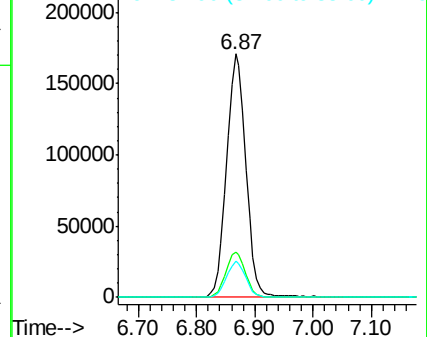

#35

Dibromofluoromethane

Concen: 42.89 ug/l

RT: 5.51 min Scan# 807

Delta R.T. -0.01 min

Lab File: VX001723.D

Acq: 14 May 2018 21:50


Tgt Ion:113 Resp: 143474

Ion Ratio Lower Upper

113 100

111 102.5 82.0 123.0



192 26.9 21.6 32.4

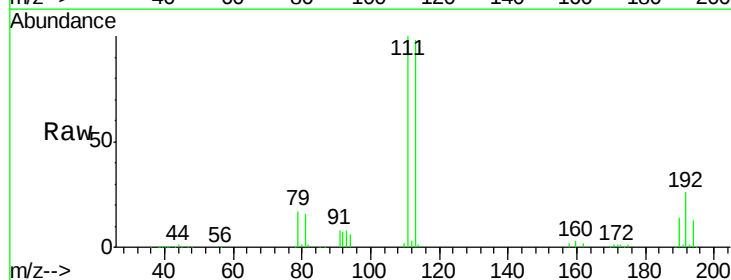


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V




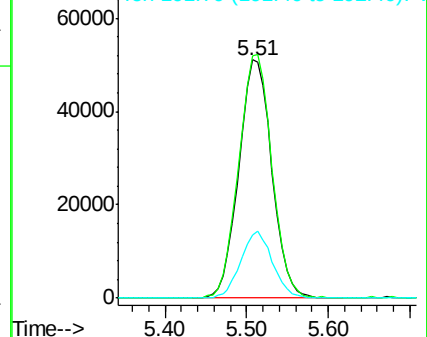


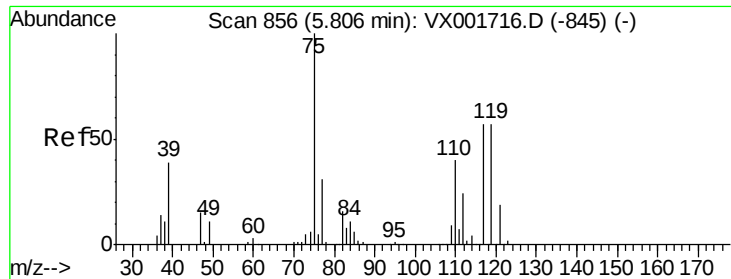

#36
 1,1-Dichloropropene
 Concen: 0.21 ug/l
 RT: 5.81 min Scan# 857
 Delta R.T. 0.01 min
 Lab File: VX001723.D
 Acq: 14 May 2018 21:50




Instrument :
 MSVOA_X
 ClientSampleId :
 FB050918


Tgt Ion: 75 Resp: 960
 Ion Ratio Lower Upper
 75 100
 110 16.7 19.1 57.1#
 77 6.6 24.6 37.0#

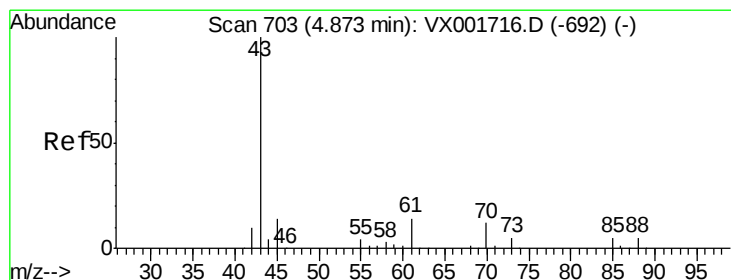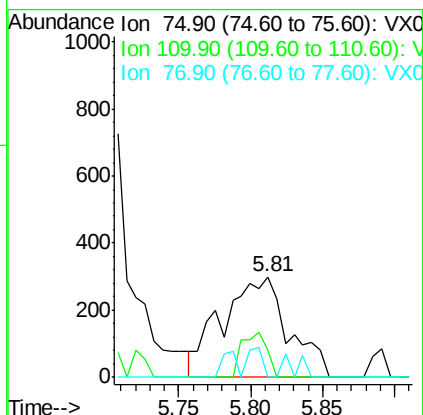

#37
 Ethyl Acetate
 Concen: 1.94 ug/l
 RT: 4.73 min Scan# 679
 Delta R.T. -0.15 min
 Lab File: VX001723.D
 Acq: 14 May 2018 21:50

Tgt Ion: 43 Resp: 9232
 Ion Ratio Lower Upper
 43 100
 61 0.0 10.9 16.3#
 70 0.0 8.8 13.2#

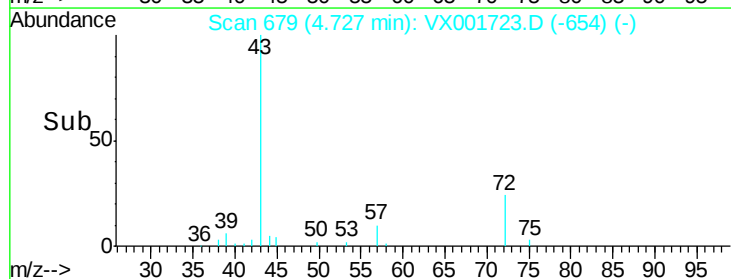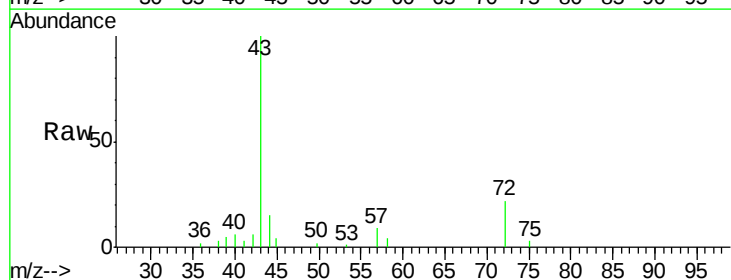


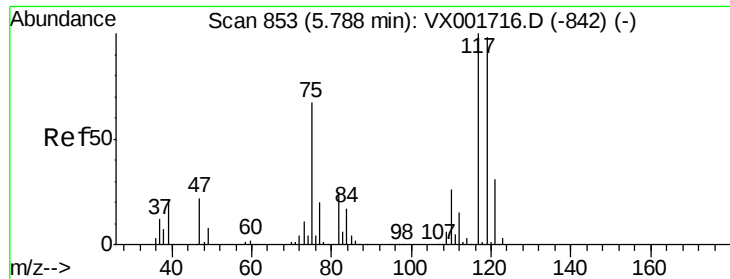




#38
Carbon Tetrachloride
Concen: 5.14 ug/l
RT: 5.67 min Scan# 834
Delta R.T. -0.12 min
Lab File: VX001723.D
Acq: 14 May 2018 21:50

Instrument :
MSVOA_X
ClientSampleId :
FB050918

Tgt Ion: 117 Resp: 24554
Ion Ratio Lower Upper
117 100
119 6.2 77.6 116.4#
121 0.0 24.6 36.8#

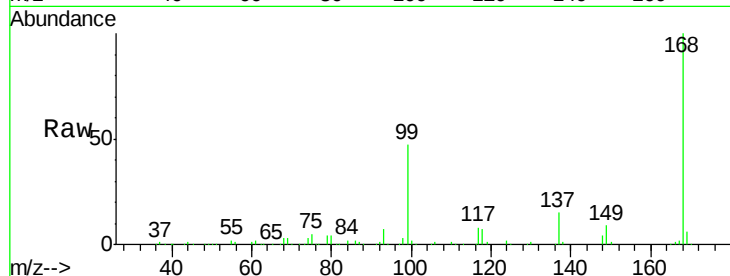


Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V


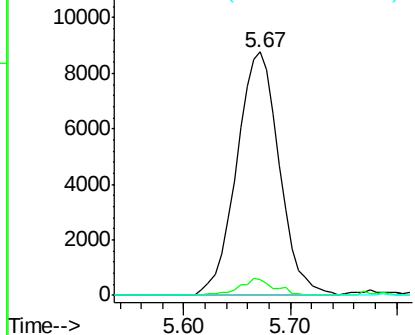



#50
Toluene-d8
Concen: 45.38 ug/l
RT: 8.72 min Scan# 1334
Delta R.T. -0.00 min
Lab File: VX001723.D
Acq: 14 May 2018 21:50

Tgt Ion: 98 Resp: 543643
Ion Ratio Lower Upper
98 100
100 66.6 54.0 81.0



Abundance Ion 98.00 (97.70 to 98.70): VX0
Ion 100.00 (99.70 to 100.70): V

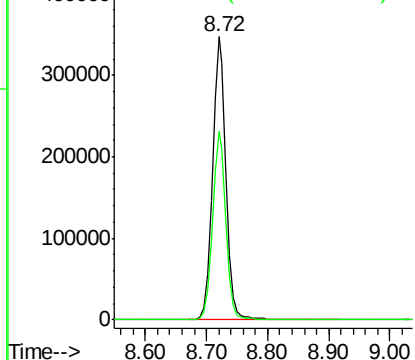



#62

4-Bromofluorobenzene

Concen: 40.91 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.00 min

Lab File: VX001723.D

Acq: 14 May 2018 21:50

Instrument :

MSVOA_X

ClientSampleId :

FB050918


Tgt Ion: 95 Resp: 176494

Ion Ratio Lower Upper

95 100

174 101.5 0.0 201.8

176 98.9 0.0 196.8



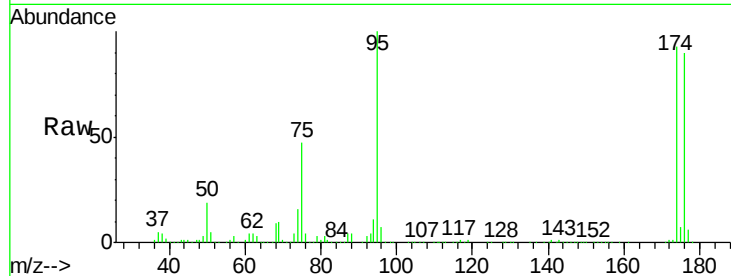


Abundance Ion 94.90 (94.60 to 95.60): VX001716.D (-1724) (-)

Ion 173.80 (173.50 to 174.50): VX001716.D (-1724) (-)

Ion 175.80 (175.50 to 176.50): VX001716.D (-1724) (-)

Time-->

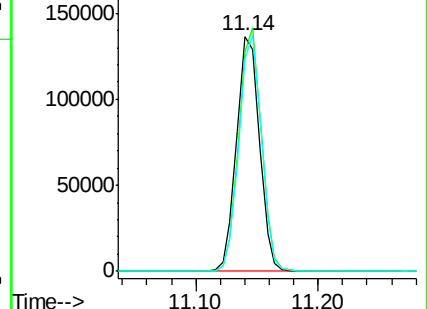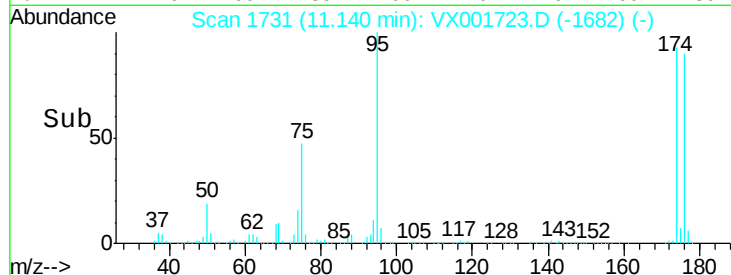

#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 10.12 min Scan# 1564

Delta R.T. 0.01 min

Lab File: VX001723.D

Acq: 14 May 2018 21:50


Tgt Ion: 117 Resp: 342880

Ion Ratio Lower Upper

117 100

82 49.5 41.4 62.2

119 32.6 25.6 38.4






Abundance Ion 116.90 (116.60 to 117.60): VX001716.D (-1555) (-)

Ion 82.00 (81.70 to 82.70): VX001716.D (-1555) (-)

Ion 118.90 (118.60 to 119.60): VX001716.D (-1555) (-)

Time-->

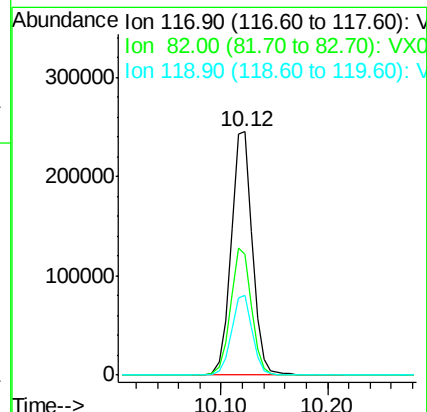


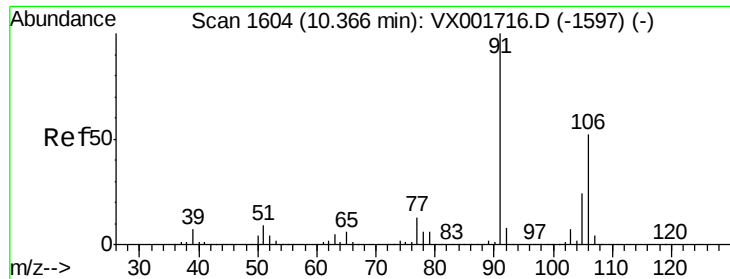




#68
m/p-Xylenes
Concen: 0.39 ug/l
RT: 10.37 min Scan# 1604
Delta R.T. -0.00 min
Lab File: VX001723.D
Acq: 14 May 2018 21:50

Instrument :
MSVOA_X
ClientSampleId :
FB050918

Tgt Ion:106 Resp: 2341
Ion Ratio Lower Upper
106 100
91 207.6 155.4 233.2

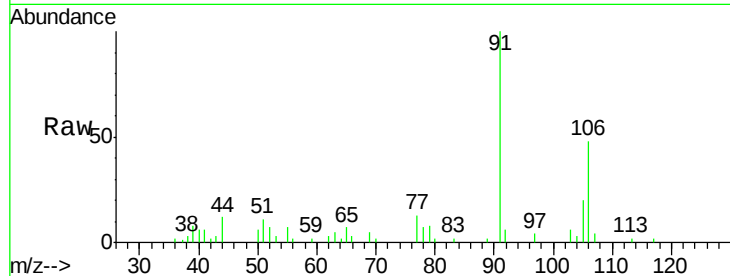


Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VX0


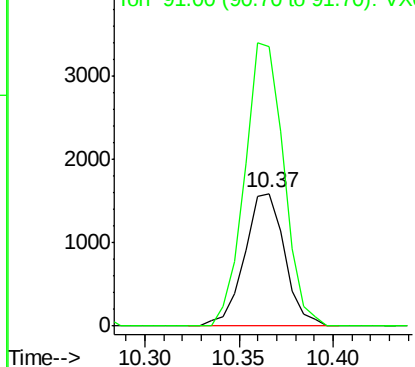



#71
Bromoform
Concen: 2.94 ug/l
RT: 10.85 min Scan# 1684
Delta R.T. -0.01 min
Lab File: VX001723.D
Acq: 14 May 2018 21:50

Tgt Ion:173 Resp: 51
Ion Ratio Lower Upper
173 100
175 0.0 24.3 72.8#
254 0.0 0.2 0.2#



Abundance Ion 172.70 (172.40 to 173.40): V
Ion 174.70 (174.40 to 175.40): V
Ion 254.40 (254.10 to 255.10): V

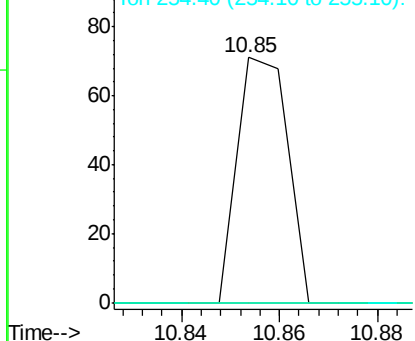



#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.09 min Scan# 1886

Delta R.T. -0.00 min

Lab File: VX001723.D

Acq: 14 May 2018 21:50

Instrument :

MSVOA_X

ClientSampleId :

FB050918


Tgt Ion:152 Resp: 190051

Ion Ratio Lower Upper

152 100

115 52.5 37.4 112.2




150 155.5 0.0 344.8

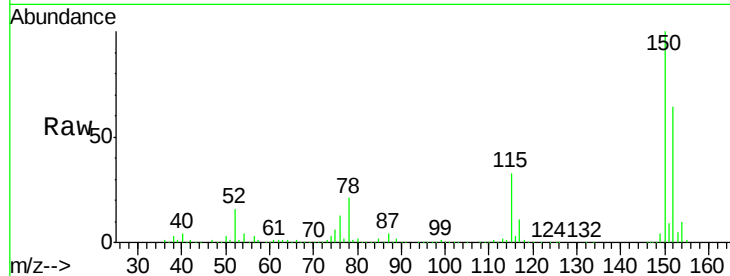

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

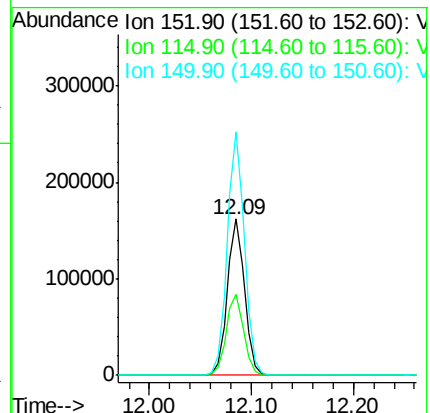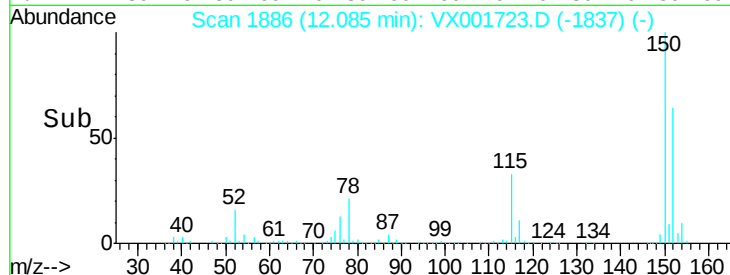

#76

1,2,3-Trichloropropane

Concen: 23.27 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.16 min

Lab File: VX001723.D


Acq: 14 May 2018 21:50

Tgt Ion: 75 Resp: 84085

Ion Ratio Lower Upper



75 100


77 1.3 18.9 56.7#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0



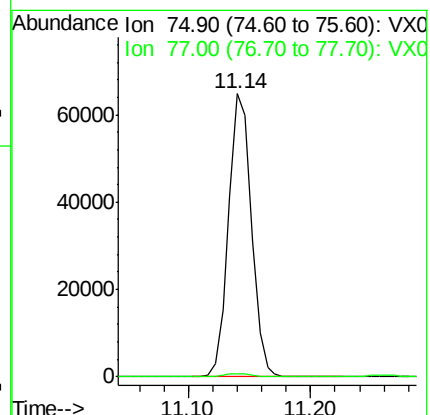



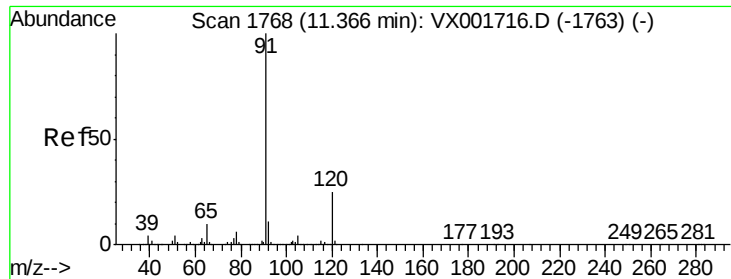

#78
n-propylbenzene
Concen: 0.21 ug/l
RT: 11.37 min Scan# 1768
Delta R.T. -0.00 min
Lab File: VX001723.D
Acq: 14 May 2018 21:50




Instrument :
MSVOA_X
ClientSampleId :
FB050918


Tgt Ion: 91 Resp: 2972
Ion Ratio Lower Upper
91 100
120 25.4 12.5 37.5

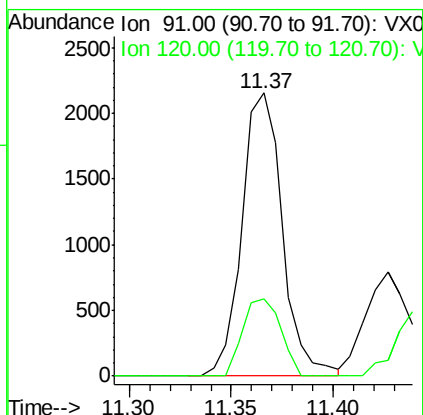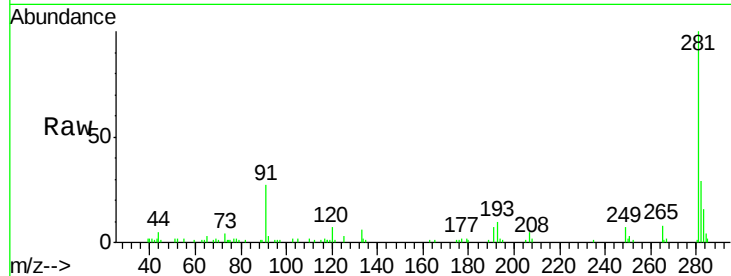

#80
1,3,5-Trimethylbenzene
Concen: 0.22 ug/l
RT: 11.51 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX001723.D
Acq: 14 May 2018 21:50

Tgt Ion: 105 Resp: 2210
Ion Ratio Lower Upper
105 100
120 46.9 25.7 77.0





#81

trans-1,4-Dichloro-2-butene

Concen: 68.06 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.06 min

Lab File: VX001723.D

Acq: 14 May 2018 21:50

Instrument :

MSVOA_X

ClientSampleId :

FB050918


Tgt Ion: 75 Resp: 84085

Ion Ratio Lower Upper

75 100

53 0.1 79.4 119.2#




89 0.0 38.8 58.2#

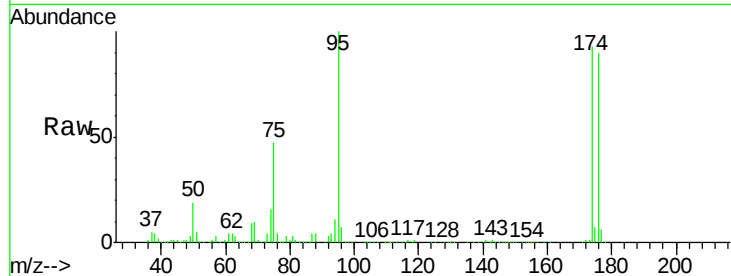

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

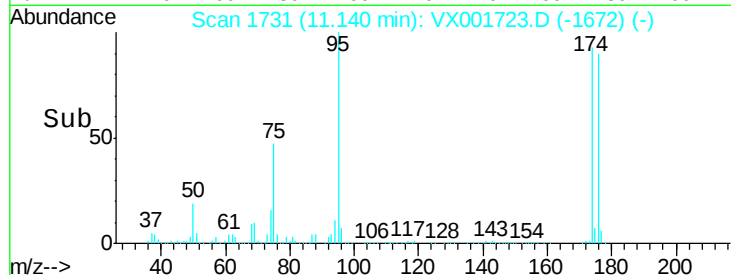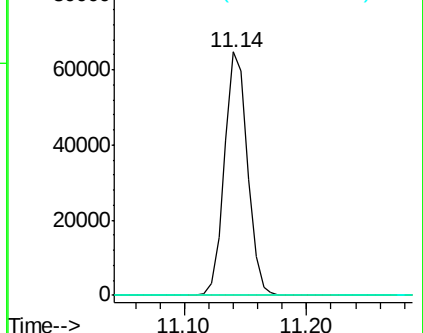

#82

4-Chlorotoluene

Concen: 0.21 ug/l

RT: 11.51 min Scan# 1792

Delta R.T. -0.01 min

Lab File: VX001723.D


Acq: 14 May 2018 21:50

Tgt Ion: 91 Resp: 2120

Ion Ratio Lower Upper



91 100


126 31.4 16.4 49.1



Abundance Ion 91.00 (90.70 to 91.70): VX0

Ion 125.90 (125.60 to 126.60): V



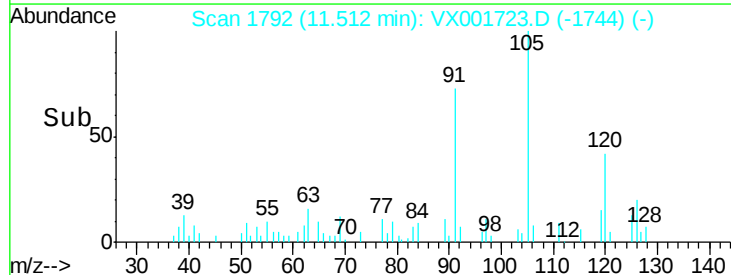
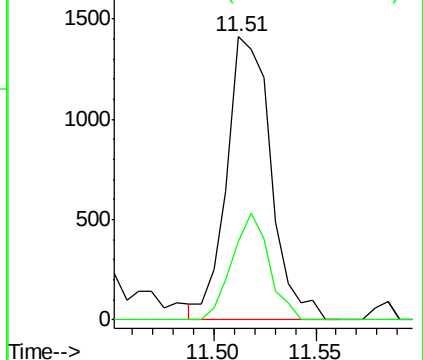


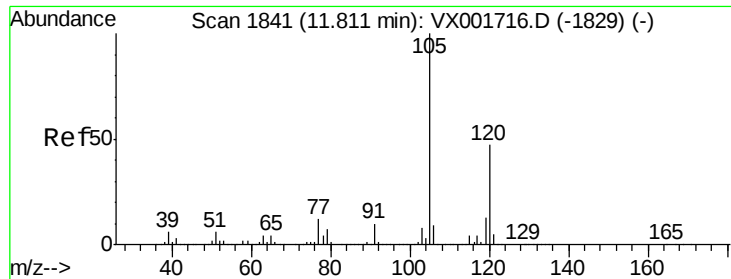

#84
 1,2,4-Trimethylbenzene
 Concen: 0.39 ug/l
 RT: 11.81 min Scan# 1841
 Delta R.T. -0.00 min
 Lab File: VX001723.D
 Acq: 14 May 2018 21:50




Instrument :
 MSVOA_X
 ClientSampleId :
 FB050918


Tgt Ion:105 Resp: 4188
 Ion Ratio Lower Upper
 105 100
 120 49.9 23.5 70.5

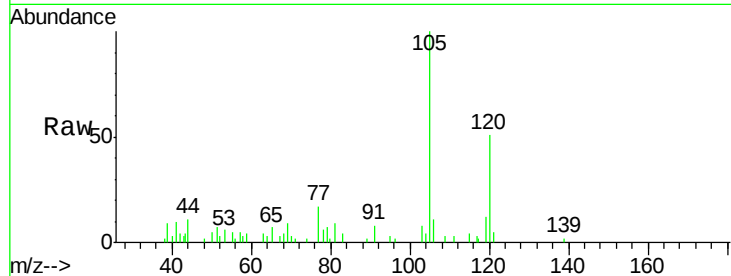

#87
 1,3-Dichlorobenzene
 Concen: 0.28 ug/l
 RT: 12.03 min Scan# 1877
 Delta R.T. -0.00 min
 Lab File: VX001723.D
 Acq: 14 May 2018 21:50

Tgt Ion:146 Resp: 1903
 Ion Ratio Lower Upper
 146 100
 111 42.9 17.8 53.4
 148 61.3 32.1 96.3



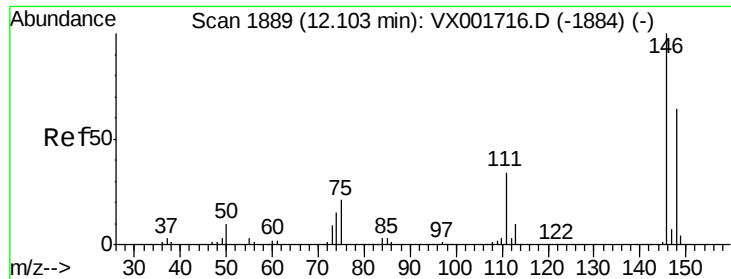

#88

1,4-Dichlorobenzene

Concen: 0.27 ug/l

RT: 12.03 min Scan# 1877

Delta R.T. -0.07 min

Lab File: VX001723.D

Acq: 14 May 2018 21:50

Instrument :

MSVOA_X

ClientSampleId :

FB050918


Tgt Ion:146 Resp: 1903

Ion Ratio Lower Upper

146 100

111 42.9 17.3 52.0




148 61.3 32.3 96.9



Abundance Ion 145.90 (145.60 to 146.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 147.90 (147.60 to 148.60): V

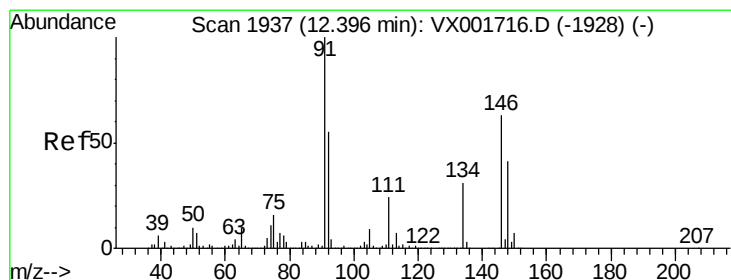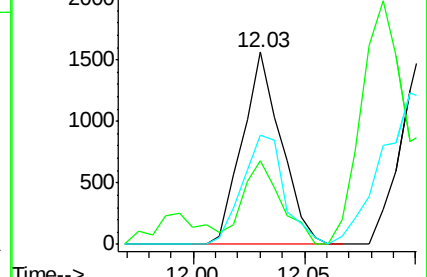

#89

n-Butylbenzene

Concen: 0.31 ug/l

RT: 12.40 min Scan# 1937

Delta R.T. -0.00 min

Lab File: VX001723.D

Acq: 14 May 2018 21:50


Tgt Ion: 91 Resp: 3107

Ion Ratio Lower Upper

91 100

92 46.5 27.3 81.9



134 38.0 14.7 44.1




Abundance Ion 91.00 (90.70 to 91.70): VX0

Ion 92.00 (91.70 to 92.70): VX0

Ion 134.00 (133.70 to 134.70): V




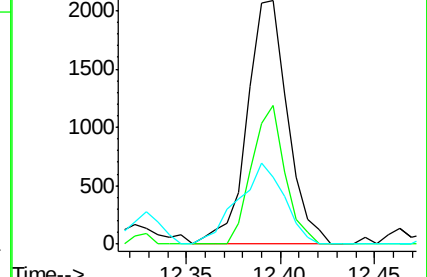




#93
 1,2,4-Trichlorobenzene
 Concen: 0.39 ug/l
 RT: 13.65 min Scan# 2143
 Delta R.T. -0.00 min
 Lab File: VX001723.D
 Acq: 14 May 2018 21:50




Instrument :
 MSVOA_X
 ClientSampleId :
 FB050918


Tgt Ion:180 Resp: 2124
 Ion Ratio Lower Upper
 180 100
 182 94.7 47.6 142.9
 145 27.2 13.4 40.1

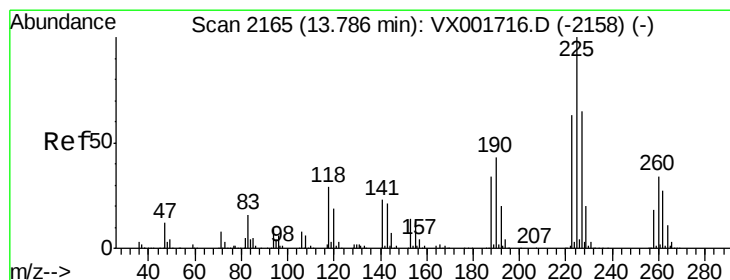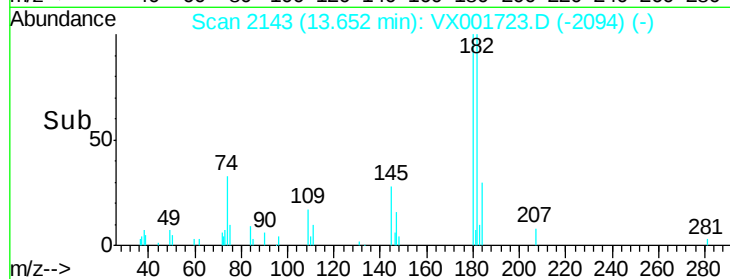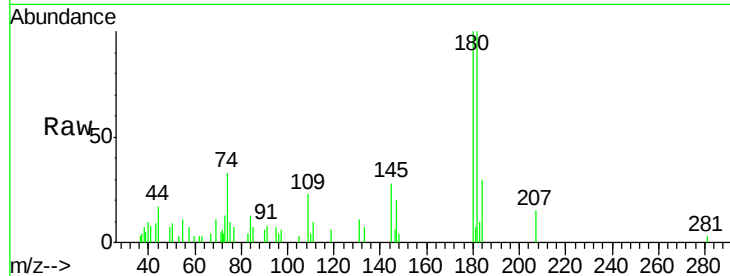

#94
 Hexachlorobutadiene
 Concen: 0.31 ug/l
 RT: 13.79 min Scan# 2165
 Delta R.T. -0.00 min
 Lab File: VX001723.D
 Acq: 14 May 2018 21:50

Tgt Ion:225 Resp: 904
 Ion Ratio Lower Upper
 225 100
 223 51.1 31.1 93.5
 227 53.3 31.9 95.5

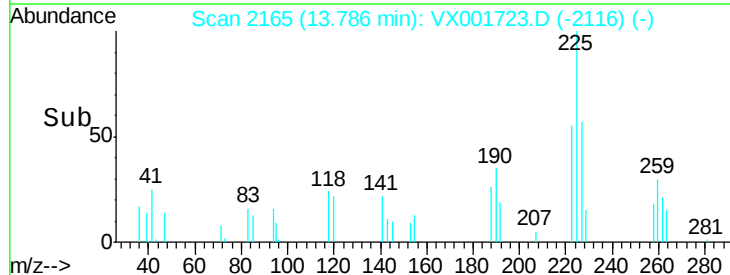

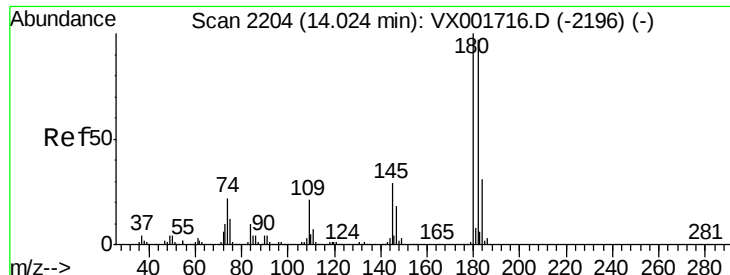

#96
 1,2,3-Trichlorobenzene
 Concen: 0.23 ug/l
 RT: 14.02 min Scan# 2204
 Delta R.T. -0.00 min
 Lab File: VX001723.D
 Acq: 14 May 2018 21:50

Instrument :
 MSVOA_X
 ClientSampleId :
 FB050918

Tgt Ion	Ratio	Lower	Upper
180	100		
182	95.4	47.9	143.7
145	33.3	14.2	42.8

