



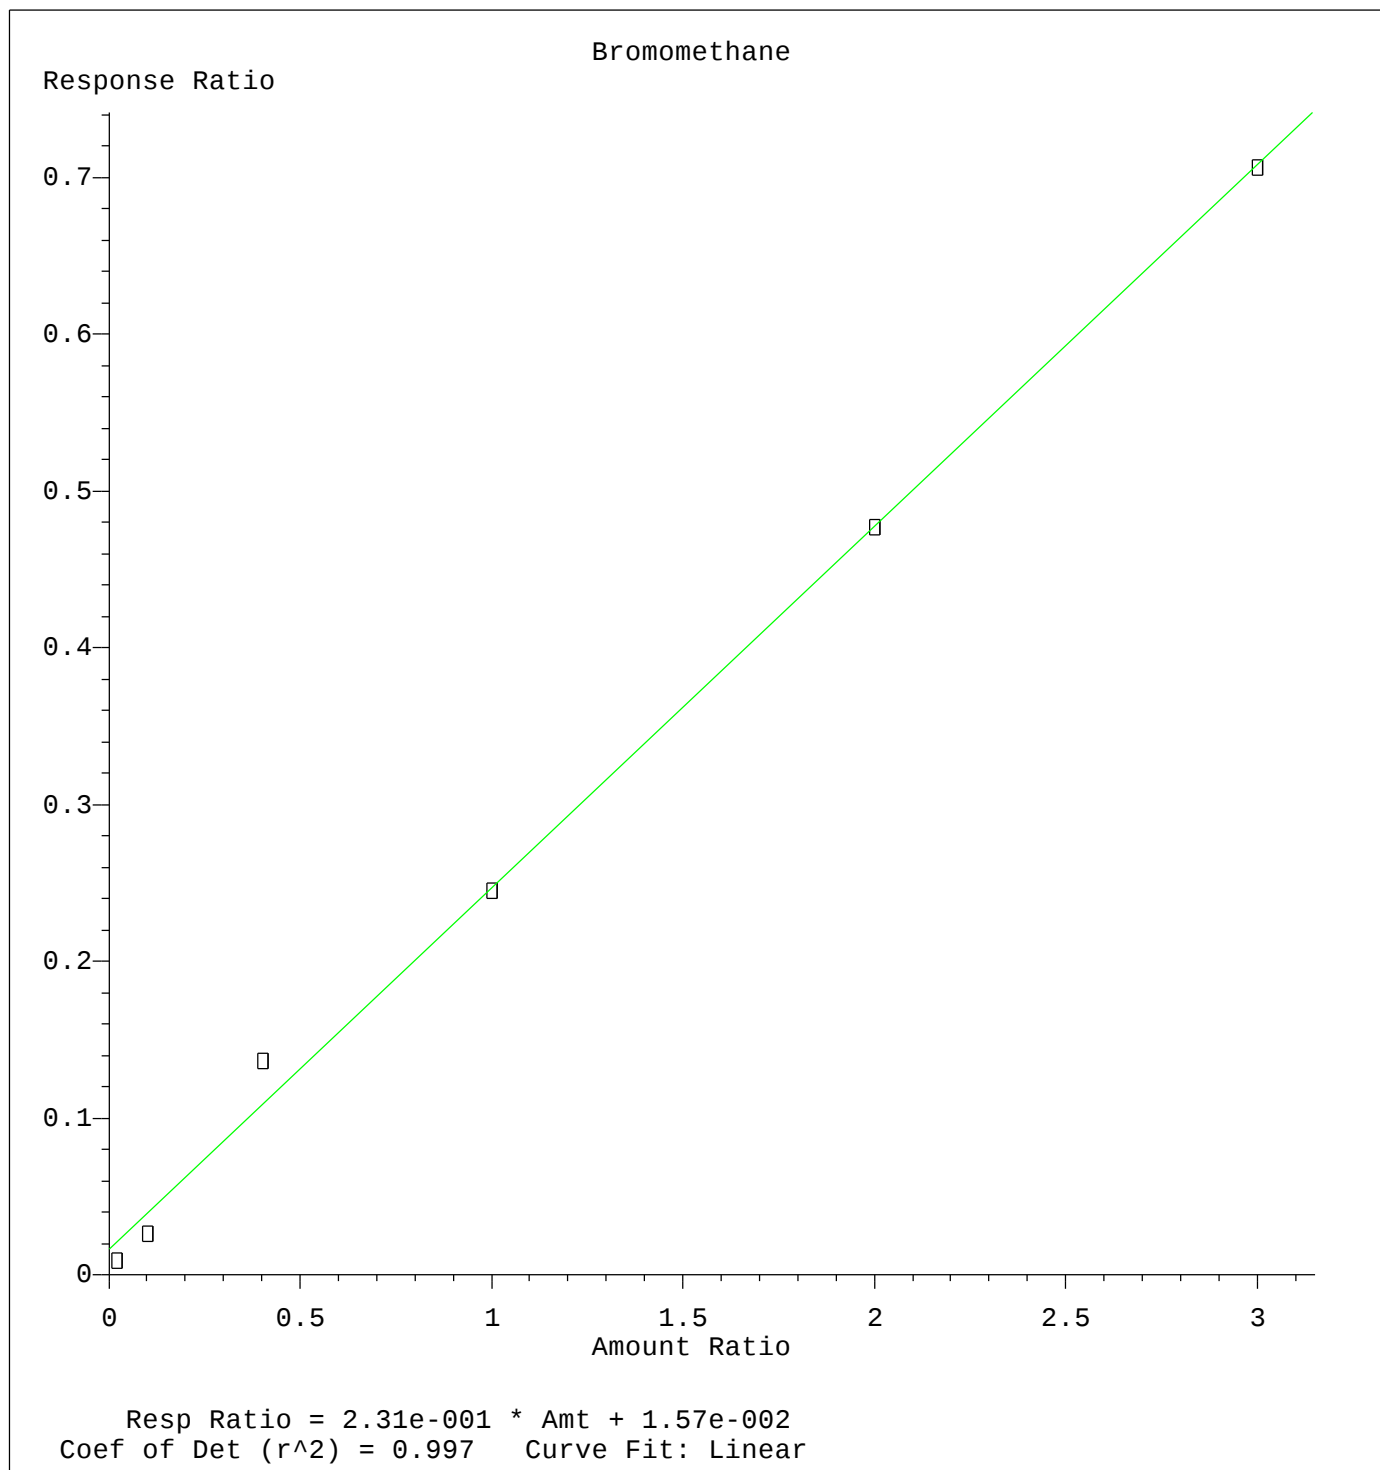

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X051518W.M
Calibration Table Last Updated: Tue May 15 01:36:22 2018


trans-1,4-Dichloro-2-butene

Response Ratio

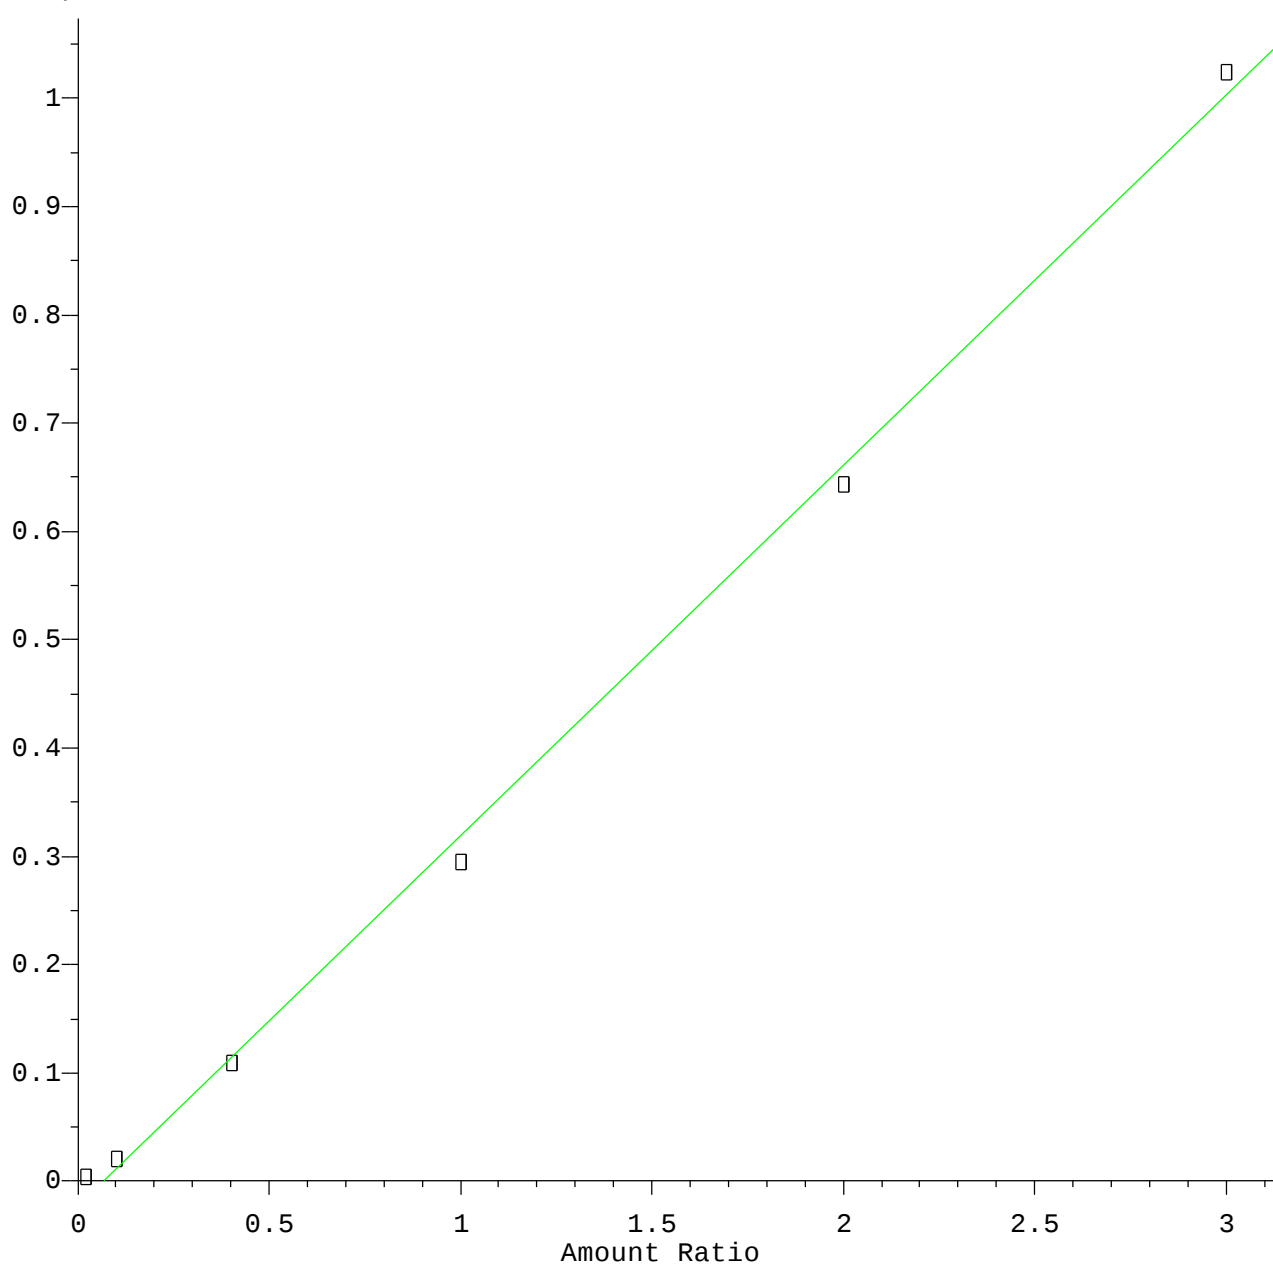

Resp Ratio = $3.42 \times 10^{-1} \times \text{Amt} - 2.26 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X051518W.M
Calibration Table Last Updated: Tue May 15 01:36:22 2018

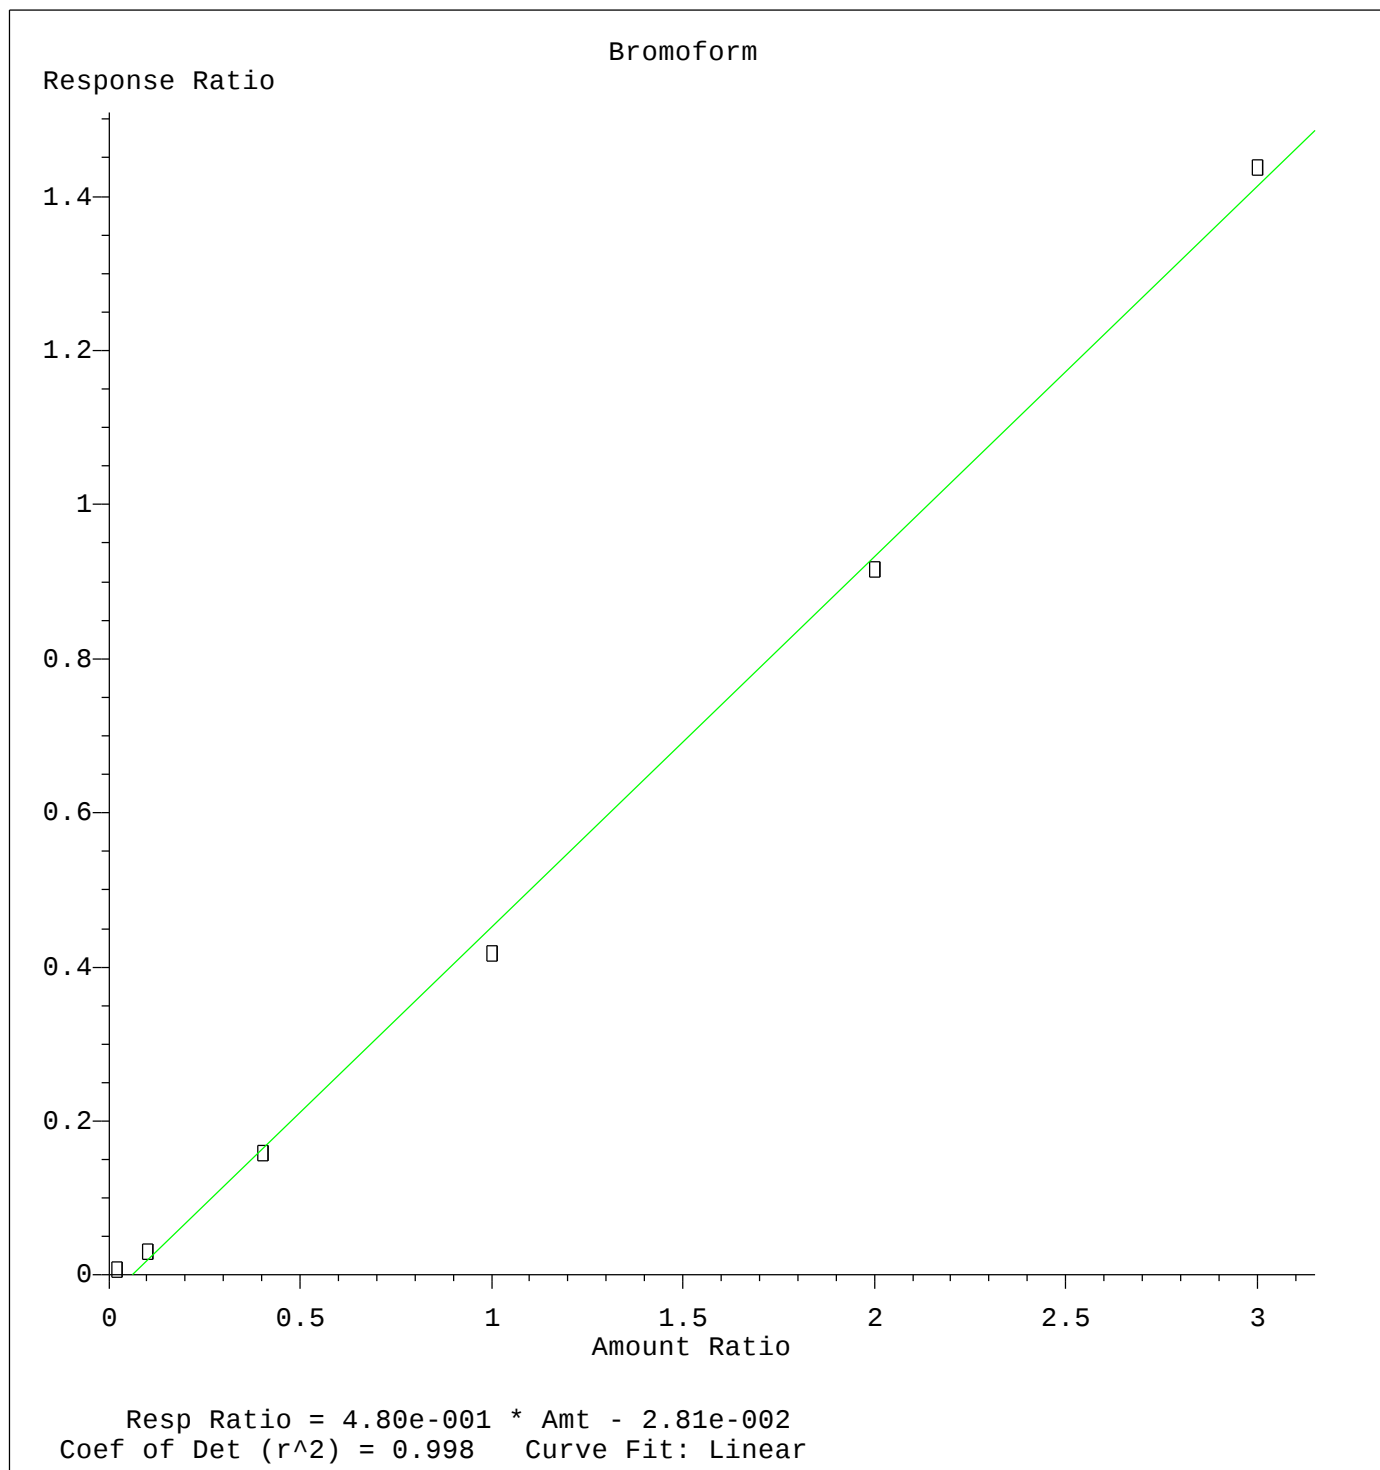

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X051518W.M
Calibration Table Last Updated: Tue May 15 01:36:22 2018