


Data Path : W:\HPCHEM1\MSVOA X\DATA\VX051518\
Data File : VX001711.D
Acq On : 14 May 2018 14:27
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X051518W.M
Title : SW846 8260
Last Update : Tue May 15 01:36:22 2018

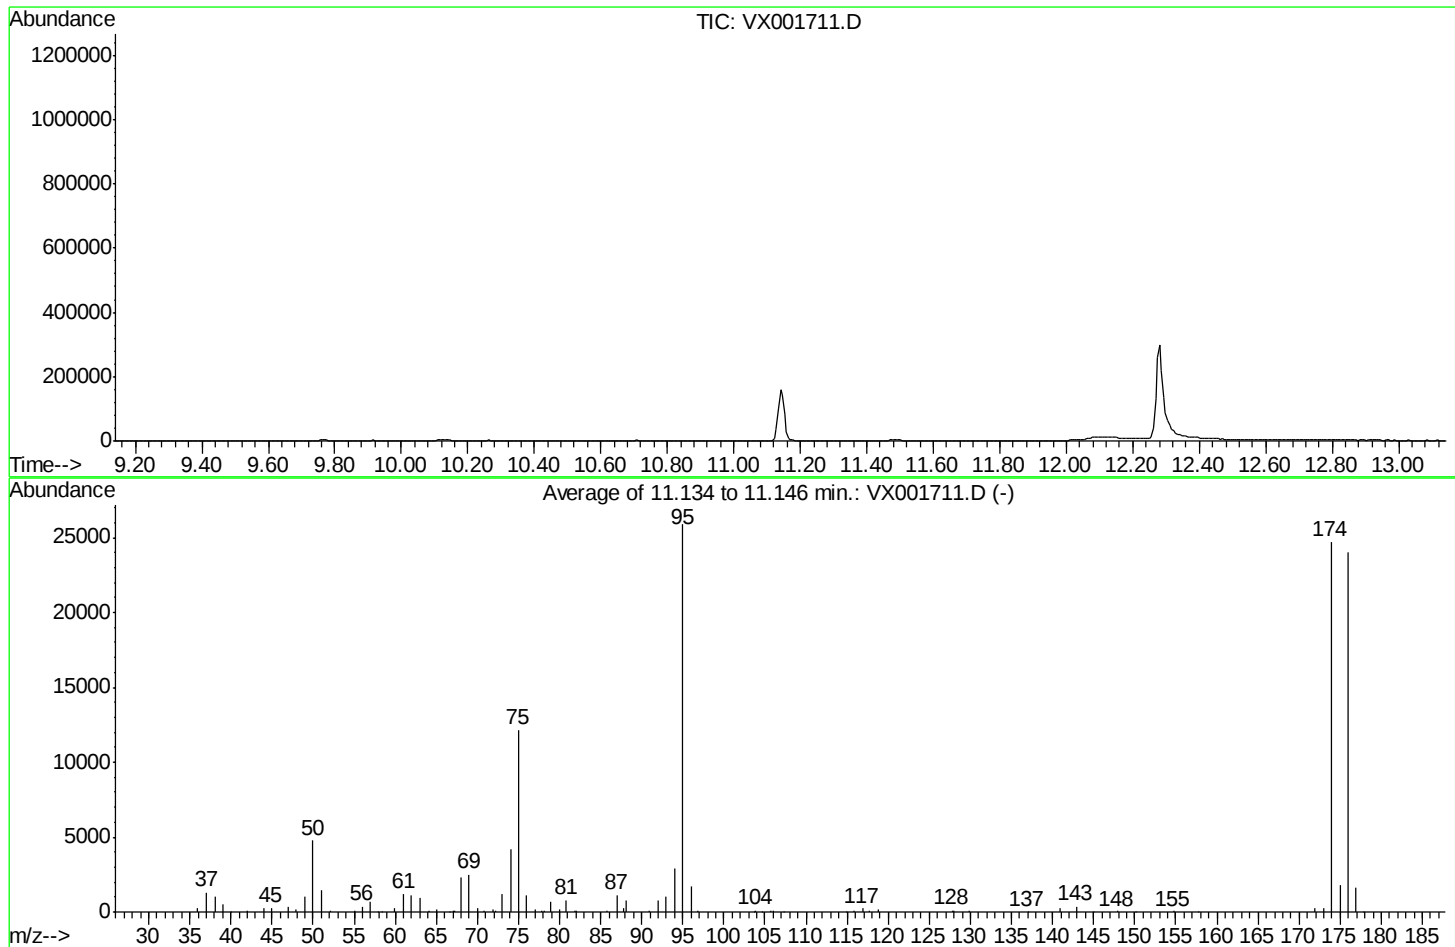

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	4775	PASS
75	95	30	60	46.9	12147	PASS
95	95	100	100	100.0	25885	PASS
96	95	5	9	6.8	1753	PASS
173	174	0.00	2	1.2	293	PASS
174	95	50	100	95.6	24736	PASS
175	174	5	9	7.4	1836	PASS
176	174	95	101	97.0	24002	PASS
177	176	5	9	6.9	1651	PASS