


Data Path : W:\HPCHEM1\MSVOA X\DATA\VX051818\
 Data File : VX001804.D
 Acq On : 18 May 2018 02:45
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\624X051818W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri May 18 10:06:03 2018

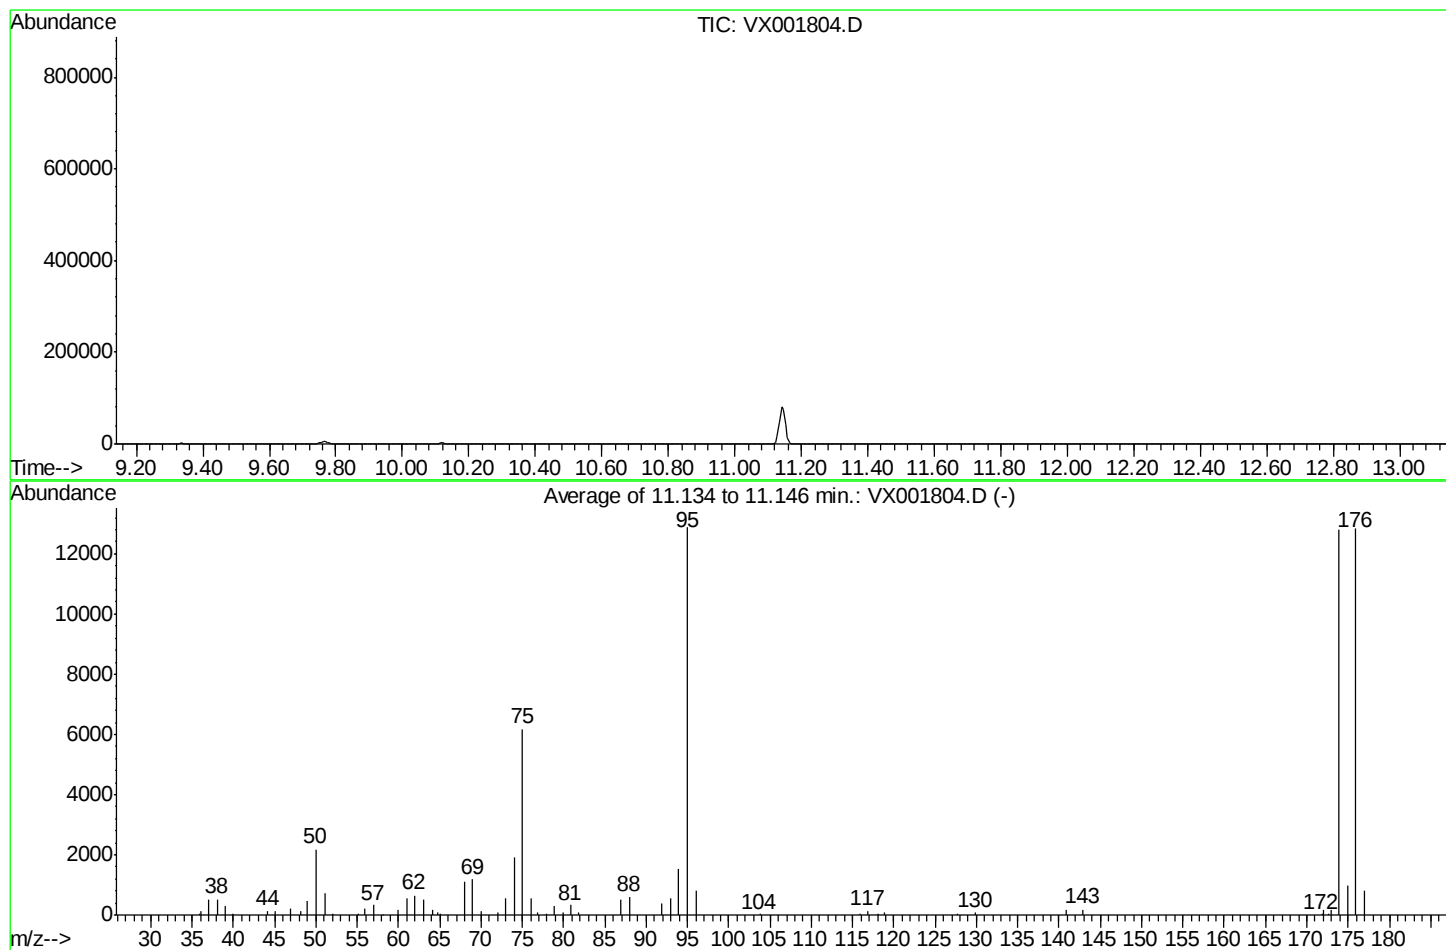

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	2188	PASS
75	95	30	60	48.0	6185	PASS
95	95	100	100	100.0	12880	PASS
96	95	5	9	6.4	824	PASS
173	174	0.00	2	1.4	180	PASS
174	95	50	100	99.5	12817	PASS
175	174	5	9	7.8	995	PASS
176	174	95	101	100.3	12852	PASS
177	176	5	9	6.4	822	PASS