


Data Path : W:\HPCHEM1\MSVOA X\DATA\VX051818\
Data File : VX001820.D
Acq On : 18 May 2018 11:57
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X051518W.M
Title : SW846 8260
Last Update : Tue May 15 01:36:22 2018

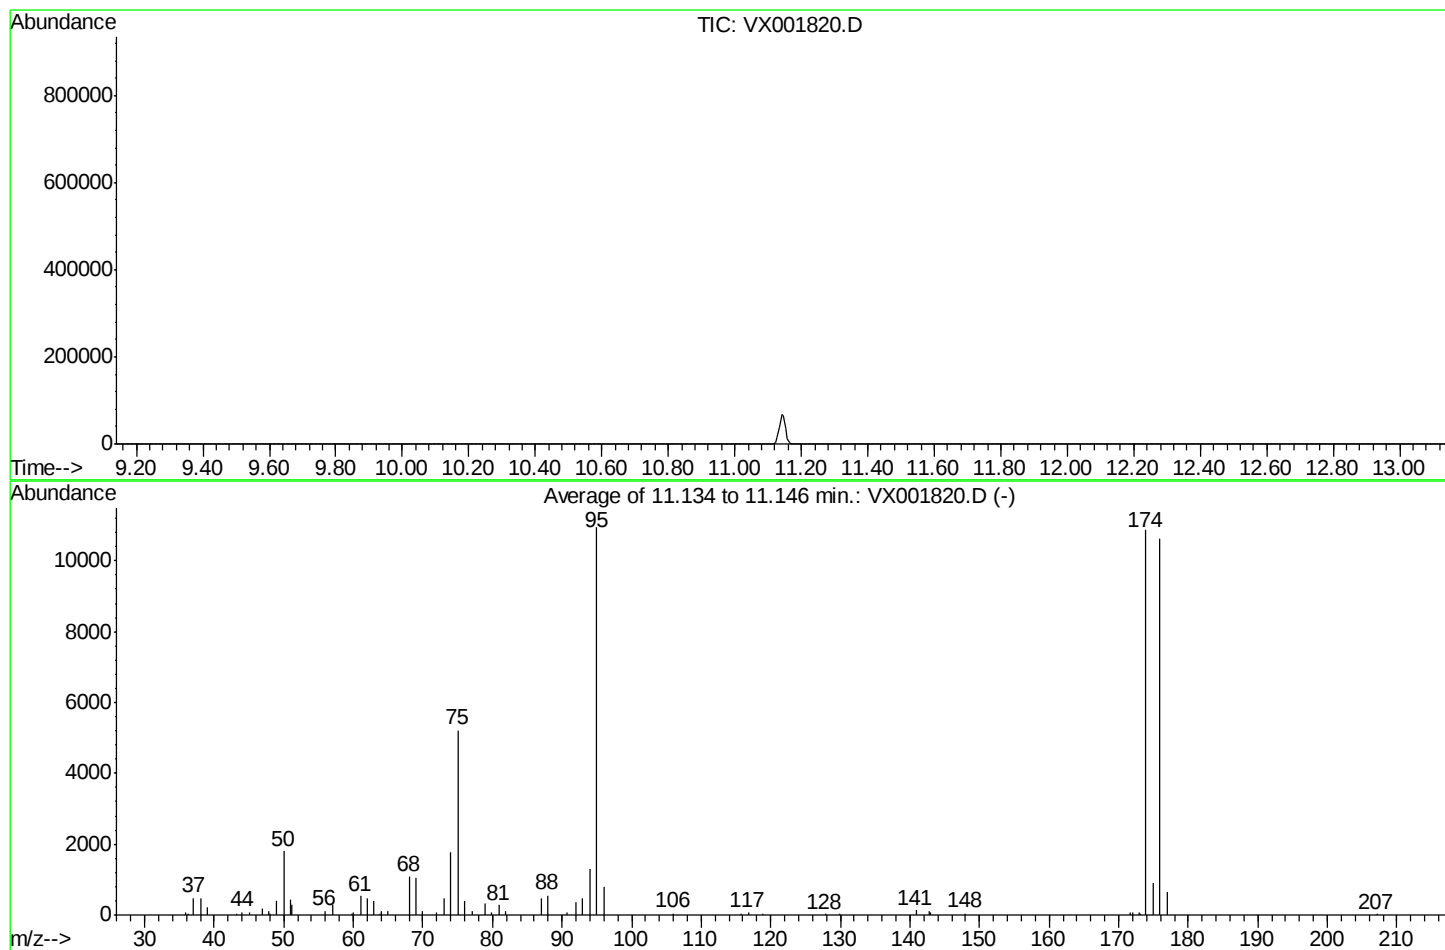

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	1795	PASS
75	95	30	60	47.6	5216	PASS
95	95	100	100	100.0	10947	PASS
96	95	5	9	7.2	785	PASS
173	174	0.00	2	0.8	82	PASS
174	95	50	100	99.3	10866	PASS
175	174	5	9	8.3	906	PASS
176	174	95	101	98.0	10644	PASS
177	176	5	9	6.0	638	PASS