


Data Path : W:\HPCHEM1\MSVOA X\DATA\VX051818\
Data File : VX001844.D
Acq On : 18 May 2018 23:21
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X051518W.M
Title : SW846 8260
Last Update : Tue May 15 01:36:22 2018

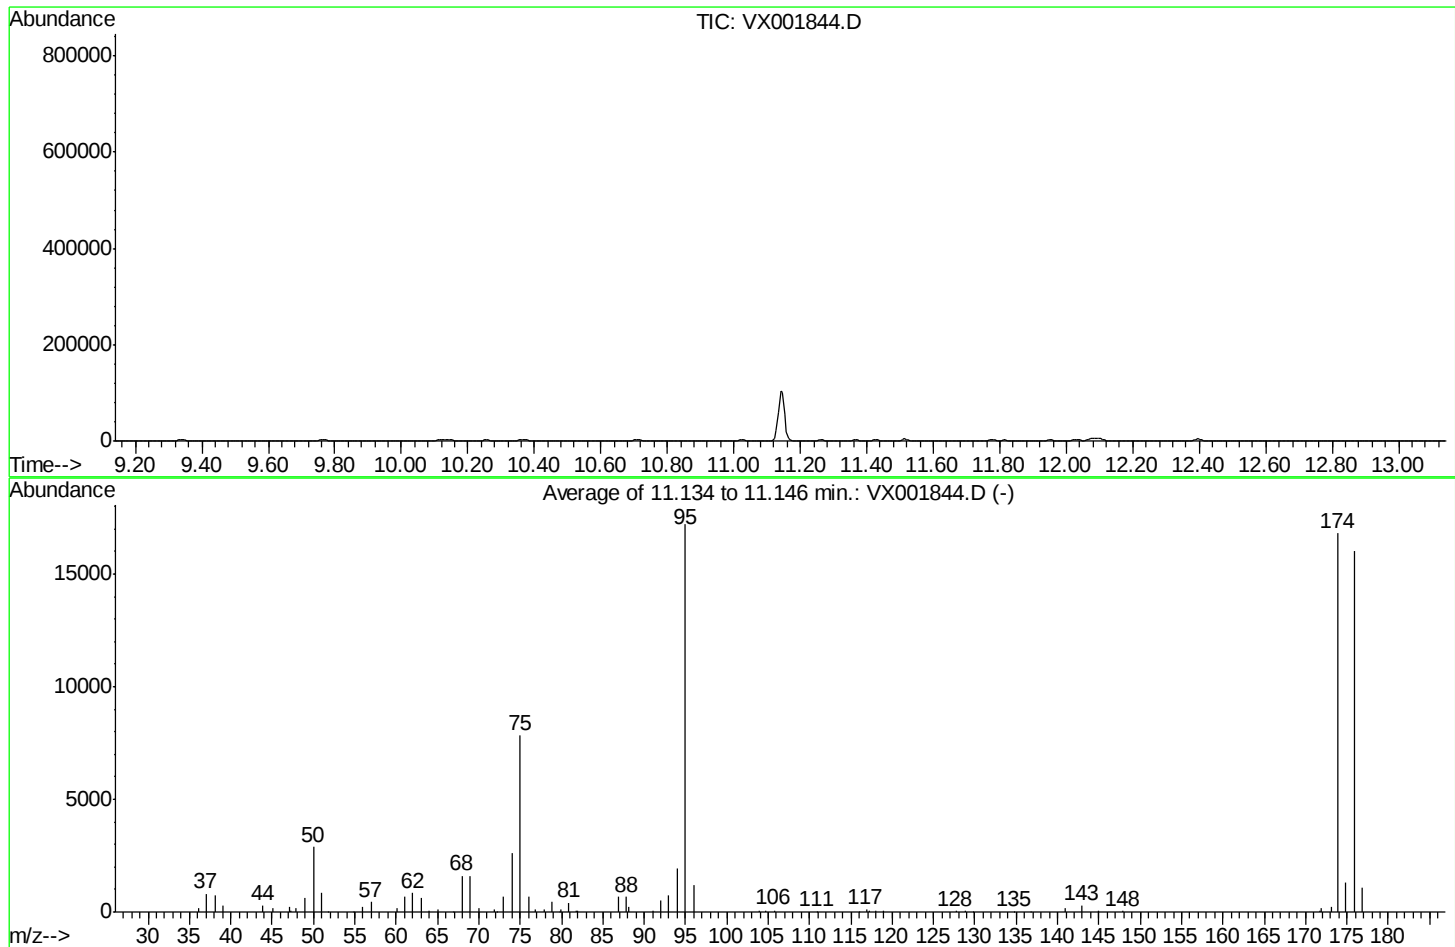

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	2890	PASS
75	95	30	60	45.6	7841	PASS
95	95	100	100	100.0	17210	PASS
96	95	5	9	7.1	1218	PASS
173	174	0.00	2	1.2	203	PASS
174	95	50	100	97.6	16800	PASS
175	174	5	9	7.7	1287	PASS
176	174	95	101	95.2	16001	PASS
177	176	5	9	6.9	1107	PASS