

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX052119\
 Data File : VX009789.D
 Acq On : 22 May 2019 08:30
 Operator : JC/SP
 Sample : K2910-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S73-0224

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.300	20	24	34	rVB	15201	18853	1.96%	0.357%
2	1.404	34	41	47	rBV2	70954	120276	12.52%	2.276%
3	1.465	47	51	57	rVV	24866	29599	3.08%	0.560%
4	1.532	58	62	68	rVV	33292	36793	3.83%	0.696%
5	1.611	68	75	81	rVV	6213	13482	1.40%	0.255%
6	1.696	85	89	99	rVB	15000	23937	2.49%	0.453%
7	1.794	99	105	111	rBV	18647	26925	2.80%	0.509%
8	1.952	127	131	135	rBV	21111	28475	2.96%	0.539%
9	2.001	135	139	148	rVB	21545	34269	3.57%	0.648%
10	2.117	153	158	166	rVB	17062	23477	2.44%	0.444%
11	2.215	169	174	179	rVB	12898	18125	1.89%	0.343%
12	2.605	229	238	245	rBV	11066	21353	2.22%	0.404%
13	2.812	259	272	280	rBV6	11955	42251	4.40%	0.799%
14	5.501	698	713	726	rBV	100793	292407	30.44%	5.533%
15	5.659	729	739	757	rVB	179464	514534	53.57%	9.736%
16	6.061	795	805	817	rBV	127406	337052	35.09%	6.378%
17	6.860	925	936	951	rBV	291826	689879	71.83%	13.054%
18	8.561	1209	1215	1222	rVB6	4799	10906	1.14%	0.206%
19	8.713	1231	1240	1249	rBV	616637	960487	100.00%	18.174%
20	10.109	1461	1469	1481	rBV	574889	788296	82.07%	14.916%
21	11.134	1632	1637	1647	rBV	465150	589027	61.33%	11.145%
22	12.073	1786	1791	1798	rBV	512748	664534	69.19%	12.574%


Sum of corrected areas: 5284937

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX052119\
Data File : VX009789.D
Acq On : 22 May 2019 08:30
Operator : JC/SP
Sample : K2910-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S73-0224

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

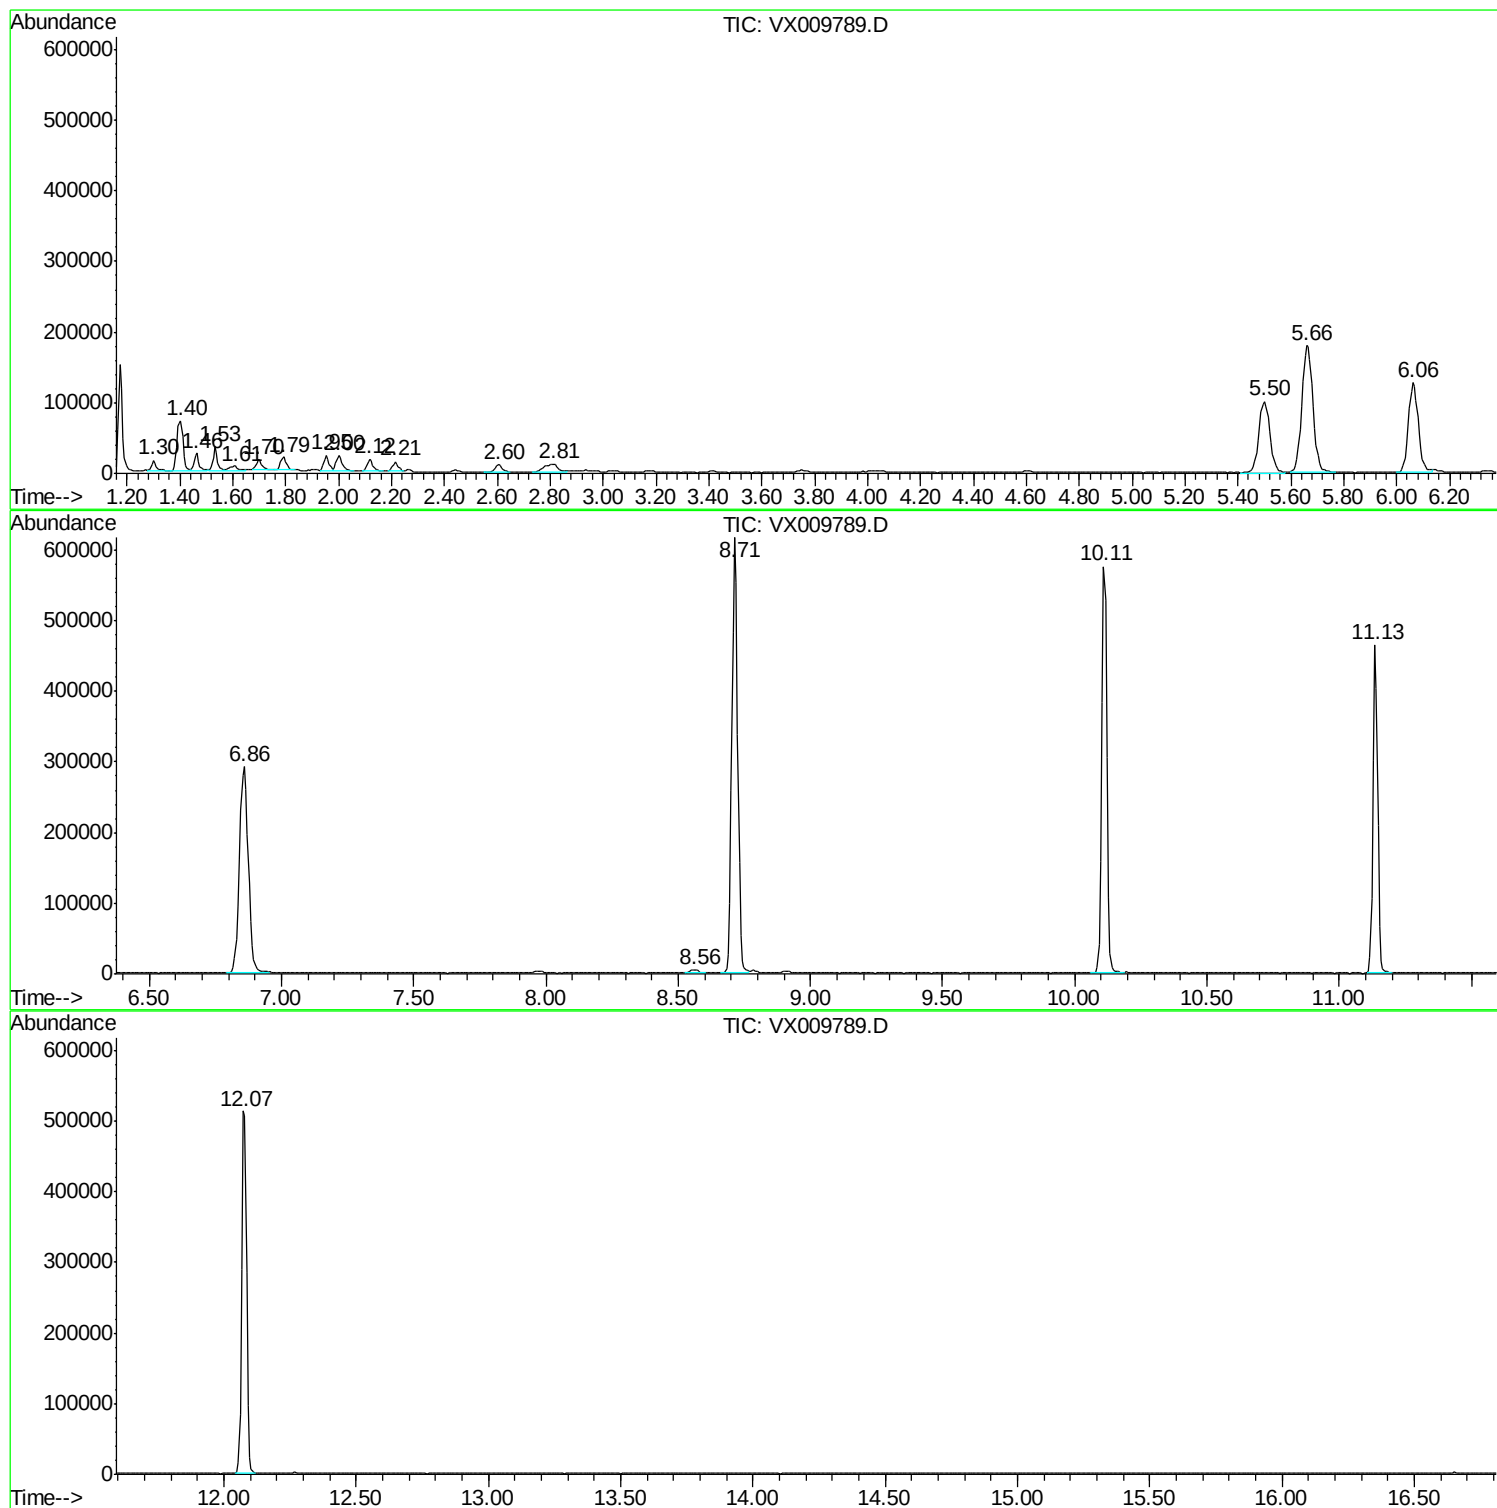

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX052119\
Data File : VX009789.D
Acq On : 22 May 2019 08:30
Operator : JC/SP
Sample : K2910-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S73-0224

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX052119\
Data File : VX009789.D
Acq On : 22 May 2019 08:30
Operator : JC/SP
Sample : K2910-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S73-0224

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc