


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX052119\
Data File : VX009769.D
Acq On : 21 May 2019 23:58
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Title : SW846 8260
Last Update : Thu May 09 07:31:15 2019

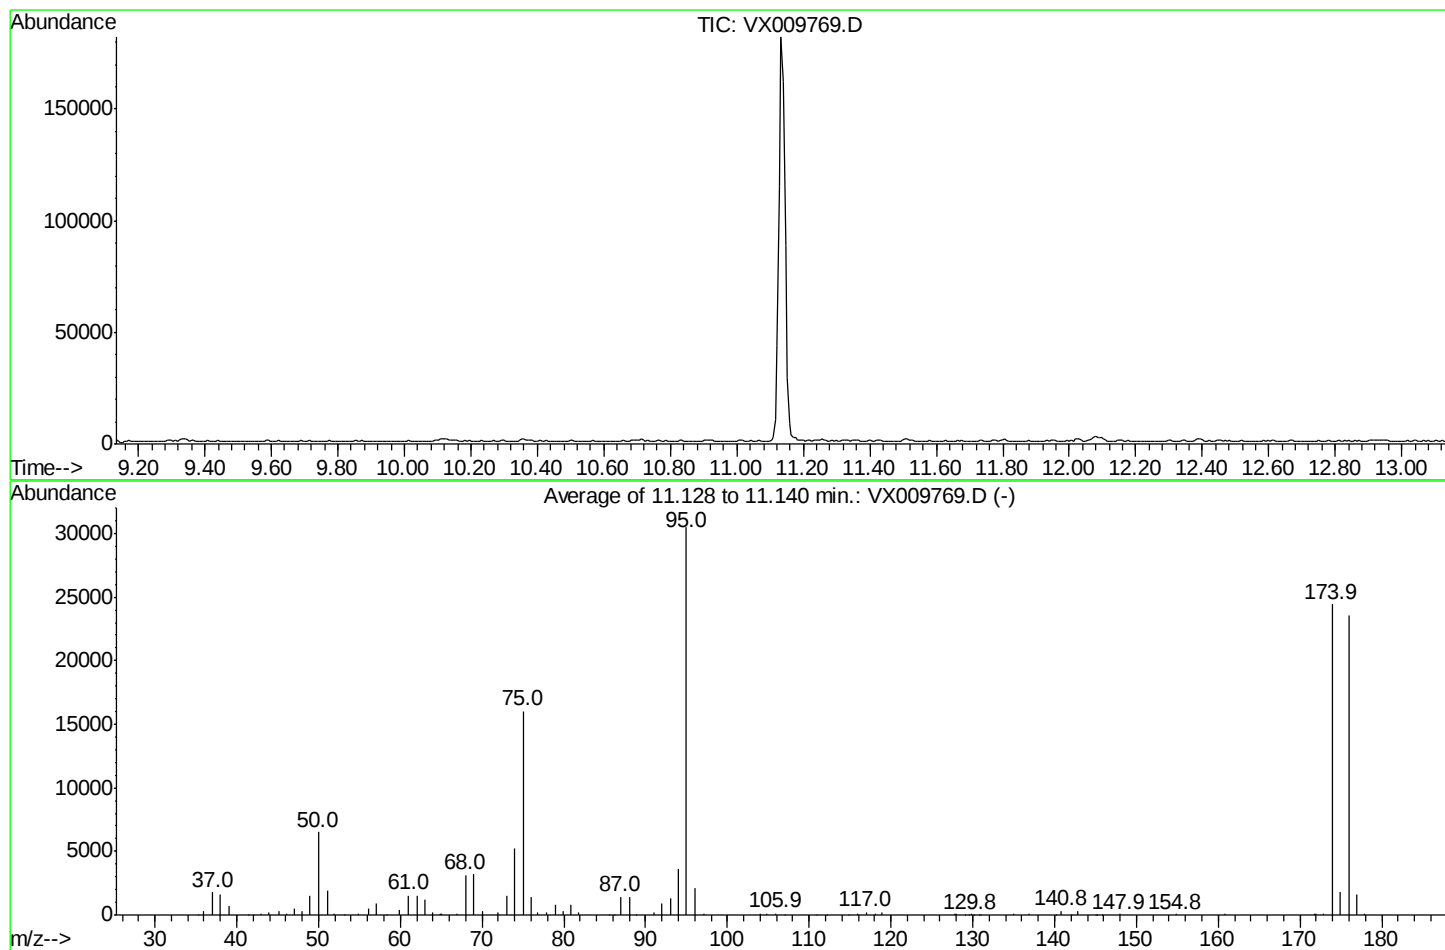

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	6497	PASS
75	95	30	60	52.7	16054	PASS
95	95	100	100	100.0	30485	PASS
96	95	5	9	7.0	2121	PASS
173	174	0.00	2	0.3	67	PASS
174	95	50	100	80.2	24448	PASS
175	174	5	9	7.5	1839	PASS
176	174	95	101	96.4	23572	PASS
177	176	5	9	7.0	1648	PASS