

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX052218\
 Data File : VX001926.D
 Acq On : 23 May 2018 06:19
 Operator : JC/MD
 Sample : PB109456ZHE#06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB109456ZHE#06

Quant Time: May 23 06:57:35 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X051518W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 15 01:36:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	248741	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	336484	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	278712	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	153724	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.08	65	156828	47.04	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.08%	
35) Dibromofluoromethane	5.51	113	130586	45.99	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.98%	
50) Toluene-d8	8.72	98	478019	47.00	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.00%	
62) 4-Bromofluorobenzene	11.14	95	139452	38.08	ug/l	0.00
Spiked Amount 50.000			Recovery	=	76.16%	
Target Compounds						
16) Acetone	2.45	43	8895	6.79	ug/l	96
18) Methyl Acetate	2.78	43	23335	6.10	ug/l	99
20) Methylene Chloride	2.86	84	6389	2.28	ug/l	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX052218\
Data File : VX001926.D
Acq On : 23 May 2018 06:19
Operator : JC/MD
Sample : PB109456ZHE#06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB109456ZHE#06

Quant Time: May 23 06:57:35 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X051518W.M
Quant Title : SW846 8260
QLast Update : Tue May 15 01:36:22 2018
Response via : Initial Calibration

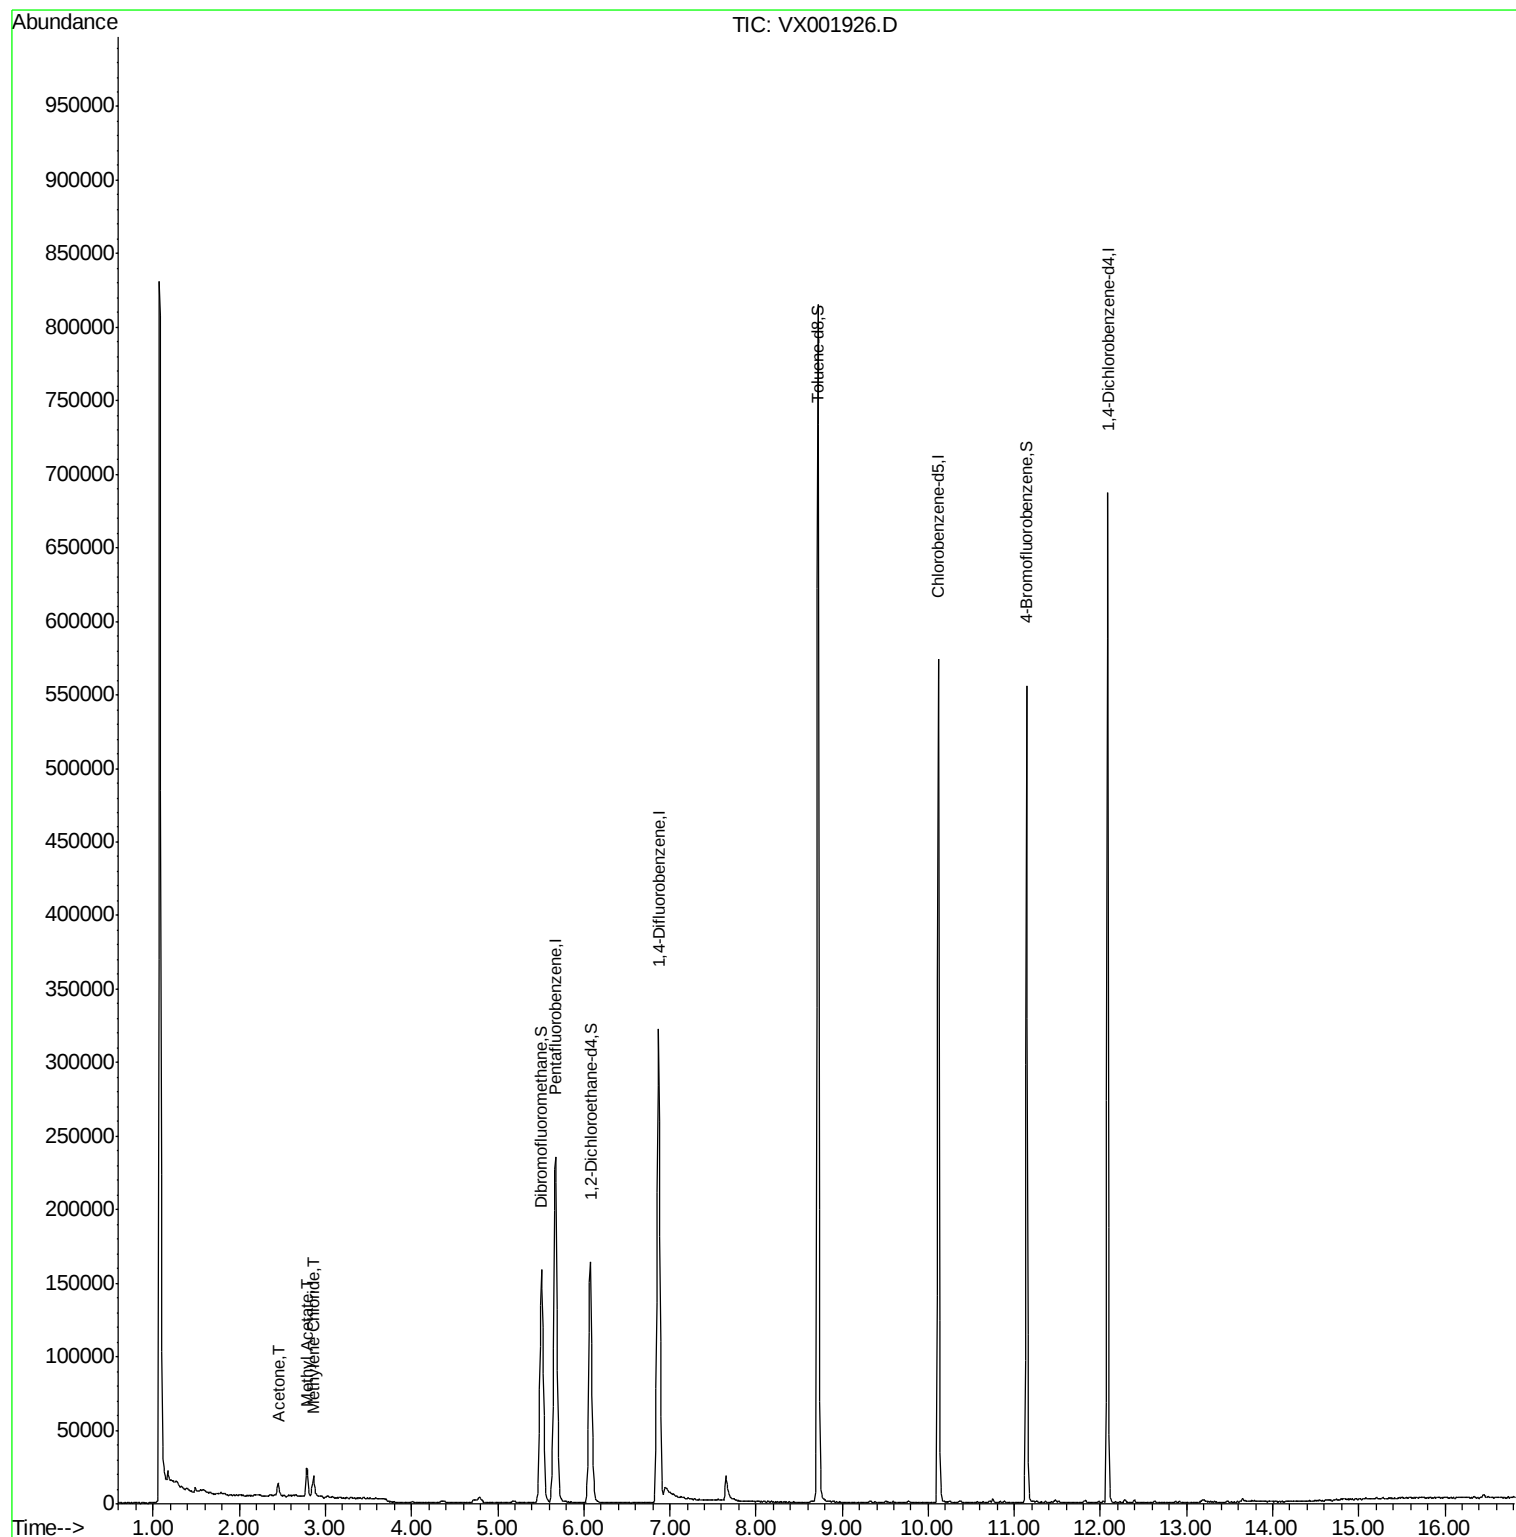



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.00 min

Lab File: VX001926.D

Acq: 23 May 2018 06:19

Instrument :

MSVOA_X

ClientSampleId :


PB109456ZHE#06

Tot Ion:168 Resp: 248741

Ion Ratio Lower Upper

168 100

99 47.5 35.0 52.4

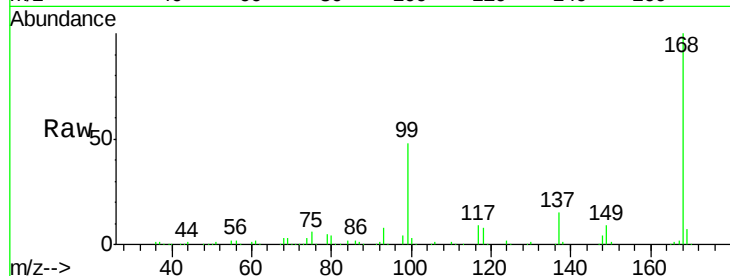

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

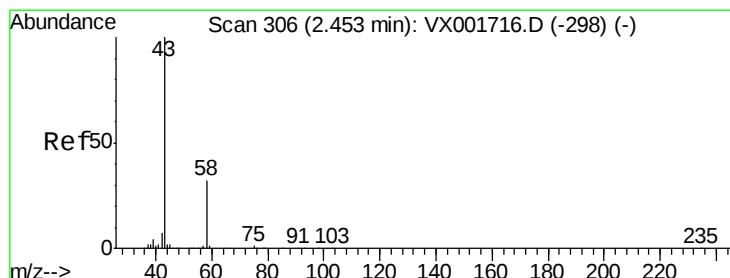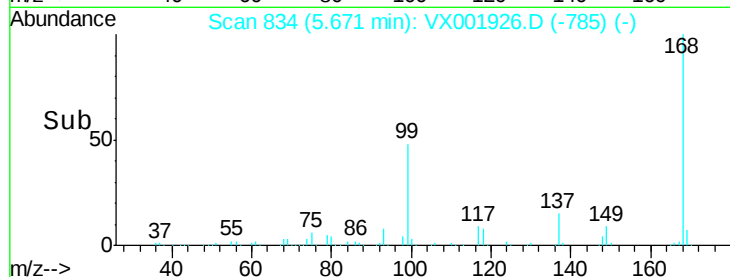

#16

Acetone

Concen: 6.79 ug/l

RT: 2.45 min Scan# 306

Delta R.T. -0.00 min

Lab File: VX001926.D


Acq: 23 May 2018 06:19

Tgt Ion: 43 Resp: 8895

Ion Ratio Lower Upper

43 100

58 33.8 25.3 37.9

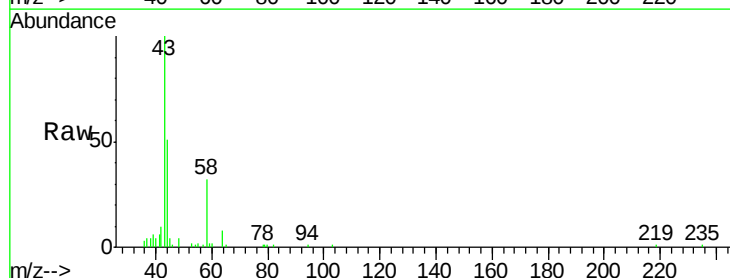

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.45

6000

5000

4000


3000


2000

1000

0

Time--> 2.40 2.45 2.50




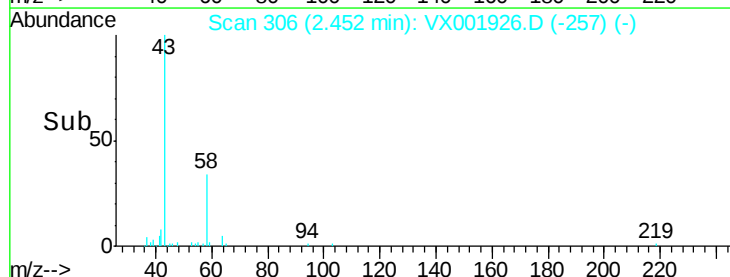


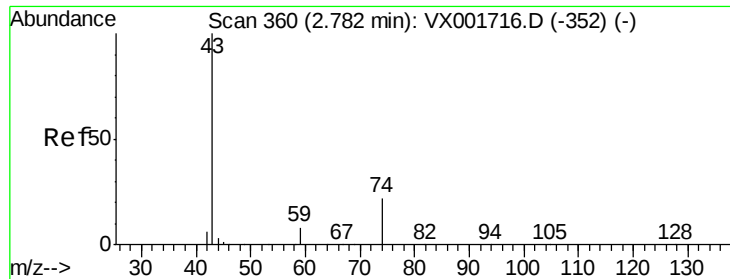

#18
Methvl Acetate
Concen: 6.10 ug/l
RT: 2.78 min Scan# 360
Delta R.T. -0.00 min
Lab File: VX001926.D
Acq: 23 May 2018 06:19




Instrument :
MSVOA_X
ClientSampleId :
PB109456ZHE#06


Tot Ion: 43 Resp: 23335
Ion Ratio Lower Upper
43 100
74 23.0 18.2 27.2

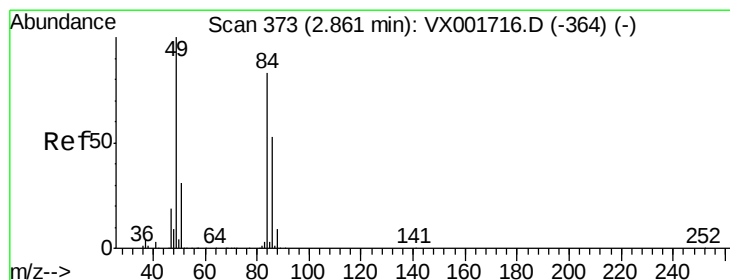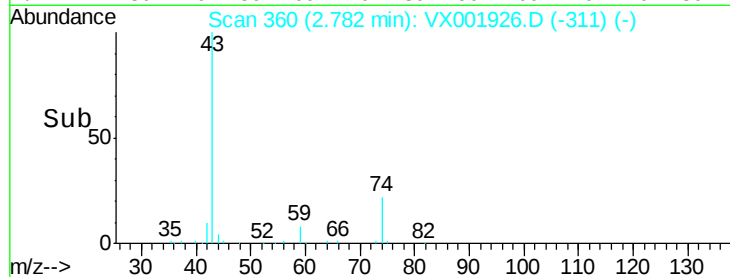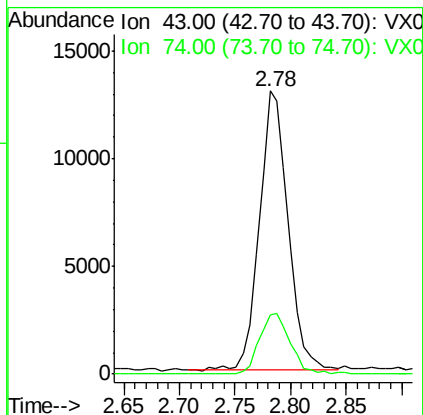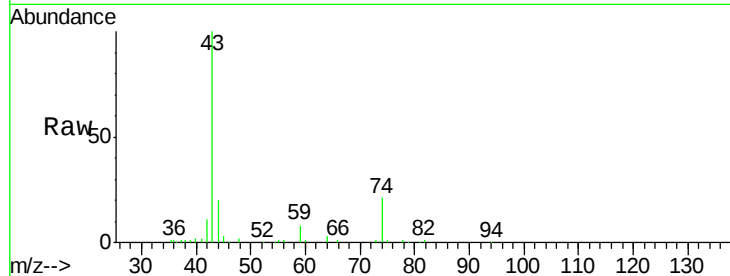

#20
Methylene Chloride
Concen: 2.28 ug/l
RT: 2.86 min Scan# 373
Delta R.T. -0.00 min
Lab File: VX001926.D
Acq: 23 May 2018 06:19

Tgt Ion: 84 Resp: 6389
Ion Ratio Lower Upper
84 100
49 126.4 96.3 144.5
51 36.9 29.8 44.6
86 64.4 51.0 76.6

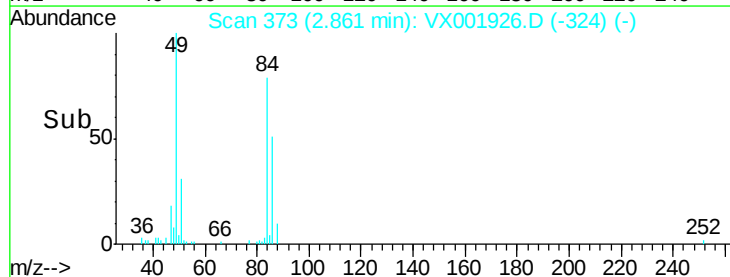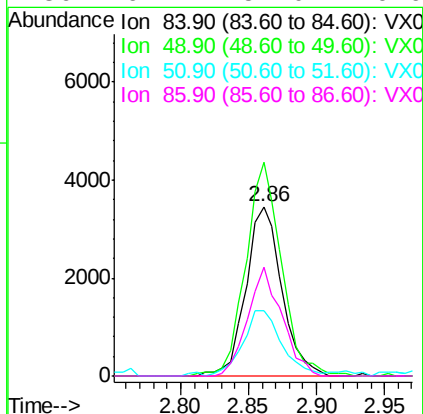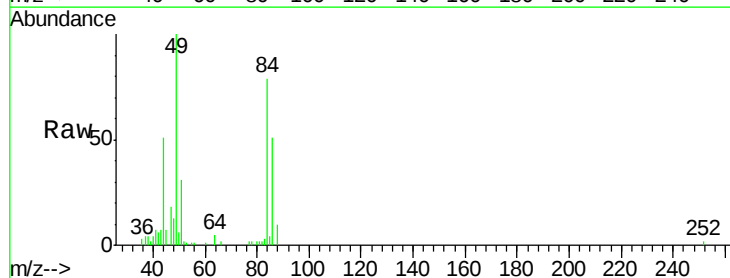

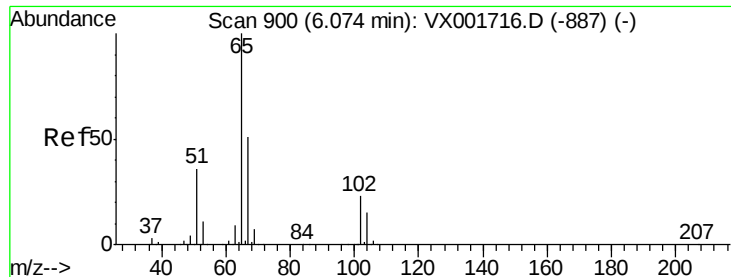

#33

1,2-Dichloroethane-d4

Concen: 47.04 ug/l

RT: 6.08 min Scan# 901

Delta R.T. 0.01 min

Lab File: VX001926.D

Acq: 23 May 2018 06:19

Instrument :

MSVOA_X

ClientSampleId :


PB109456ZHE#06

Tot Ion: 65 Resp: 156828

Ion Ratio Lower Upper




65 100

67 51.8 0.0 102.8

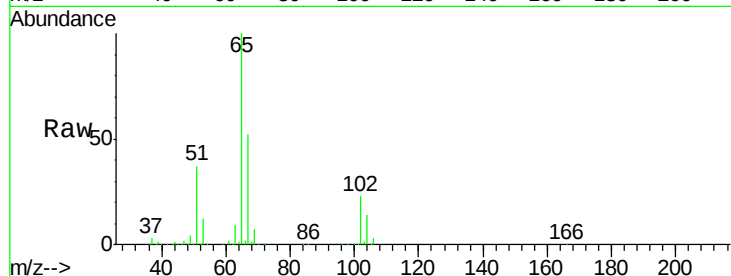

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

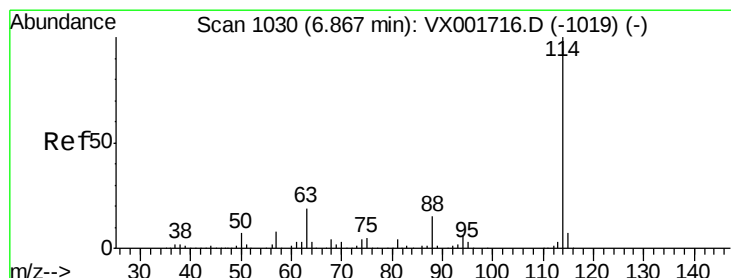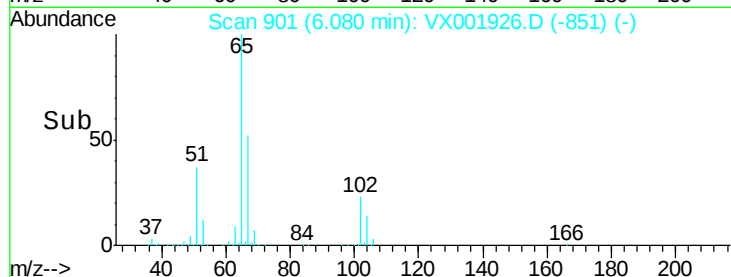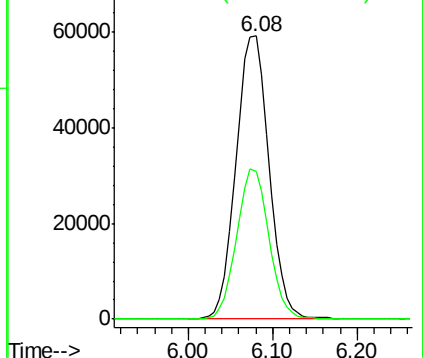

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. -0.00 min

Lab File: VX001926.D

Acq: 23 May 2018 06:19


Tgt Ion: 114 Resp: 336484

Ion Ratio Lower Upper

114 100

63 19.3 0.0 37.0



88 14.4 0.0 29.8

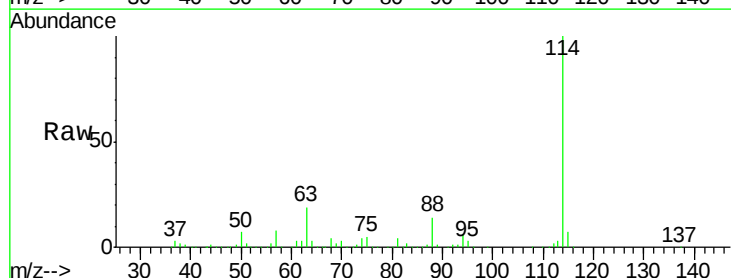


Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0



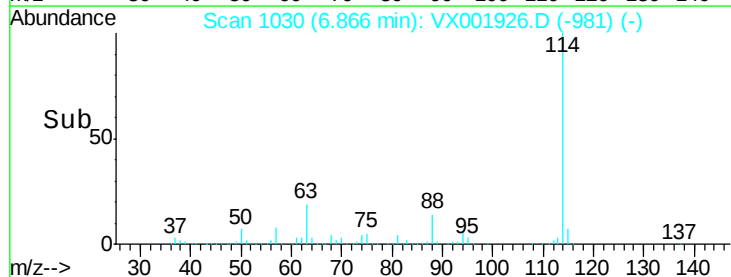
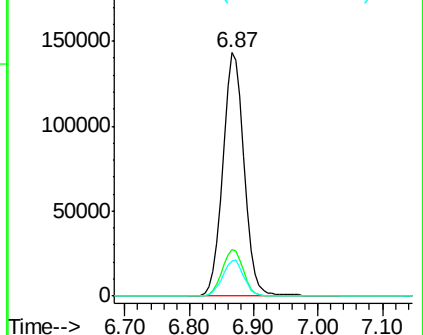


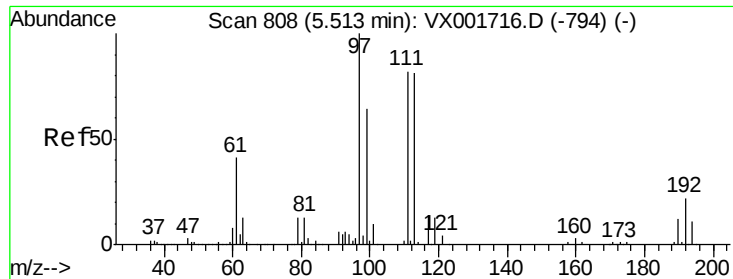

#35
 Dibromofluoromethane
 Concen: 45.99 ug/l
 RT: 5.51 min Scan# 808
 Delta R.T. -0.00 min
 Lab File: VX001926.D
 Acq: 23 May 2018 06:19




Instrument :
 MSVOA_X
 ClientSampleId :
 PB109456ZHE#06

Tot Ion:113 Resp: 130586
 Ion Ratio Lower Upper
 113 100
 111 102.5 82.0 123.0
 192 27.1 21.6 32.4

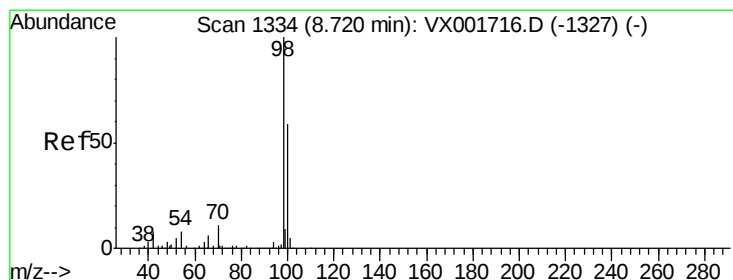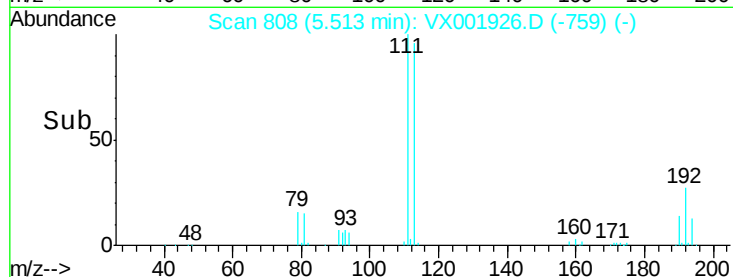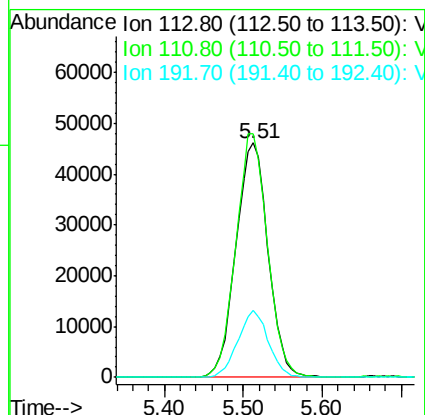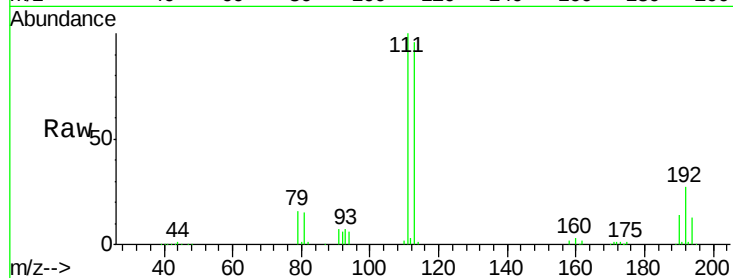

#50
 Toluene-d8
 Concen: 47.00 ug/l
 RT: 8.72 min Scan# 1334
 Delta R.T. -0.00 min
 Lab File: VX001926.D
 Acq: 23 May 2018 06:19

Tgt Ion: 98 Resp: 478019
 Ion Ratio Lower Upper
 98 100
 100 66.5 54.0 81.0

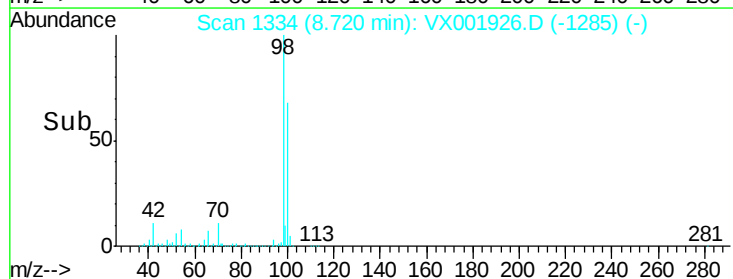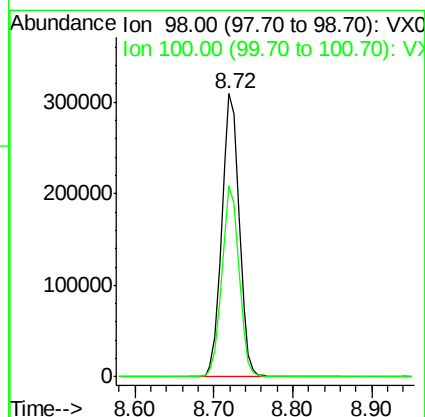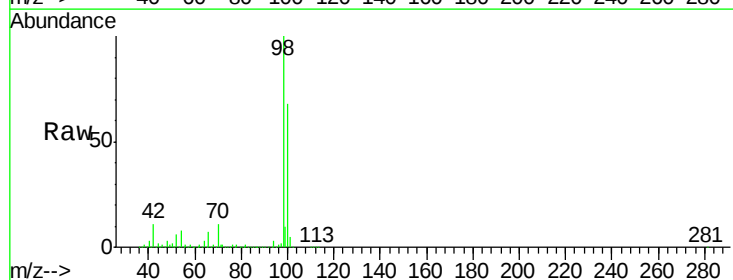



#62

4-Bromofluorobenzene

Concen: 38.08 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.00 min

Lab File: VX001926.D

Acq: 23 May 2018 06:19

Instrument :

MSVOA_X

ClientSampleId :

PB109456ZHE#06


Tot Ion: 95 Resp: 139452

Ion Ratio Lower Upper

95 100

174 103.4 0.0 201.8




176 99.4 0.0 196.8

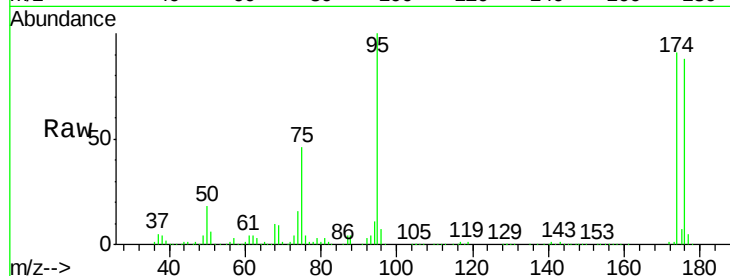

Abundance Ion 94.90 (94.60 to 95.60): VX001926.D (-1682) (-)

Ion 173.80 (173.50 to 174.50): VX001926.D (-1682) (-)

Ion 175.80 (175.50 to 176.50): VX001926.D (-1682) (-)

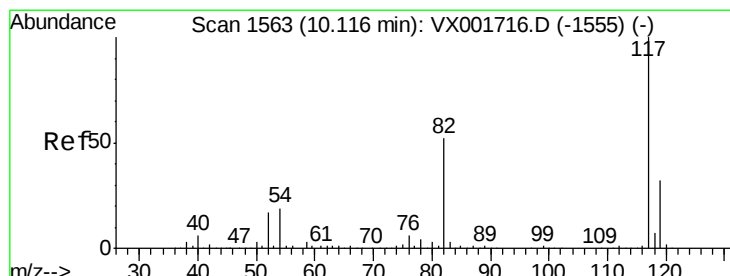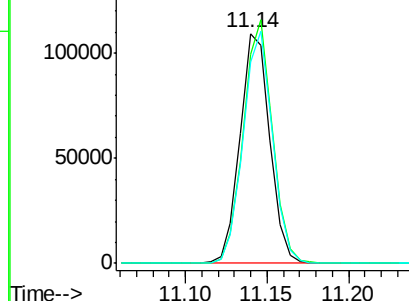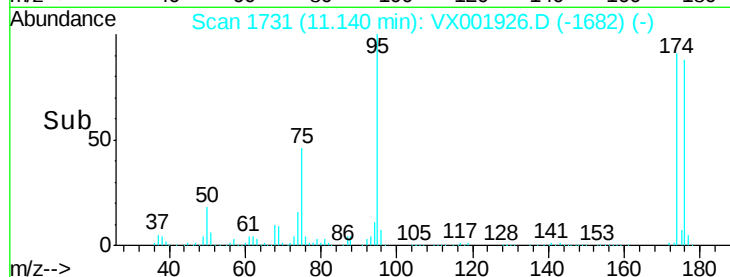

#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 10.12 min Scan# 1564

Delta R.T. 0.01 min

Lab File: VX001926.D

Acq: 23 May 2018 06:19


Tgt Ion: 117 Resp: 278712

Ion Ratio Lower Upper

117 100

82 49.1 41.4 62.2



119 32.7 25.6 38.4

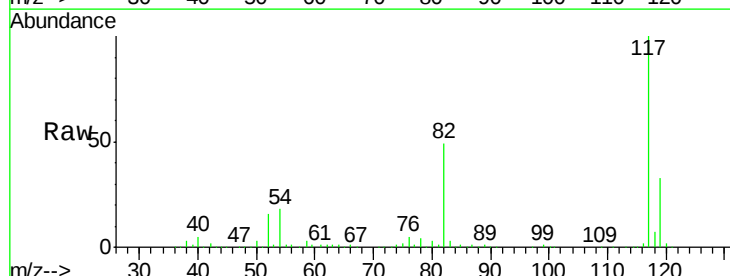


Abundance Ion 116.90 (116.60 to 117.60): VX001926.D (-1514) (-)

Ion 82.00 (81.70 to 82.70): VX001926.D (-1514) (-)

Ion 118.90 (118.60 to 119.60): VX001926.D (-1514) (-)

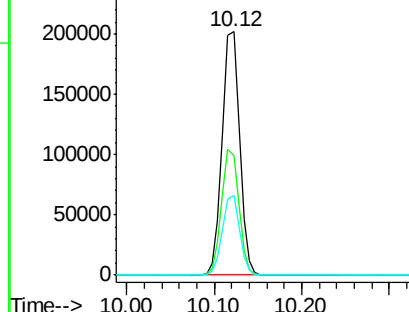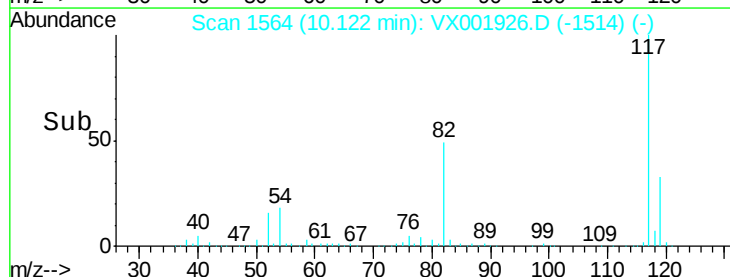

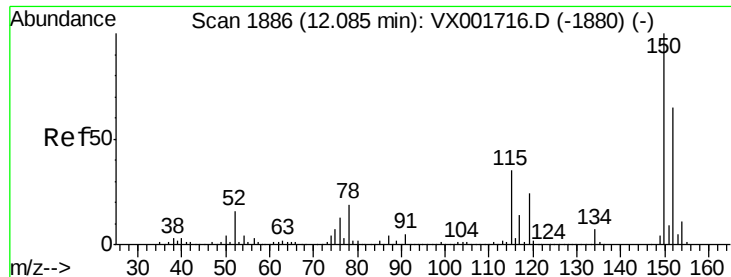

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.08 min Scan# 1886

Delta R.T. -0.00 min

Lab File: VX001926.D


Acq: 23 May 2018 06:19

Instrument :

MSVOA_X

ClientSampleId :

PB109456ZHE#06

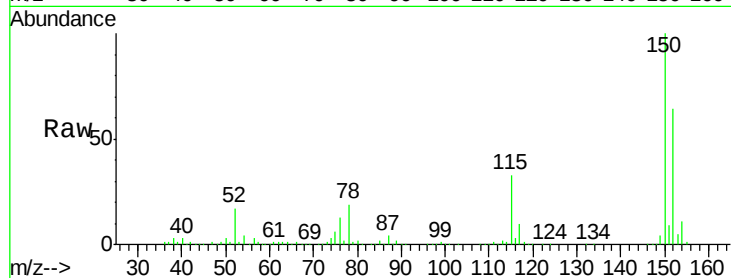


Tot Ion:152 Resp: 153724

Ion Ratio Lower Upper

152 100

115 51.2 37.4 112.2

150 155.5 0.0 344.8

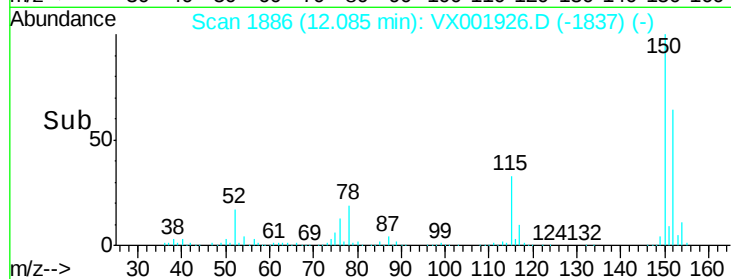

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

