


Dichlorodifluoromethane

Response Ratio

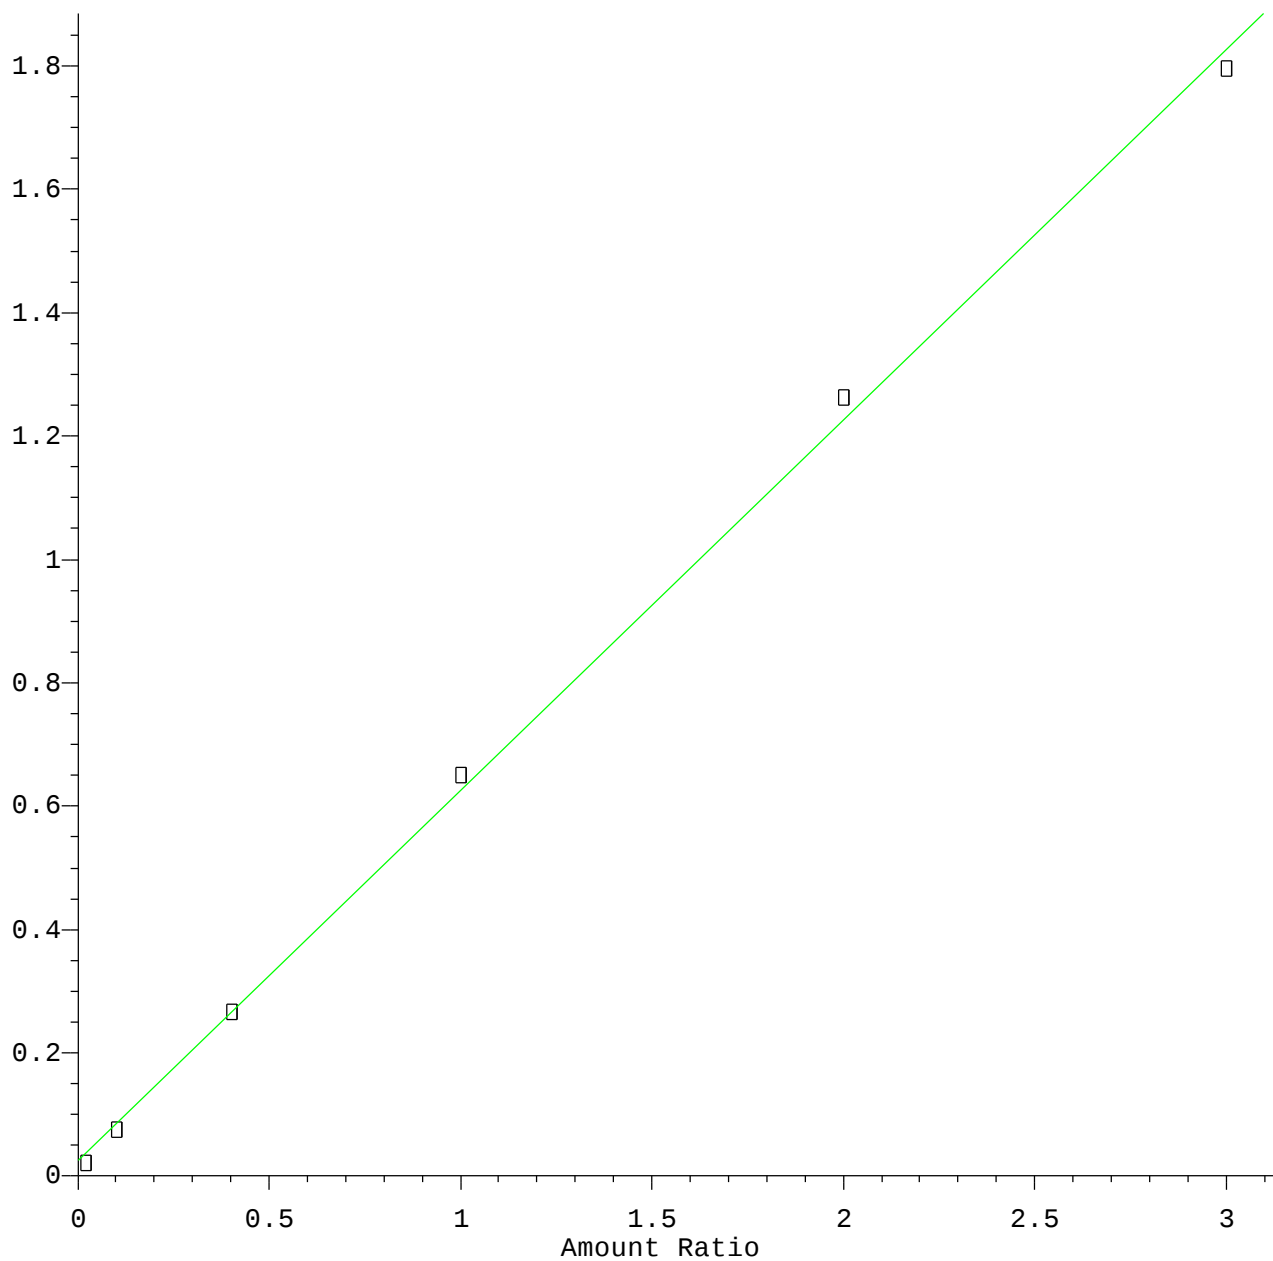


Resp Ratio = $6.00 \times 10^{-1} \times \text{Amt} + 2.54 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Calibration Table Last Updated: Thu May 24 13:09:03 2018

2-Chlorotoluene

Response Ratio

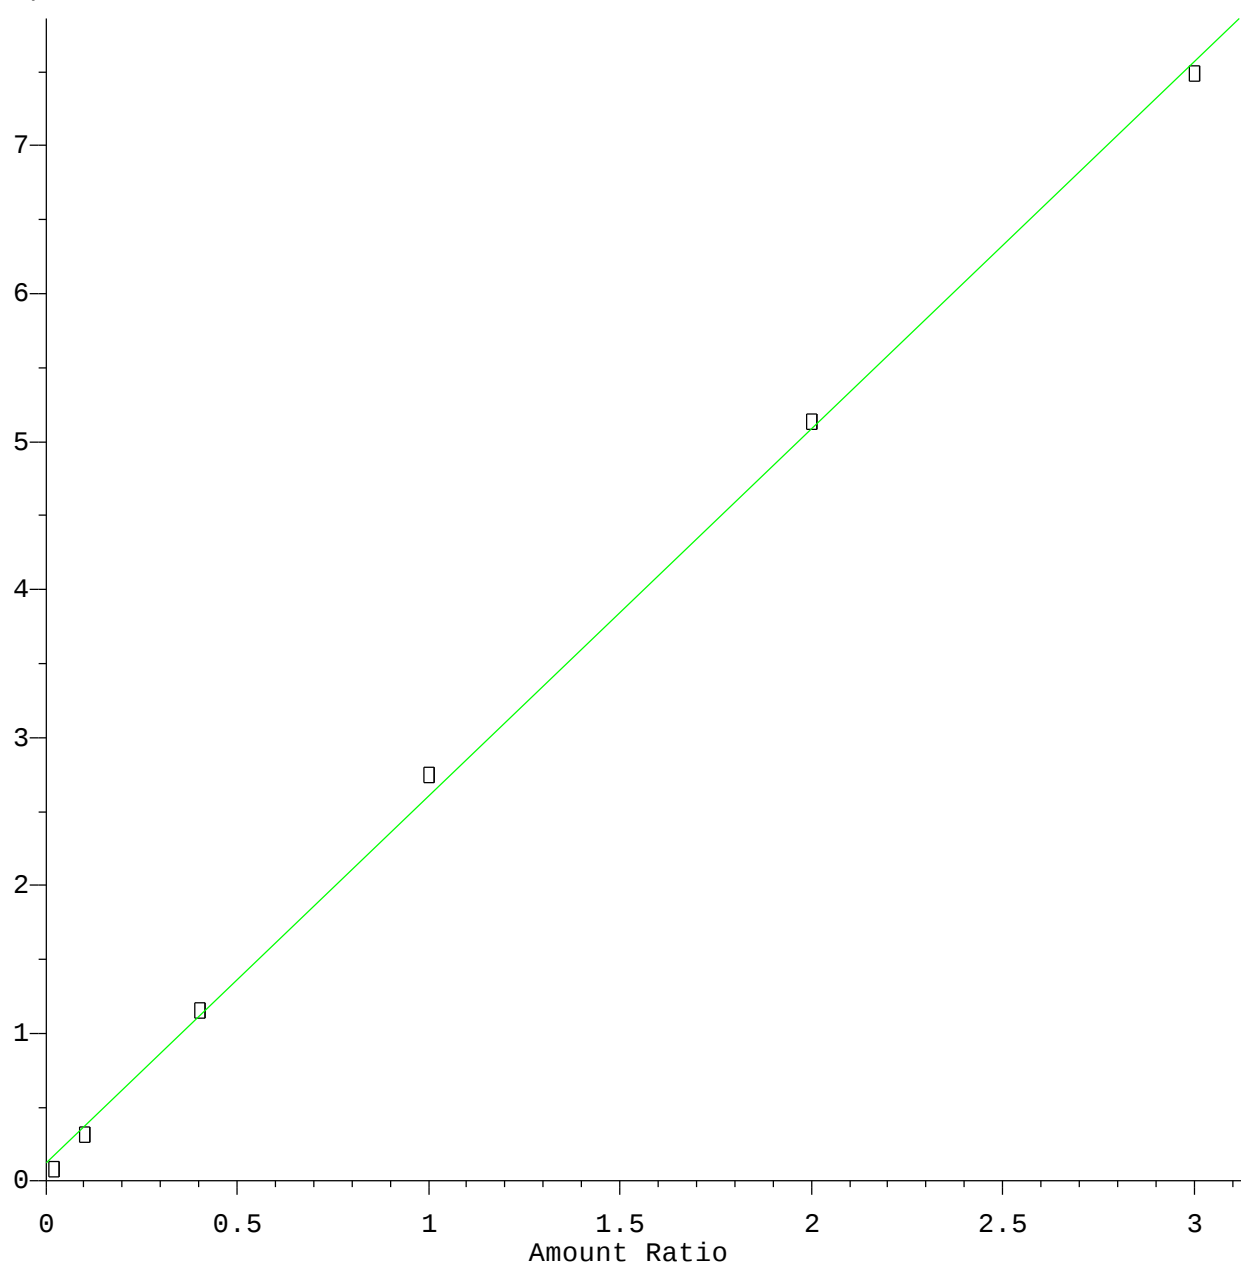


Resp Ratio = 2.48e+000 * Amt + 1.20e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Calibration Table Last Updated: Thu May 24 13:09:03 2018


1,1,2,2-Tetrachloroethane

Response Ratio

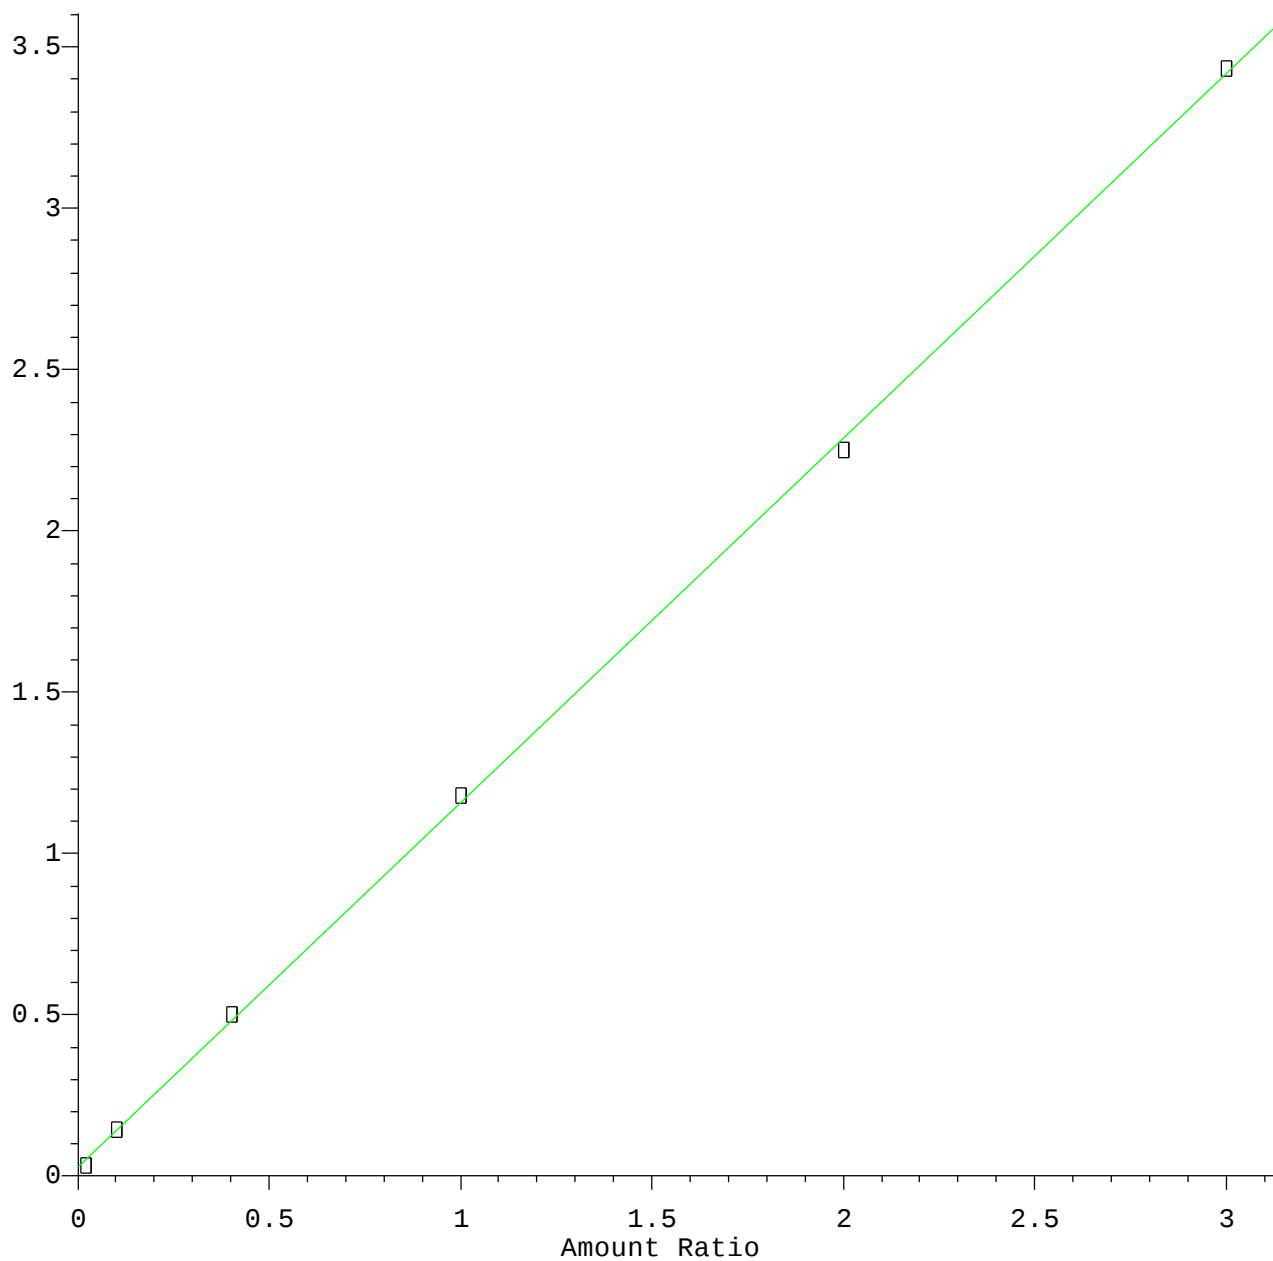


Resp Ratio = 1.13e+000 * Amt + 2.93e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Calibration Table Last Updated: Thu May 24 13:09:03 2018

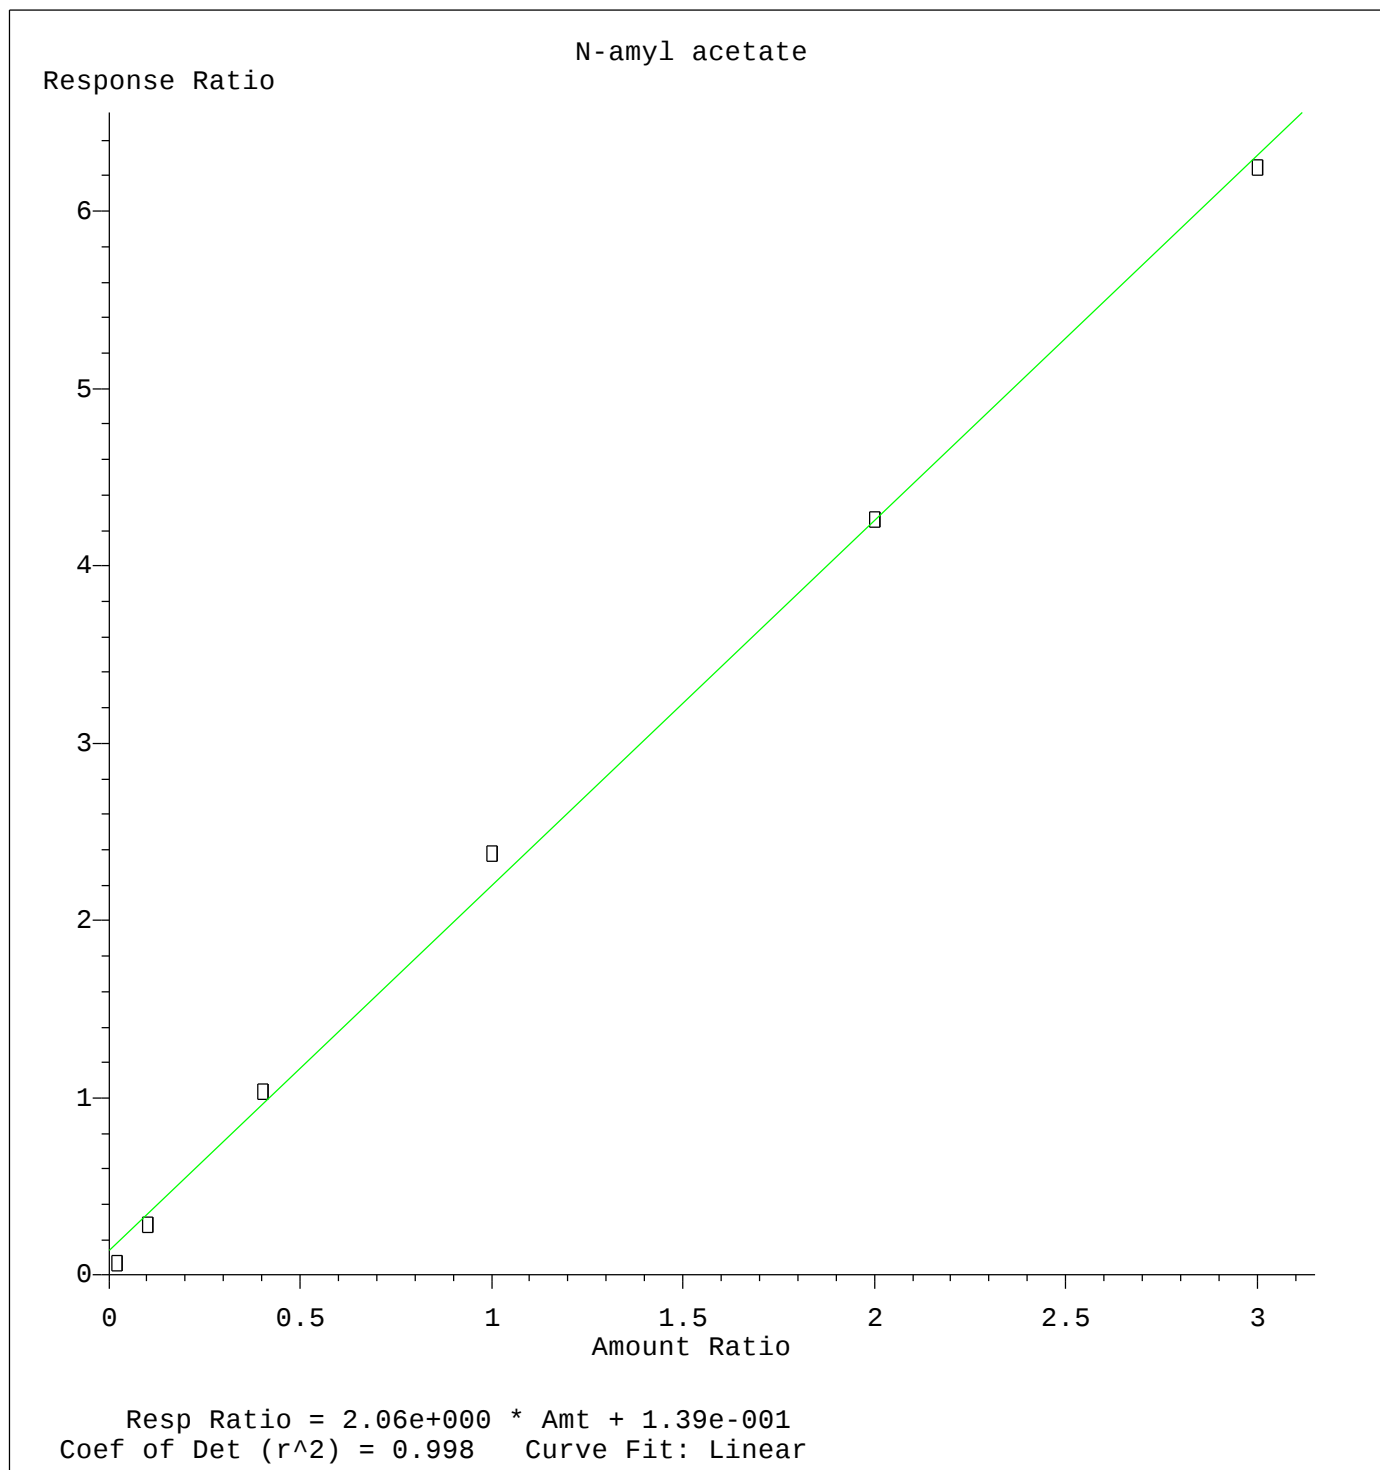


Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Calibration Table Last Updated: Thu May 24 13:09:03 2018

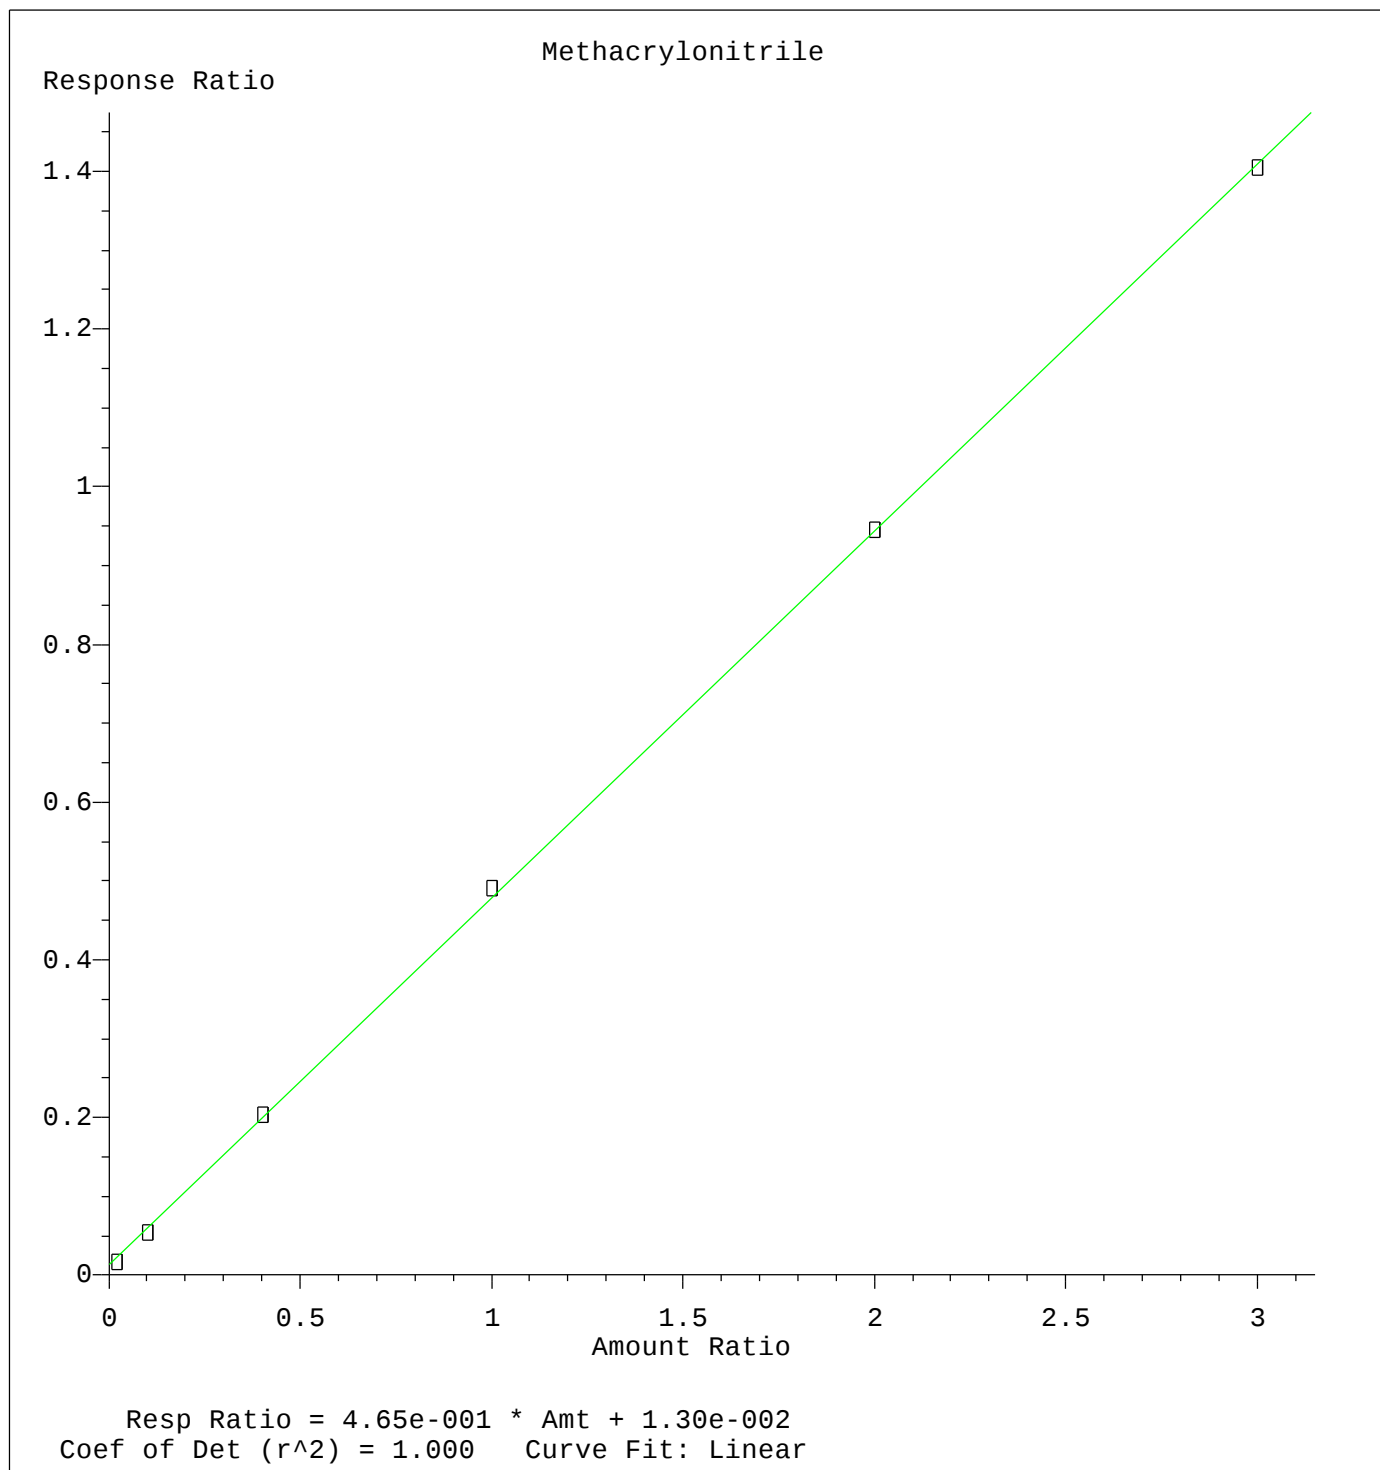

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Calibration Table Last Updated: Thu May 24 13:09:03 2018

Bromochloromethane

Response Ratio

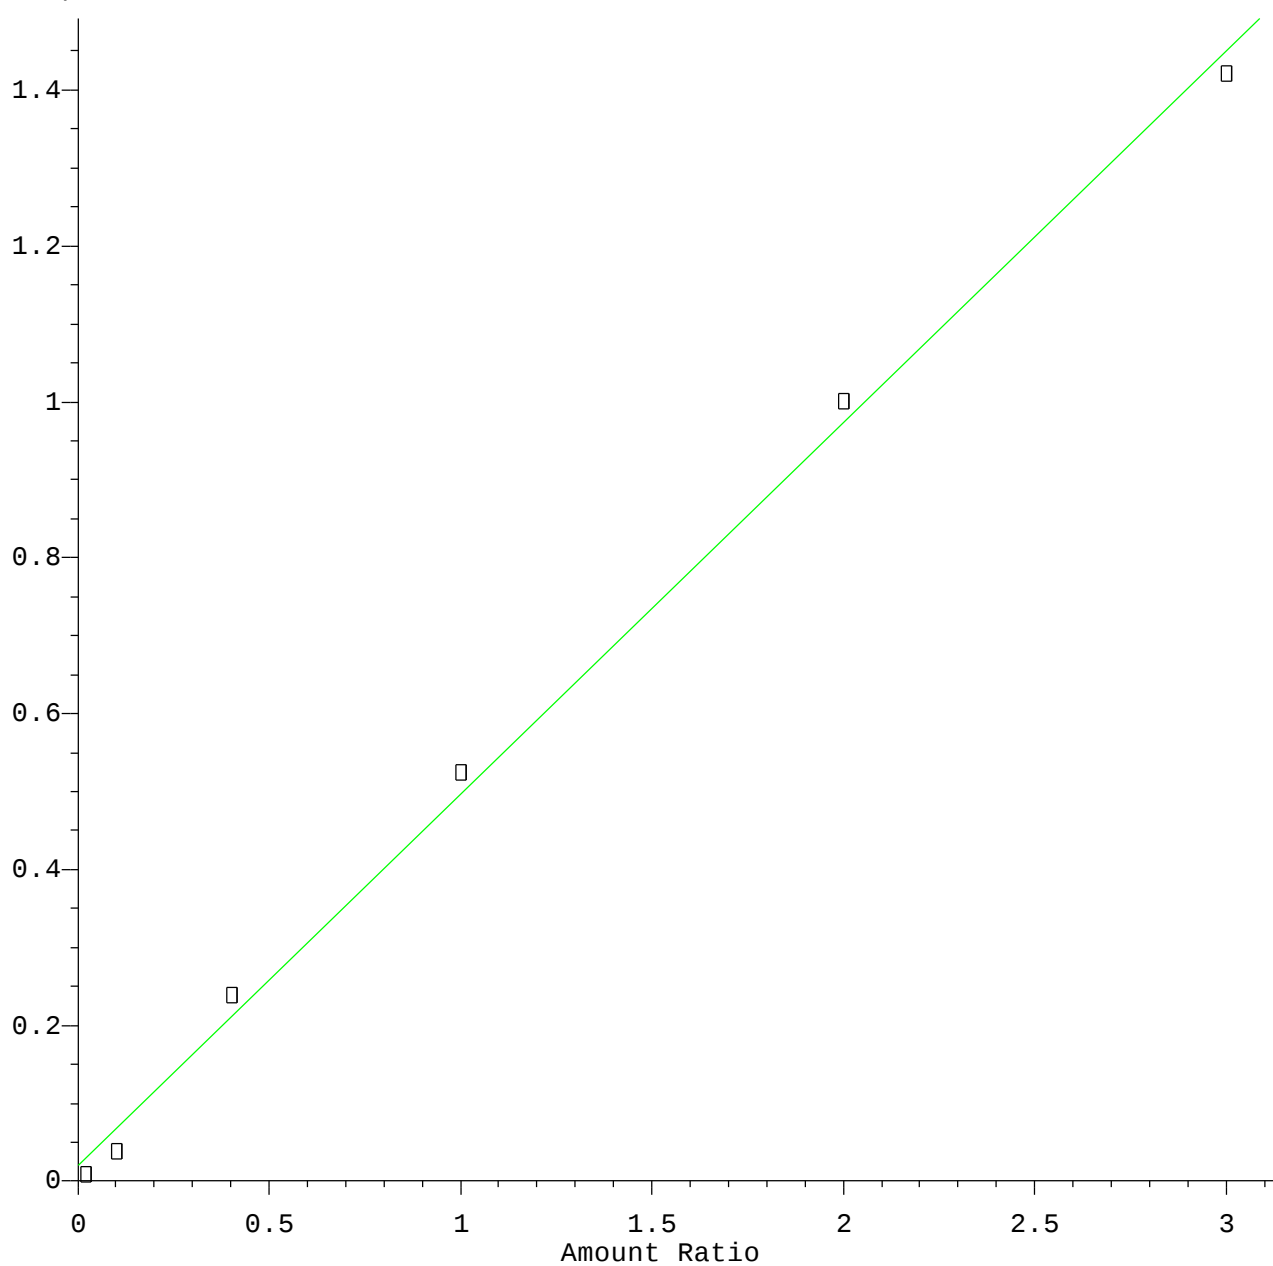


Resp Ratio = $4.76 \times 10^{-1} \times \text{Amt} + 2.03 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Calibration Table Last Updated: Thu May 24 13:09:03 2018

trans-1,2-Dichloroethene

Response Ratio

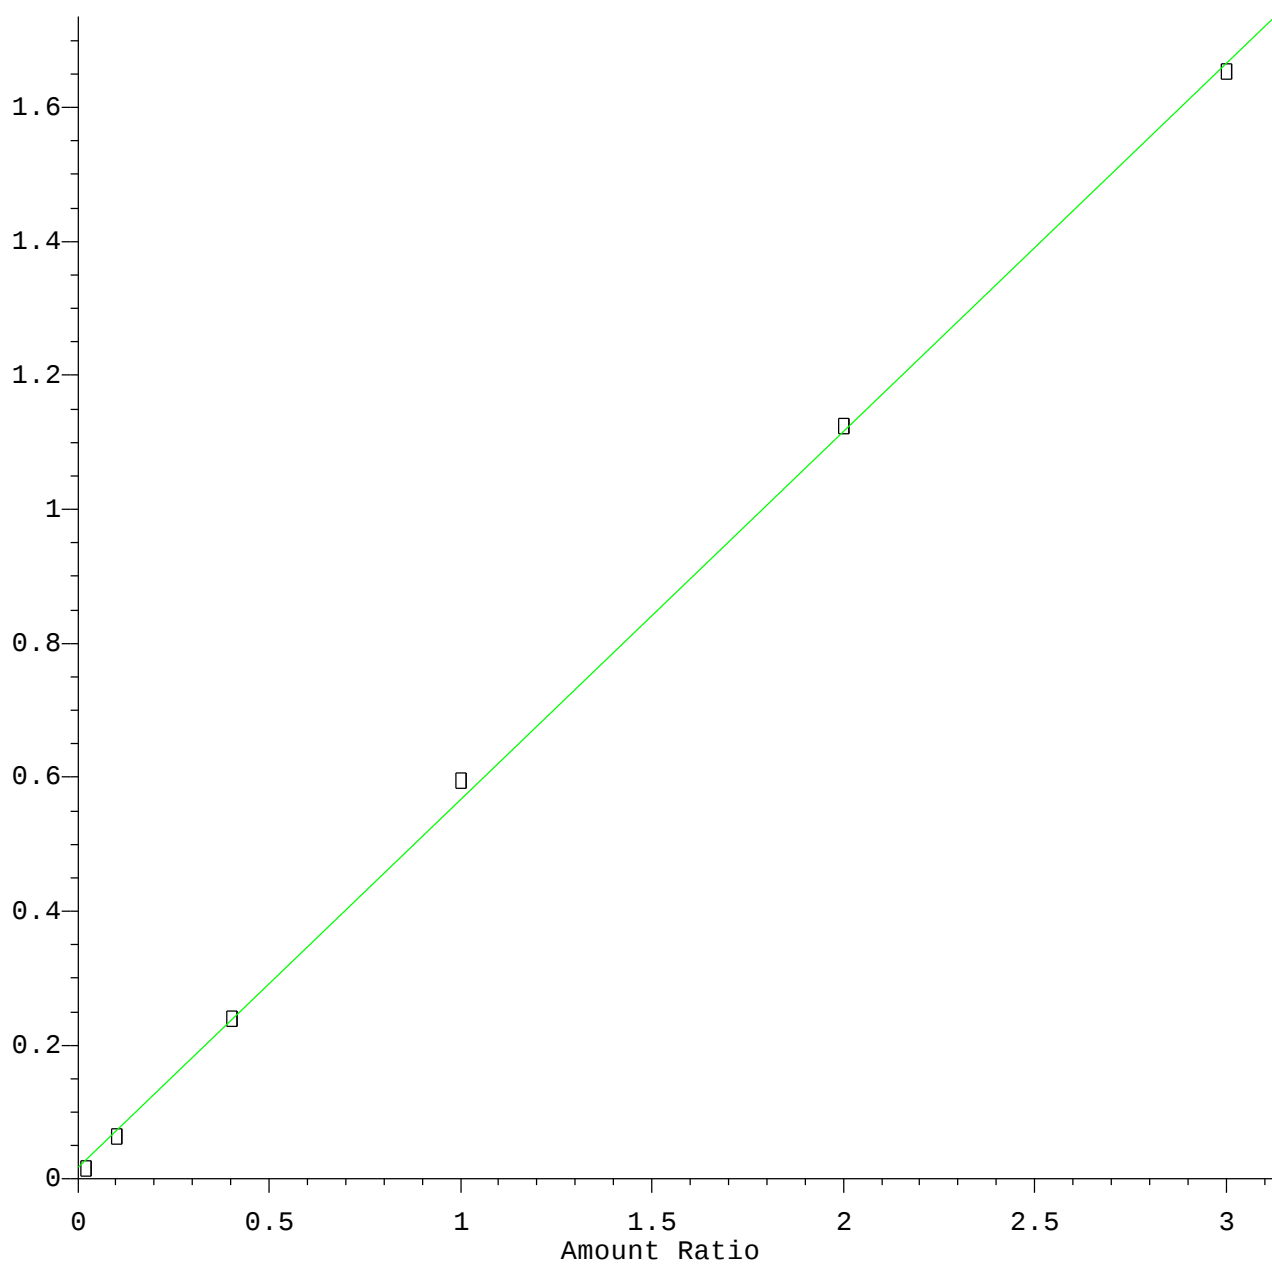


Resp Ratio = 5.49e-001 * Amt + 1.79e-002
Coef of Det (r²) = 0.999 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Calibration Table Last Updated: Thu May 24 13:09:03 2018


Methylene Chloride

Response Ratio

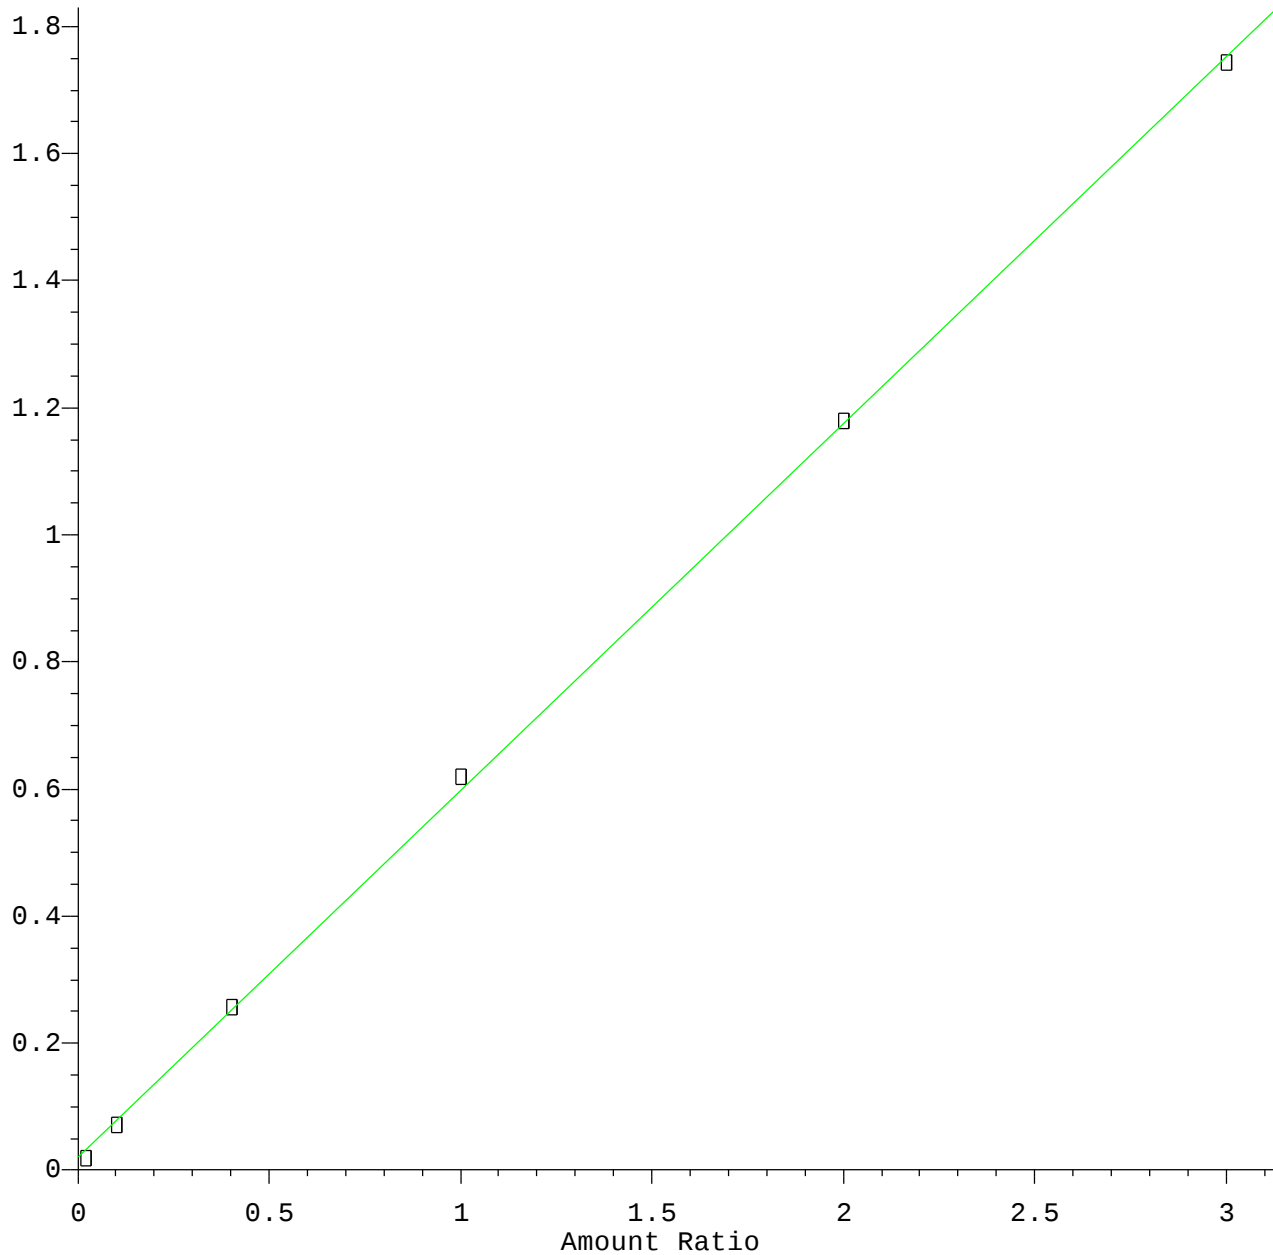


Resp Ratio = 5.77e-001 * Amt + 1.99e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Calibration Table Last Updated: Thu May 24 13:09:03 2018

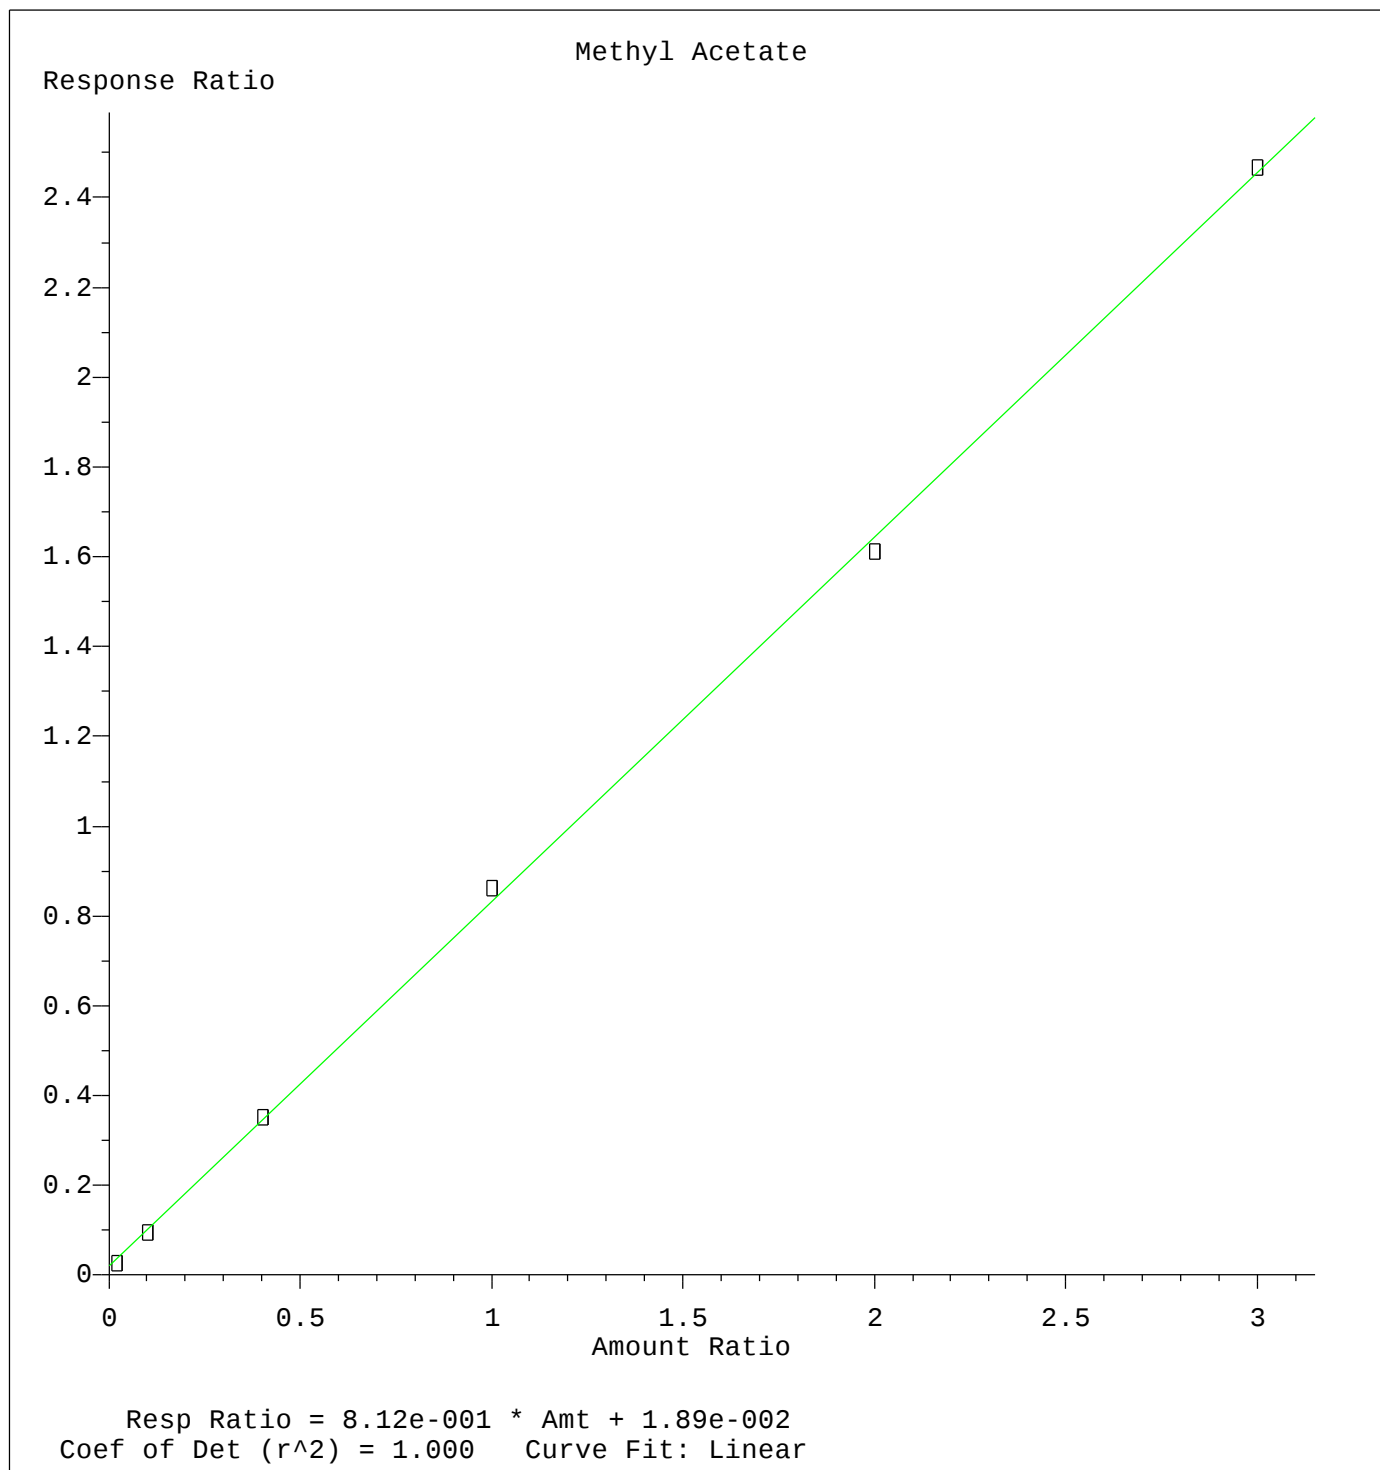

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Calibration Table Last Updated: Thu May 24 13:09:03 2018

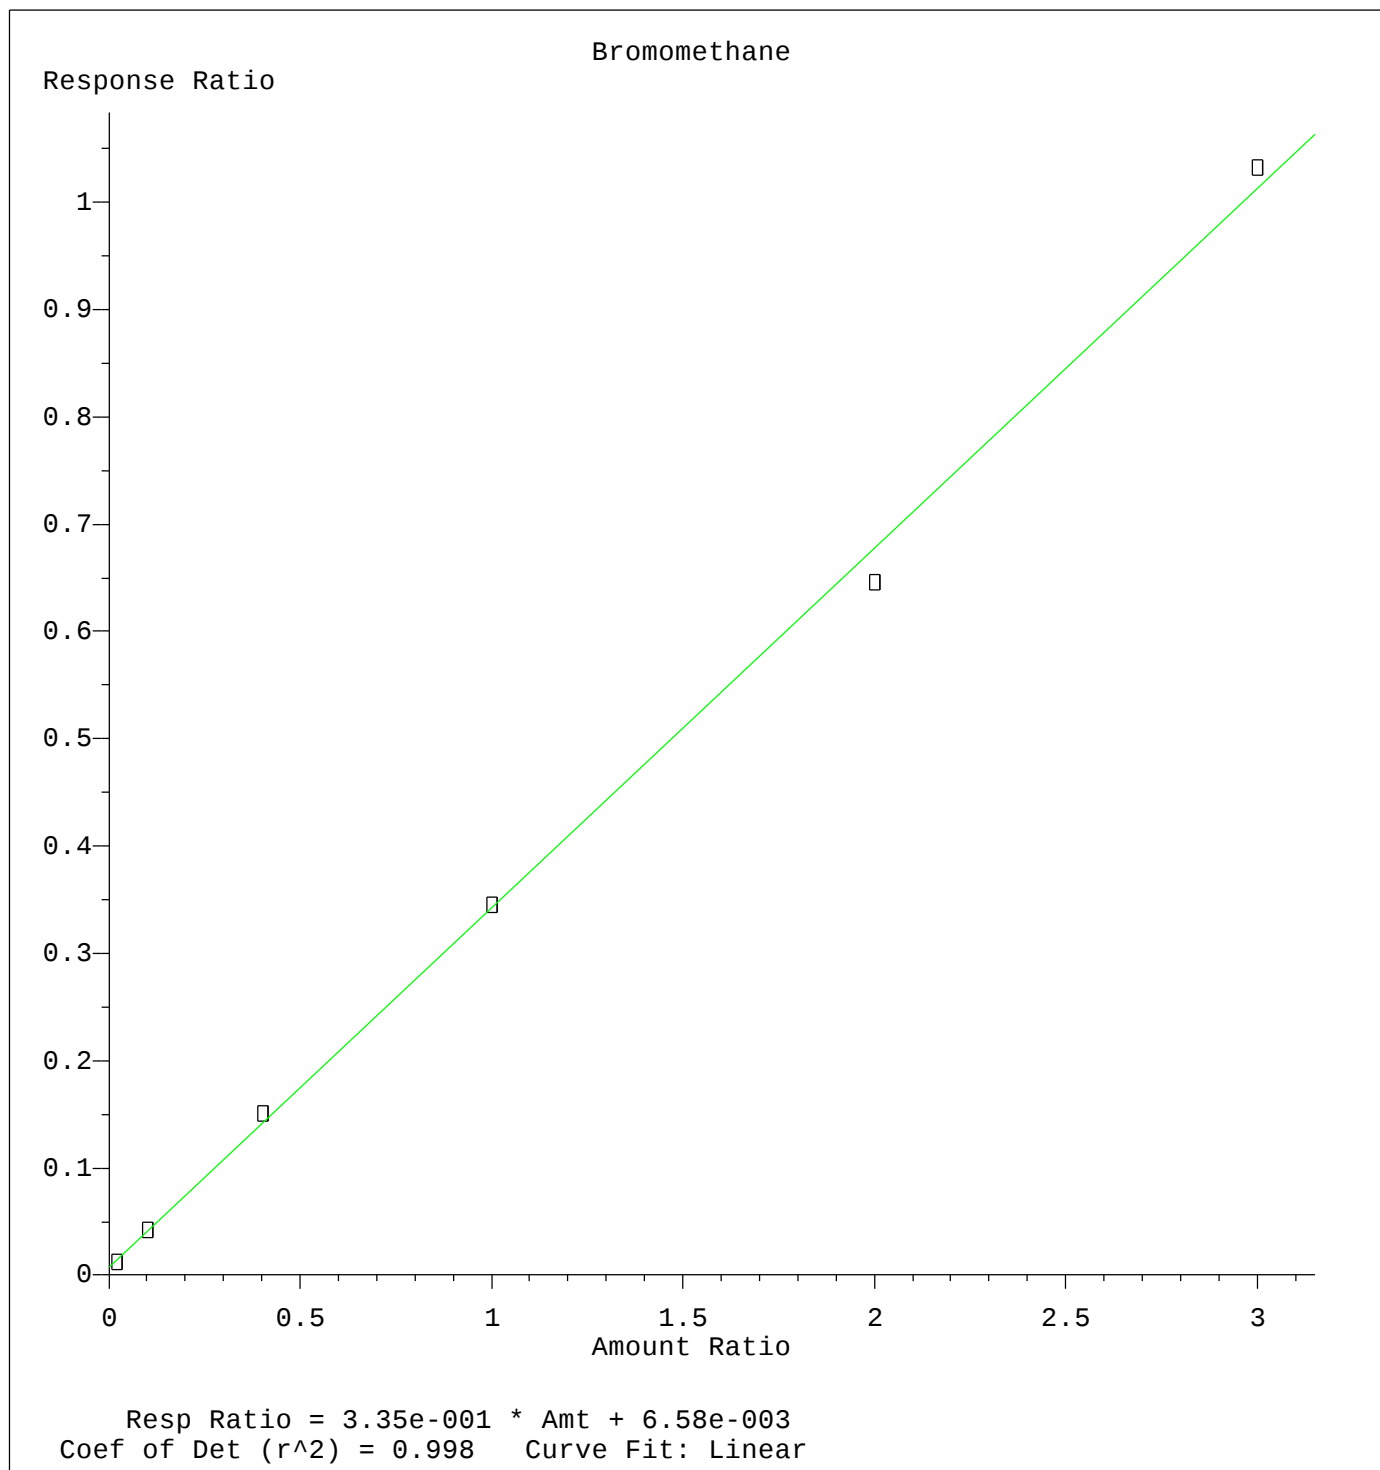

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Calibration Table Last Updated: Thu May 24 13:09:03 2018