


Data Path : W:\HPCHEM1\MSVOA X\Data\VX052518\
 Data File : VX001955.D
 Acq On : 24 May 2018 22:04
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\624X052518W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri May 25 02:17:15 2018

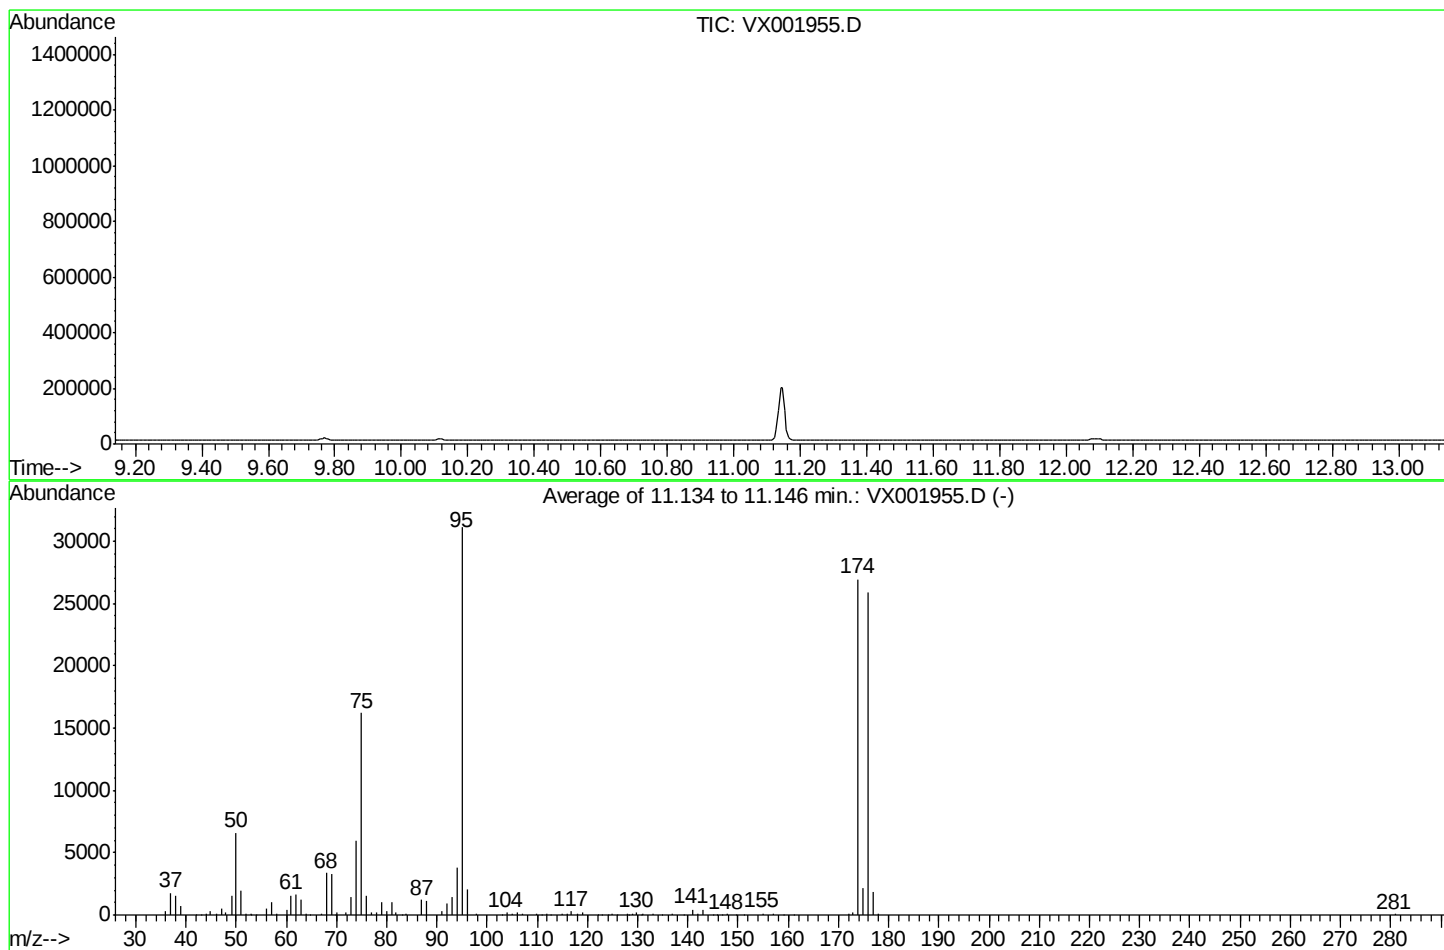

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	6617	PASS
75	95	30	60	52.1	16208	PASS
95	95	100	100	100.0	31116	PASS
96	95	5	9	6.7	2072	PASS
173	174	0.00	2	0.8	228	PASS
174	95	50	100	86.5	26920	PASS
175	174	5	9	8.1	2189	PASS
176	174	95	101	96.4	25938	PASS
177	176	5	9	7.3	1898	PASS