


Data Path : W:\HPCHEM1\MSVOA X\DATA\VX052518\
Data File : VX001966.D
Acq On : 25 May 2018 09:27
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Title : SW846 8260
Last Update : Thu May 24 13:09:03 2018

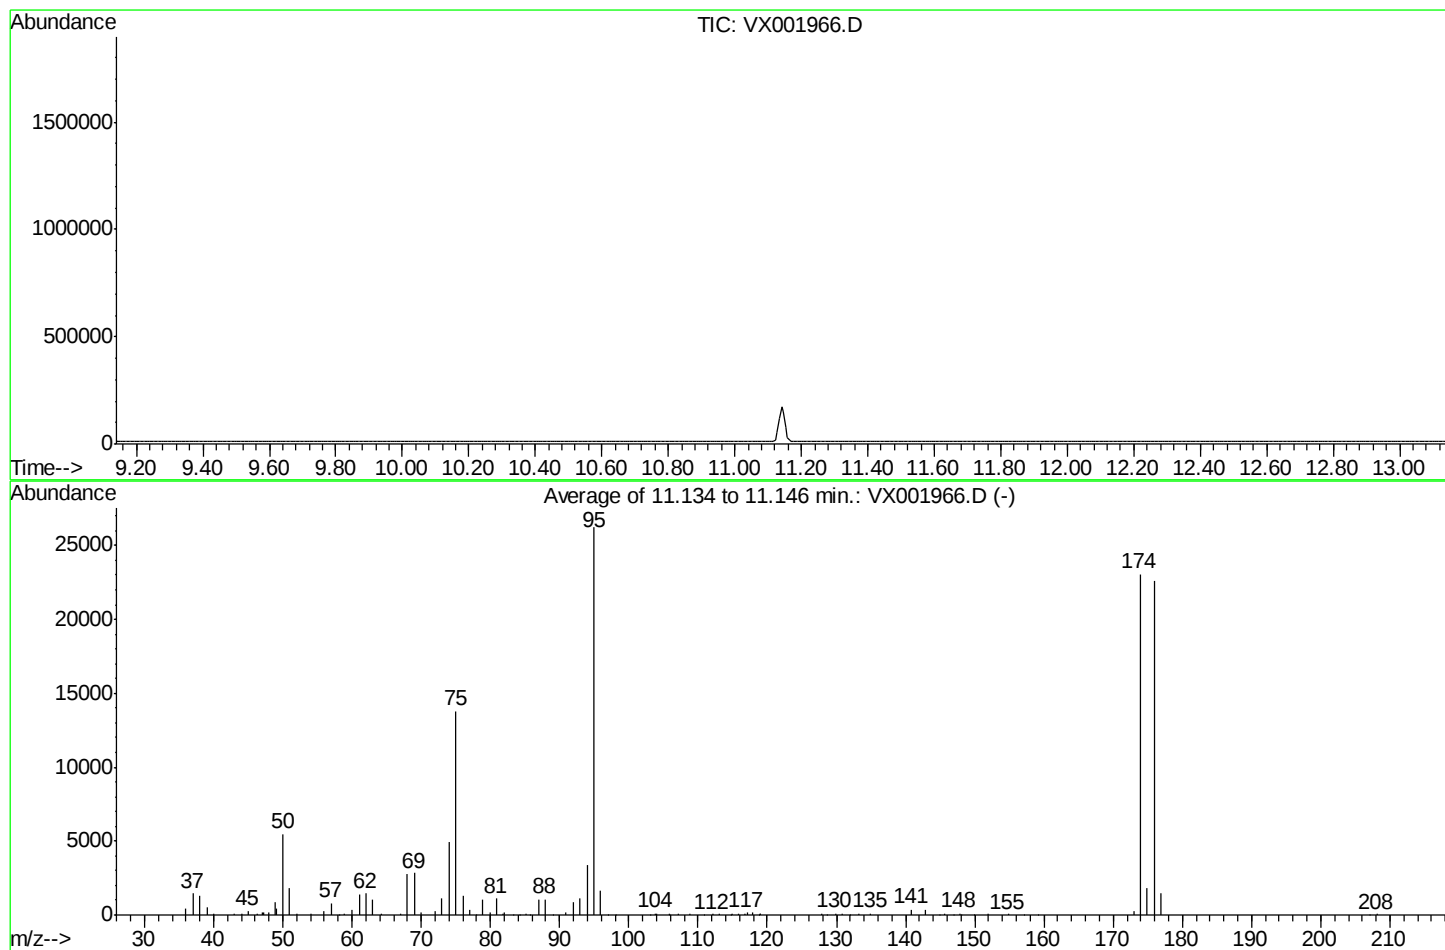

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	5481	PASS
75	95	30	60	52.7	13813	PASS
95	95	100	100	100.0	26226	PASS
96	95	5	9	6.1	1605	PASS
173	174	0.00	2	1.0	239	PASS
174	95	50	100	88.0	23066	PASS
175	174	5	9	7.9	1820	PASS
176	174	95	101	97.9	22590	PASS
177	176	5	9	6.4	1454	PASS