


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX052518\
 Data File : VX001989.D
 Acq On : 25 May 2018 21:03
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
 Title : SW846 8260
 Last Update : Thu May 24 13:09:03 2018

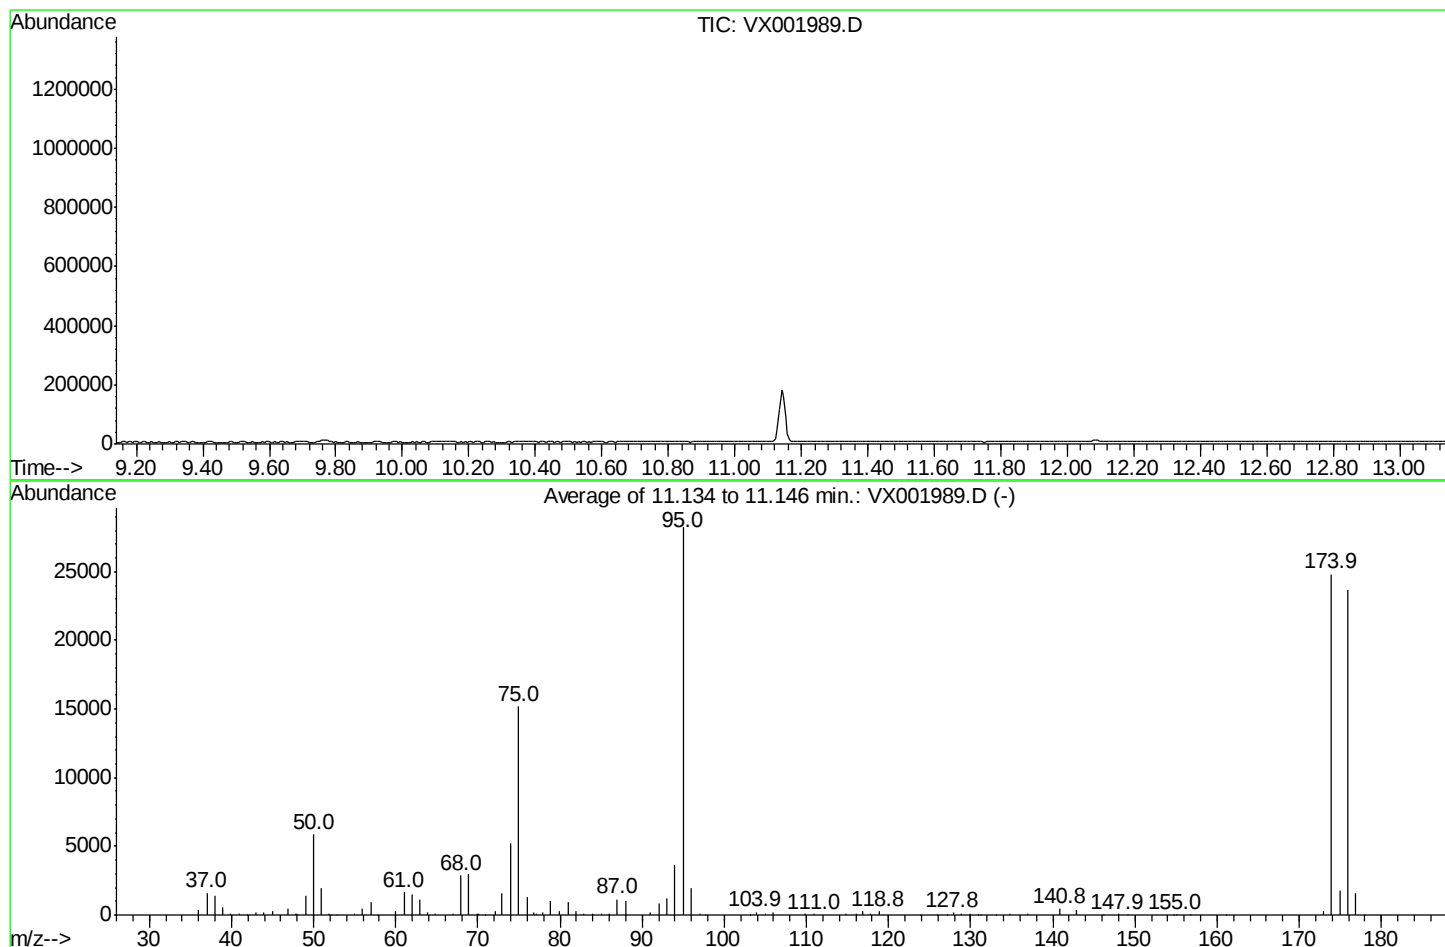

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1721

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	5843	PASS
75	95	30	60	53.7	15152	PASS
95	95	100	100	100.0	28229	PASS
96	95	5	9	7.0	1987	PASS
173	174	0.00	2	1.2	299	PASS
174	95	50	100	87.8	24797	PASS
175	174	5	9	7.3	1801	PASS
176	174	95	101	95.6	23711	PASS
177	176	5	9	6.6	1574	PASS