


Data Path : W:\HPCHEM1\MSVOA X\Data\VX052618\
 Data File : VX002038.D
 Acq On : 27 May 2018 00:19
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
 Title : SW846 8260
 Last Update : Thu May 24 13:09:03 2018

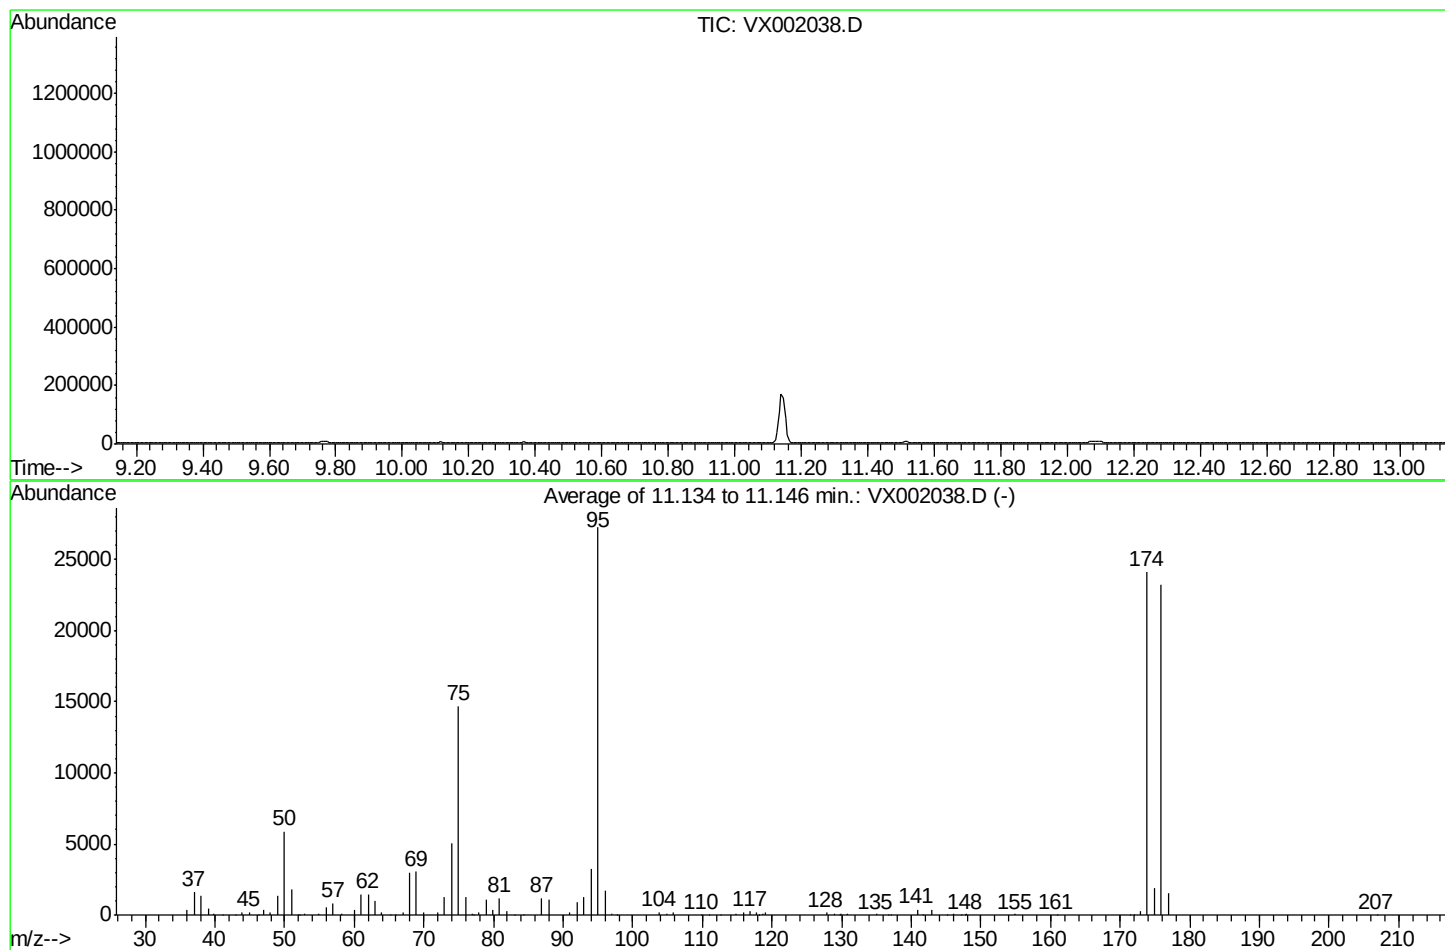

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	5894	PASS
75	95	30	60	53.9	14698	PASS
95	95	100	100	100.0	27277	PASS
96	95	5	9	6.3	1711	PASS
173	174	0.00	2	1.2	283	PASS
174	95	50	100	88.6	24171	PASS
175	174	5	9	7.7	1852	PASS
176	174	95	101	96.1	23234	PASS
177	176	5	9	6.8	1577	PASS