

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX052718\
 Data File : VX002073.D
 Acq On : 27 May 2018 17:18
 Operator : JC/MD
 Sample : J2679-28
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: May 29 02:58:04 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 24 13:09:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	319980	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	447550	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	408775	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	236654	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	210997	36.89	ug/l	0.00
Spiked Amount			Recovery	=	73.78%	
35) Dibromofluoromethane	5.51	113	162223	36.25	ug/l	0.00
Spiked Amount			Recovery	=	72.50%	
50) Toluene-d8	8.72	98	638678	39.42	ug/l	0.00
Spiked Amount			Recovery	=	78.84%	
62) 4-Bromofluorobenzene	11.14	95	235946	37.22	ug/l	0.00
Spiked Amount			Recovery	=	74.44%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.21	85	45	Below Cal	#	41
3) Chloromethane	1.33	50	4597	0.93	ug/l	100
5) Bromomethane	1.65	94	598	Below Cal	#	72
11) Tert butyl alcohol	3.02	59	3212	2.86	ug/l	81
13) Acrolein	2.30	56	246	0.51	ug/l	14
14) Allyl chloride	2.86	41	205252	26.22	ug/l	26
16) Acetone	2.45	43	18458	8.36	ug/l	98
18) Methyl Acetate	2.78	43	25433	3.73	ug/l	100
20) Methylene Chloride	2.86	84	5404541	1461.12	ug/l	95
21) trans-1,2-Dichloroethene	3.17	96	481	Below Cal	#	20
25) 2-Butanone	4.71	43	2930	0.72	ug/l	90
28) Bromochloromethane	5.03	49	1181	Below Cal	#	93
29) Tetrahydrofuran	5.18	42	1480	0.56	ug/l	68
30) Chloroform	5.21	83	3641	0.43	ug/l	94
36) 1,1-Dichloropropene	5.67	75	22287	3.58	ug/l	52
38) Carbon Tetrachloride	5.67	117	29782	4.10	ug/l	15
41) Methacrylonitrile	5.09	41	79	Below Cal	#	1
68) m/p-Xylenes	10.36	106	1913	0.22	ug/l	98
69) o-Xylene	10.71	106	1768	0.21	ug/l	93
74) N-amyl acetate	6.46	43	409	Below Cal	#	60
75) 1,1,2,2-Tetrachloroethane	11.26	83	94	Below Cal	#	25
76) 1,2,3-Trichloropropane	11.14	75	122883	21.62	ug/l	33
79) 2-Chlorotoluene	11.44	91	2123	Below Cal	#	40
80) 1,3,5-Trimethylbenzene	11.51	105	7207	0.42	ug/l	93
81) trans-1,4-Dichloro-2-buten	11.14	75	122883	51.96	ug/l	10
83) tert-Butylbenzene	11.81	119	4572	0.27	ug/l	66
84) 1,2,4-Trimethylbenzene	11.81	105	34381	1.94	ug/l	100
95) Naphthalene	13.84	128	60244	2.82	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX052718\
Data File : VX002073.D
Acq On : 27 May 2018 17:18
Operator : JC/MD
Sample : J2679-28
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: May 29 02:58:04 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Quant Title : SW846 8260
QLast Update : Thu May 24 13:09:03 2018
Response via : Initial Calibration

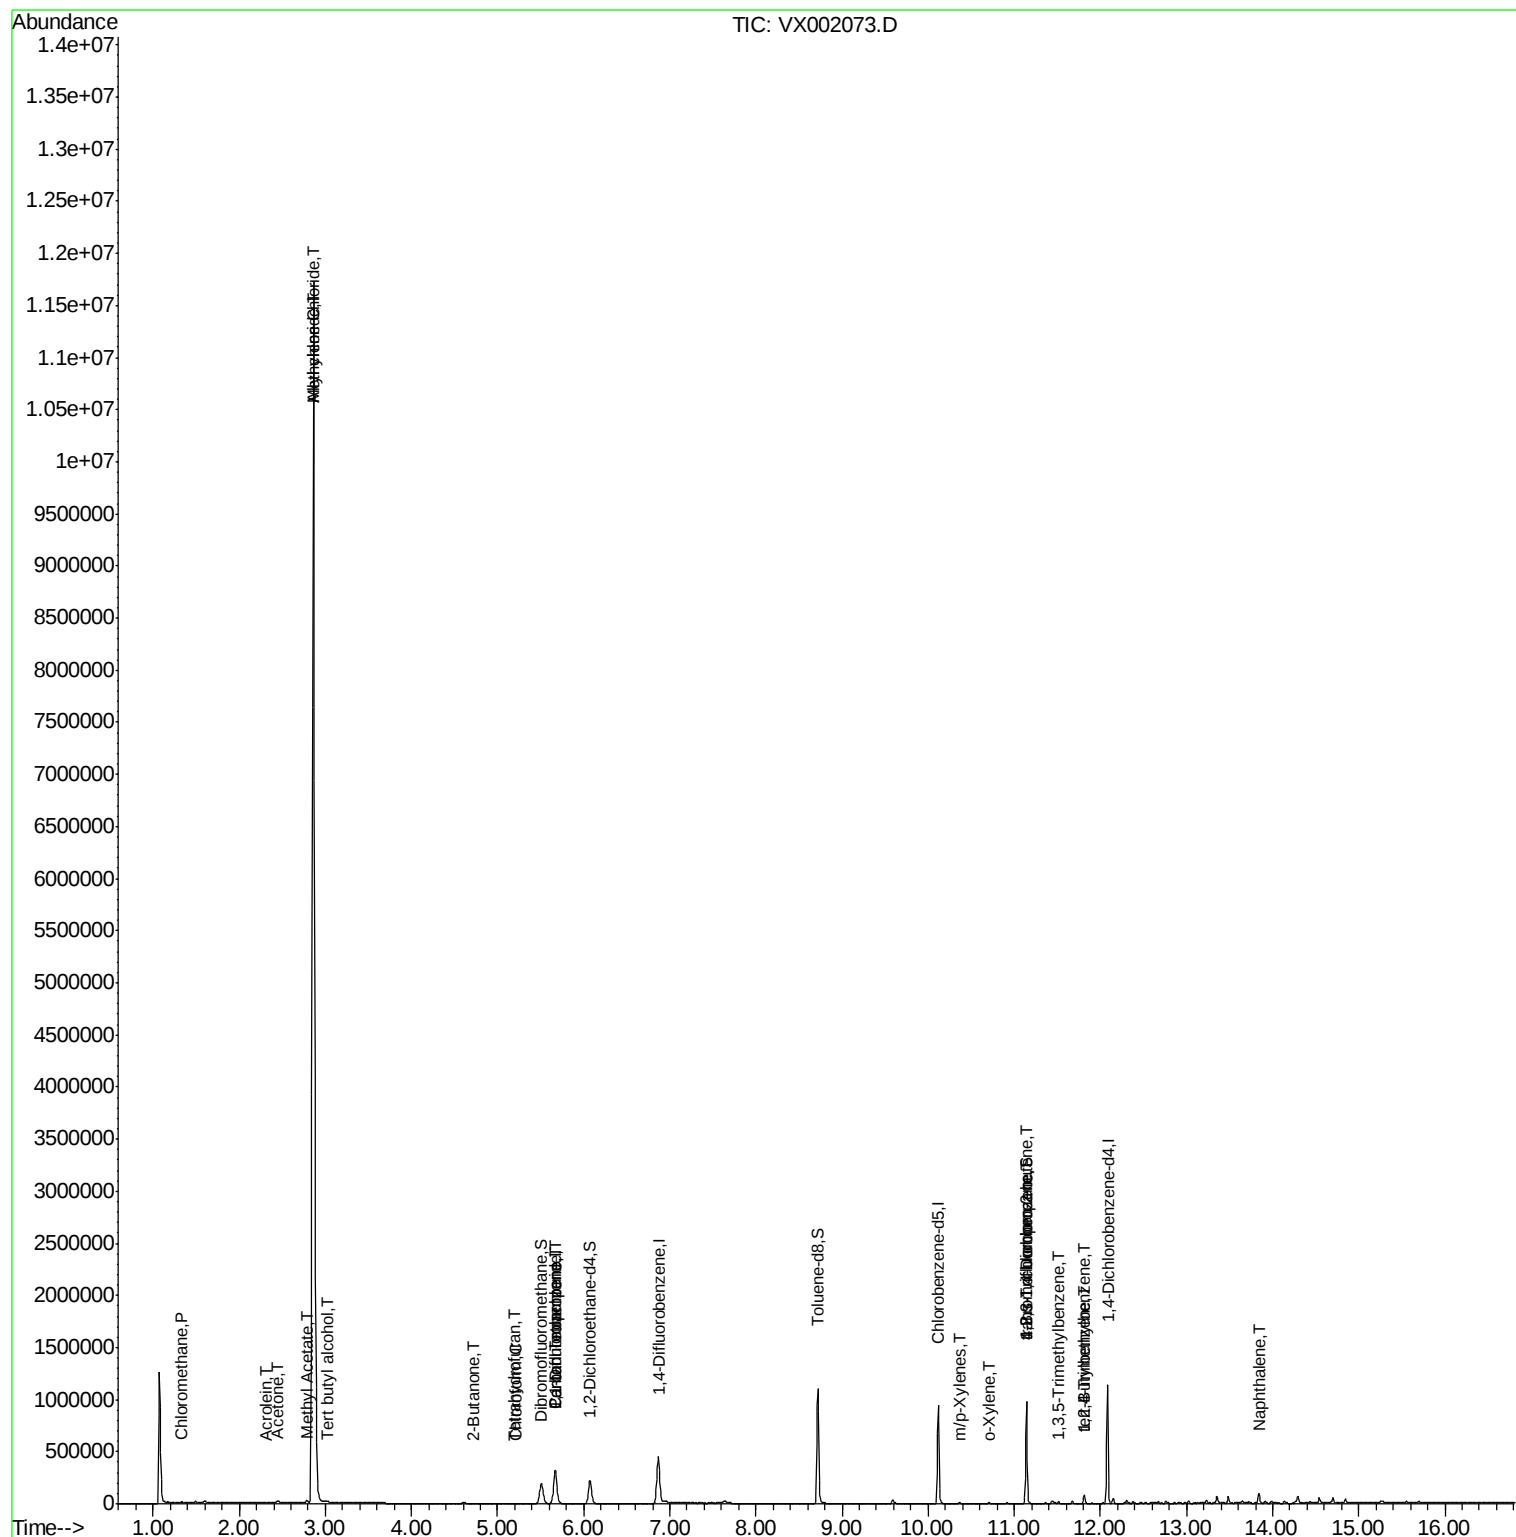



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.00 min

Lab File: VX002073.D

Acq: 27 May 2018 17:18

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion:168 Resp: 319980

Ion Ratio Lower Upper




168 100

99 52.2 41.0 61.4



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

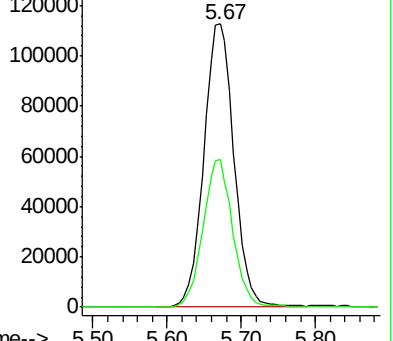

#2

Dichlorodifluoromethane

Concen: Below Cal

RT: 1.21 min Scan# 102

Delta R.T. 0.01 min

Lab File: VX002073.D


Acq: 27 May 2018 17:18

Tgt Ion: 85 Resp: 45

Ion Ratio Lower Upper



85 100


87 0.0 16.7 50.0#



Abundance Ion 84.90 (84.60 to 85.60): VX0

Ion 86.90 (86.60 to 87.60): VX0

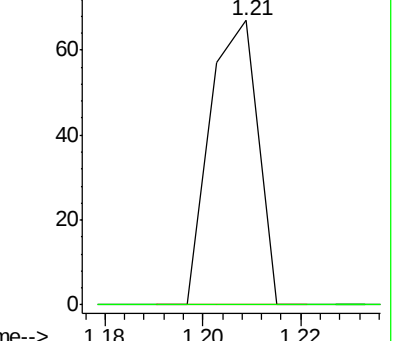



#3

Chloromethane

Concen: 0.93 ug/l

RT: 1.33 min Scan# 122

Delta R.T. 0.01 min

Lab File: VX002073.D

Acq: 27 May 2018 17:18

Instrument :

MSVOA_X





ClientSampled :

Tot Ion: 50 Resp: 4597

Ion Ratio Lower Upper

50 100

52 32.5 26.0 39.0

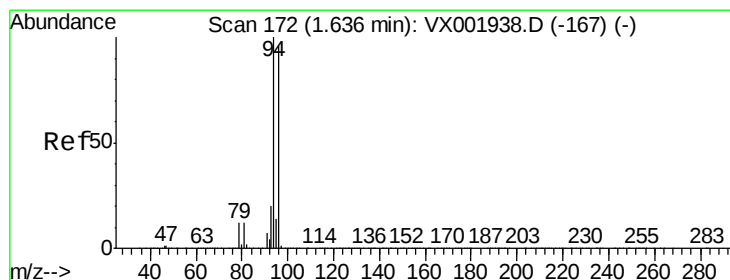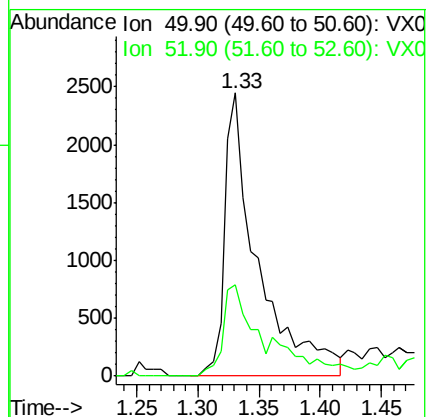

#5

Bromomethane

Concen: Below Cal

RT: 1.65 min Scan# 174

Delta R.T. 0.01 min

Lab File: VX002073.D




Acq: 27 May 2018 17:18


Tgt Ion: 94 Resp: 598

Ion Ratio Lower Upper

94 100

96 67.4 75.9 113.9#



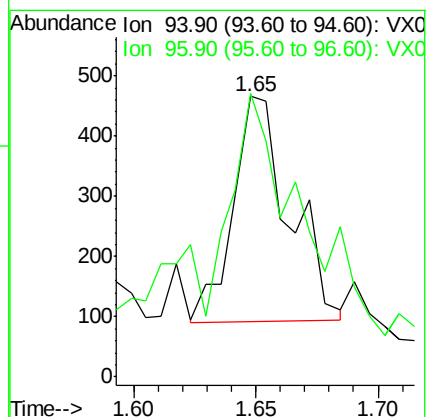



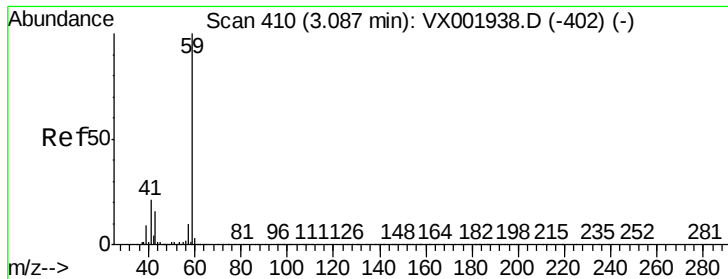

#11
Tert butvl alcohol
Concen: 2.86 ug/l
RT: 3.02 min Scan# 399
Delta R.T. -0.07 min
Lab File: VX002073.D
Acq: 27 May 2018 17:18




Instrument :
MSVOA_X
ClientSampled :


Tot Ion: 59 Resp: 3212
Ion Ratio Lower Upper
59 100
57 4.0 8.9 13.3#

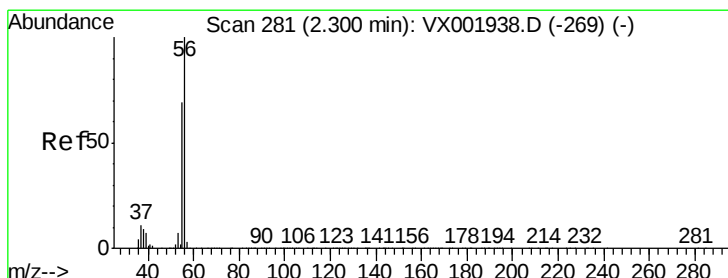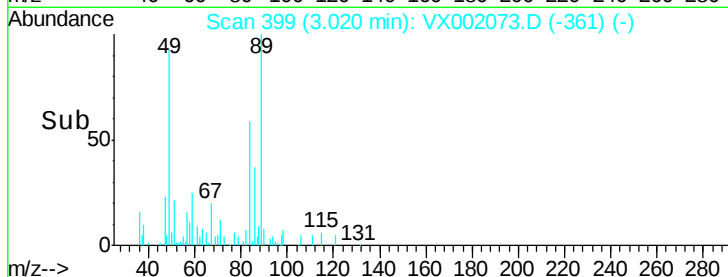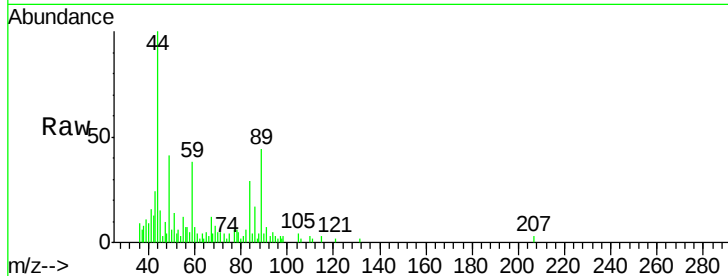

#13
Acrolein
Concen: 0.51 ug/l
RT: 2.30 min Scan# 281
Delta R.T. -0.00 min
Lab File: VX002073.D
Acq: 27 May 2018 17:18

Tgt Ion: 56 Resp: 246
Ion Ratio Lower Upper
56 100
55 0.0 56.8 85.2#


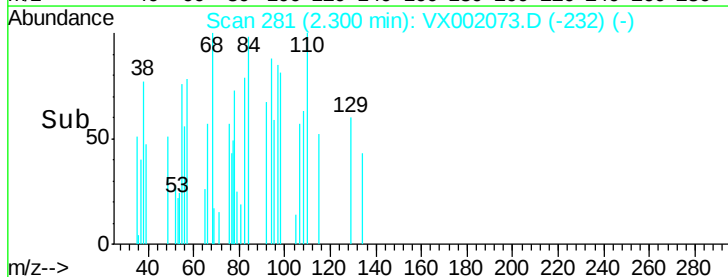

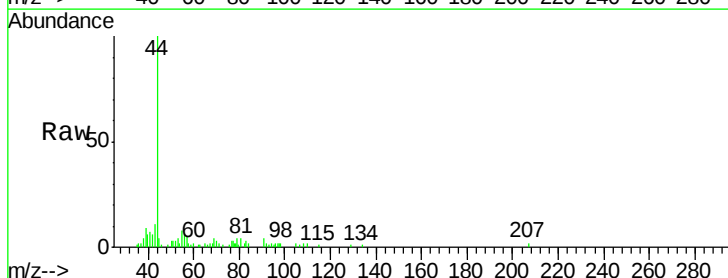




#14
Allvl chloride
Concen: 26.22 ug/l
RT: 2.86 min Scan# 373
Delta R.T. 0.13 min
Lab File: VX002073.D
Acq: 27 May 2018 17:18




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
41	100		
39	1.2	54.3	81.5#
76	0.0	24.2	36.4#

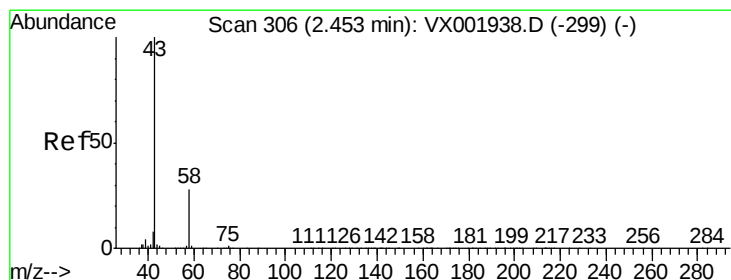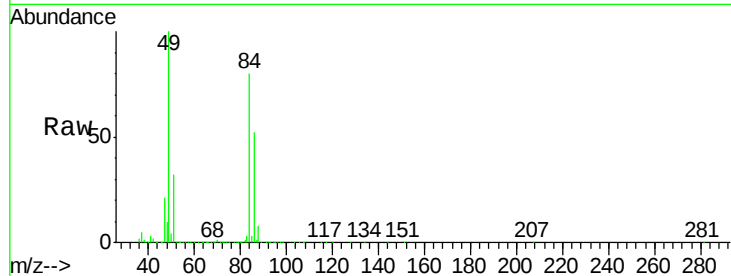

#16
Acetone
Concen: 8.36 ug/l
RT: 2.45 min Scan# 305
Delta R.T. -0.01 min
Lab File: VX002073.D
Acq: 27 May 2018 17:18

Tgt Ion	Ratio	Lower	Upper
43	100		
58	26.7	22.3	33.5


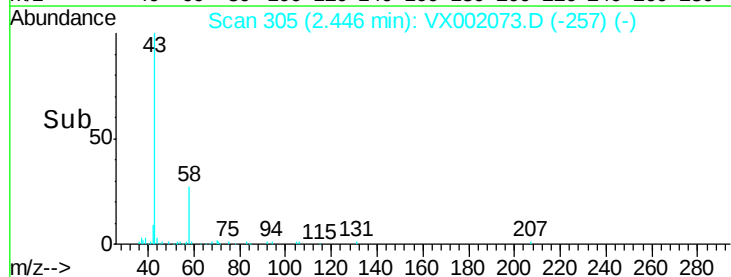






#18
Methvl Acetate
Concen: 3.73 ug/l
RT: 2.78 min Scan# 360
Delta R.T. 0.00 min
Lab File: VX002073.D
Acq: 27 May 2018 17:18




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 43 Resp: 25433
Ion Ratio Lower Upper
43 100
74 21.0 16.8 25.2

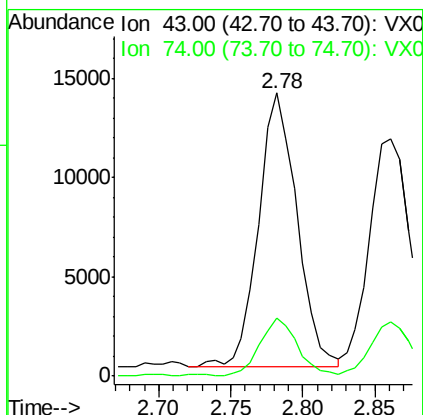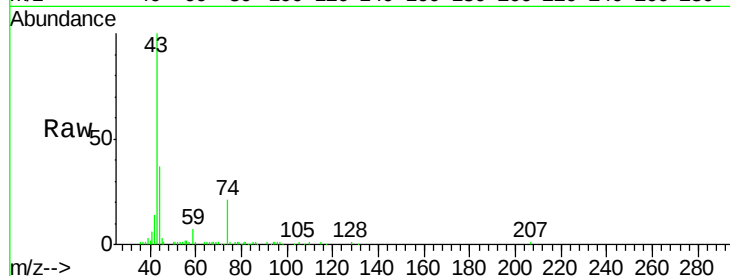

#20
Methylene Chloride
Concen: 1461.12 ug/l
RT: 2.86 min Scan# 373
Delta R.T. 0.01 min
Lab File: VX002073.D
Acq: 27 May 2018 17:18

Tgt Ion: 84 Resp: 5404541
Ion Ratio Lower Upper
84 100
49 125.8 107.2 160.8
51 39.8 32.4 48.6
86 65.4 50.4 75.6





#21

trans-1,2-Dichloroethene

Concen: Below Cal

RT: 3.17 min Scan# 423

Delta R.T. -0.00 min





Lab File: VX002073.D

Acq: 27 May 2018 17:18

Instrument :
MSVOA_X
ClientSampleId :

Tot Ion: 96 Resp: 481

Ion	Ratio	Lower	Upper
96	100		
61	22.1	113.3	169.9#
98	31.8	51.7	77.5#

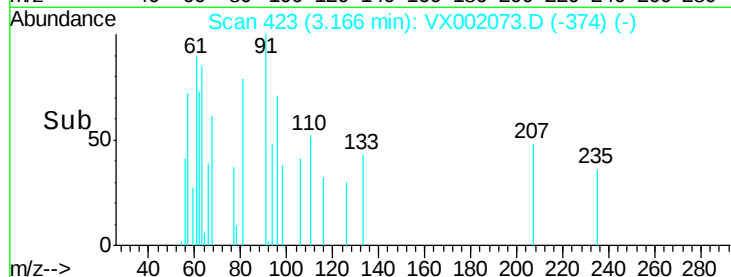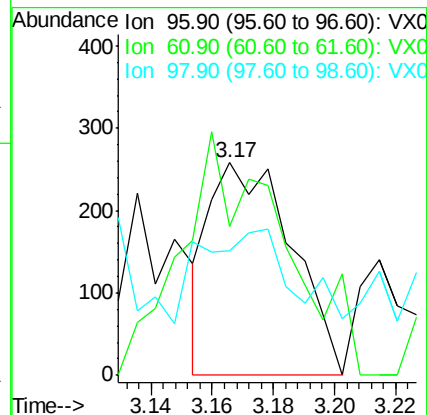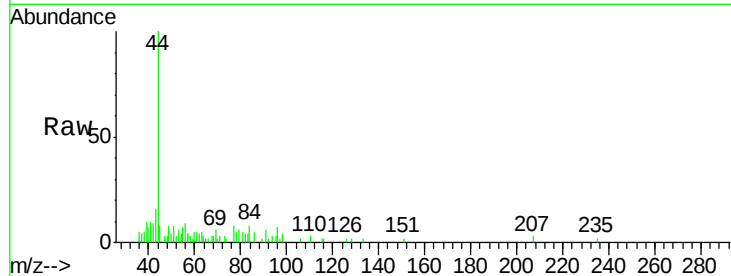

#25

2-Butanone

Concen: 0.72 ug/l

RT: 4.71 min Scan# 677




Delta R.T. -0.01 min


Lab File: VX002073.D

Acq: 27 May 2018 17:18

Tgt Ion: 43 Resp: 2930

Ion	Ratio	Lower	Upper
43	100		
72	17.8	17.9	26.9#

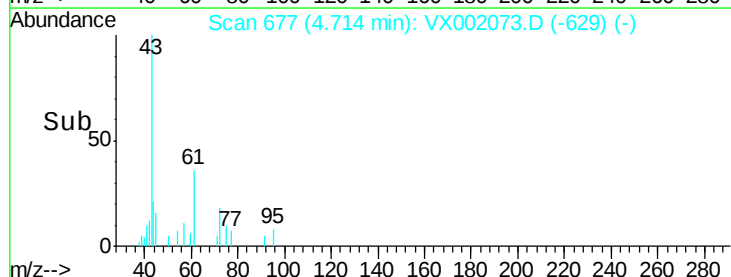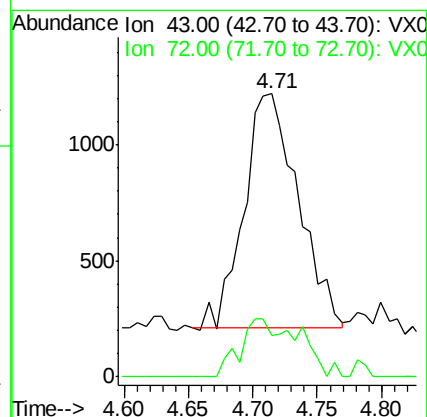



#28

Bromochloromethane

Concen: Below Cal

RT: 5.03 min Scan# 729





Delta R.T. 0.01 min

Lab File: VX002073.D

Acq: 27 May 2018 17:18

Instrument :
MSVOA_X
ClientSampled :

Tot Ion:	49	Resp:	1181
Ion	Ratio	Lower	Upper
49	100		
129	0.0	0.0	3.8
130	68.1	59.4	89.2

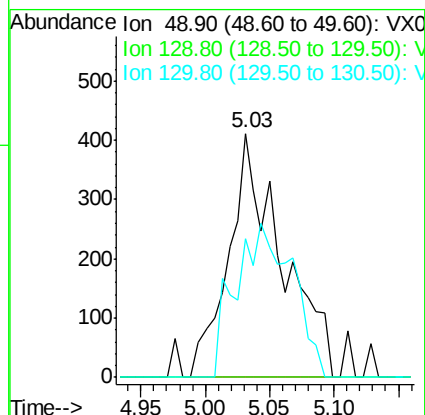

#29

Tetrahydrofuran

Concen: 0.56 ug/l




RT: 5.18 min Scan# 754


Delta R.T. 0.01 min

Lab File: VX002073.D

Acq: 27 May 2018 17:18

Tgt Ion:	42	Resp:	1480
Ion	Ratio	Lower	Upper
42	100		
72	37.0	31.4	47.0
71	0.0	29.5	44.3#



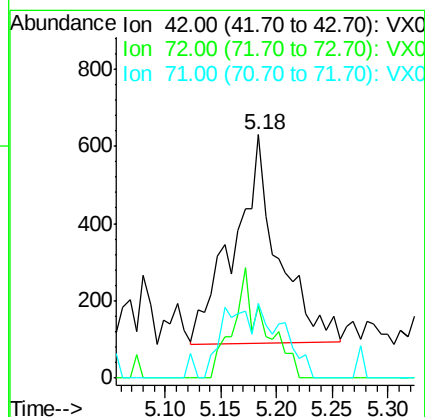





#30
Chloroform
Concen: 0.43 ug/l
RT: 5.21 min Scan# 759
Delta R.T. -0.01 min
Lab File: VX002073.D
Acq: 27 May 2018 17:18




Instrument :
MSVOA_X
ClientSampled :


Tot Ion: 83 Resp: 3641
Ion Ratio Lower Upper
83 100
85 58.5 50.9 76.3

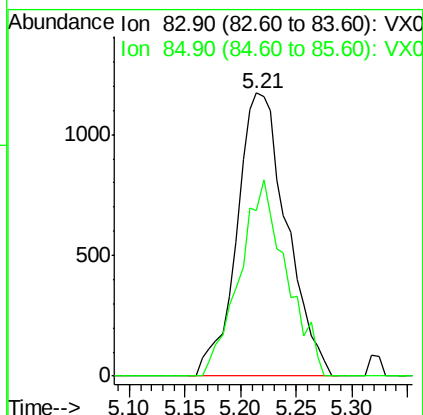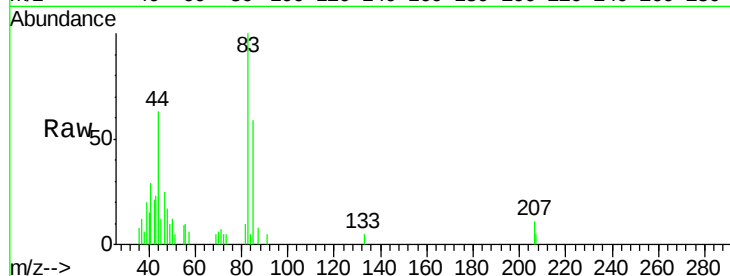

#33
1,2-Dichloroethane-d4
Concen: 36.89 ug/l
RT: 6.07 min Scan# 900
Delta R.T. -0.00 min
Lab File: VX002073.D
Acq: 27 May 2018 17:18

Tgt Ion: 65 Resp: 210997
Ion Ratio Lower Upper
65 100
67 52.1 0.0 104.0



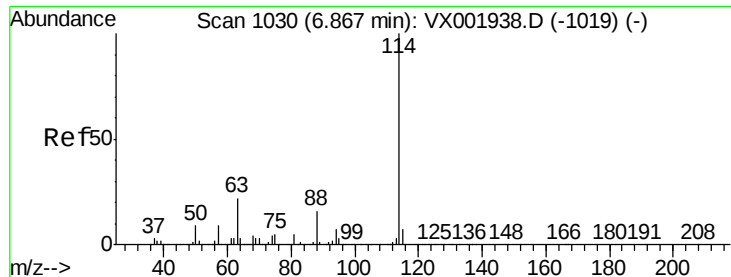

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. -0.00 min

Lab File: VX002073.D

Acq: 27 May 2018 17:18

Instrument :
MSVOA_X
ClientSampled :


Tot Ion:114 Resp: 447550

Ion Ratio Lower Upper




114 100

63 20.9 0.0 43.2

88 15.6 0.0 31.6

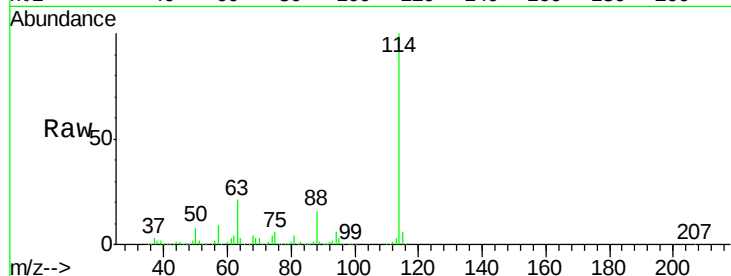

Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VX0
Ion 87.90 (87.60 to 88.60): VX0

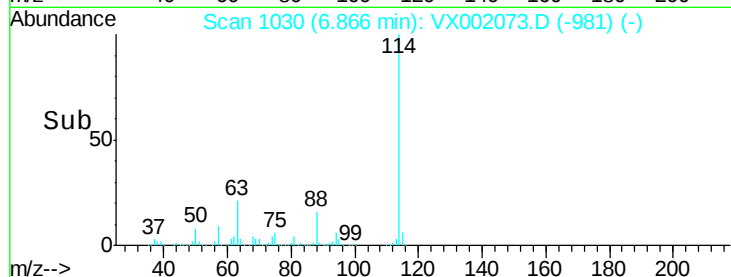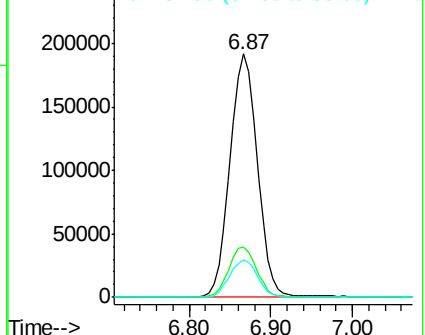

#35

Dibromofluoromethane

Concen: 36.25 ug/l

RT: 5.51 min Scan# 808

Delta R.T. -0.00 min

Lab File: VX002073.D

Acq: 27 May 2018 17:18


Tgt Ion:113 Resp: 162223

Ion Ratio Lower Upper



113 100


111 102.8 82.0 123.0

192 23.4 18.9 28.3



Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V




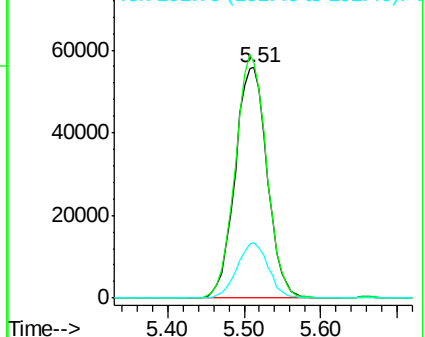




#36
 1,1-Dichloropropene
 Concen: 3.58 ug/l
 RT: 5.67 min Scan# 834
 Delta R.T. -0.13 min
 Lab File: VX002073.D
 Acq: 27 May 2018 17:18




Instrument :
 MSVOA_X
 ClientSampled :




Tot Ion	Ratio	Lower	Upper
75	100		
110	10.8	17.4	52.2#
77	0.1	24.4	36.6#

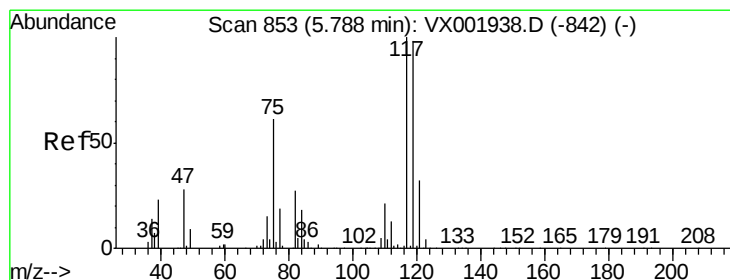

#38
 Carbon Tetrachloride
 Concen: 4.10 ug/l
 RT: 5.67 min Scan# 833
 Delta R.T. -0.12 min
 Lab File: VX002073.D
 Acq: 27 May 2018 17:18

Tgt Ion	Ratio	Lower	Upper
117	100		
119	4.7	78.5	117.7#
121	0.0	25.5	38.3#




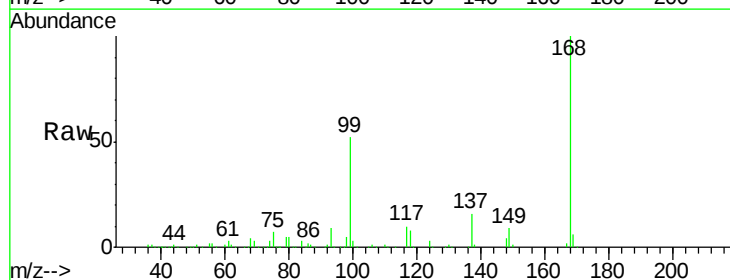


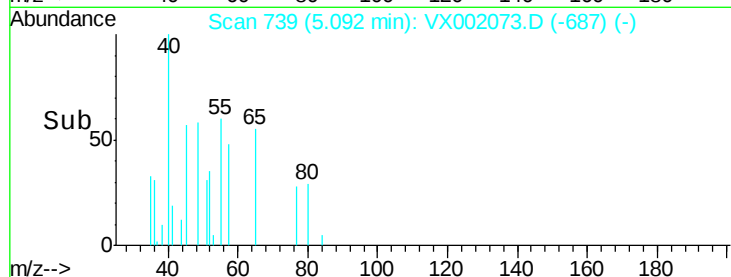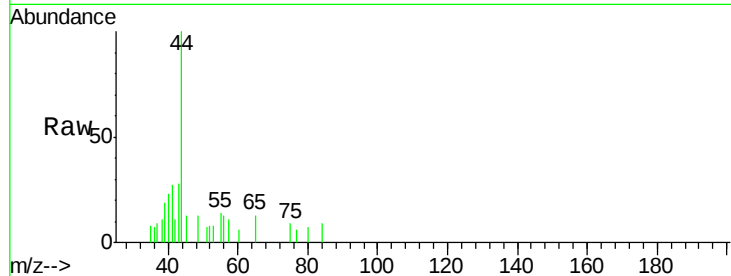

#41
Methacrylonitrile
Concen: Below Cal
RT: 5.09 min Scan# 739
Delta R.T. 0.02 min
Lab File: VX002073.D
Acq: 27 May 2018 17:18


Instrument :
MSVOA_X
ClientSampleId :


Tot Ion:	41	Resp:	79
Ion	Ratio	Lower	Upper
41	100		
39	225.3	46.0	69.0#
67	24.1	50.6	75.8#
52	67.1	21.9	32.9#

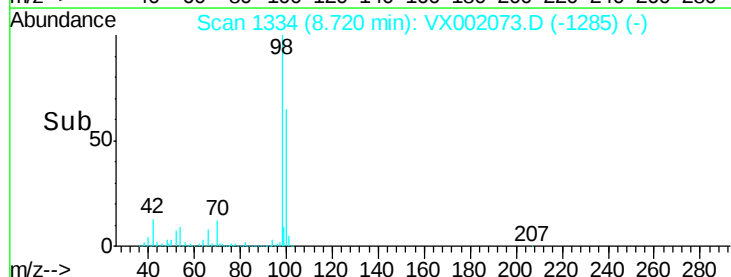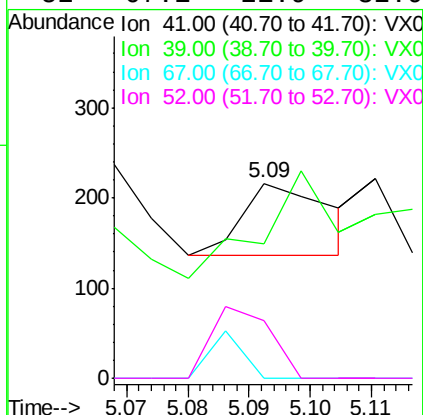

#50
Toluene-d8
Concen: 39.42 ug/l
RT: 8.72 min Scan# 1334
Delta R.T. 0.00 min
Lab File: VX002073.D
Acq: 27 May 2018 17:18

Tgt Ion:	98	Resp:	638678
Ion	Ratio	Lower	Upper
98	100		
100	64.0	51.5	77.3




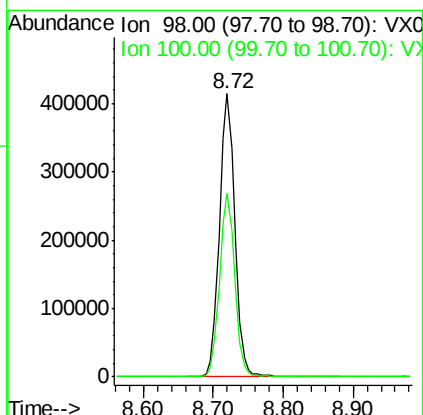




#62
4-Bromofluorobenzene
Concen: 37.22 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. 0.00 min
Lab File: VX002073.D
Acq: 27 May 2018 17:18




Instrument :
MSVOA_X
ClientSampled :


Tot Ion: 95 Resp: 235946
Ion Ratio Lower Upper
95 100
174 91.8 0.0 178.8
176 89.4 0.0 175.6

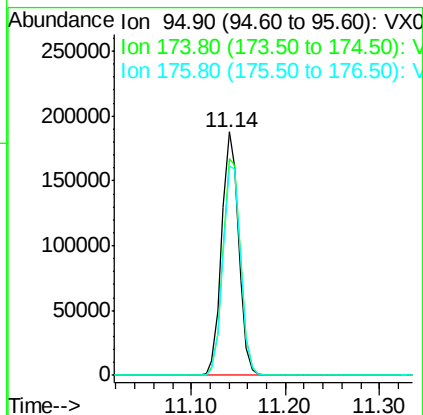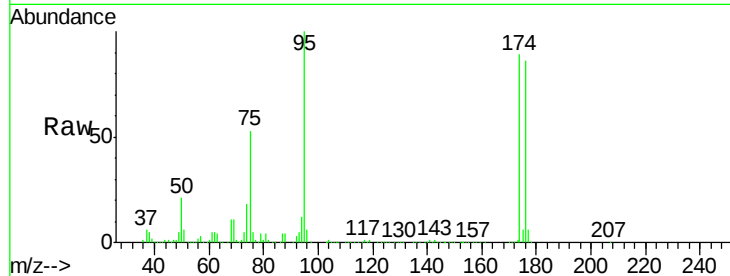

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. -0.00 min
Lab File: VX002073.D
Acq: 27 May 2018 17:18

Tgt Ion: 117 Resp: 408775
Ion Ratio Lower Upper
117 100
82 55.1 44.8 67.2
119 32.0 25.5 38.3


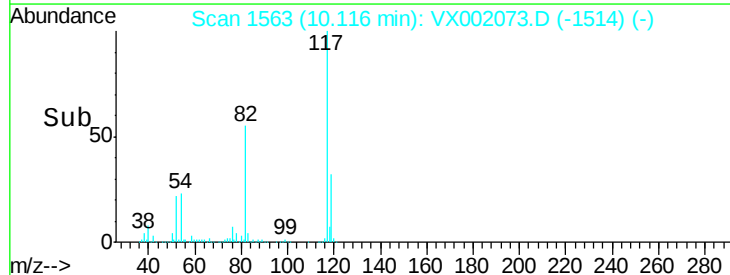
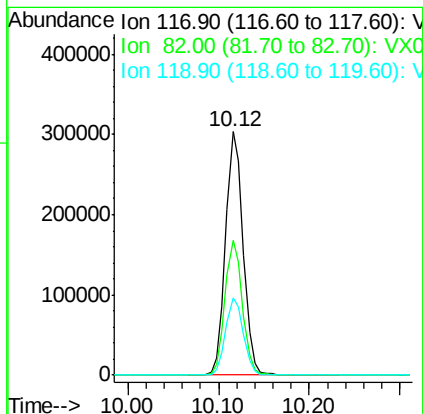





#68
m/p-Xylenes
Concen: 0.22 ug/l
RT: 10.36 min Scan# 1603
Delta R.T. -0.01 min
Lab File: VX002073.D
Acq: 27 May 2018 17:18




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion:106 Resp: 1913
Ion Ratio Lower Upper
106 100
91 208.9 165.0 247.6

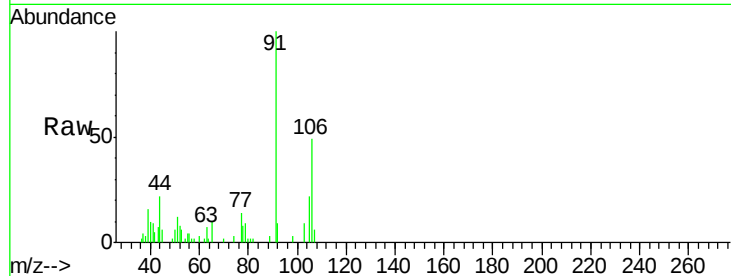

#69
o-Xylene
Concen: 0.21 ug/l
RT: 10.71 min Scan# 1660
Delta R.T. 0.01 min
Lab File: VX002073.D
Acq: 27 May 2018 17:18

Tgt Ion:106 Resp: 1768
Ion Ratio Lower Upper
106 100
91 227.9 108.7 325.9

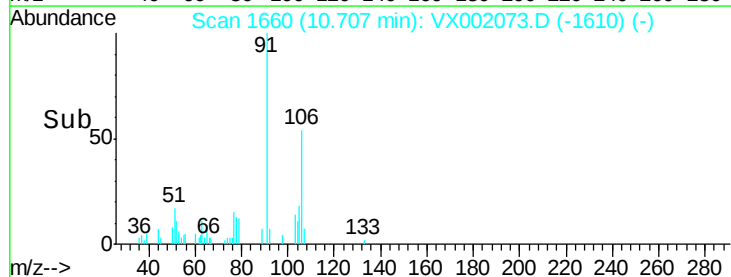




#72




1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.08 min Scan# 1886
Delta R.T. -0.00 min
Lab File: VX002073.D
Acq: 27 May 2018 17:18

Instrument :
MSVOA_X
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
115	54.8	42.3	126.8
150	155.1	0.0	351.0

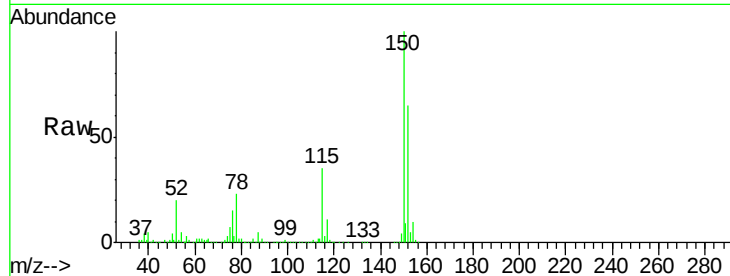


Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

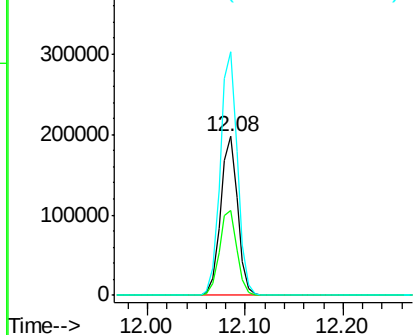



#74


N-ethyl acetate
Concen: Below Cal
RT: 6.46 min Scan# 964
Delta R.T. -0.01 min
Lab File: VX002073.D
Acq: 27 May 2018 17:18

Tgt Ion	Ratio	Lower	Upper
43	100		
70	0.0	0.1	0.1#
55	0.0	0.1	0.1#
61	0.0	14.5	21.7#



Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 70.00 (69.70 to 70.70): VX0
Ion 55.00 (54.70 to 55.70): VX0
Ion 61.00 (60.70 to 61.70): VX0

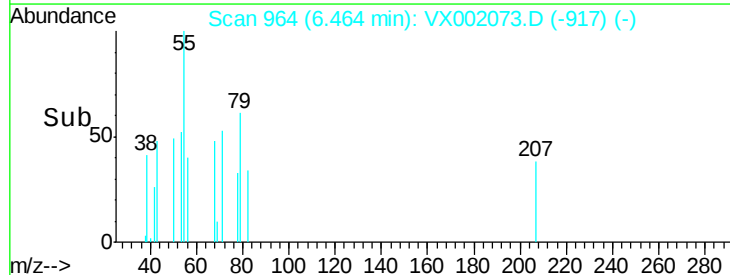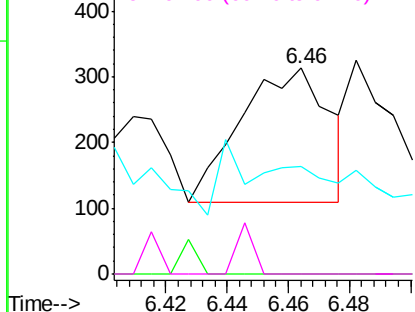

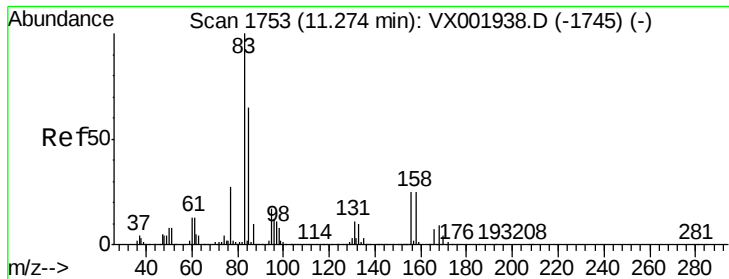

#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 11.26 min Scan# 1751

Delta R.T. -0.01 min

Lab File: VX002073.D

Acq: 27 May 2018 17:18

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion: 83 Resp: 94

Ion Ratio Lower Upper

83 100

131 0.0 5.7 17.0#




85 0.0 32.6 97.7#

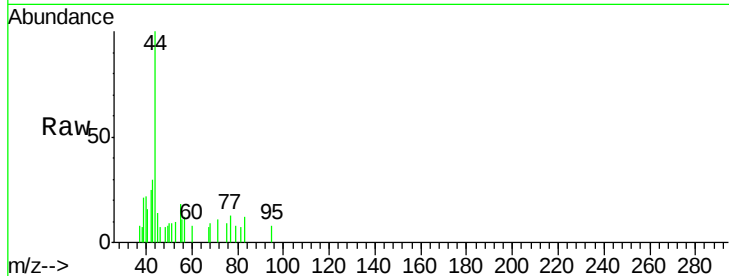

Abundance Ion 82.90 (82.60 to 83.60): VX0

Ion 130.80 (130.50 to 131.50): VX0

Ion 84.90 (84.60 to 85.60): VX0

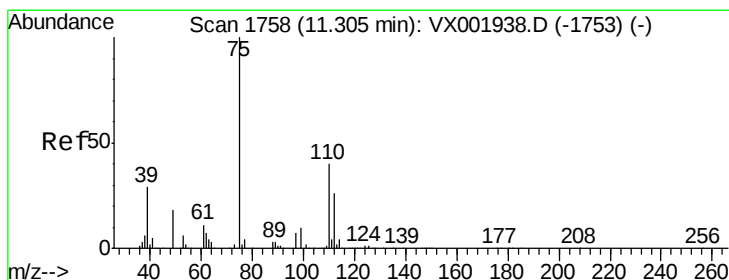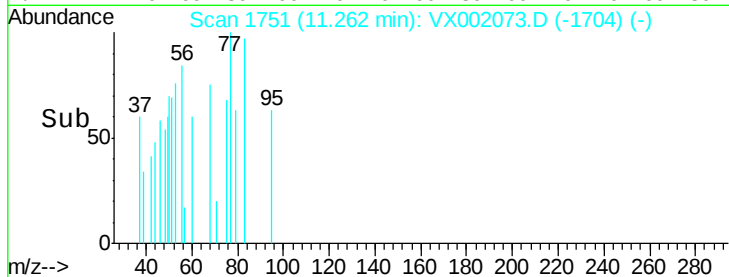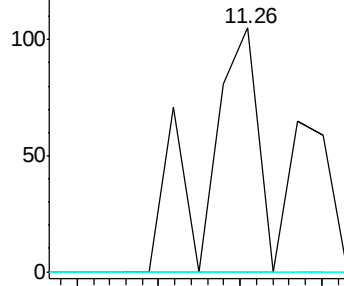

#76

1,2,3-Trichloropropane

Concen: 21.62 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.16 min

Lab File: VX002073.D


Acq: 27 May 2018 17:18

Tgt Ion: 75 Resp: 122883

Ion Ratio Lower Upper



75 100


77 1.2 22.8 68.3#

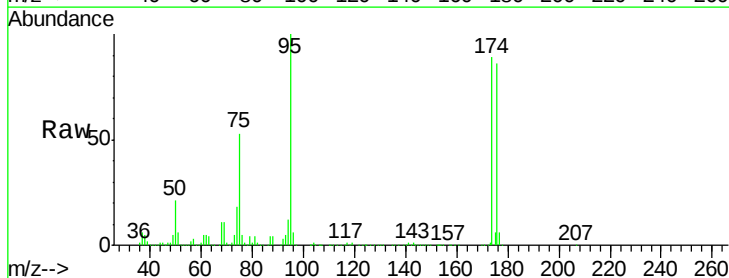

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

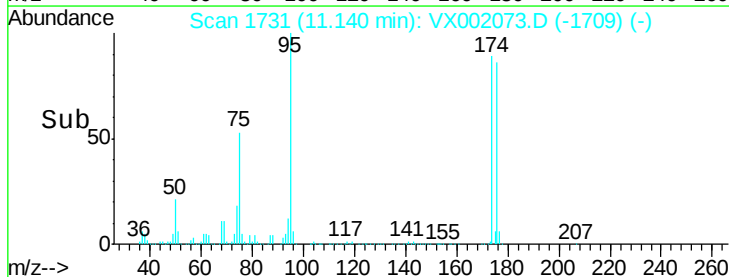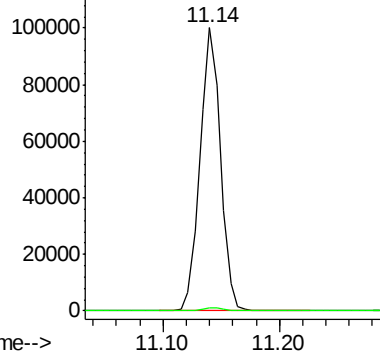



#79

2-Chlorotoluene

Concen: Below Cal

RT: 11.44 min Scan# 1780

Delta R.T. 0.01 min

Lab File: VX002073.D

Acq: 27 May 2018 17:18

Instrument :

MSVOA_X





ClientSampleId :

Tot Ion: 91 Resp: 2123

Ion Ratio Lower Upper

91 100

126 0.0 17.4 52.2#

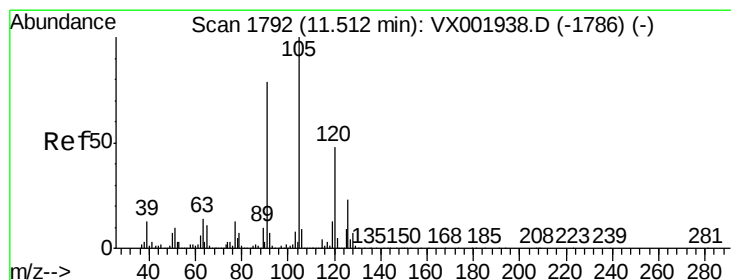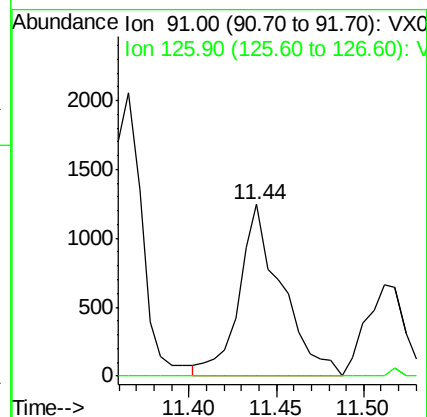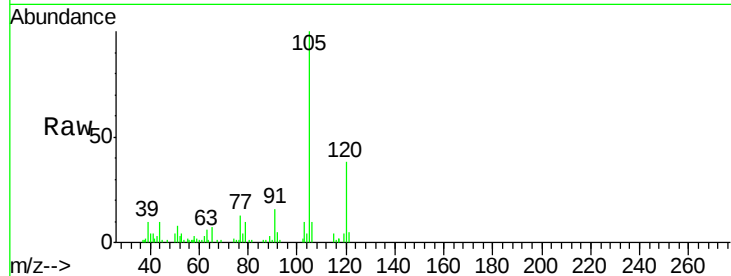

#80

1,3,5-Trimethylbenzene

Concen: 0.42 ug/l

RT: 11.51 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX002073.D




Acq: 27 May 2018 17:18


Tgt Ion: 105 Resp: 7207

Ion Ratio Lower Upper

105 100

120 52.8 24.1 72.4

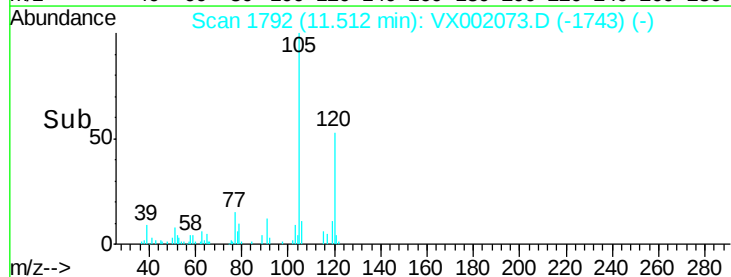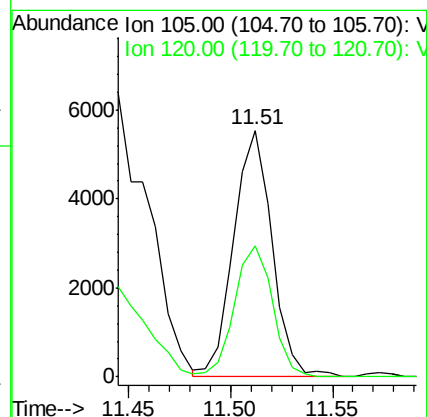

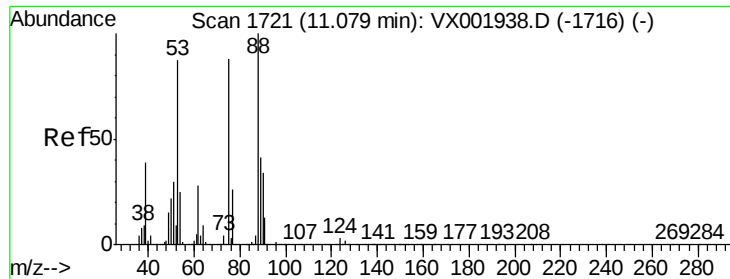

#81

trans-1,4-Dichloro-2-butene

Concen: 51.96 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.06 min

Lab File: VX002073.D

Acq: 27 May 2018 17:18

Instrument :

MSVOA_X

ClientSampled :


Tot Ion: 75 Resp: 122883

Ion Ratio Lower Upper

75 100

53 0.2 78.0 117.0#




89 0.0 39.4 59.2#

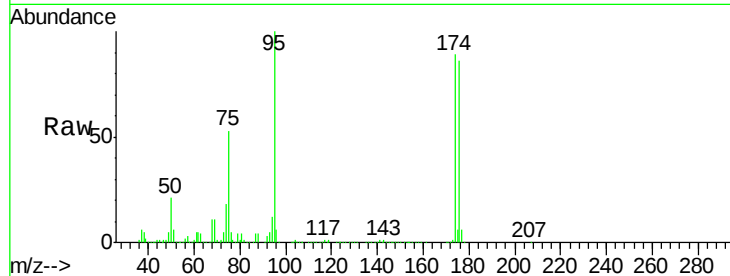

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

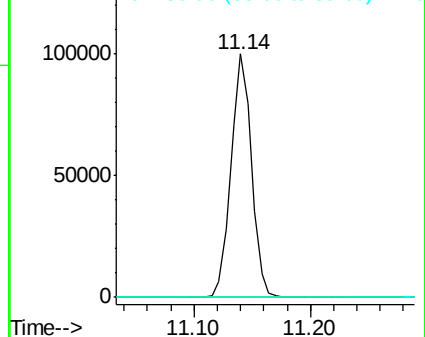

#83

tert-Butylbenzene

Concen: 0.27 ug/l

RT: 11.81 min Scan# 1841

Delta R.T. 0.04 min

Lab File: VX002073.D

Acq: 27 May 2018 17:18


Tgt Ion: 119 Resp: 4572

Ion Ratio Lower Upper

119 100

91 83.2 30.6 91.8



134 0.0 11.7 35.0#




Abundance Ion 119.00 (118.70 to 119.70): V

Ion 91.00 (90.70 to 91.70): VX0

Ion 134.00 (133.70 to 134.70): V

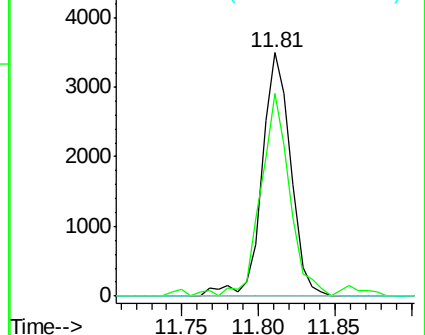



#84

1,2,4-Trimethylbenzene

Concen: 1.94 ug/l

RT: 11.81 min Scan# 1841

Delta R.T. -0.00 min

Lab File: VX002073.D

Acq: 27 May 2018 17:18

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion:105 Resp: 34381

Ion Ratio Lower Upper




105 100

120 44.4 22.1 66.5

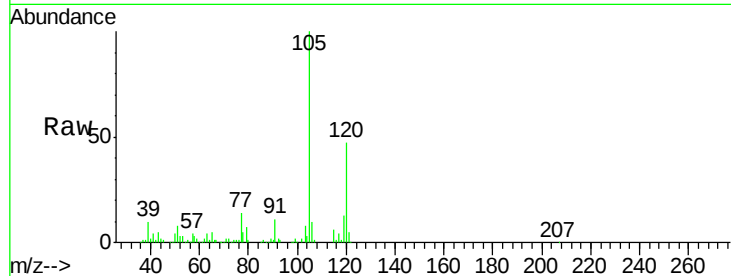

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

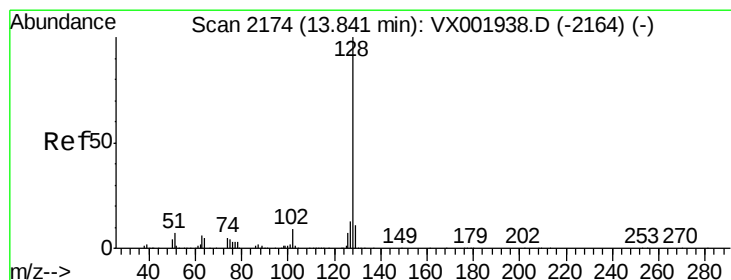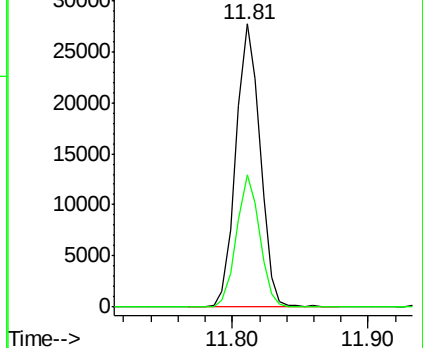

#95

Naphthalene

Concen: 2.82 ug/l

RT: 13.84 min Scan# 2174

Delta R.T. -0.00 min

Lab File: VX002073.D

Acq: 27 May 2018 17:18


Tgt Ion:128 Resp: 60244

Ion Ratio Lower Upper

128 100

127 12.8 10.4 15.6

129 11.6 8.8 13.2



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

