

Data Path : W:\HPCHEM1\MSVOA X\DATA\X052718\
 Data File : VX002074.D
 Acq On : 27 May 2018 17:45
 Operator : JC/MD
 Sample : J2679-30
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: May 29 02:58:28 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 24 13:09:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	313013	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	439875	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	397416	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	222546	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	204947	36.63	ug/l	0.00
Spiked Amount	50.000		Recovery	=	73.26%	
35) Dibromofluoromethane	5.51	113	158257	35.98	ug/l	0.00
Spiked Amount	50.000		Recovery	=	71.96%	
50) Toluene-d8	8.72	98	628842	39.49	ug/l	0.00
Spiked Amount	50.000		Recovery	=	78.98%	
62) 4-Bromofluorobenzene	11.14	95	224389	36.01	ug/l	0.00
Spiked Amount	50.000		Recovery	=	72.02%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.20	85	143	Below Cal	#	41
3) Chloromethane	1.33	50	3941	0.82	ug/l	# 88
5) Bromomethane	1.64	94	552	Below Cal	#	29
11) Tert butyl alcohol	3.03	59	3203	2.92	ug/l	# 81
13) Acrolein	2.30	56	290	0.61	ug/l	# 58
16) Acetone	2.45	43	19057	8.83	ug/l	97
18) Methyl Acetate	2.78	43	24491	3.65	ug/l	98
20) Methylene Chloride	2.86	84	99797	25.89	ug/l	98
21) trans-1,2-Dichloroethene	3.17	96	213	Below Cal	#	44
25) 2-Butanone	4.71	43	3455	0.87	ug/l	99
28) Bromochloromethane	5.02	49	67	Below Cal	#	14
29) Tetrahydrofuran	5.18	42	1217	0.47	ug/l	97
30) Chloroform	5.22	83	3559	0.43	ug/l	93
36) 1,1-Dichloropropene	5.67	75	22084	3.61	ug/l	# 52
38) Carbon Tetrachloride	5.67	117	29087	4.08	ug/l	# 15
41) Methacrylonitrile	5.09	41	244	Below Cal	#	32
68) m/p-Xylenes	10.36	106	3583	0.43	ug/l	99
69) o-Xylene	10.70	106	2815	0.34	ug/l	99
74) N-amyl acetate	6.49	43	146	Below Cal	#	59
75) 1,1,2,2-Tetrachloroethane	11.26	83	90	Below Cal	#	25
76) 1,2,3-Trichloropropane	11.14	75	116722	21.84	ug/l	# 33
78) n-propylbenzene	11.36	91	4470	0.21	ug/l	100
79) 2-Chlorotoluene	11.44	91	3184	Below Cal	#	52
80) 1,3,5-Trimethylbenzene	11.51	105	9151	0.57	ug/l	97
81) trans-1,4-Dichloro-2-buten	11.14	75	116722	52.48	ug/l	# 10
84) 1,2,4-Trimethylbenzene	11.81	105	40618	2.44	ug/l	98
89) n-Butylbenzene	12.39	91	3029	0.21	ug/l	# 31
95) Naphthalene	13.84	128	116804	5.81	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX052718\
Data File : VX002074.D
Acq On : 27 May 2018 17:45
Operator : JC/MD
Sample : J2679-30
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: May 29 02:58:28 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Quant Title : SW846 8260
QLast Update : Thu May 24 13:09:03 2018
Response via : Initial Calibration

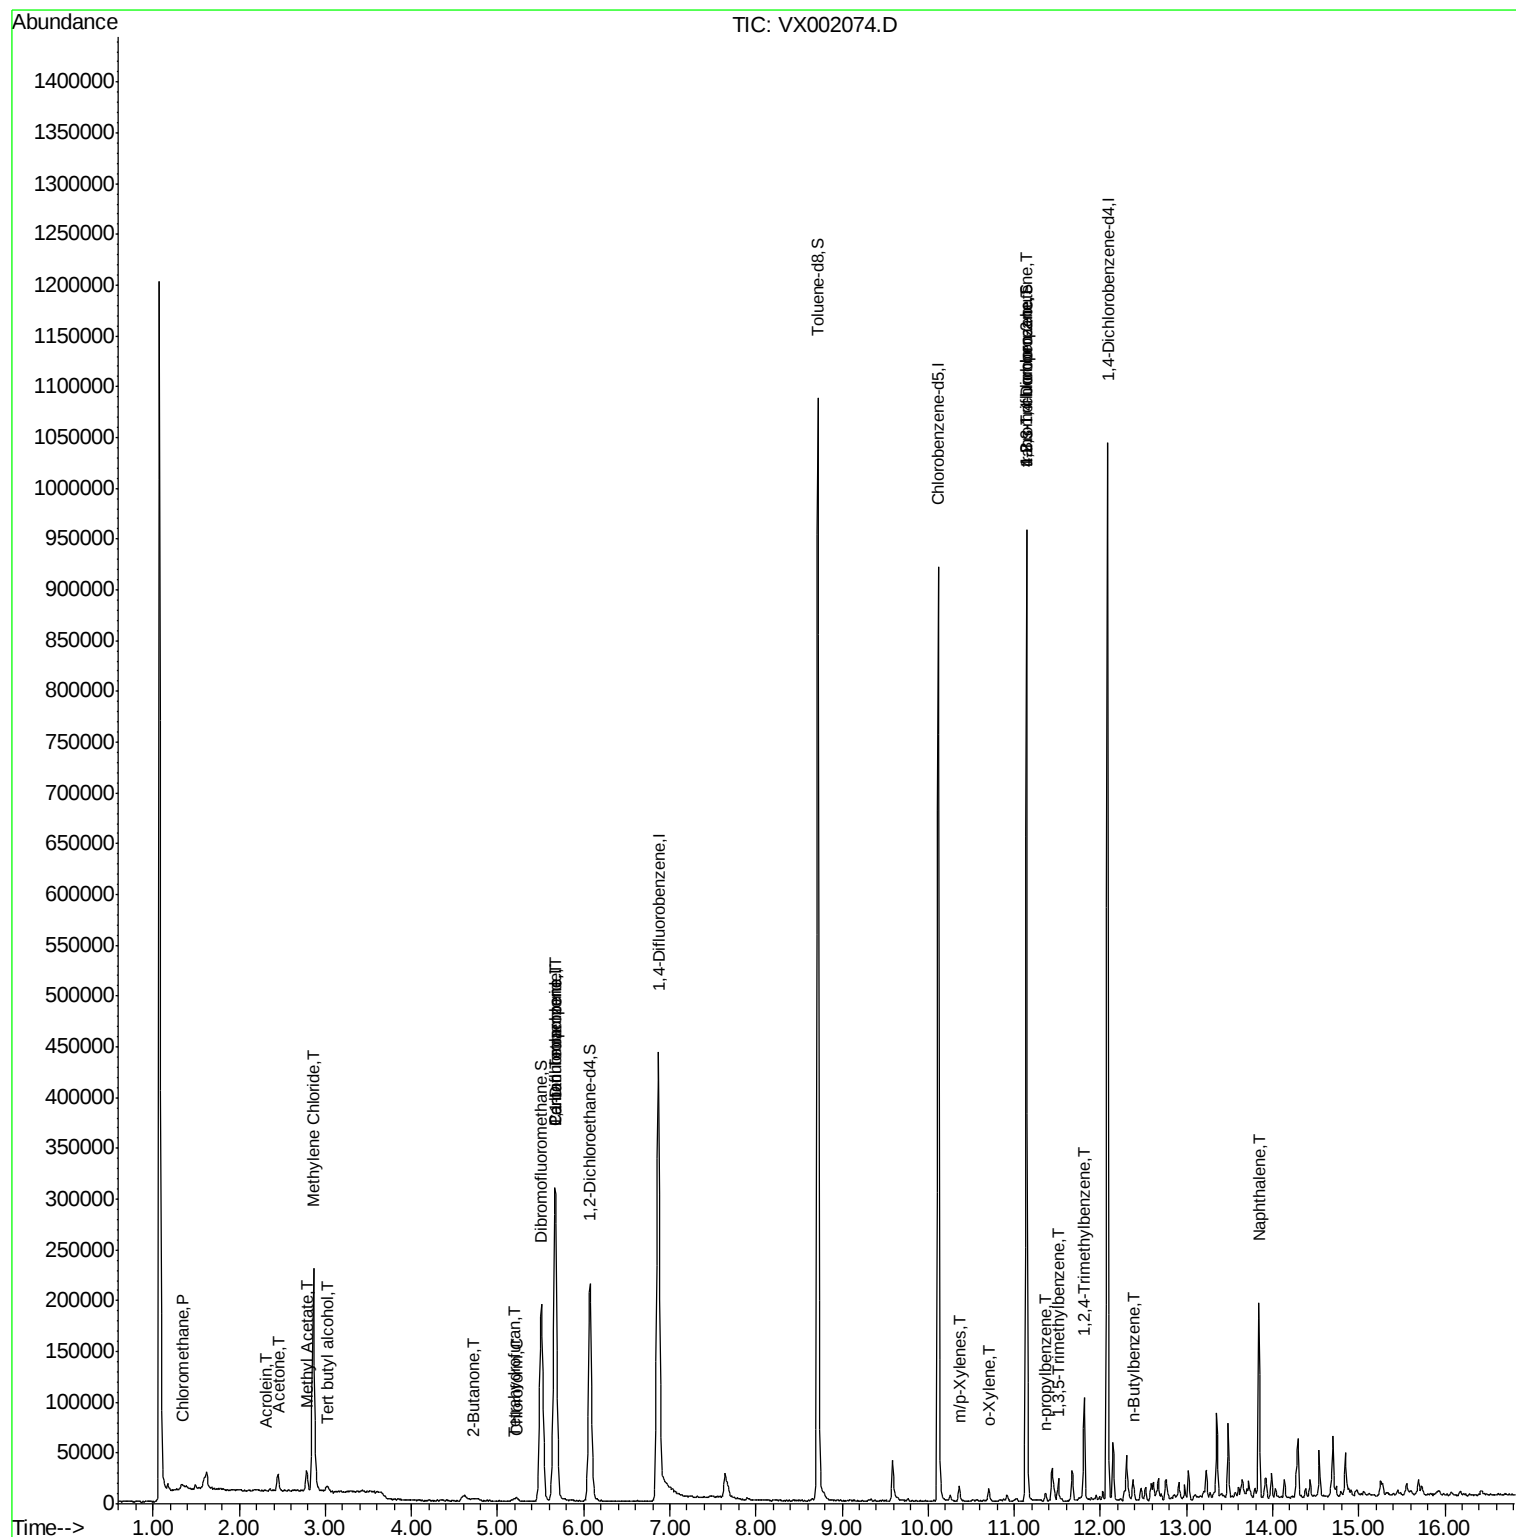



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.00 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45


Instrument :
MSVOA_X
ClientSampleId :

Tot Ion:168 Resp: 313013

Ion Ratio Lower Upper

168 100

99 50.0 41.0 61.4



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

120000

100000

80000



60000

40000

20000

0

Time-->



#2

Dichlorodifluoromethane

Concen: Below Cal

RT: 1.20 min Scan# 100

Delta R.T. 0.00 min

Lab File: VX002074.D


Acq: 27 May 2018 17:45

Tgt Ion: 85 Resp: 143

Ion Ratio Lower Upper

85 100

87 0.0 16.7 50.0#



Abundance Ion 84.90 (84.60 to 85.60): VX0

Ion 86.90 (86.60 to 87.60): VX0

1.20


150


100

50

0

Time-->



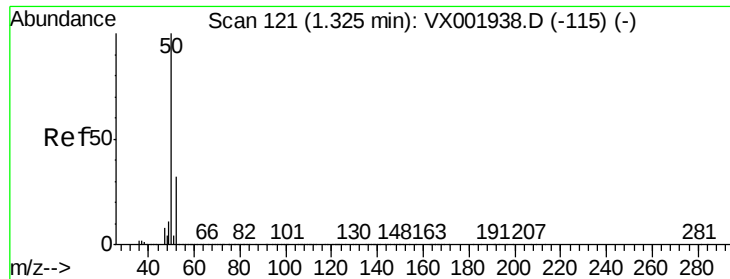

#3

Chloromethane

Concen: 0.82 ug/l

RT: 1.33 min Scan# 122

Delta R.T. 0.01 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45

Instrument :

MSVOA_X





ClientSampleId :

Tot Ion: 50 Resp: 3941

Ion Ratio Lower Upper

50 100

52 25.5 26.0 39.0#

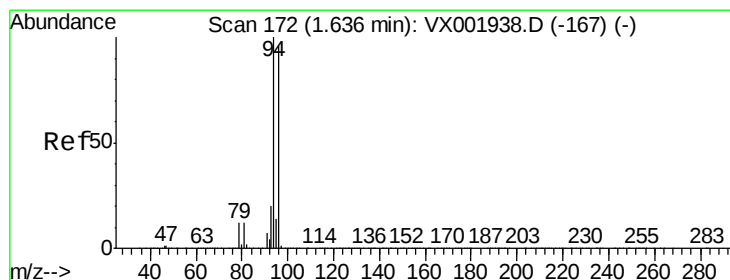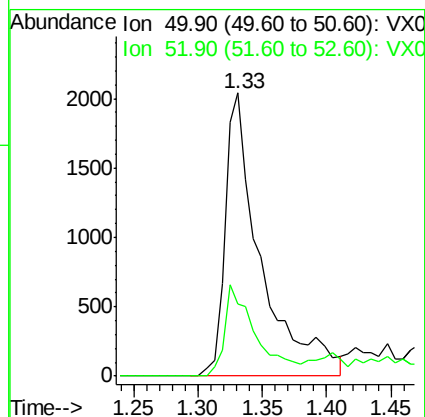

#5

Bromomethane

Concen: Below Cal

RT: 1.64 min Scan# 173

Delta R.T. 0.01 min

Lab File: VX002074.D




Acq: 27 May 2018 17:45


Tgt Ion: 94 Resp: 552

Ion Ratio Lower Upper

94 100

96 26.0 75.9 113.9#

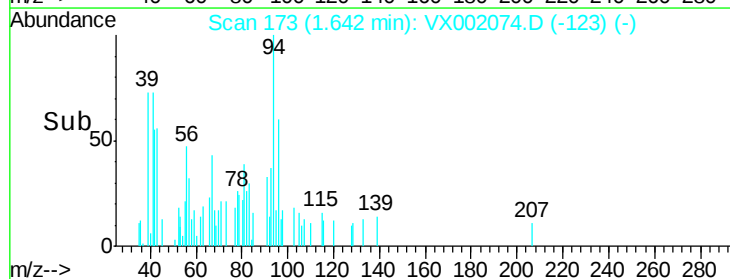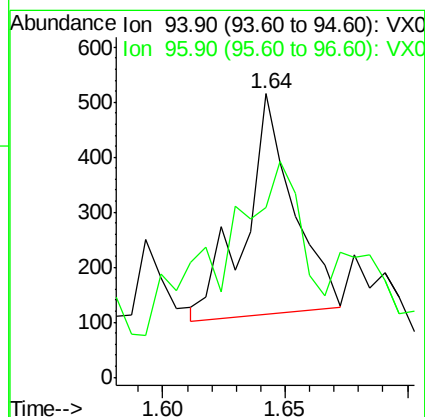







#11

Tert butvl alcohol
 Concen: 2.92 ug/l
 RT: 3.03 min Scan# 400
 Delta R.T. -0.06 min
 Lab File: VX002074.D
 Acq: 27 May 2018 17:45

Instrument :
 MSVOA_X
 ClientSampleId :




Tot Ion: 59 Resp: 3203
 Ion Ratio Lower Upper
 59 100
 57 4.0 8.9 13.3#

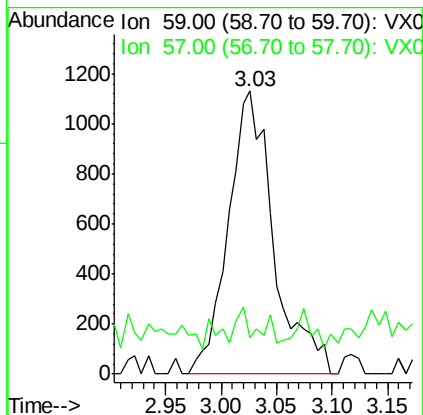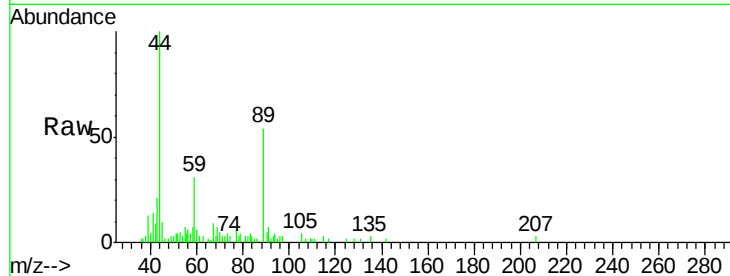


#13

Acrolein
 Concen: 0.61 ug/l
 RT: 2.30 min Scan# 281
 Delta R.T. 0.00 min
 Lab File: VX002074.D
 Acq: 27 May 2018 17:45

Tgt Ion: 56 Resp: 290
 Ion Ratio Lower Upper
 56 100
 55 105.9 56.8 85.2#

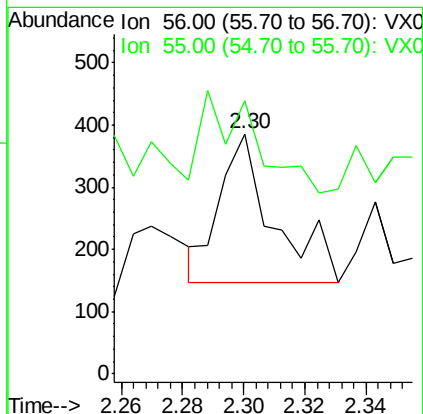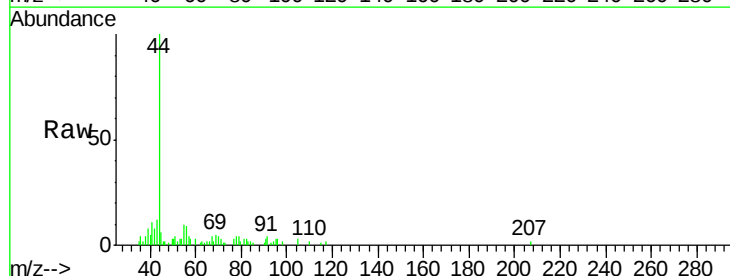



#16

Acetone

Concen: 8.83 ug/l

RT: 2.45 min Scan# 305

Delta R.T. -0.01 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 43 Resp: 19057

Ion Ratio Lower Upper

43 100

58 26.5 22.3 33.5



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

12000

10000

8000

6000



4000

2000

0

2.35 2.40 2.45 2.50

Time-->



#18

Methyl Acetate

Concen: 3.65 ug/l

RT: 2.78 min Scan# 360

Delta R.T. 0.00 min

Lab File: VX002074.D


Acq: 27 May 2018 17:45

Tgt Ion: 43 Resp: 24491

Ion Ratio Lower Upper

43 100

74 22.0 16.8 25.2



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0

15000


10000


5000

0

2.70 2.75 2.80 2.85

Time-->







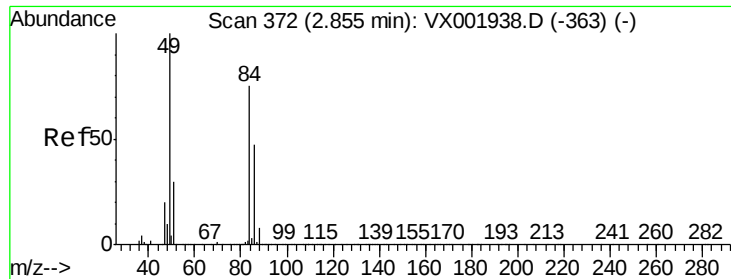

#20
Methvlene Chloride
Concen: 25.89 ua/l
RT: 2.86 min Scan# 373
Delta R.T. 0.01 min
Lab File: VX002074.D
Acq: 27 May 2018 17:45




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion:	84	Resp:	99797
Ion	Ratio	Lower	Upper
84	100		
49	131.3	107.2	160.8
51	40.7	32.4	48.6
86	65.7	50.4	75.6

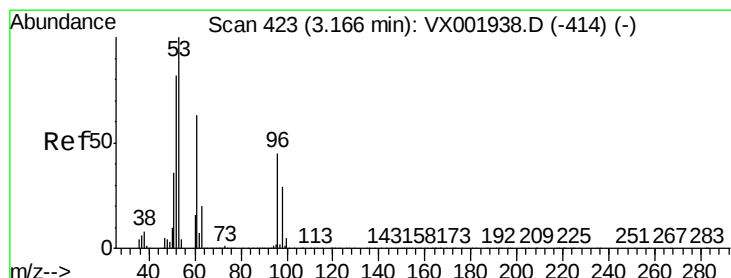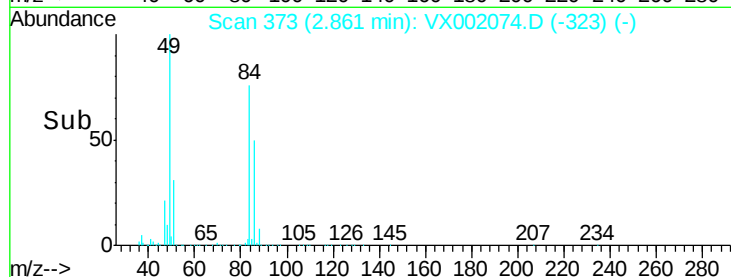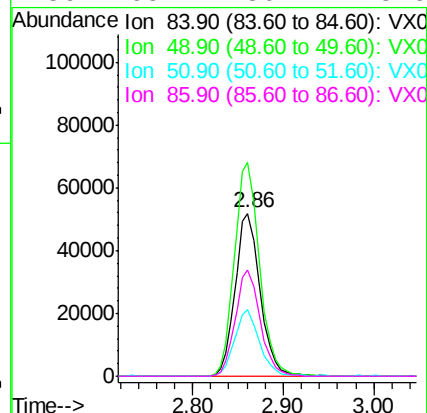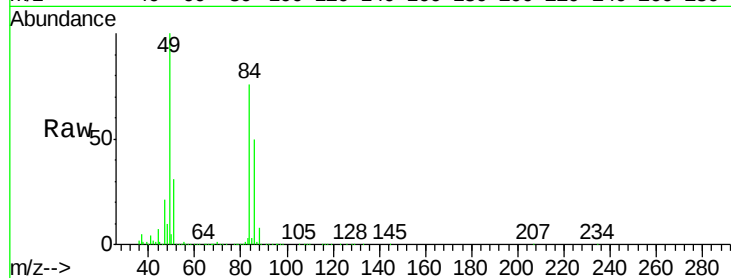

#21
trans-1,2-Dichloroethene
Concen: Below Cal
RT: 3.17 min Scan# 424
Delta R.T. 0.01 min
Lab File: VX002074.D
Acq: 27 May 2018 17:45

Tgt Ion:	96	Resp:	213
Ion	Ratio	Lower	Upper
96	100		
61	65.2	113.3	169.9#
98	97.8	51.7	77.5#

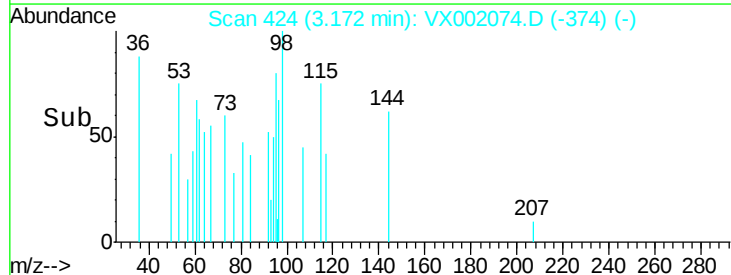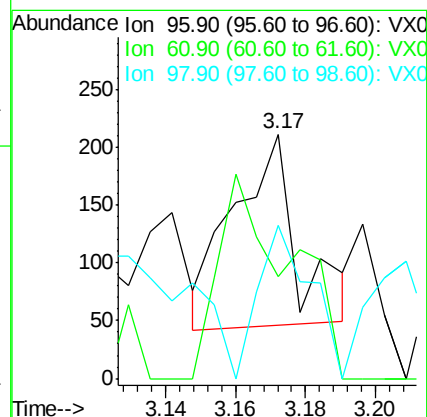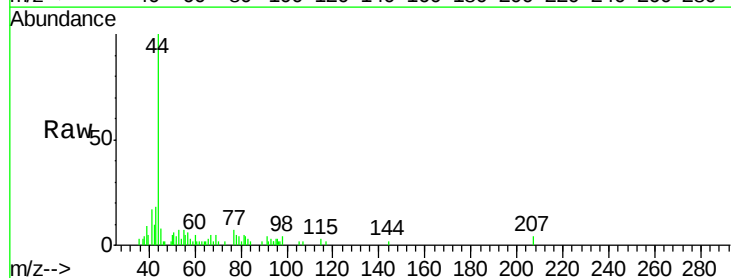



#25

2-Butanone

Concen: 0.87 ug/l

RT: 4.71 min Scan# 677

Delta R.T. -0.01 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45

Instrument :

MSVOA_X





ClientSampled :

Tot Ion: 43 Resp: 3455

Ion Ratio Lower Upper

43 100

72 21.7 17.9 26.9

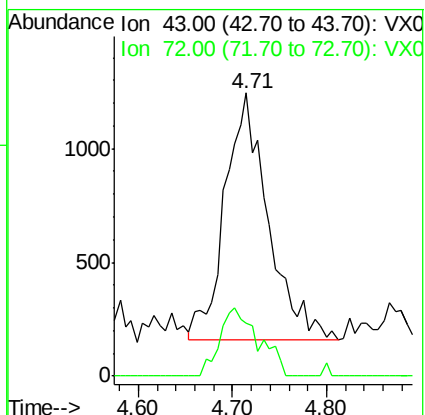

#28

Bromochloromethane

Concen: Below Cal

RT: 5.02 min Scan# 727

Delta R.T. -0.01 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45




Tgt Ion: 49 Resp: 67


Ion Ratio Lower Upper

49 100

129 0.0 0.0 3.8

130 0.0 59.4 89.2#

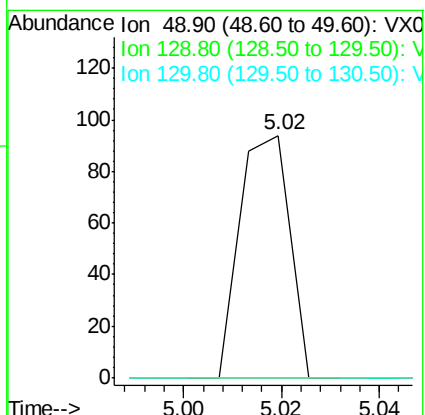



#29

Tetrahydrofuran

Concen: 0.47 ug/l

RT: 5.18 min Scan# 754





Delta R.T. 0.01 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45

Instrument :
MSVOA_X
ClientSampleId :

Tot Ion:	42	Resp:	1217
Ion	Ratio	Lower	Upper
42	100		
72	38.3	31.4	47.0
71	34.5	29.5	44.3

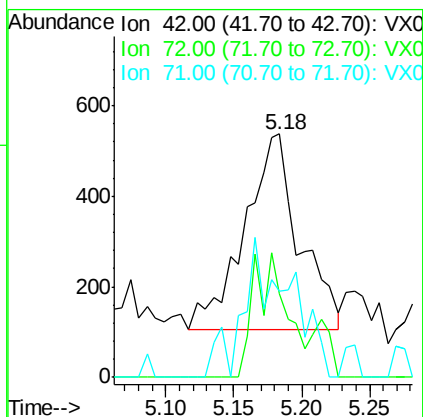

#30

Chloroform

Concen: 0.43 ug/l




RT: 5.22 min Scan# 760


Delta R.T. -0.00 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45

Tgt Ion:	83	Resp:	3559
Ion	Ratio	Lower	Upper
83	100		
85	57.9	50.9	76.3

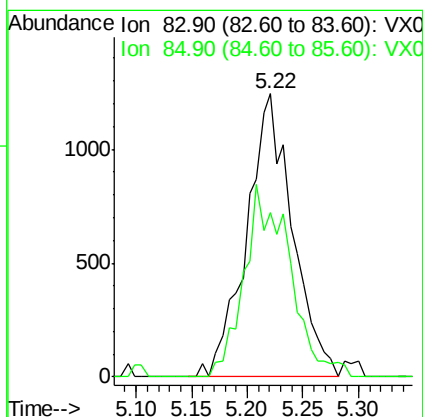



#33

1,2-Dichloroethane-d4

Concen: 36.63 ug/l

RT: 6.07 min Scan# 900

Delta R.T. 0.00 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 65 Resp: 204947

Ion Ratio Lower Upper




65 100

67 51.6 0.0 104.0

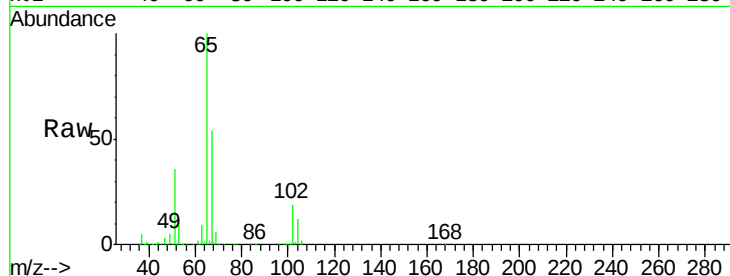

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

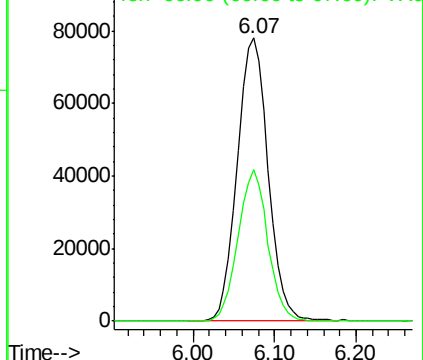

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. 0.00 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45


Tgt Ion: 114 Resp: 439875

Ion Ratio Lower Upper

114 100

63 21.6 0.0 43.2



88 16.0 0.0 31.6




Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

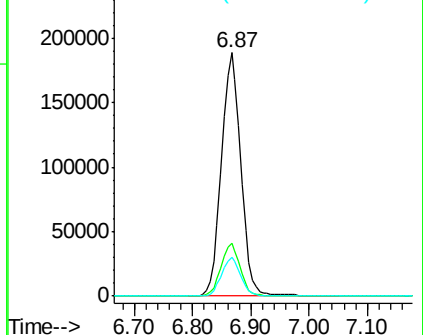

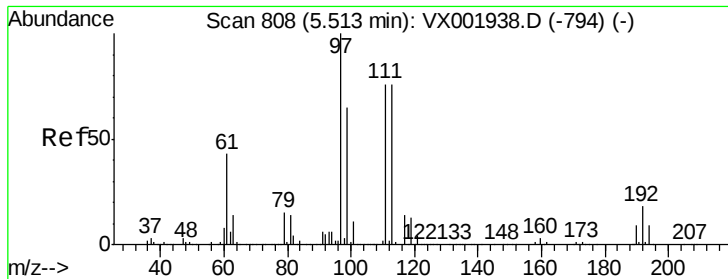

#35

Dibromofluoromethane

Concen: 35.98 ug/l

RT: 5.51 min Scan# 807


Delta R.T. -0.01 min

Lab File: VX002074.D




Acq: 27 May 2018 17:45

Instrument :
MSVOA_X
ClientSampleId :

Tot Ion:	113	Resp:	158257
Ion	Ratio	Lower	Upper
113	100		
111	102.3	82.0	123.0
192	23.8	18.9	28.3

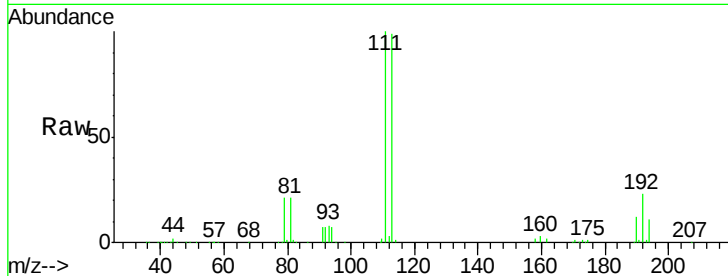

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

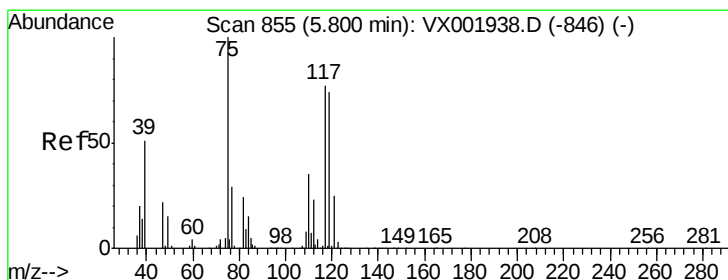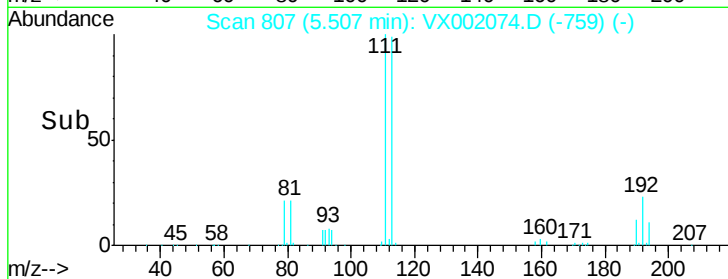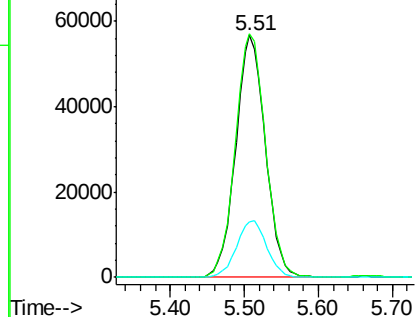

#36

1,1-Dichloropropene

Concen: 3.61 ug/l


RT: 5.67 min Scan# 833

Delta R.T. -0.13 min



Lab File: VX002074.D


Acq: 27 May 2018 17:45

Tgt Ion:	75	Resp:	22084
Ion	Ratio	Lower	Upper
75	100		
110	10.6	17.4	52.2#
77	0.5	24.4	36.6#

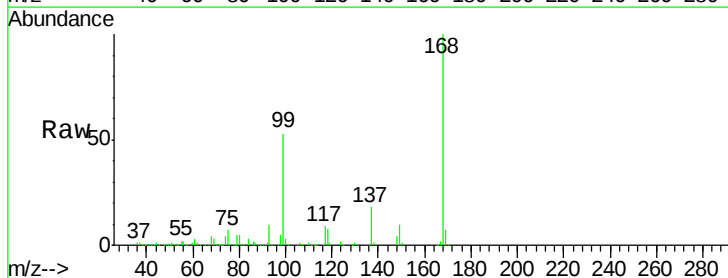

Abundance Ion 74.90 (74.60 to 75.60): VX0
Ion 109.90 (109.60 to 110.60): V
Ion 76.90 (76.60 to 77.60): VX0

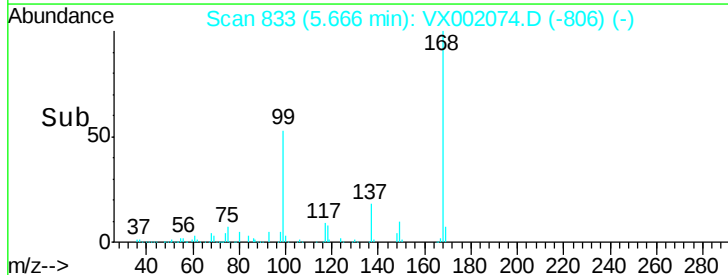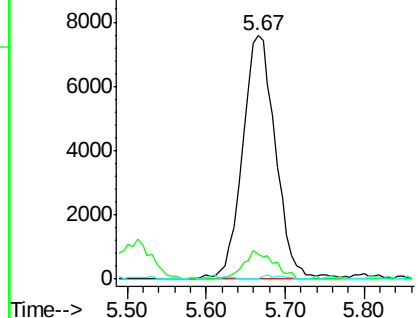

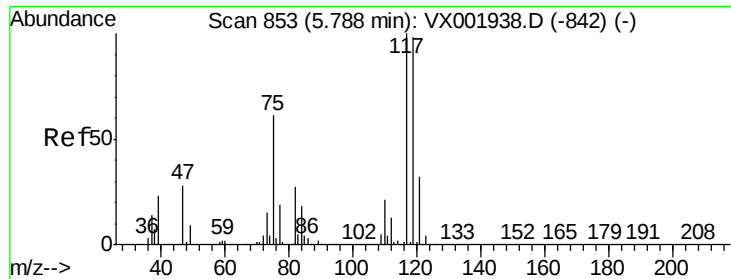

#38

Carbon Tetrachloride

Concen: 4.08 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.12 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45

Instrument :
MSVOA_X
ClientSampled :


Tot Ion:117 Resp: 29087

Ion Ratio Lower Upper




117 100

119 5.4 78.5 117.7#

121 0.0 25.5 38.3#

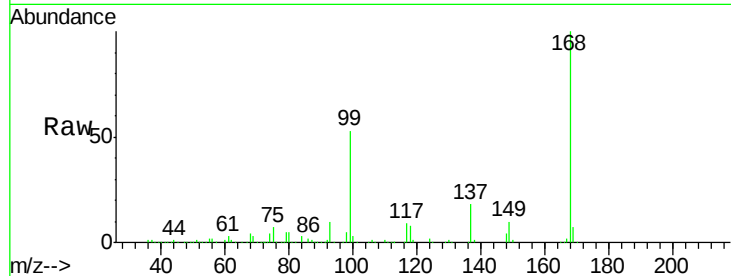

Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V

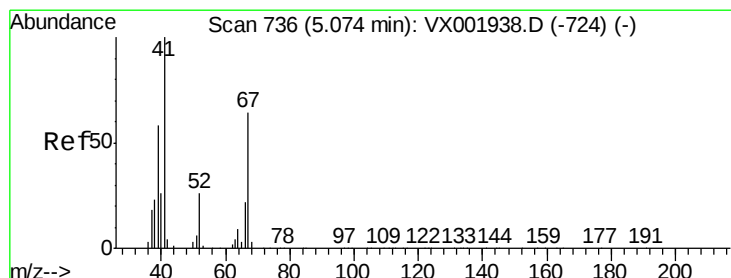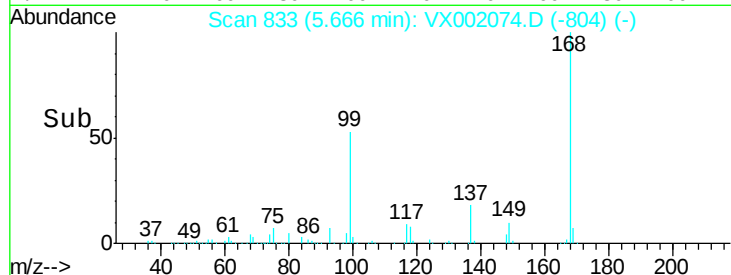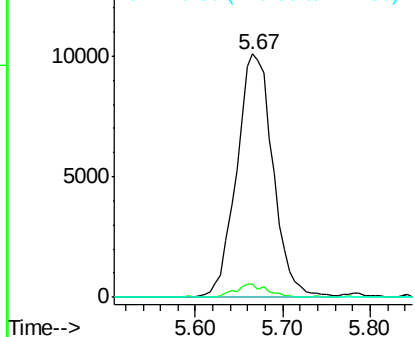

#41

Methacrylonitrile

Concen: Below Cal

RT: 5.09 min Scan# 738

Delta R.T. 0.01 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45

Tgt Ion: 41 Resp: 244


Ion Ratio Lower Upper

41 100



39 12.7 46.0 69.0#


67 0.0 50.6 75.8#

52 0.0 21.9 32.9#

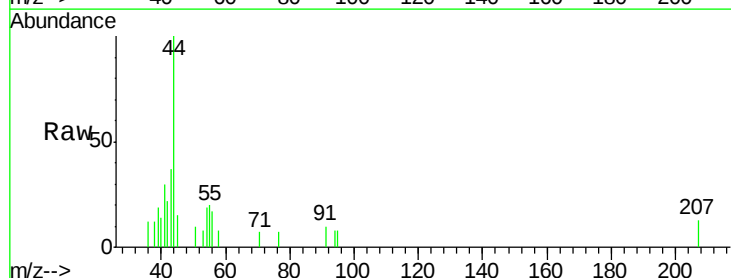

Abundance Ion 41.00 (40.70 to 41.70): VX0
Ion 39.00 (38.70 to 39.70): VX0
Ion 67.00 (66.70 to 67.70): VX0
Ion 52.00 (51.70 to 52.70): VX0

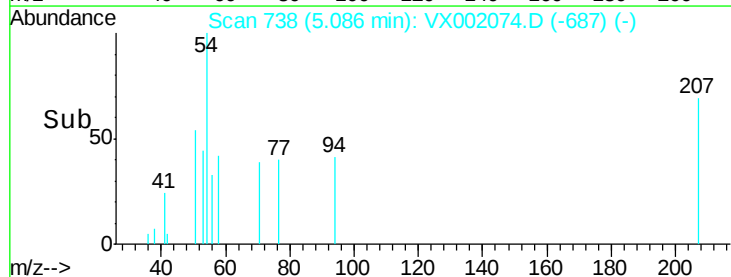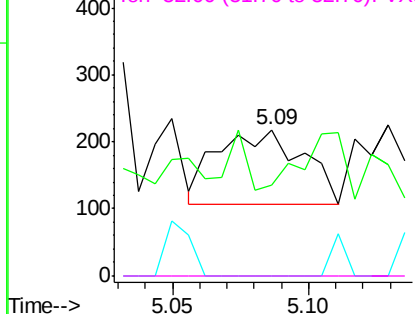

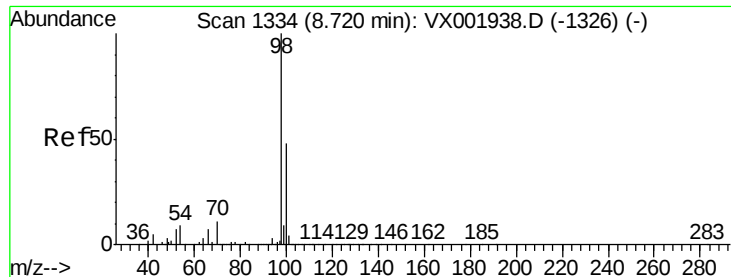

#50

Toluene-d8

Concen: 39.49 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. 0.00 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45

Instrument :

MSVOA_X





ClientSampleId :

Tot Ion: 98 Resp: 628842

Ion Ratio Lower Upper

98 100

100 63.0 51.5 77.3

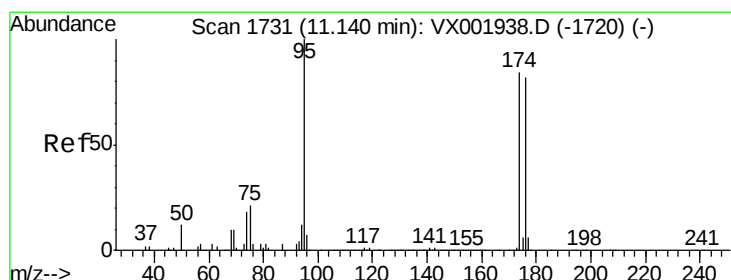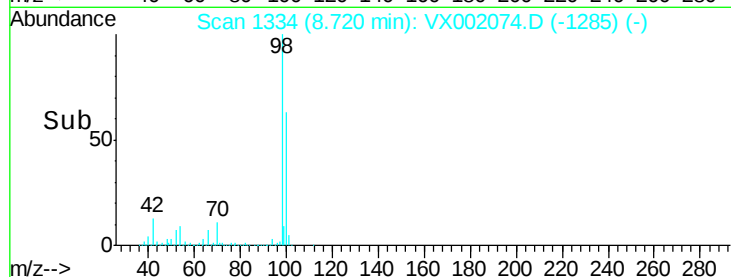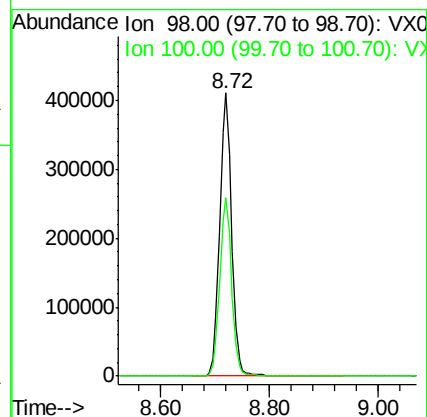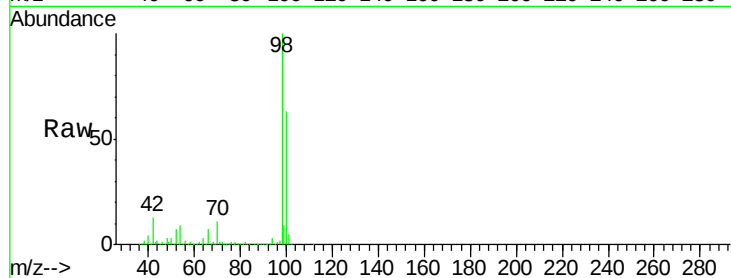

#62

4-Bromofluorobenzene

Concen: 36.01 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.00 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45




Tgt Ion: 95 Resp: 224389


Ion Ratio Lower Upper

95 100

174 93.1 0.0 178.8

176 90.1 0.0 175.6


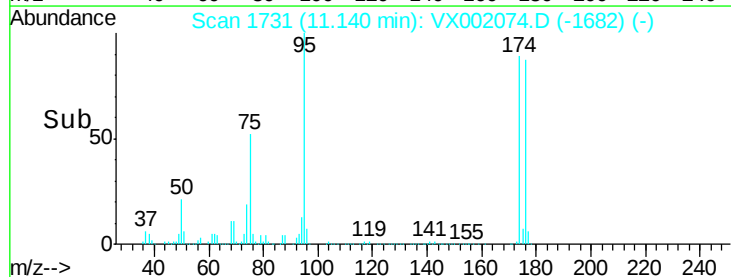
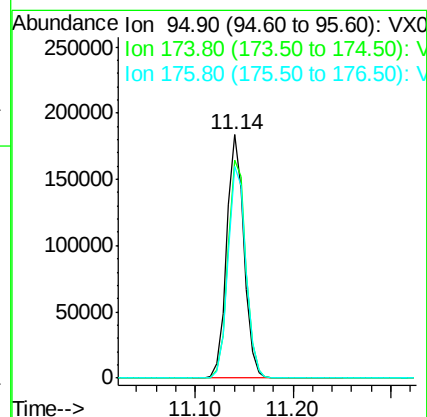
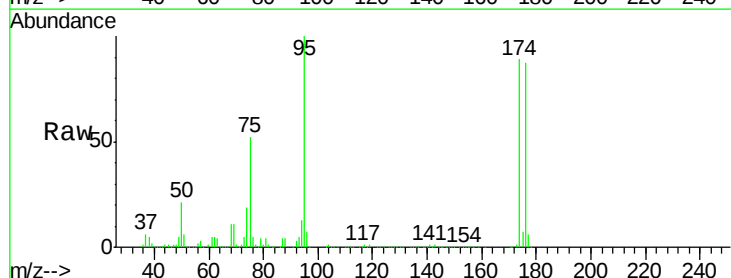




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. 0.00 min
Lab File: VX002074.D
Acq: 27 May 2018 17:45




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
117	100		
82	56.1	44.8	67.2
119	32.2	25.5	38.3

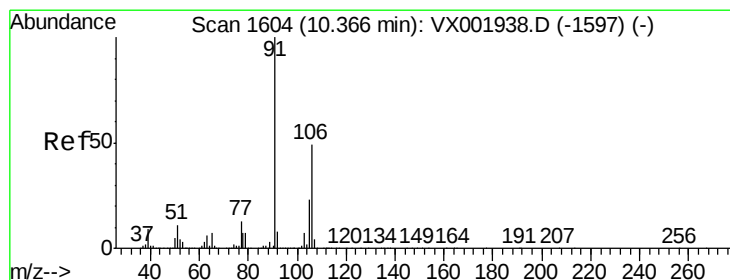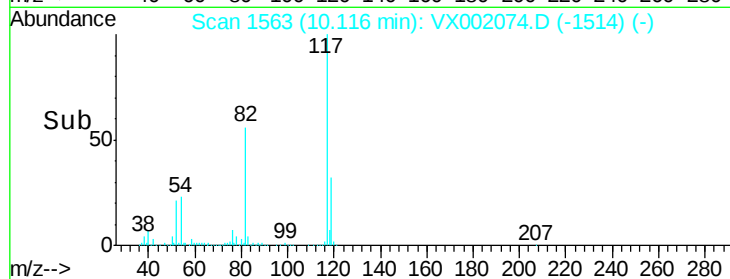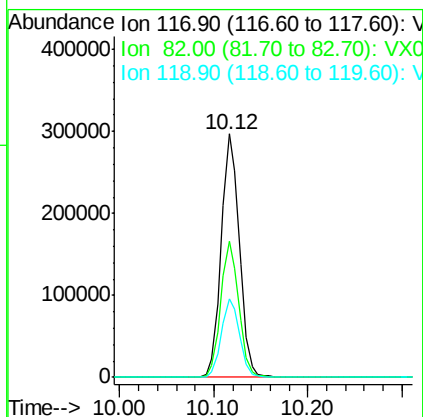

#68
m/p-Xylenes
Concen: 0.43 ug/l
RT: 10.36 min Scan# 1603
Delta R.T. -0.01 min
Lab File: VX002074.D
Acq: 27 May 2018 17:45

Tgt Ion	Ratio	Lower	Upper
106	100		
91	208.5	165.0	247.6


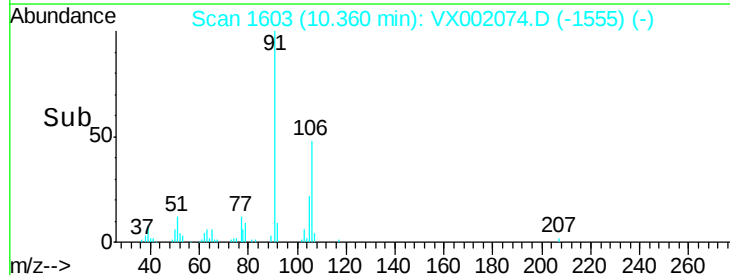
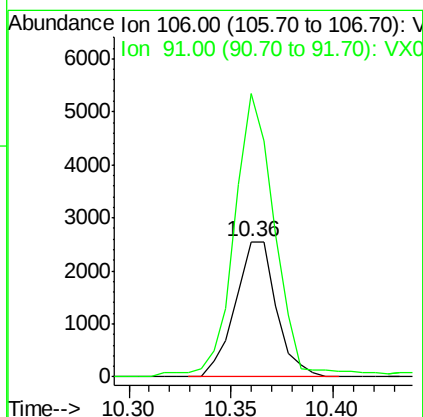





#69
o-Xylene
Concen: 0.34 ug/l
RT: 10.70 min Scan# 1659
Delta R.T. -0.00 min
Lab File: VX002074.D
Acq: 27 May 2018 17:45




Instrument :
MSVOA_X
ClientSampled :


Tot Ion:106 Resp: 2815
Ion Ratio Lower Upper
106 100
91 215.2 108.7 325.9

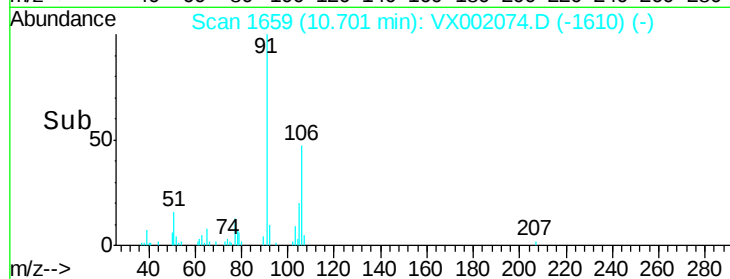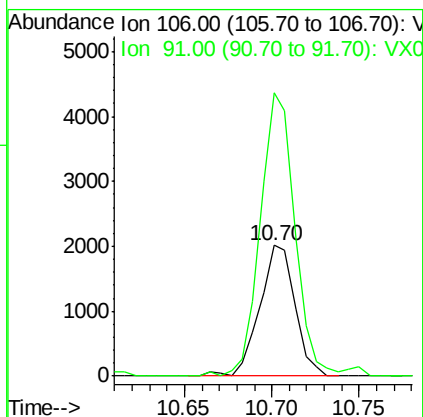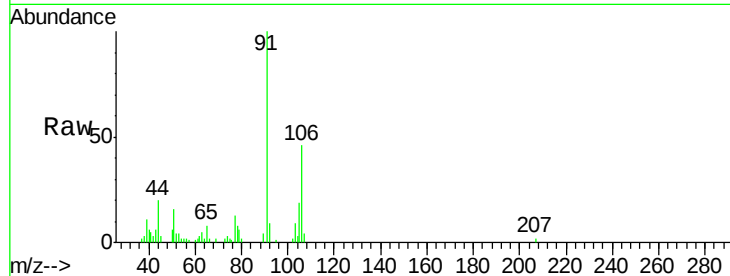

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.09 min Scan# 1886
Delta R.T. -0.00 min
Lab File: VX002074.D
Acq: 27 May 2018 17:45

Tgt Ion:152 Resp: 222546
Ion Ratio Lower Upper
152 100
115 54.6 42.3 126.8
150 156.4 0.0 351.0

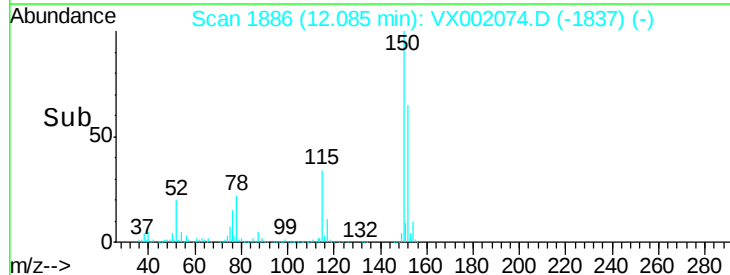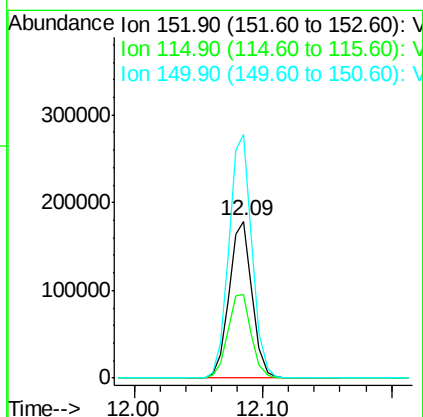



#74

N-amvl acetate

Concen: Below Cal

RT: 6.49 min Scan# 968





Delta R.T. 0.01 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45

Instrument :
MSVOA_X
ClientSampleId :

Tot Ion:	43	Resp:	146
Ion	Ratio	Lower	Upper
43	100		
70	15.8	0.1	0.1#
55	72.6	0.1	0.1#
61	0.0	14.5	21.7#

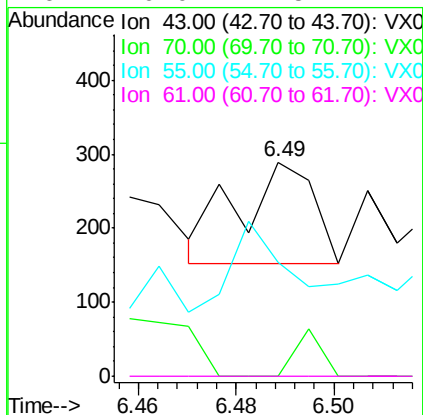

#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal




RT: 11.26 min Scan# 1751


Delta R.T. -0.01 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45

Tgt Ion:	83	Resp:	90
Ion	Ratio	Lower	Upper
83	100		
131	0.0	5.7	17.0#
85	0.0	32.6	97.7#

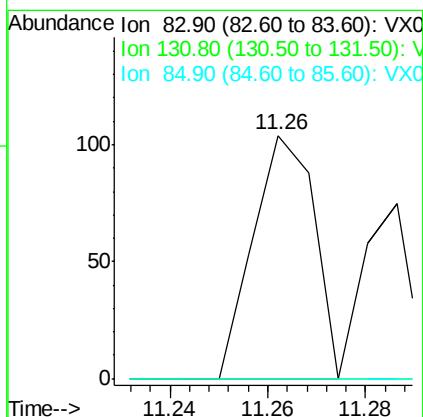

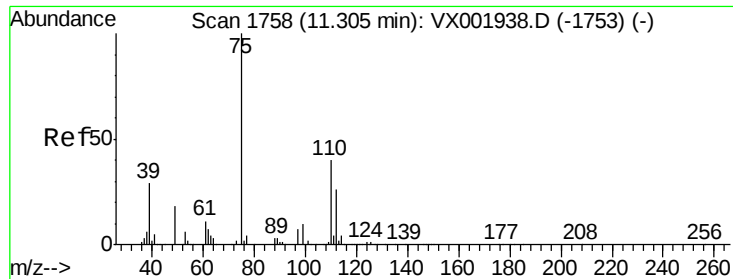

#76

1,2,3-Trichloropropane

Concen: 21.84 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.16 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 75 Resp: 116722

Ion Ratio Lower Upper




75 100

77 1.3 22.8 68.3#

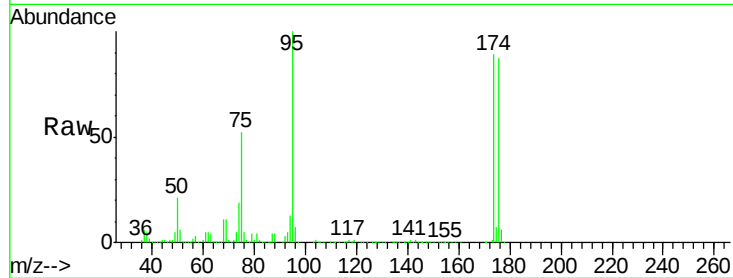

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

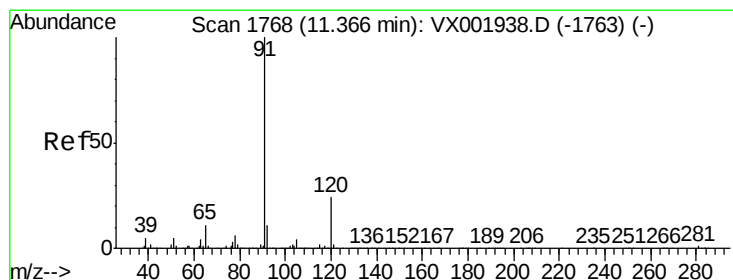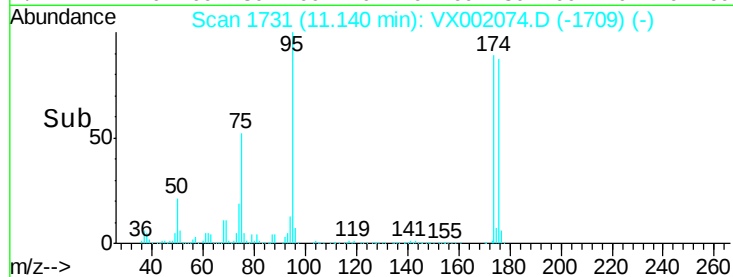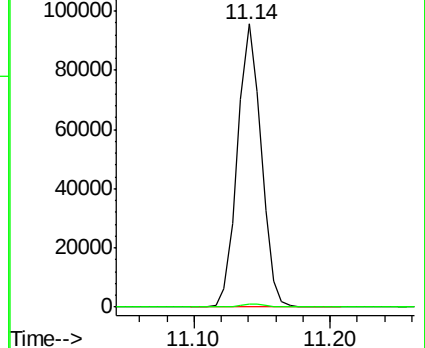

#78

n-propylbenzene

Concen: 0.21 ug/l

RT: 11.36 min Scan# 1767

Delta R.T. -0.01 min

Lab File: VX002074.D


Acq: 27 May 2018 17:45

Tgt Ion: 91 Resp: 4470

Ion Ratio Lower Upper



91 100


120 23.9 11.9 35.7

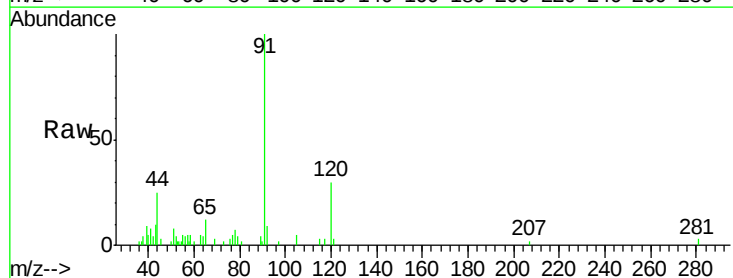

Abundance Ion 91.00 (90.70 to 91.70): VX0

Ion 120.00 (119.70 to 120.70): V

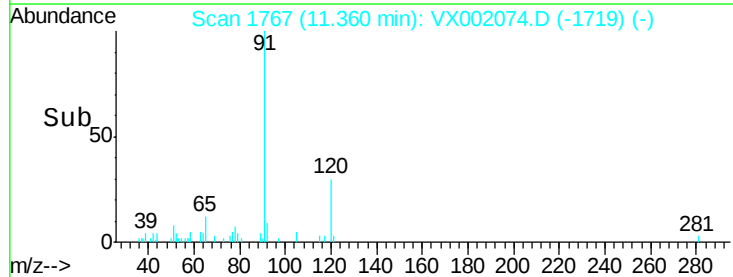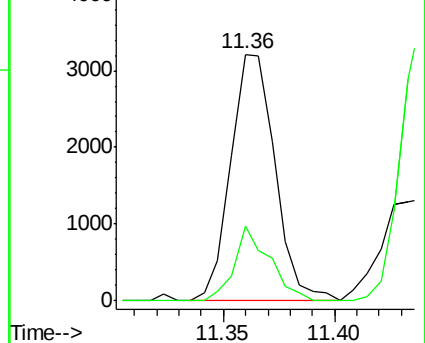

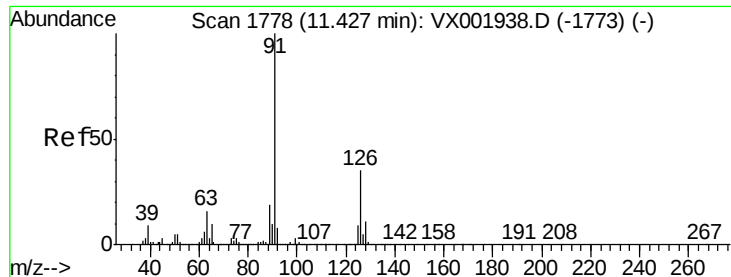

#79

2-Chlorotoluene

Concen: Below Cal

RT: 11.44 min Scan# 1780

Delta R.T. 0.01 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45

Instrument :

MSVOA_X





ClientSampleId :

Tot Ion: 91 Resp: 3184

Ion Ratio Lower Upper

91 100

126 7.2 17.4 52.2#

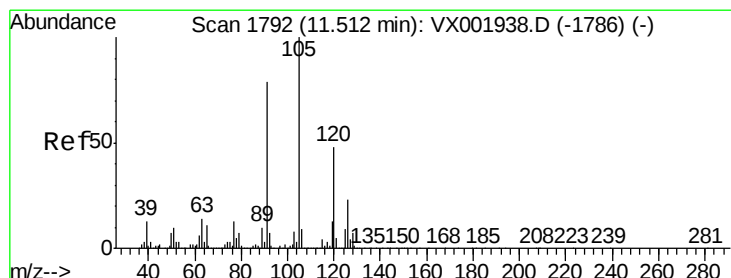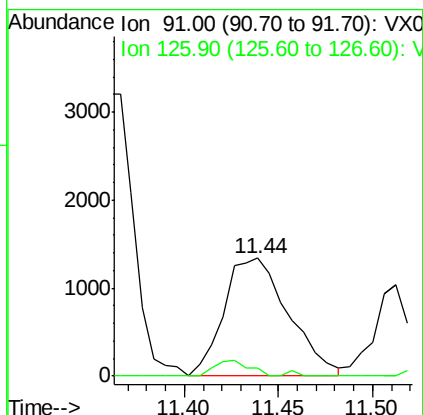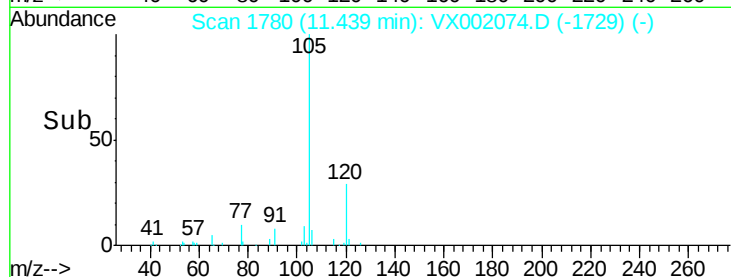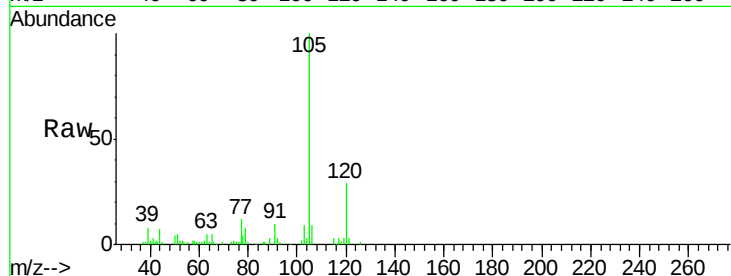

#80

1,3,5-Trimethylbenzene

Concen: 0.57 ug/l

RT: 11.51 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX002074.D




Acq: 27 May 2018 17:45


Tgt Ion: 105 Resp: 9151

Ion Ratio Lower Upper

105 100

120 50.1 24.1 72.4

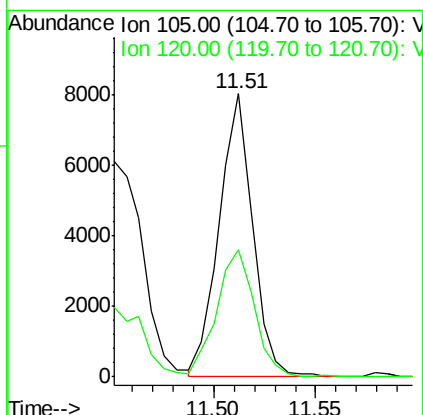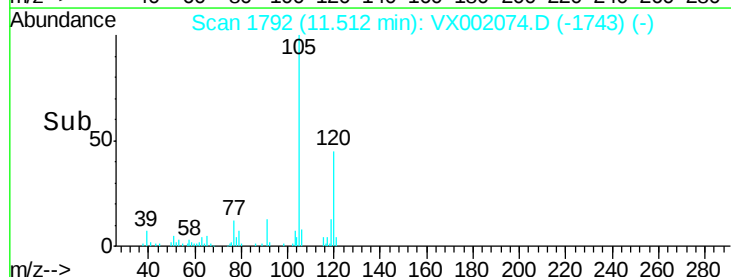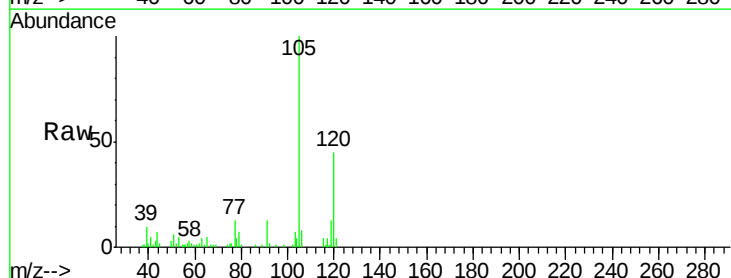

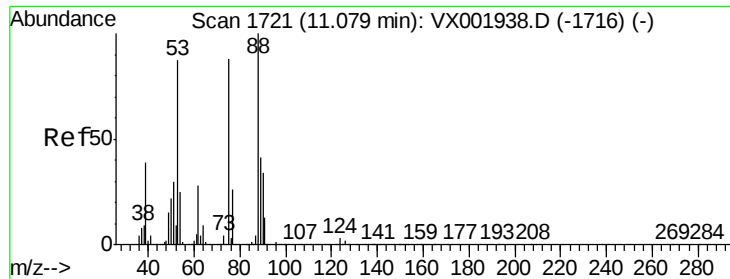

#81

trans-1,4-Dichloro-2-butene

Concen: 52.48 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.06 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45

Instrument :

MSVOA_X

ClientSampled :


Tot Ion: 75 Resp: 116722

Ion Ratio Lower Upper

75 100

53 0.1 78.0 117.0#




89 0.0 39.4 59.2#

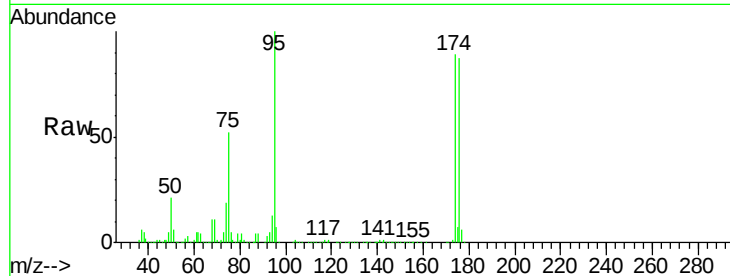

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

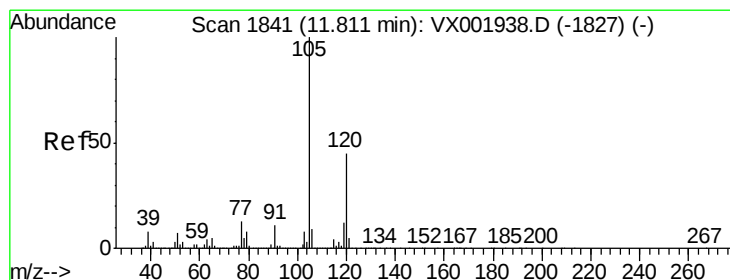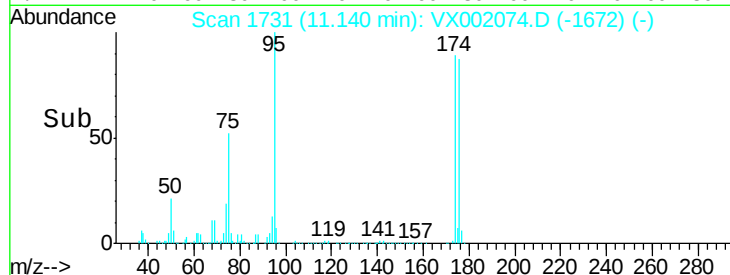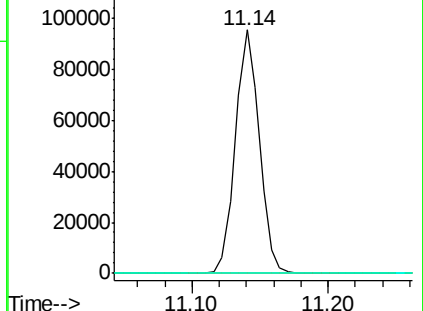

#84

1,2,4-Trimethylbenzene

Concen: 2.44 ug/l

RT: 11.81 min Scan# 1841

Delta R.T. 0.00 min

Lab File: VX002074.D


Acq: 27 May 2018 17:45

Tgt Ion: 105 Resp: 40618

Ion Ratio Lower Upper



105 100


120 45.7 22.1 66.5



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

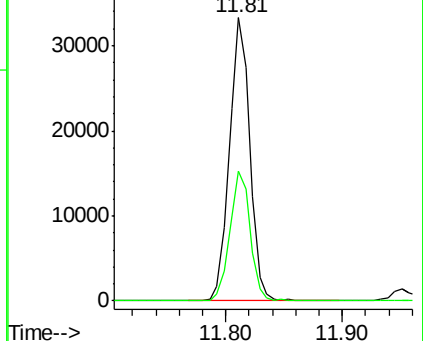

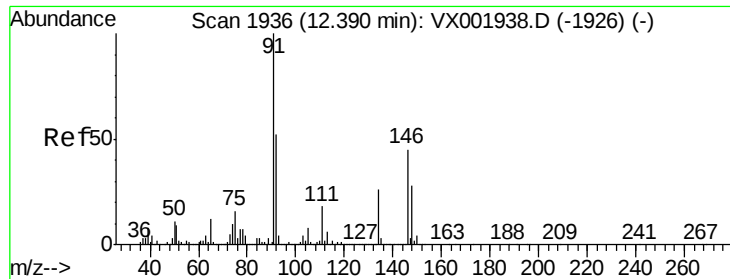

#89

n-Butylbenzene

Concen: 0.21 ug/l

RT: 12.39 min Scan# 1936

Delta R.T. 0.00 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45

Instrument :

MSVOA_X

ClientSampled :





Tot Ion: 91 Resp: 3029

Ion Ratio Lower Upper

91 100

92 35.3 26.3 78.9

134 107.4 13.6 40.7#

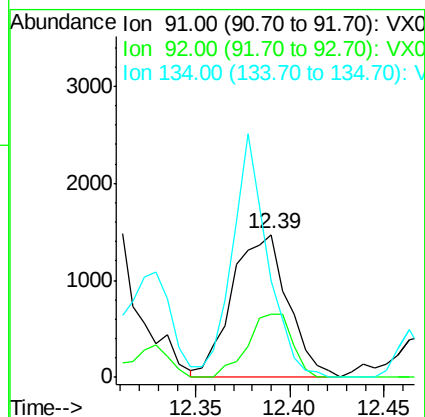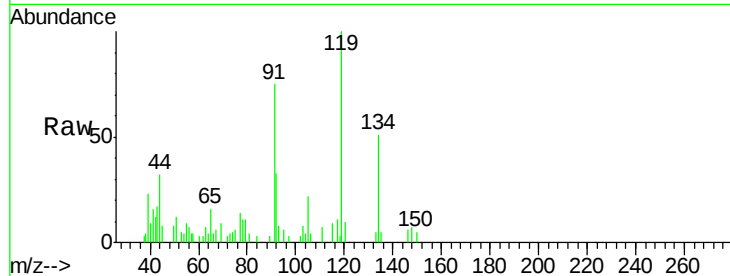

#95

Naphthalene

Concen: 5.81 ug/l

RT: 13.84 min Scan# 2174

Delta R.T. -0.00 min

Lab File: VX002074.D

Acq: 27 May 2018 17:45

Tgt Ion: 128 Resp: 116804

Ion Ratio Lower Upper

128 100

127 13.5 10.4 15.6

129 11.0 8.8 13.2

