


Data Path : W:\HPCHEM1\MSVOA X\Data\VX052718\
Data File : VX002060.D
Acq On : 27 May 2018 10:53
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Title : SW846 8260
Last Update : Thu May 24 13:09:03 2018

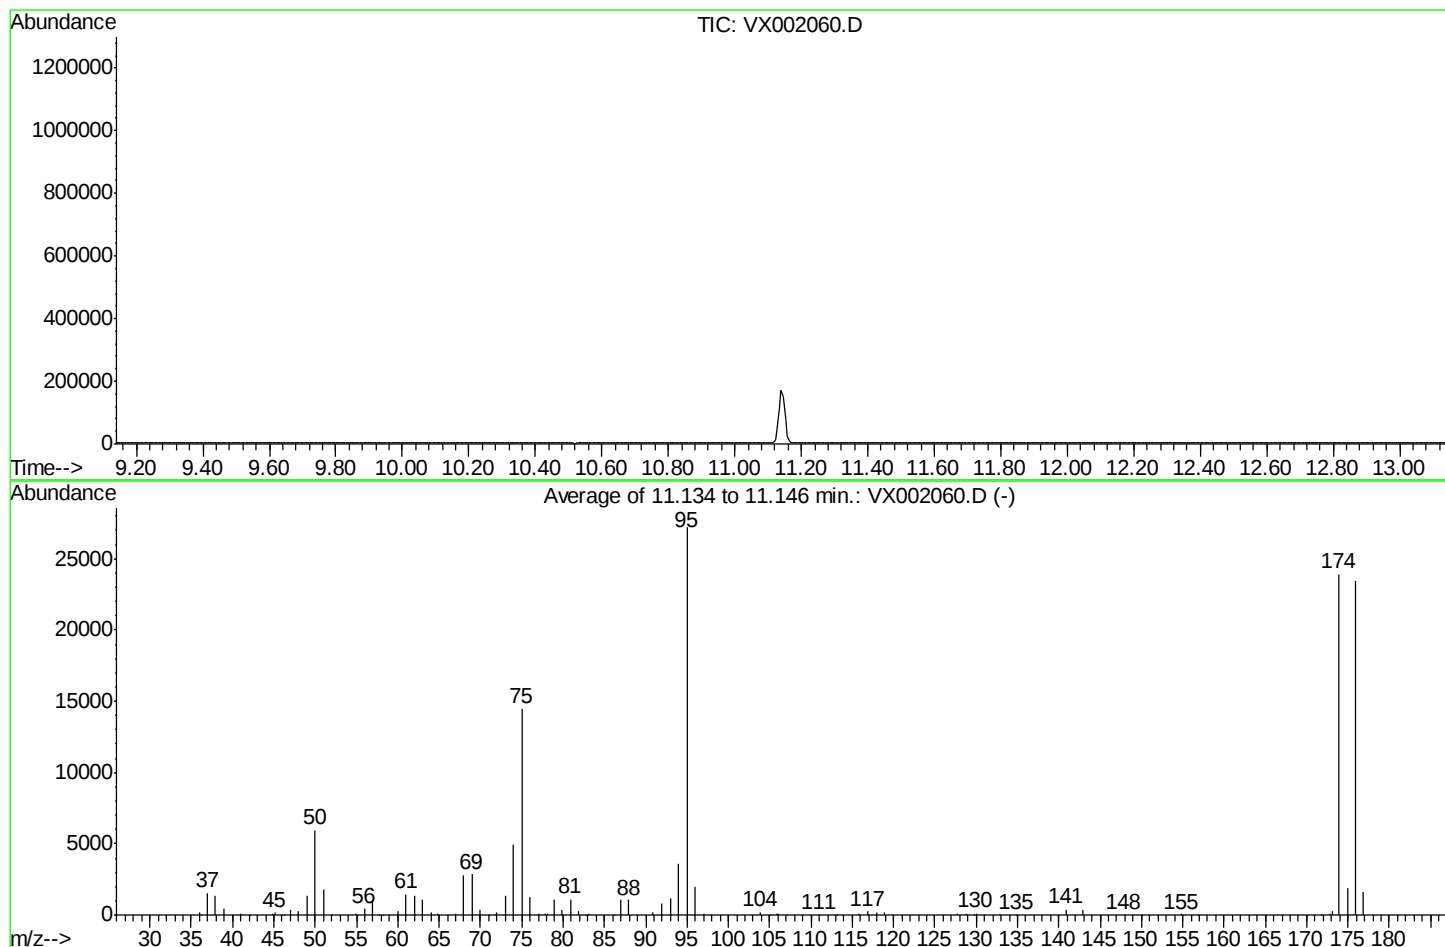

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	5945	PASS
75	95	30	60	53.3	14509	PASS
95	95	100	100	100.0	27208	PASS
96	95	5	9	7.2	1970	PASS
173	174	0.00	2	1.1	259	PASS
174	95	50	100	87.9	23919	PASS
175	174	5	9	7.9	1895	PASS
176	174	95	101	97.9	23422	PASS
177	176	5	9	6.8	1581	PASS